


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072521\
 Data File : BN015689.D
 Acq On : 24 Jul 2021 15:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 26 02:17:00 2021

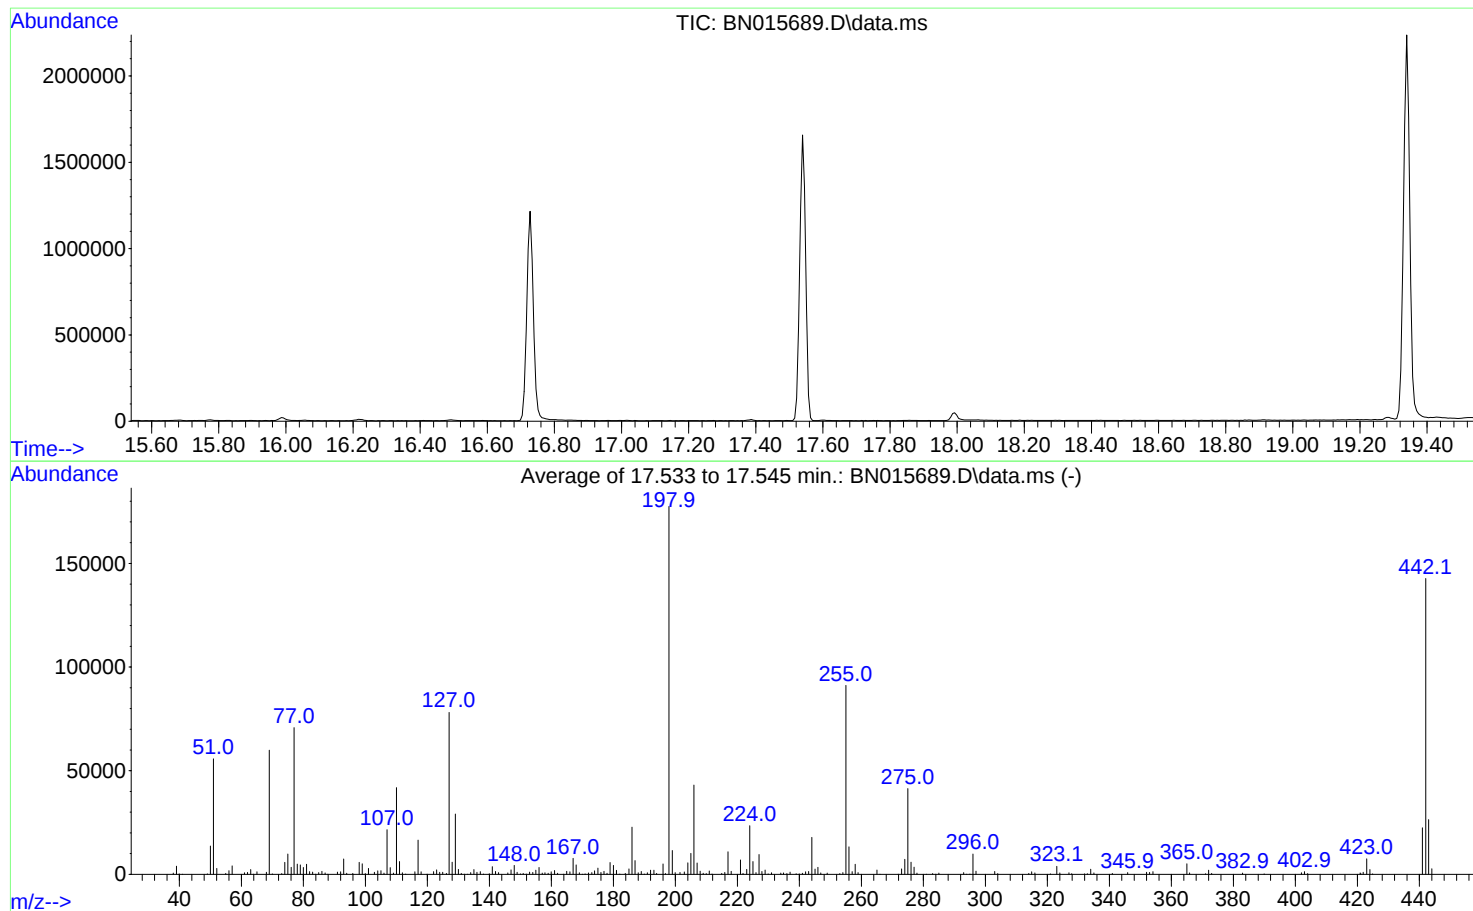




AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	55755	PASS
68	69	0.00	2	1.7	1041	PASS
69	198	0.00	100	33.8	59891	PASS
70	69	0.00	2	0.4	228	PASS
127	198	10	80	44.0	78141	PASS
197	198	0.00	2	0.2	405	PASS
198	198	100	100	100.0	177451	PASS
199	198	5	9	6.5	11521	PASS
275	198	10	60	23.3	41411	PASS
365	198	1	100	2.9	5067	PASS
441	198	0.01	100	12.6	22445	PASS
442	442	50	100	100.0	142680	PASS
443	442	15	24	18.5	26405	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072521\
Data File : BN015689.D
Acq On : 24 Jul 2021 15:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 26 06:53:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 06:53:05 2021
Response via : Initial Calibration

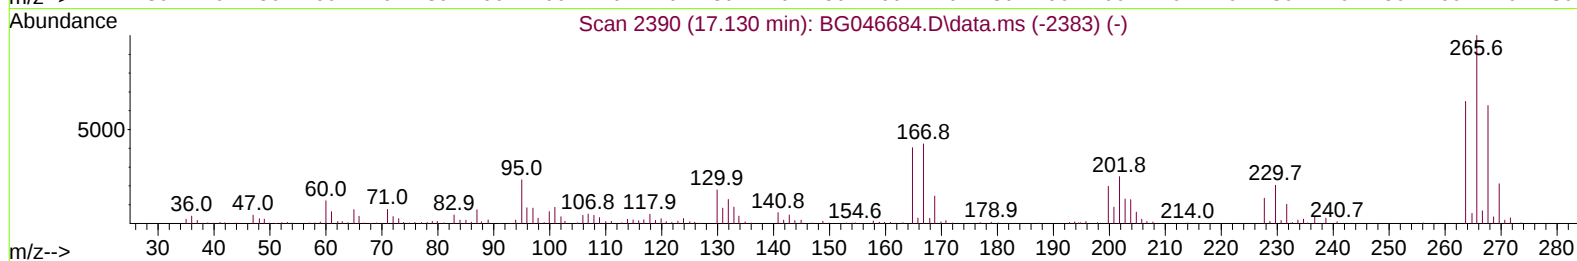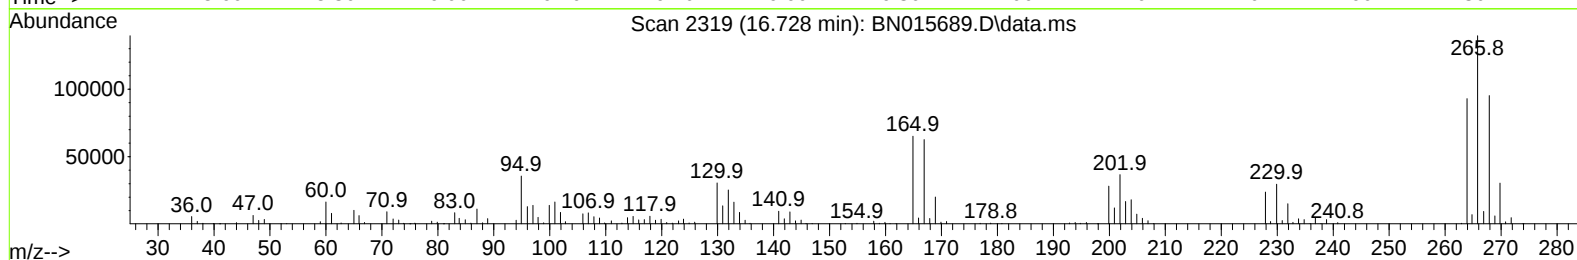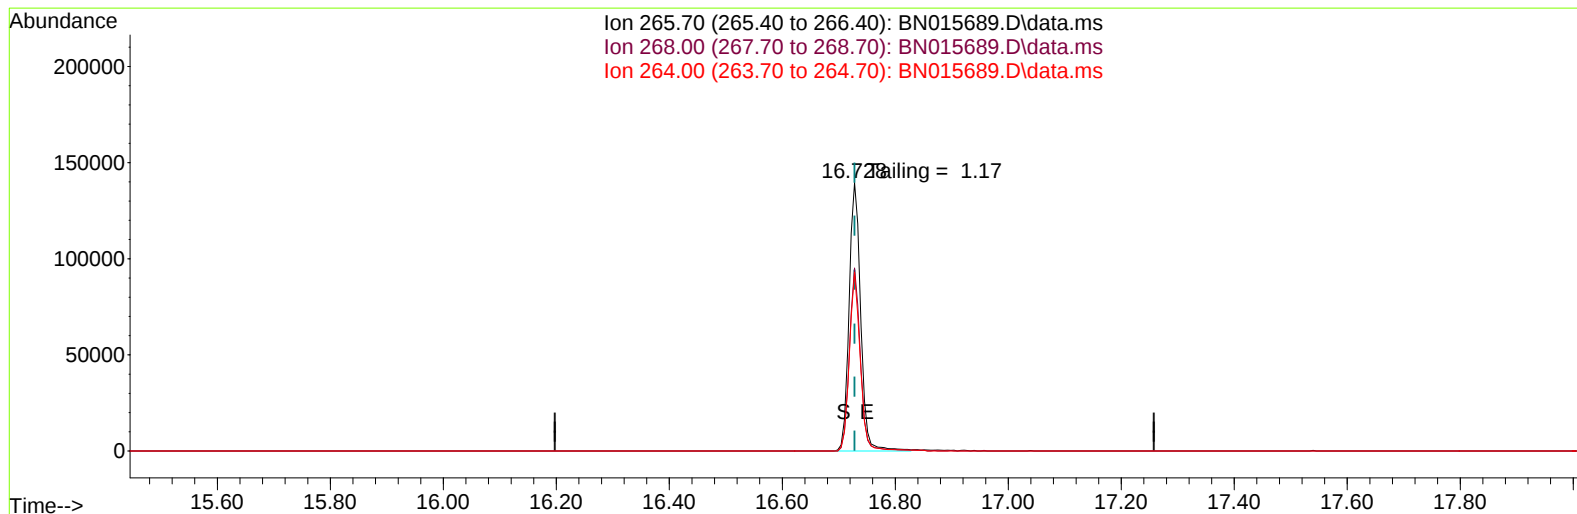

TIC: BN015689.D\data.ms

(70) Pentachlorophenol (C)

16.728min (0.000) 26744.29 ng




response 200018

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.21
264.00	61.60	66.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072521\
Data File : BN015689.D
Acq On : 24 Jul 2021 15:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 26 06:53:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 06:53:05 2021
Response via : Initial Calibration

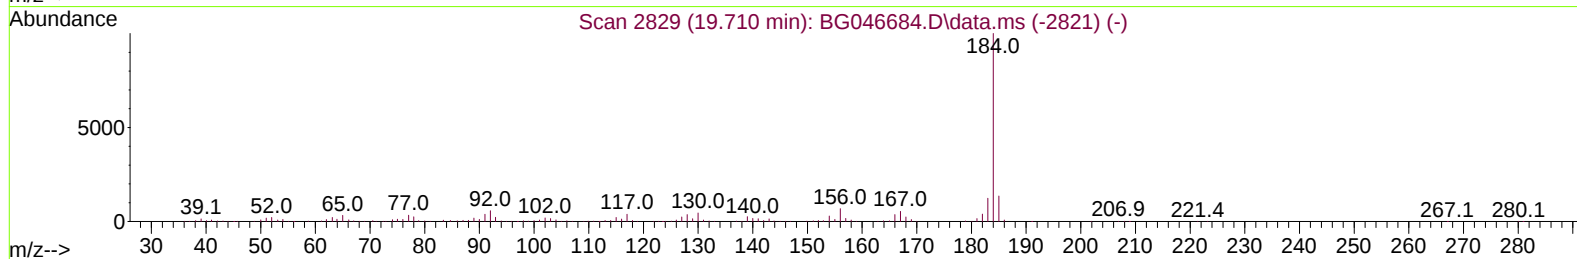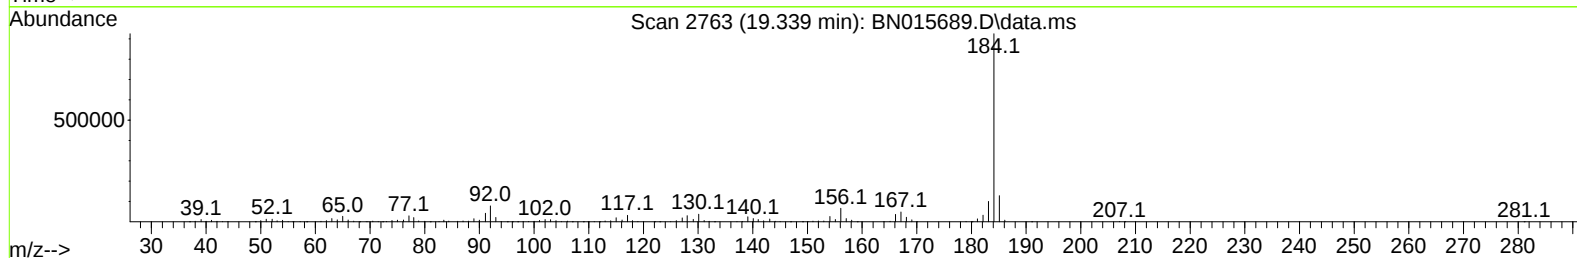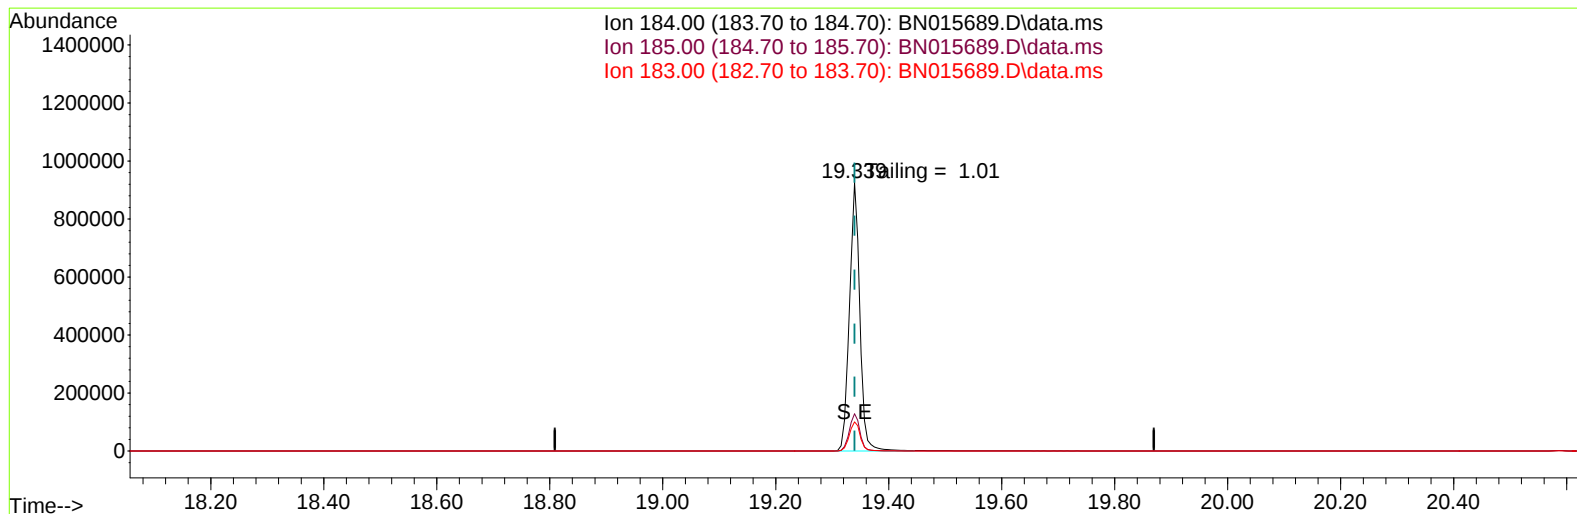

TIC: BN015689.D\data.ms

(77) Benzidine

19.339min (0.000) 0.00 ng

response 1187049

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.90
183.00	13.20	10.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/25/2021	BNA_N	<u>BN015689.D</u>
Compound Name	Response	Retention Time
DDT	492886	20.586
DDD	50108	20.145
DDE	574	19.633
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
50682	543568	9.32

Instrument :
BNA_N
ClientSampleId :
DFTPP