

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
 Data File : BN020833.D
 Acq On : 25 Jul 2022 19:58
 Operator : CG/JU
 Sample : PB146371BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK3711

Quant Time: Jul 26 00:31:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 18:06:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	2486	0.400	ng/ul	0.00
4) Naphthalene-d8	10.612	136	10914	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.470	164	6792	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.217	188	14288	0.400	ng/ul	0.00
17) Chrysene-d12	21.432	240	11639	0.400	ng/ul	0.00
23) Perylene-d12	23.764	264	12326	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.214	96	22972	7.690	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.223	152	5797	0.350	ng/ul	0.00
18) Fluoranthene-d10	19.258	212	14033	0.377	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.460	166	1941	0.065	ng/ul#	14
20) Pyrene	19.620	202	1959	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.615	252	3857	0.072	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
Data File : BN020833.D
Acq On : 25 Jul 2022 19:58
Operator : CG/JU
Sample : PB146371BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK3711

Quant Time: Jul 26 00:31:23 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 18:06:54 2022
Response via : Initial Calibration




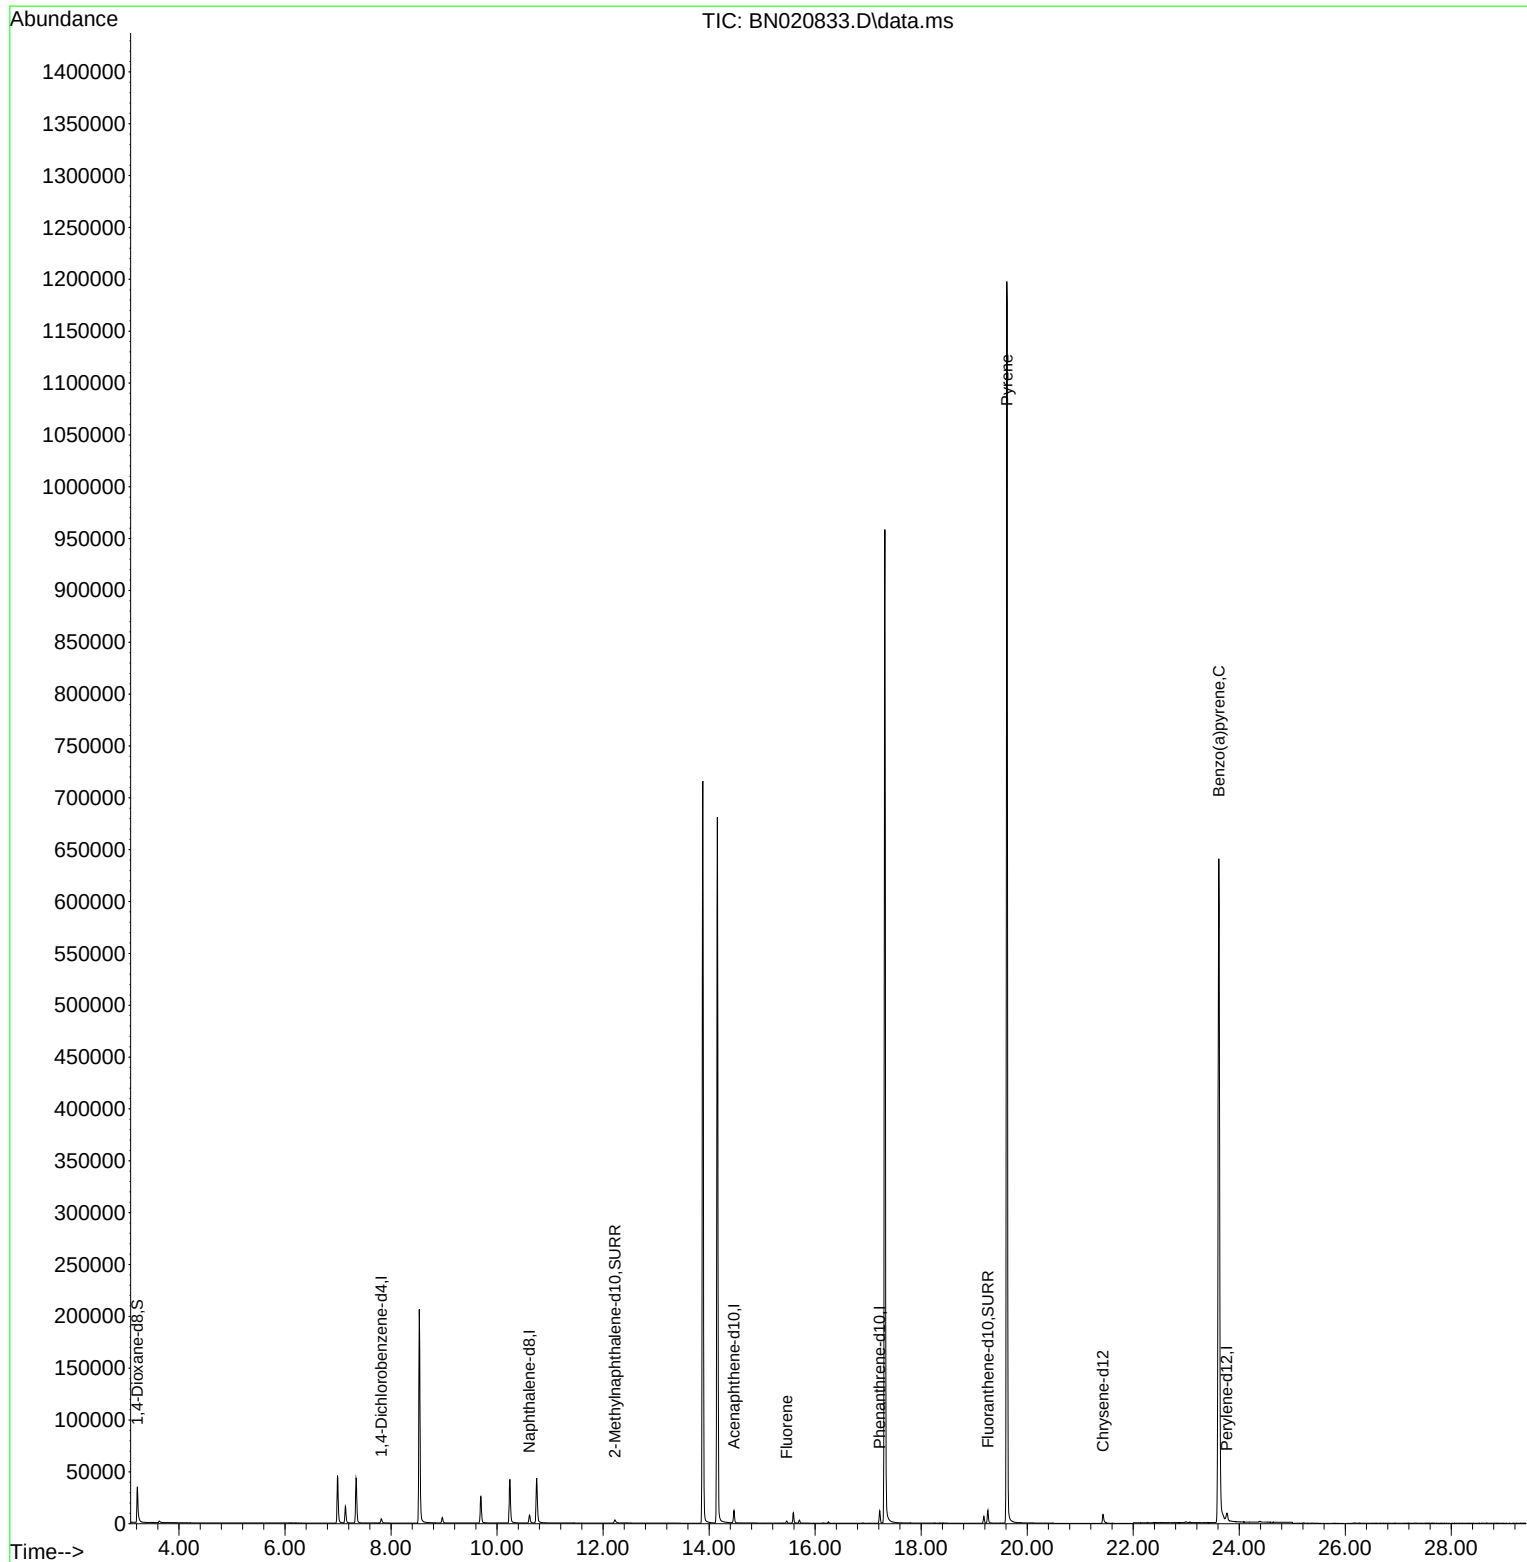


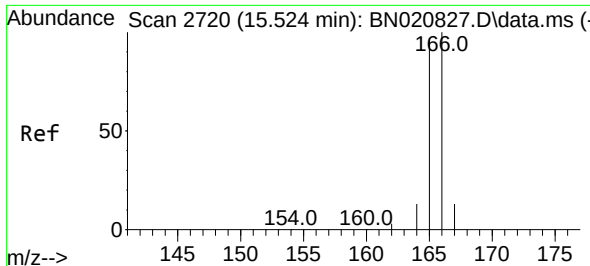

#12
Fluorene
Concen: 0.065 ng/ul
RT: 15.460 min Scan# 21
Delta R.T. -0.065 min
Lab File: BN020833.D
Acq: 25 Jul 2022 19:58




Instrument :
BNA_N
ClientSampleId :
SBLK3711


Tgt Ion:166 Resp: 1941
Ion Ratio Lower Upper
166 100
165 7.3 78.2 117.2#
167 32.0 11.3 16.9#

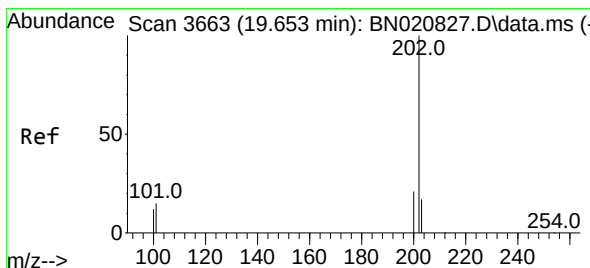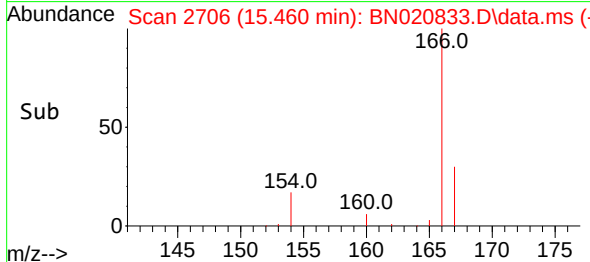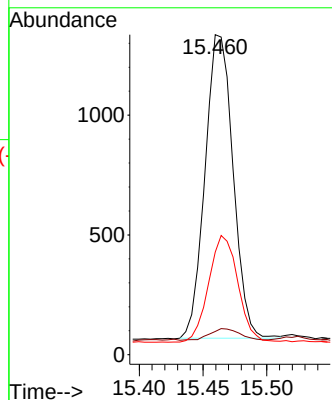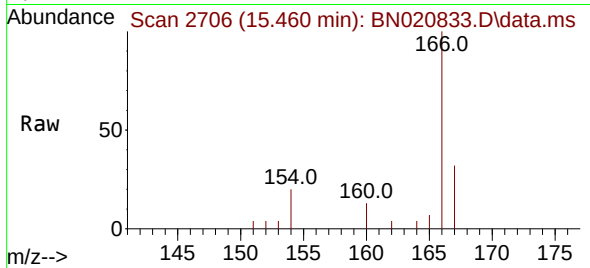

#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.620 min Scan# 3656
Delta R.T. -0.032 min
Lab File: BN020833.D
Acq: 25 Jul 2022 19:58

Tgt Ion:202 Resp: 1959
Ion Ratio Lower Upper
202 100
101 173.1 11.6 17.4#
100 1253.4 9.2 13.8#

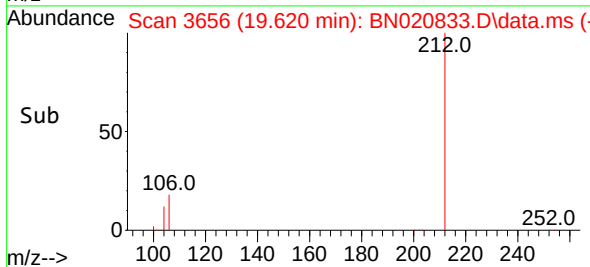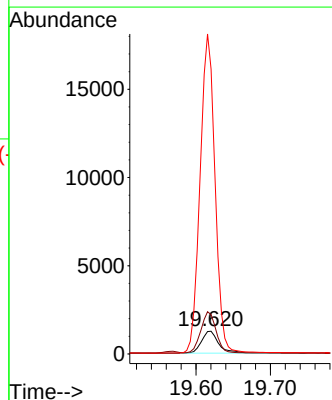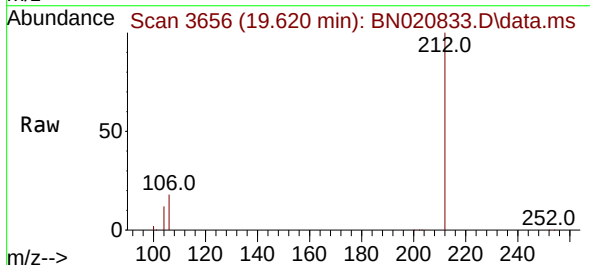

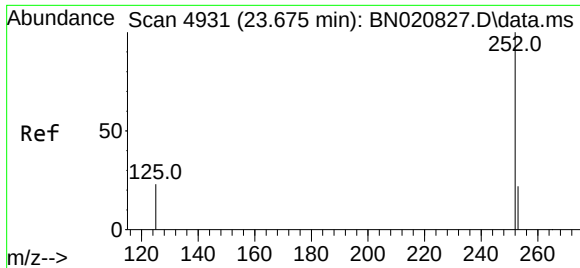

#26

Benzo(a)pyrene

Concen: 0.072 ng/ul

RT: 23.615 min Scan# 4911

Delta R.T. -0.060 min

Lab File: BN020833.D


Acq: 25 Jul 2022 19:58

Instrument :

BNA_N

ClientSampleId :

SBLK3711

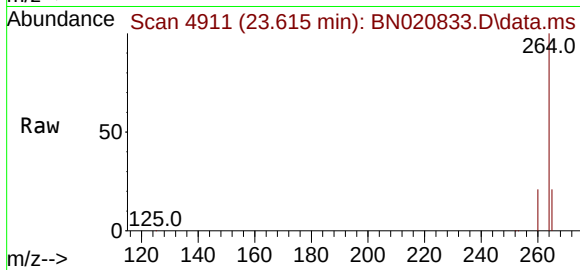

Tgt Ion:252 Resp: 3857

Ion Ratio Lower Upper

252 100

253 40.8 21.0 31.4#

125 33.0 18.8 28.2#

