

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
 Data File : BN020835.D
 Acq On : 25 Jul 2022 21:51
 Operator : CG/JU
 Sample : PB146369BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK369

Quant Time: Jul 26 00:31:31 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 18:06:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	2277	0.400	ng/ul	0.00
4) Naphthalene-d8	10.612	136	7823	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.470	164	4742	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.217	188	9735	0.400	ng/ul	0.00
17) Chrysene-d12	21.429	240	7694	0.400	ng/ul	0.00
23) Perylene-d12	23.764	264	9170	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.214	96	16798	6.140	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.223	152	4263	0.359	ng/ul	0.00
18) Fluoranthene-d10	19.258	212	9975	0.406	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.615	202	1477	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.612	252	3173	0.079	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
Data File : BN020835.D
Acq On : 25 Jul 2022 21:51
Operator : CG/JU
Sample : PB146369BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK369

Quant Time: Jul 26 00:31:31 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 18:06:54 2022
Response via : Initial Calibration




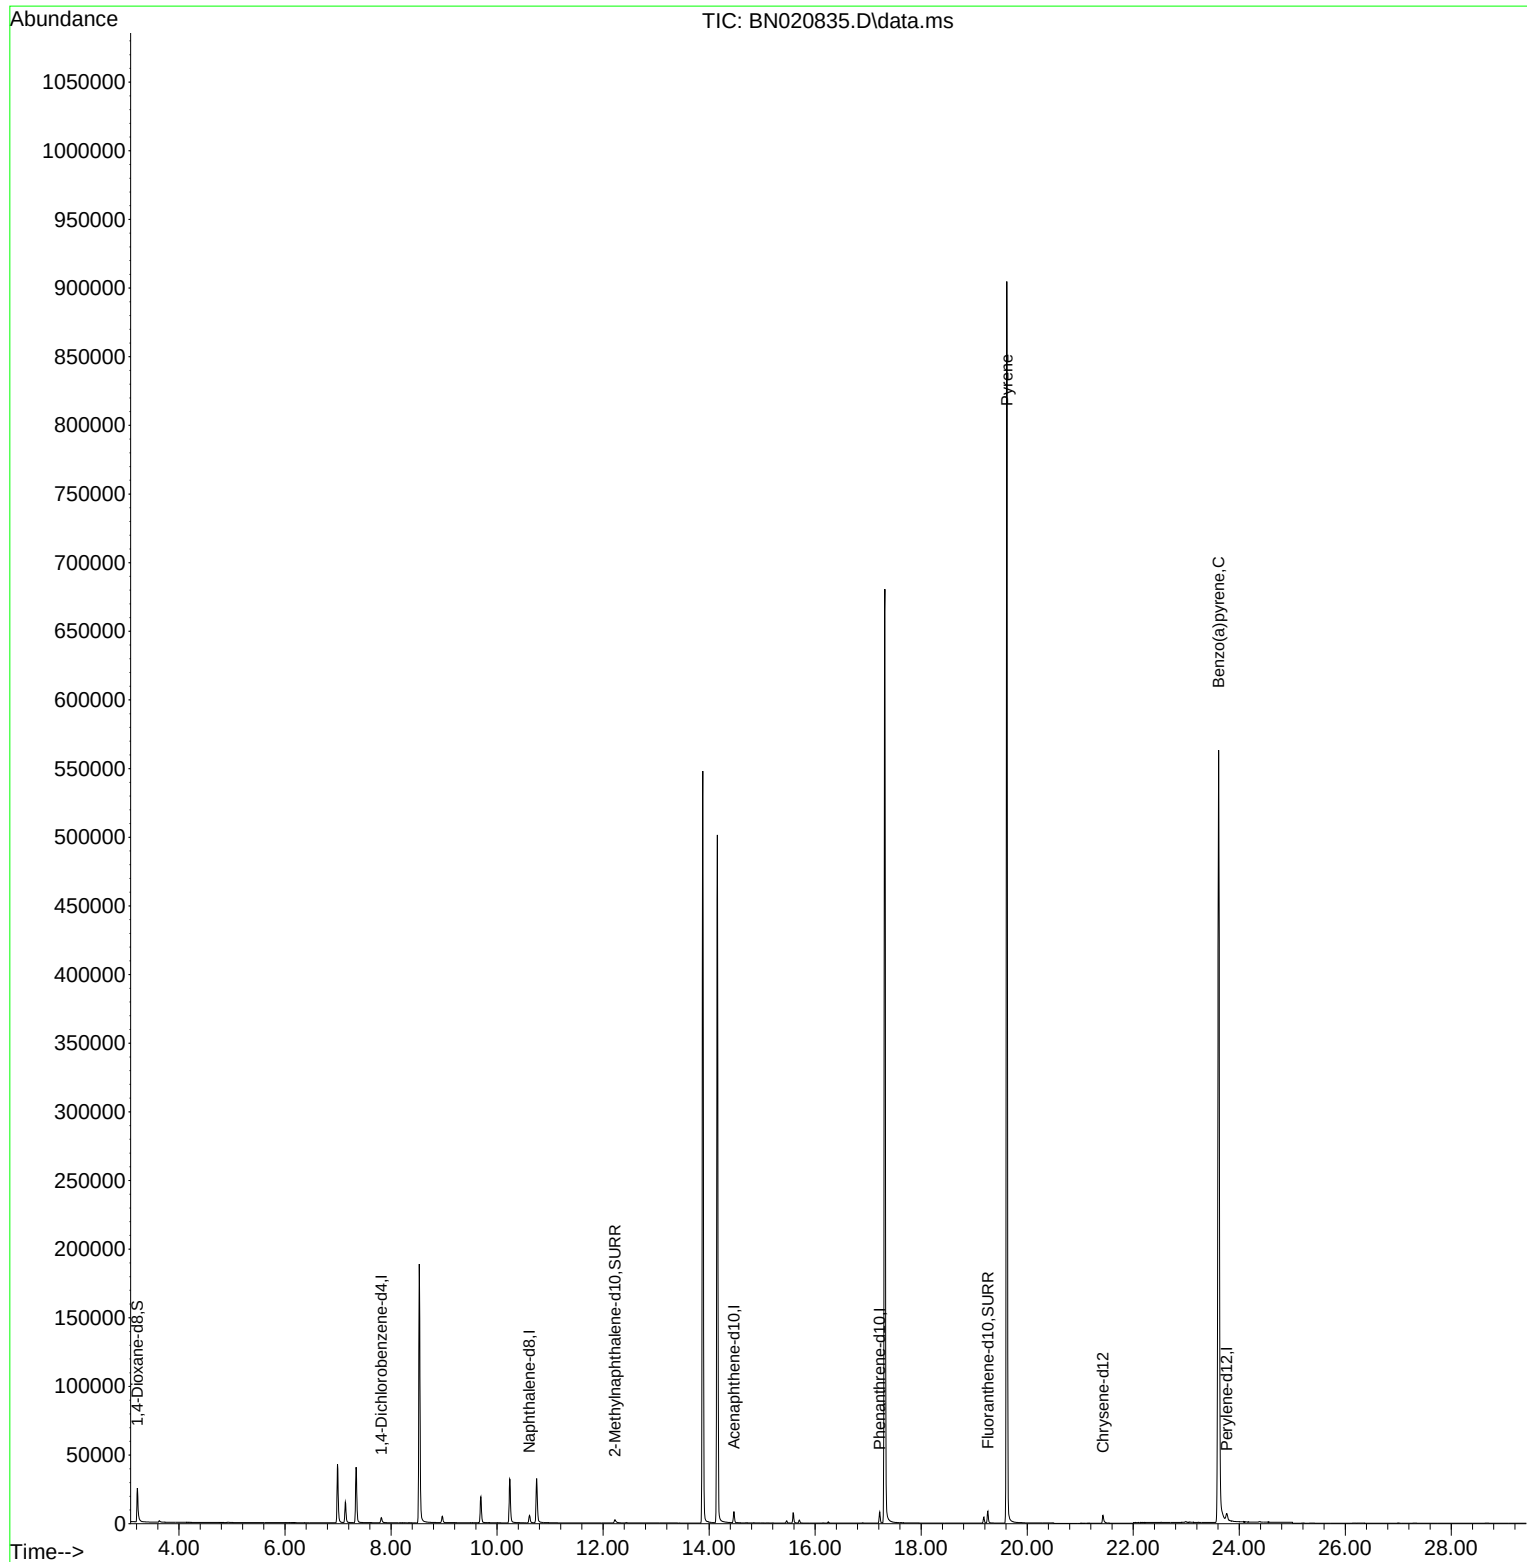


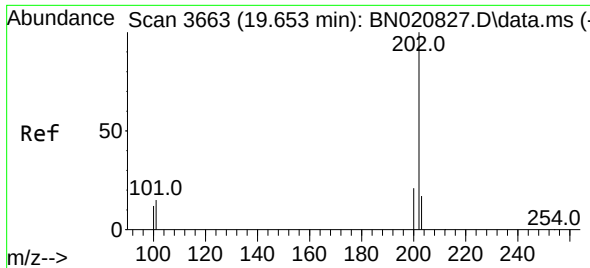

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.615 min Scan# 3655
Delta R.T. -0.037 min
Lab File: BN020835.D
Acq: 25 Jul 2022 21:51

Instrument :
BNA_N
ClientSampleId :
SBLK369

Tgt Ion:202 Resp: 1477
Ion Ratio Lower Upper
202 100
101 185.5 11.6 17.4#
100 1375.0 9.2 13.8#

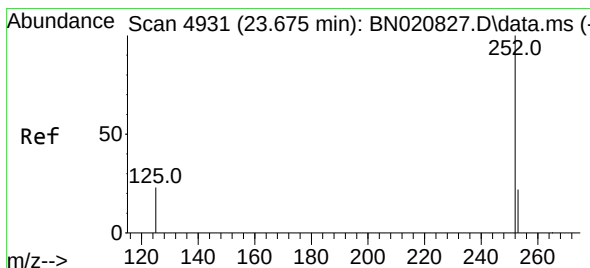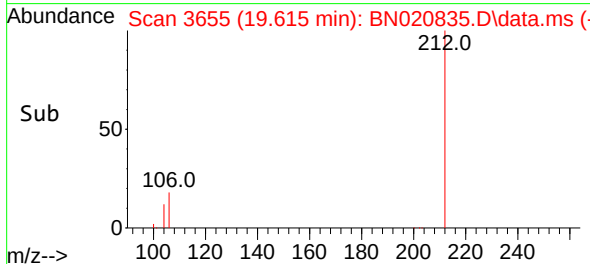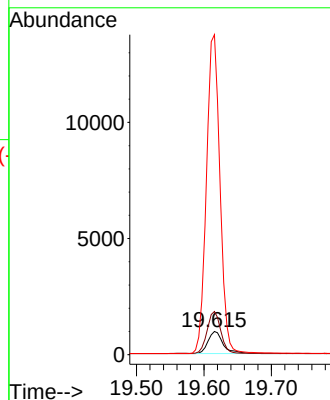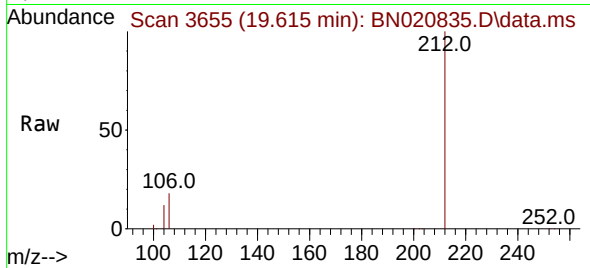

#26
Benzo(a)pyrene
Concen: 0.079 ng/ul
RT: 23.612 min Scan# 4910
Delta R.T. -0.063 min
Lab File: BN020835.D
Acq: 25 Jul 2022 21:51

Tgt Ion:252 Resp: 3173
Ion Ratio Lower Upper
252 100
253 42.4 21.0 31.4#
125 34.7 18.8 28.2#

