

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
 Data File : BN020848.D
 Acq On : 26 Jul 2022 05:54
 Operator : CG/JU
 Sample : N3801-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBHW7

Quant Time: Jul 26 06:35:18 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 18:06:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	2779	0.400	ng/ul	0.00
4) Naphthalene-d8	10.606	136	9827	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.465	164	6011	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	12895	0.400	ng/ul	0.00
17) Chrysene-d12	21.422	240	11035	0.400	ng/ul	0.00
23) Perylene-d12	23.760	264	12400	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.214	96	12841	3.846	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.212	152	4870	0.326	ng/ul	0.00
18) Fluoranthene-d10	19.253	212	13797	0.391	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.252	88	782	0.228	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
Data File : BN020848.D
Acq On : 26 Jul 2022 05:54
Operator : CG/JU
Sample : N3801-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBHW7

Quant Time: Jul 26 06:35:18 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 18:06:54 2022
Response via : Initial Calibration

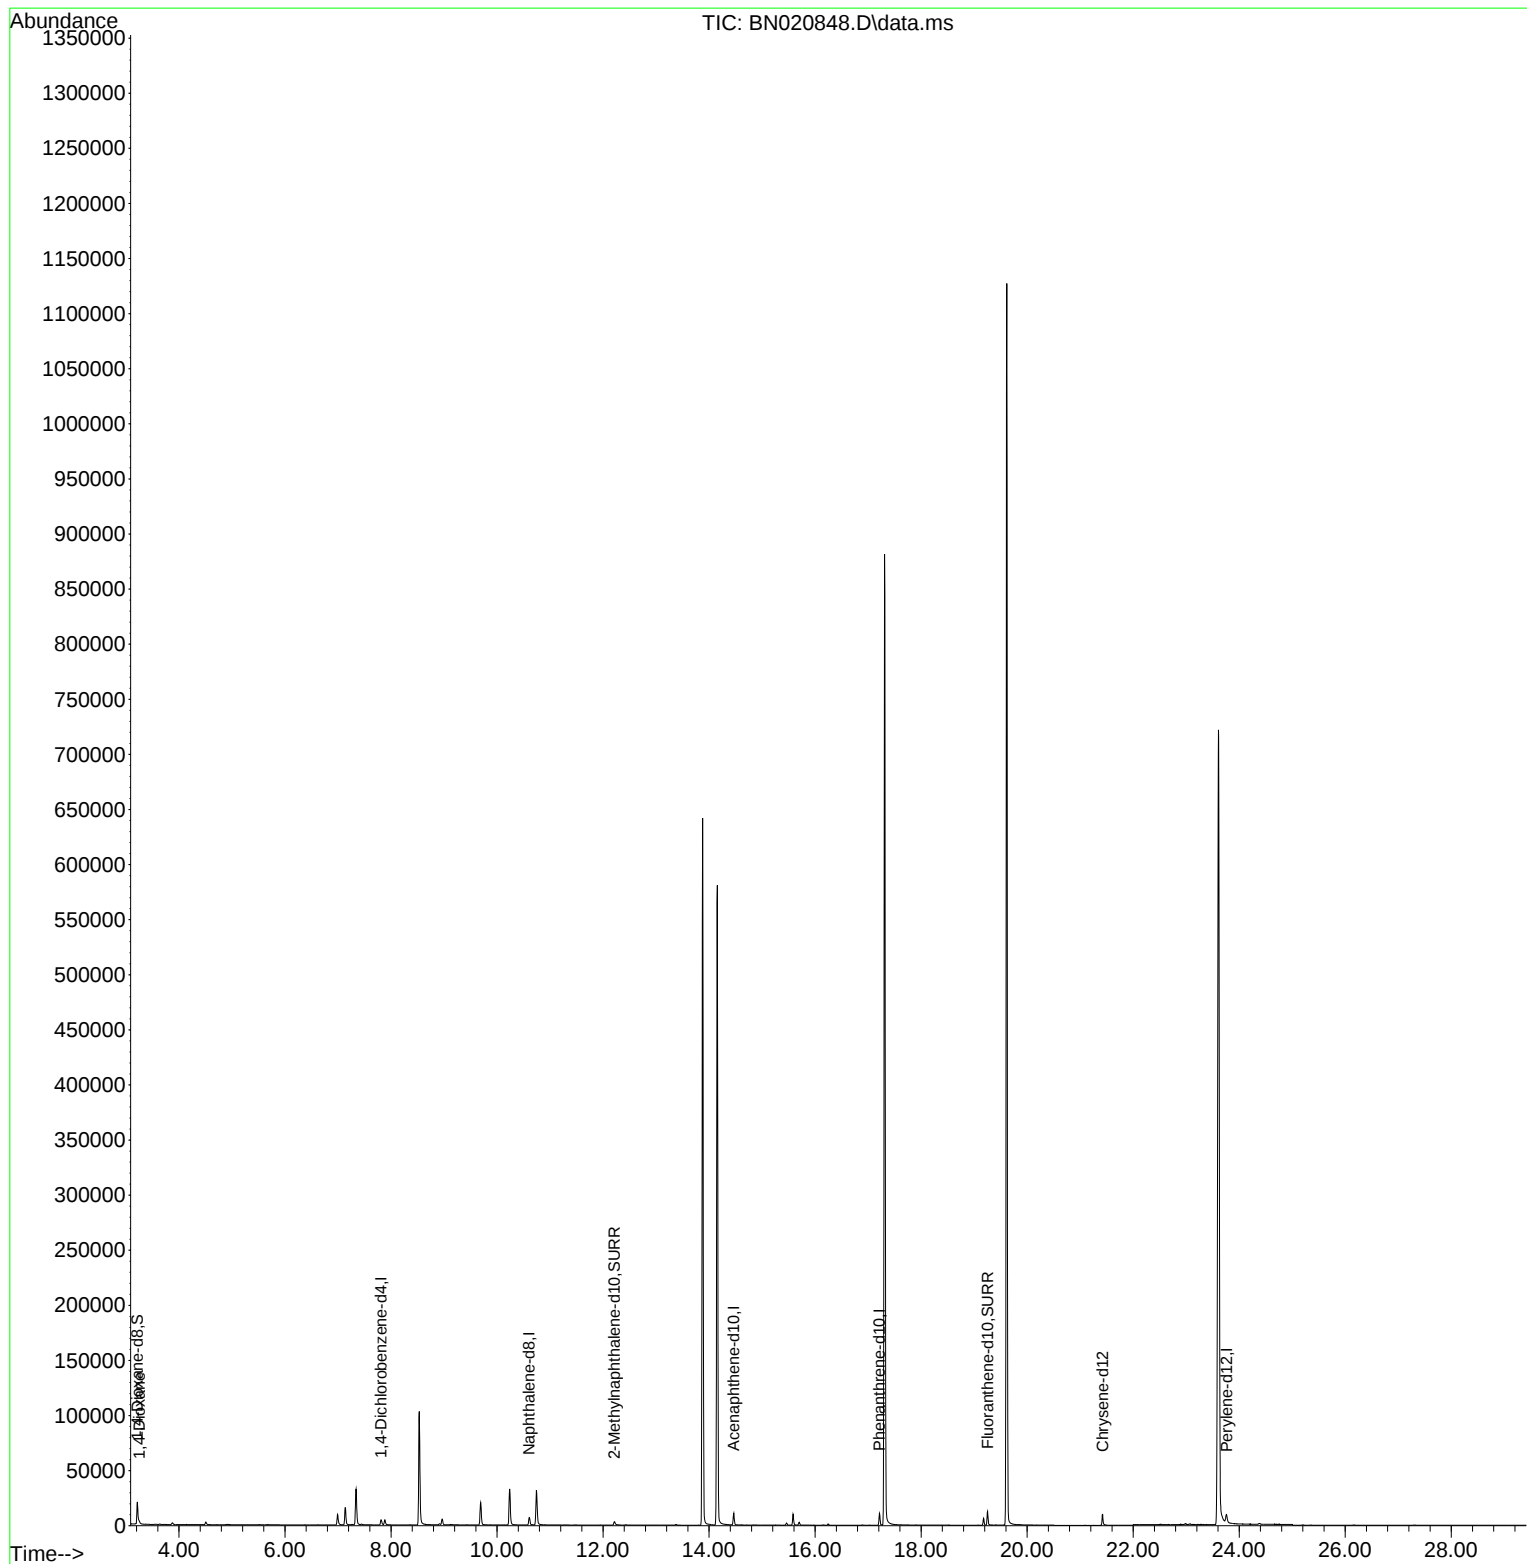

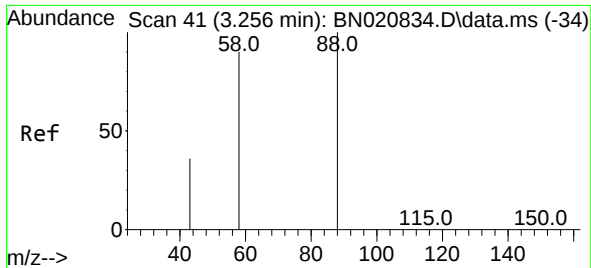

#2
 1,4-Dioxane
 Concen: 0.228 ng/ul
 RT: 3.252 min Scan# 40
 Delta R.T. -0.004 min
 Lab File: BN020848.D
 Acq: 26 Jul 2022 05:54

Instrument :
 BNA_N
 ClientSampleId :
 GBHW7

Tgt Ion:	88	Resp:	782
Ion	Ratio	Lower	Upper
88	100		
43	35.8	32.5	48.7
58	45.6	46.2	69.2#

