

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
 Data File : BN020864.D
 Acq On : 26 Jul 2022 16:20
 Operator : CG/JU
 Sample : N3801-19
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBHY4

Quant Time: Jul 26 17:21:53 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 18:06:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	2315	0.400	ng/ul	0.00
4) Naphthalene-d8	10.612	136	7821	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.465	164	4968	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	10364	0.400	ng/ul	0.00
17) Chrysene-d12	21.426	240	8455	0.400	ng/ul	0.00
23) Perylene-d12	23.764	264	8757	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.214	96	14996	5.391	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.212	152	5017	0.422	ng/ul	0.00
18) Fluoranthene-d10	19.253	212	13083	0.484	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.252	88	172	0.060	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
Data File : BN020864.D
Acq On : 26 Jul 2022 16:20
Operator : CG/JU
Sample : N3801-19
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBHY4


Quant Time: Jul 26 17:21:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 18:06:54 2022
Response via : Initial Calibration

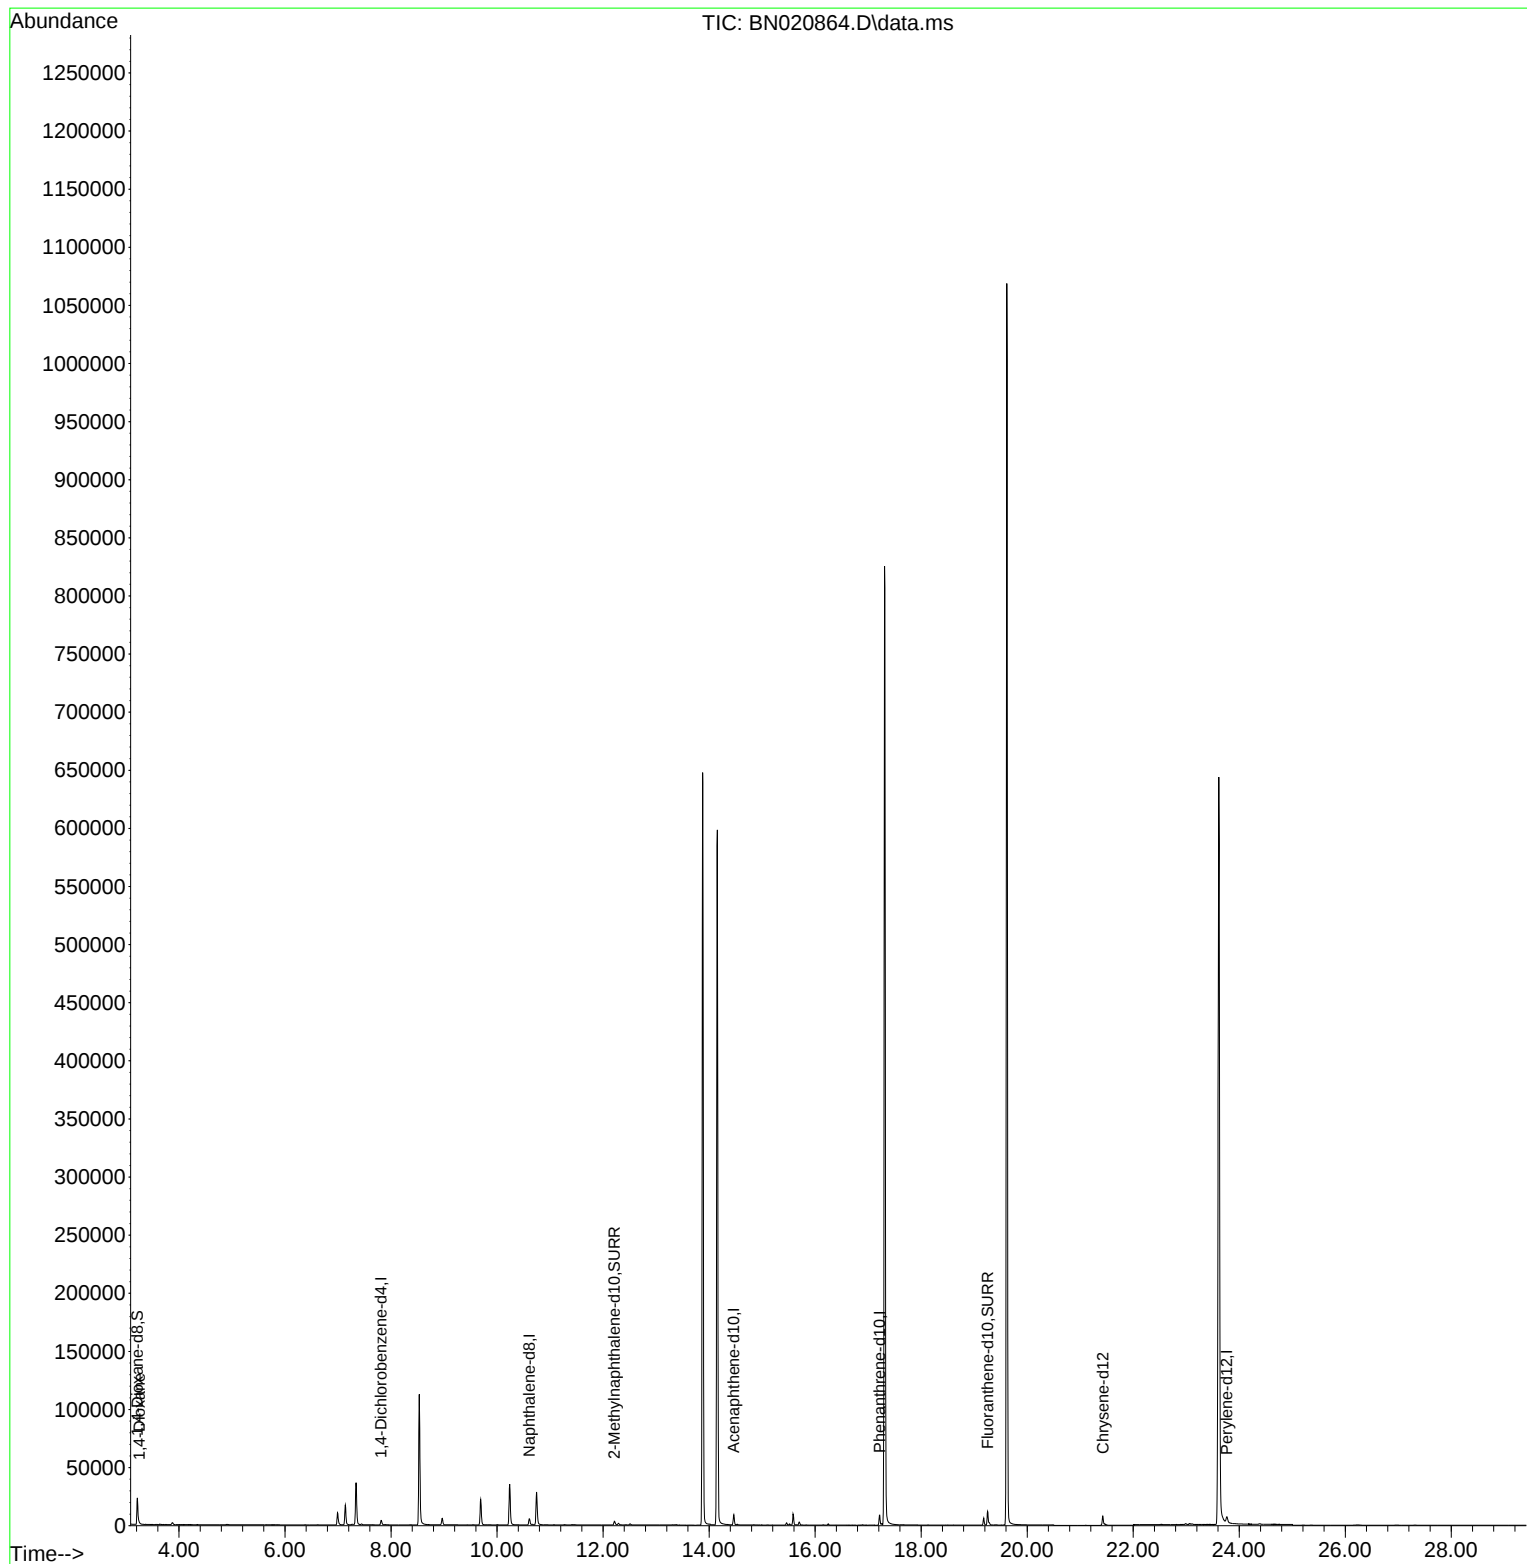

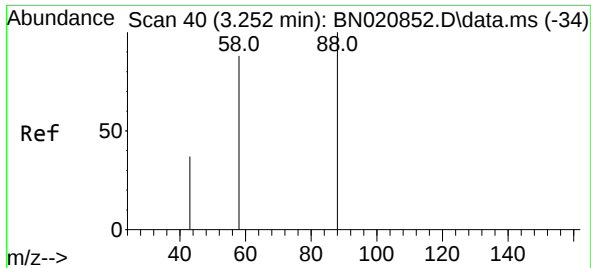

#2
 1,4-Dioxane
 Concen: 0.060 ng/ul
 RT: 3.252 min Scan# 40
 Delta R.T. -0.004 min
 Lab File: BN020864.D
 Acq: 26 Jul 2022 16:20

Instrument :
 BNA_N
 ClientSampleId :
 GBHY4

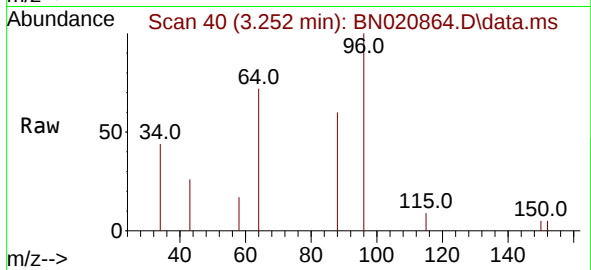

Tgt Ion: 88 Resp: 172

Ion	Ratio	Lower	Upper
88	100		
43	43.7	32.5	48.7
58	28.4	46.2	69.2

