

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
 Data File : BN020865.D
 Acq On : 26 Jul 2022 16:57
 Operator : CG/JU
 Sample : N3801-20
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBHY5

Quant Time: Jul 26 17:29:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 18:06:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	2261	0.400	ng/ul	0.00
4) Naphthalene-d8	10.606	136	7774	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.465	164	4853	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	10232	0.400	ng/ul	0.00
17) Chrysene-d12	21.426	240	8746	0.400	ng/ul	0.00
23) Perylene-d12	23.764	264	9214	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.214	96	12648	4.656	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.212	152	4198	0.355	ng/ul	0.00
18) Fluoranthene-d10	19.253	212	11381	0.407	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.252	88	228	0.082	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
Data File : BN020865.D
Acq On : 26 Jul 2022 16:57
Operator : CG/JU
Sample : N3801-20
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBHY5


Quant Time: Jul 26 17:29:04 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 18:06:54 2022
Response via : Initial Calibration

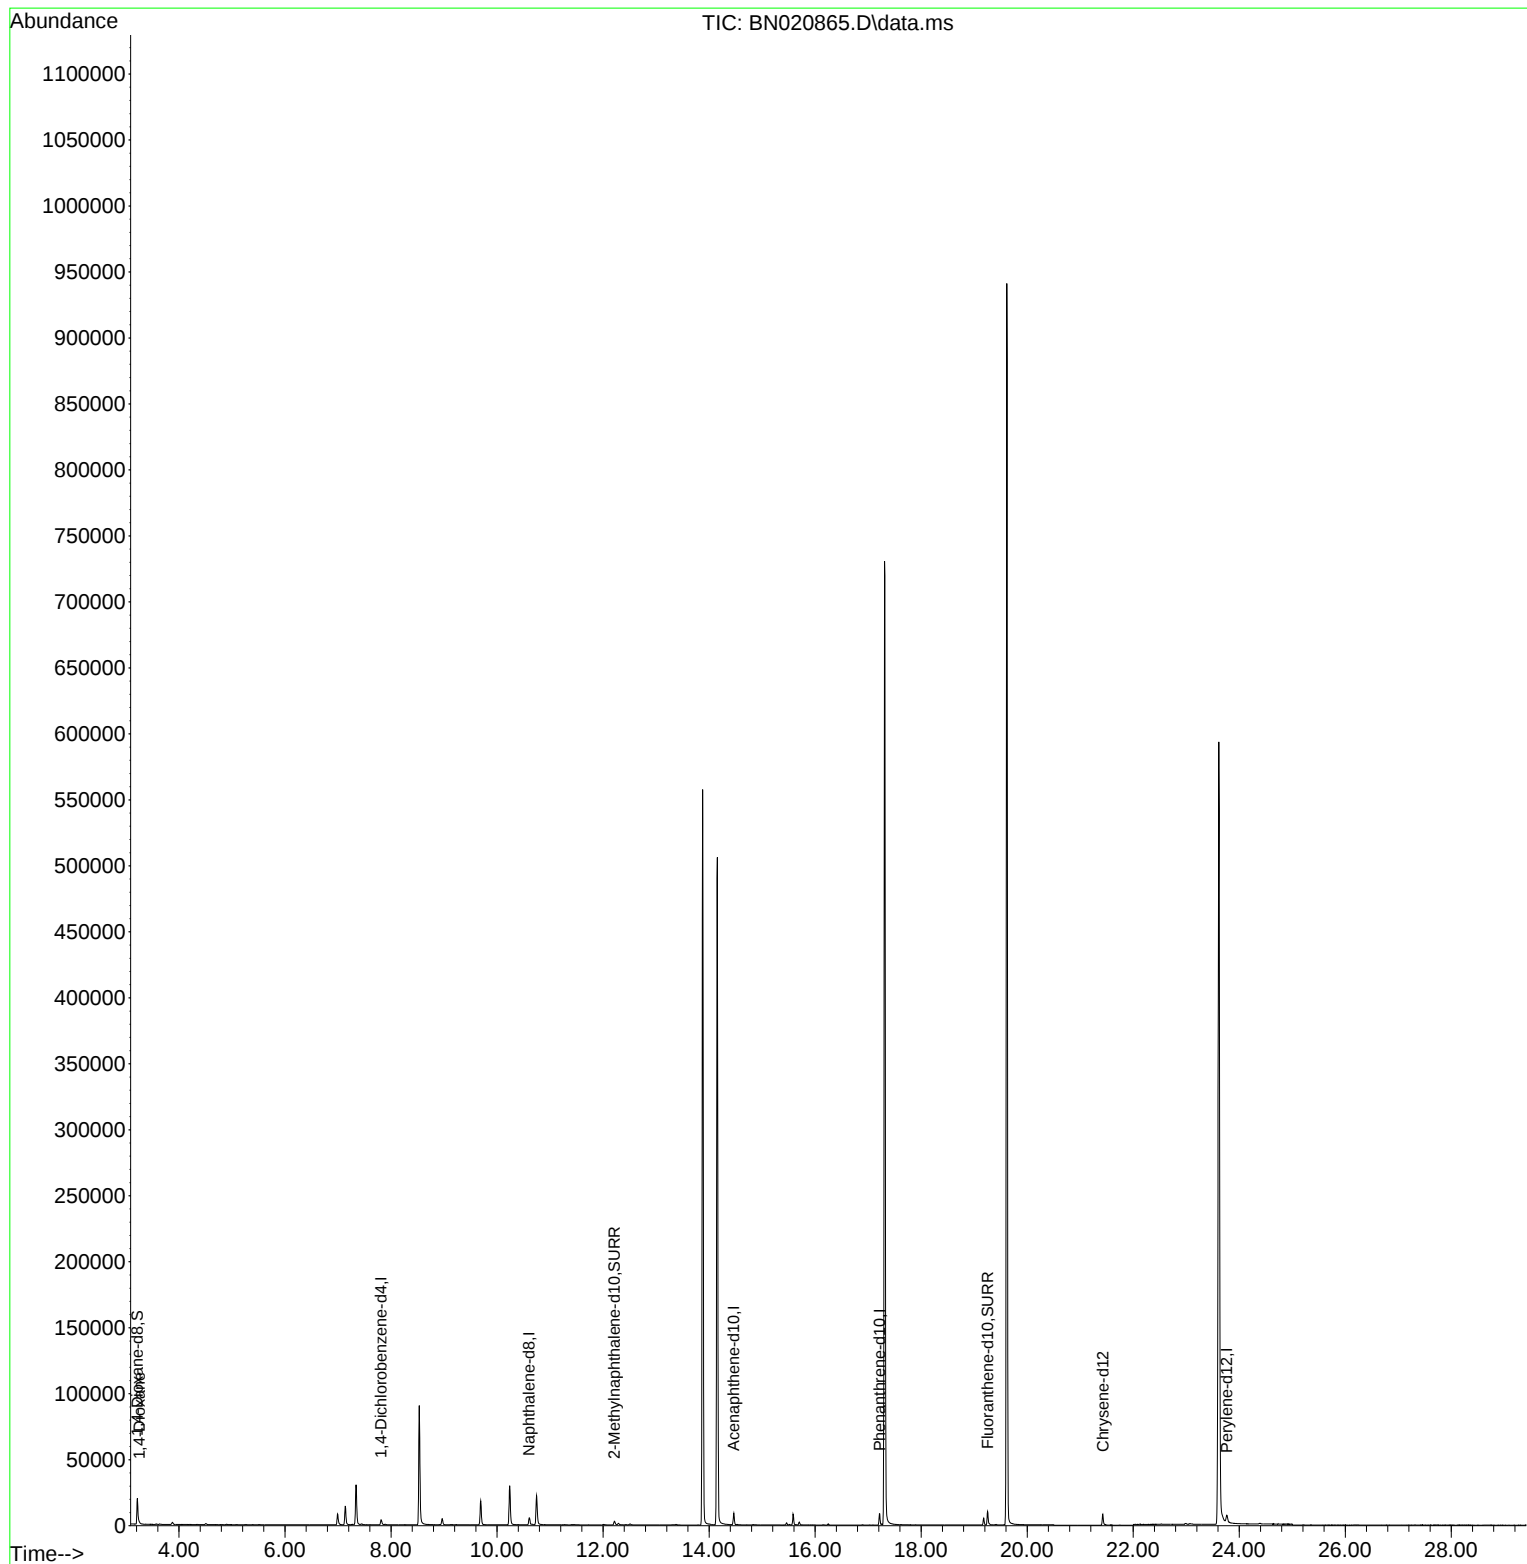

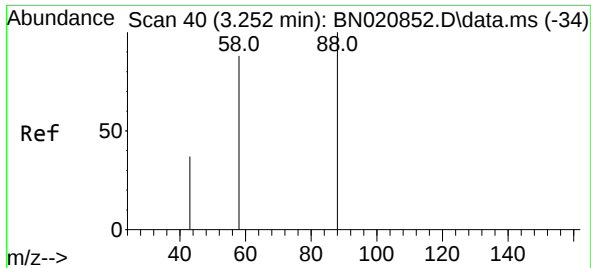

#2
 1,4-Dioxane
 Concen: 0.082 ng/ul
 RT: 3.252 min Scan# 40
 Delta R.T. -0.004 min
 Lab File: BN020865.D
 Acq: 26 Jul 2022 16:57

Instrument :
 BNA_N
 ClientSampleId :
 GBHY5

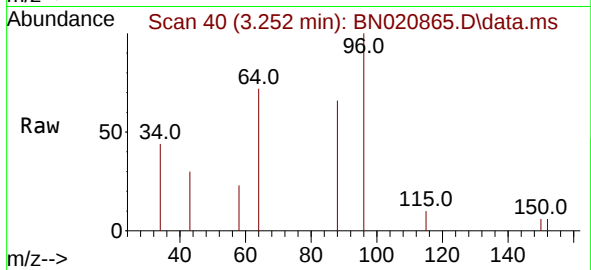

Tgt Ion: 88 Resp: 228

Ion	Ratio	Lower	Upper
88	100		
43	45.6	32.5	48.7
58	34.4	46.2	69.2#

