

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
 Data File : BN020867.D
 Acq On : 26 Jul 2022 18:12
 Operator : CG/JU
 Sample : N3801-22
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBHY7

Quant Time: Jul 26 18:38:45 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 18:06:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	2448	0.400	ng/u1	0.00
4) Naphthalene-d8	10.612	136	8350	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.465	164	5323	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.213	188	11142	0.400	ng/u1	0.00
17) Chrysene-d12	21.426	240	9184	0.400	ng/u1	0.00
23) Perylene-d12	23.764	264	10111	0.400	ng/u1	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.214	96	15910	5.409	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.218	152	4865	0.383	ng/u1	0.00
18) Fluoranthene-d10	19.253	212	12774	0.435	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.252	88	477	0.158	ng/u1	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
Data File : BN020867.D
Acq On : 26 Jul 2022 18:12
Operator : CG/JU
Sample : N3801-22
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBHY7


Quant Time: Jul 26 18:38:45 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 18:06:54 2022
Response via : Initial Calibration

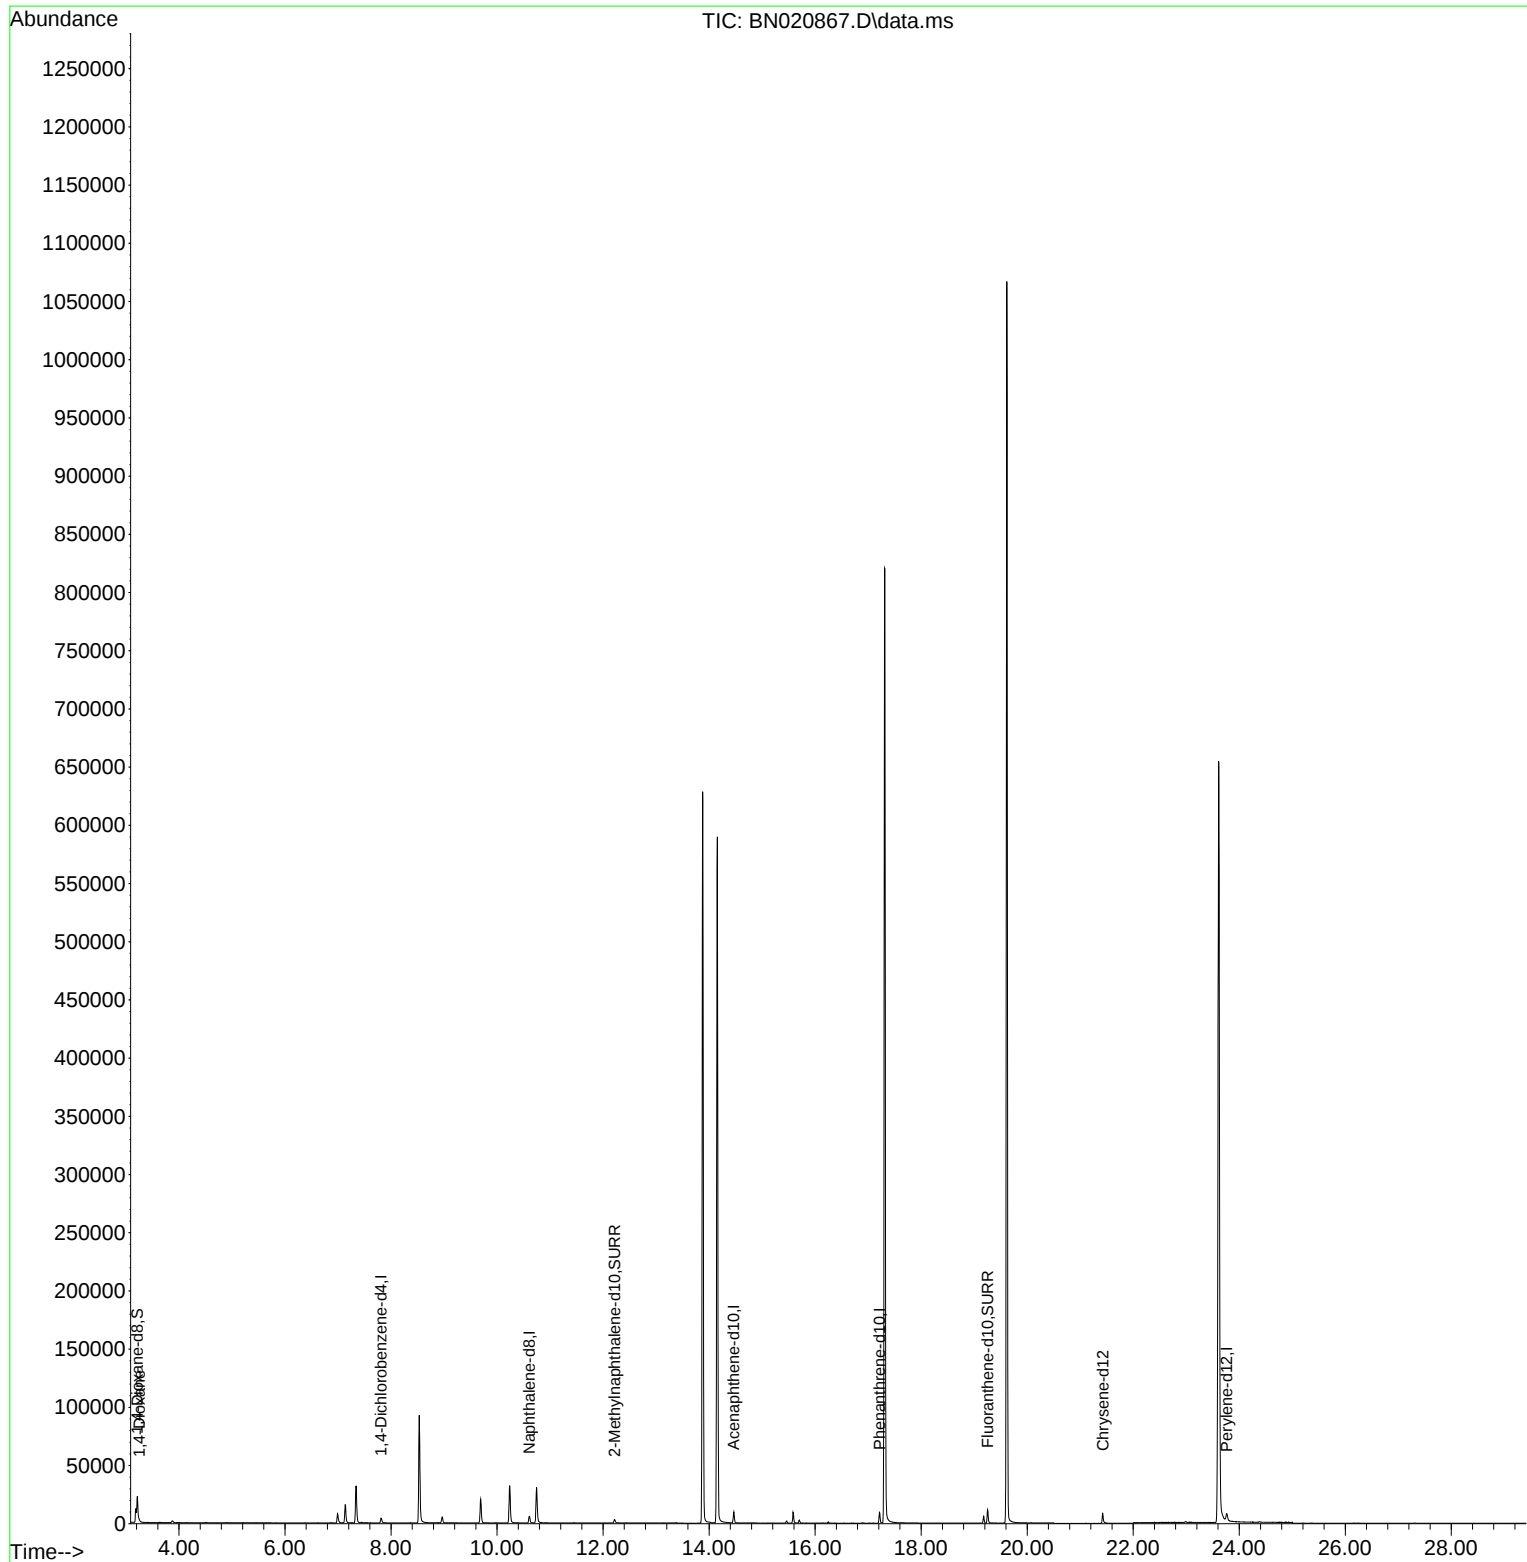

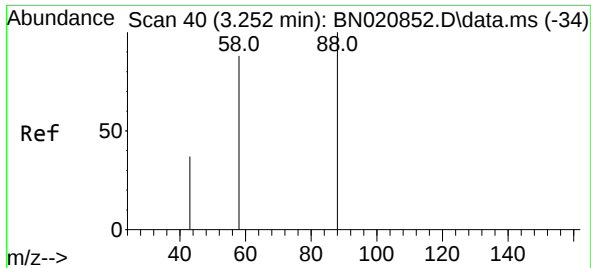

#2
 1,4-Dioxane
 Concen: 0.158 ng/ul
 RT: 3.252 min Scan# 40
 Delta R.T. -0.004 min
 Lab File: BN020867.D
 Acq: 26 Jul 2022 18:12

Instrument :
 BNA_N
 ClientSampleId :
 GBHY7

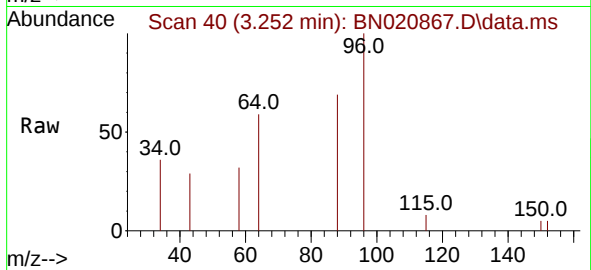

Tgt Ion:	88	Resp:	477
Ion	Ratio	Lower	Upper
88	100		
43	41.5	32.5	48.7
58	46.7	46.2	69.2

