

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
 Data File : BN020872.D
 Acq On : 26 Jul 2022 21:55
 Operator : CG/JU
 Sample : N3871-08
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBJ07

Quant Time: Jul 26 23:25:46 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 18:06:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	2472	0.400	ng/ul	0.00
4) Naphthalene-d8	10.606	136	8326	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.465	164	5216	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	11020	0.400	ng/ul	0.00
17) Chrysene-d12	21.420	240	9323	0.400	ng/ul	-0.01
23) Perylene-d12	23.761	264	9279	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.214	96	13066	4.399	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.212	152	4097	0.324	ng/ul	0.00
18) Fluoranthene-d10	19.253	212	11918	0.400	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.252	88	1511	0.495	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
Data File : BN020872.D
Acq On : 26 Jul 2022 21:55
Operator : CG/JU
Sample : N3871-08
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBJ07


Quant Time: Jul 26 23:25:46 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 18:06:54 2022
Response via : Initial Calibration

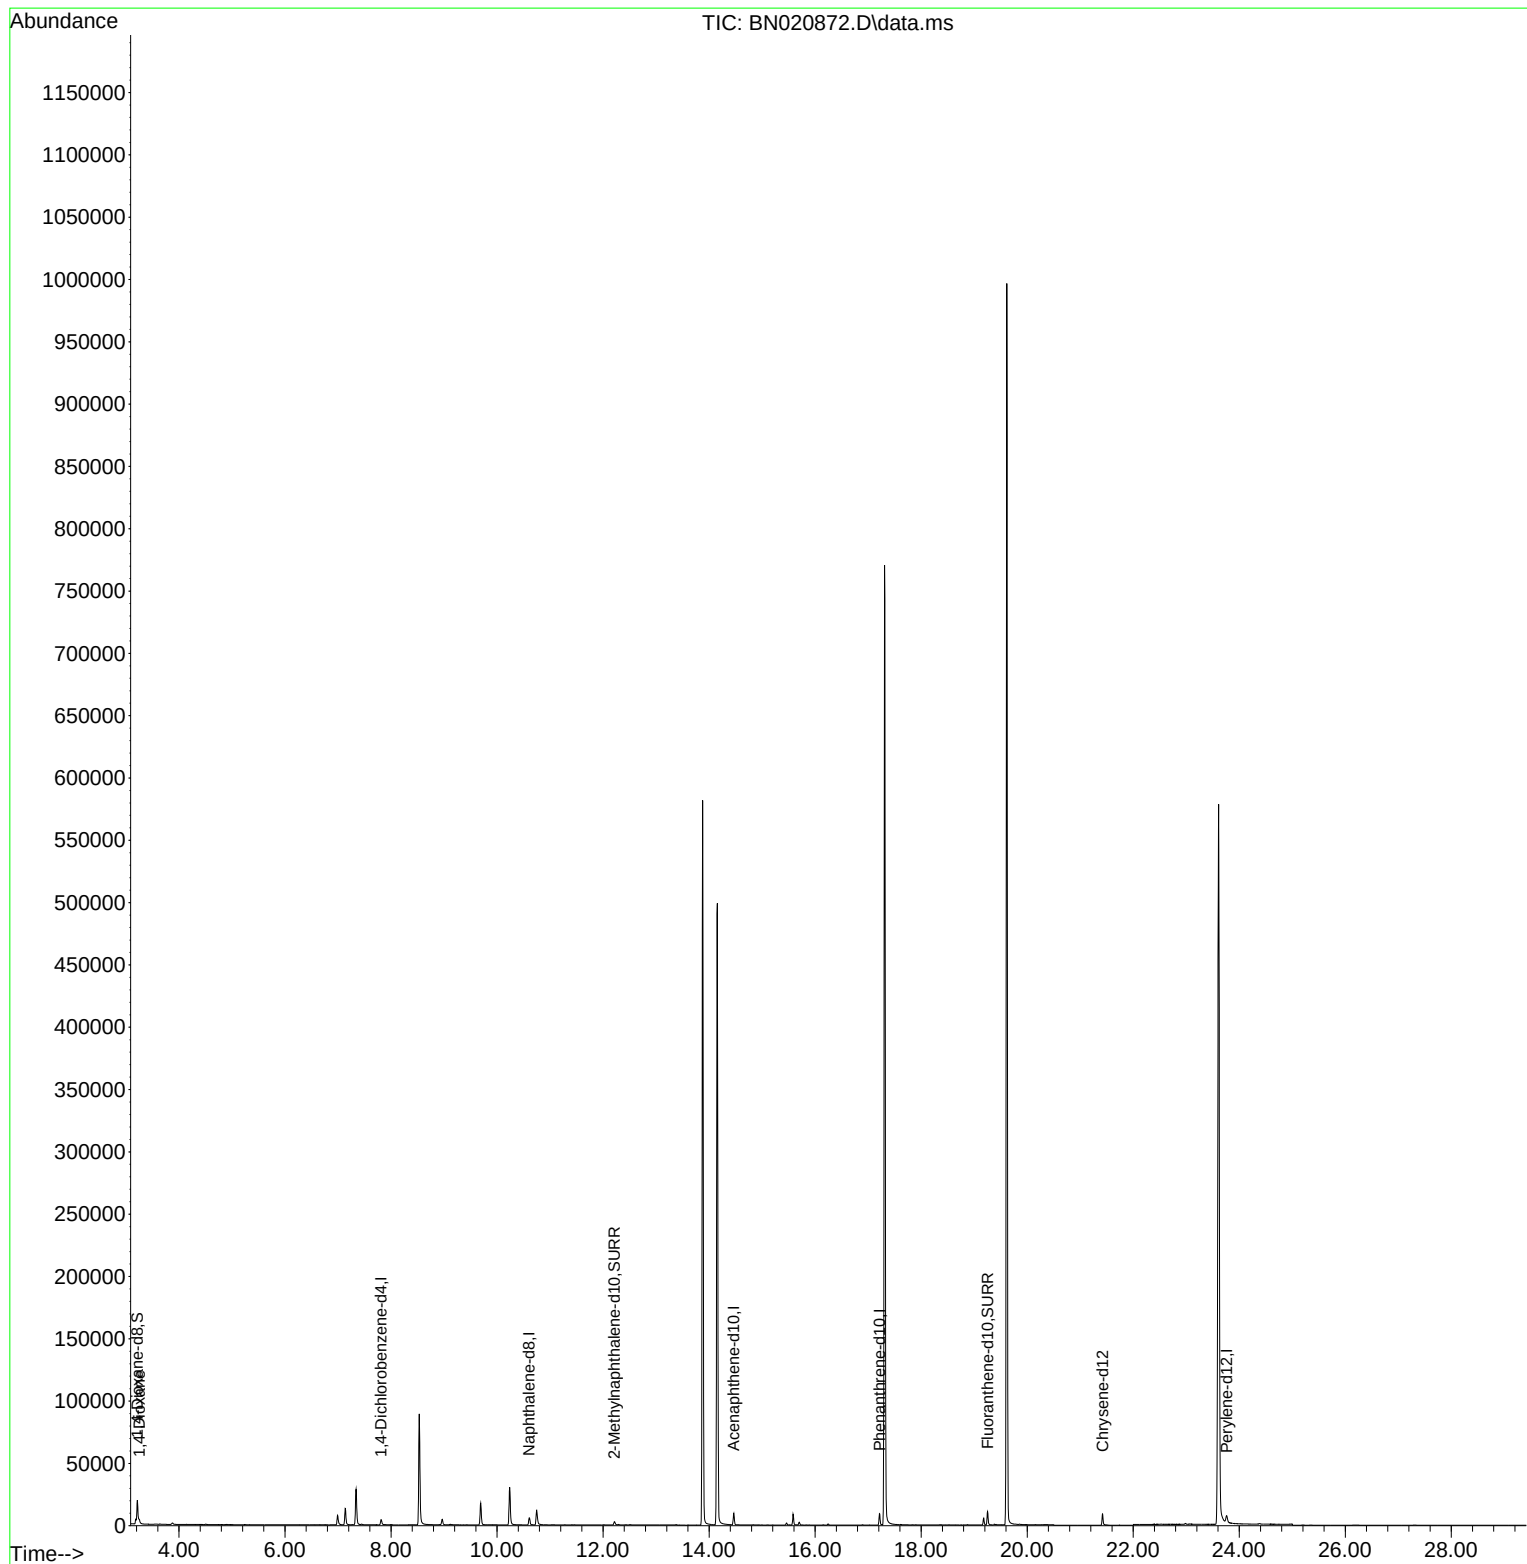

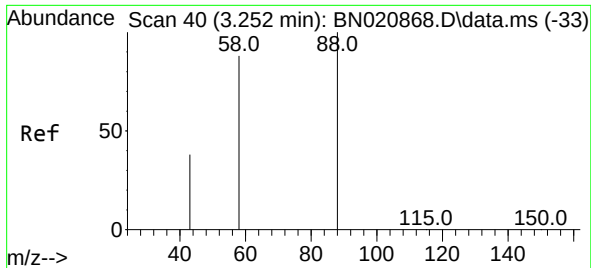

#2
 1,4-Dioxane
 Concen: 0.495 ng/ul
 RT: 3.252 min Scan# 40
 Delta R.T. -0.004 min
 Lab File: BN020872.D
 Acq: 26 Jul 2022 21:55

Instrument :
 BNA_N
 ClientSampleId :
 GBJ07

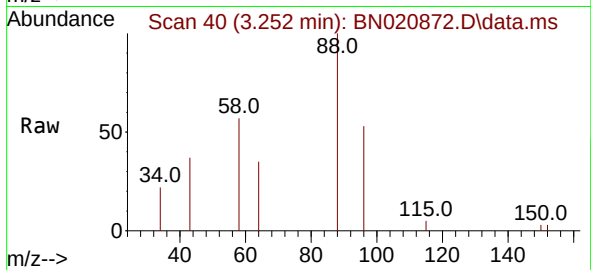

Tgt Ion:	88	Resp:	1511
Ion	Ratio	Lower	Upper
88	100		
43	36.5	32.5	48.7
58	57.2	46.2	69.2

