

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
 Data File : BN020900.D
 Acq On : 27 Jul 2022 15:38
 Operator : CG/JU
 Sample : N3871-21
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBJ18

Quant Time: Jul 27 18:15:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 18:06:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.808	152	2896	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.606	136	10103	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.460	164	6448	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	13661	0.400	ng/ul	0.00
17) Chrysene-d12	21.422	240	11478	0.400	ng/ul	0.00
23) Perylene-d12	23.760	264	11199	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.214	96	14885	4.278	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.206	152	5363	0.349	ng/ul	-0.01
18) Fluoranthene-d10	19.253	212	13516	0.369	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.252	88	816	0.228	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072522\
Data File : BN020900.D
Acq On : 27 Jul 2022 15:38
Operator : CG/JU
Sample : N3871-21
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBJ18

Quant Time: Jul 27 18:15:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 18:06:54 2022
Response via : Initial Calibration

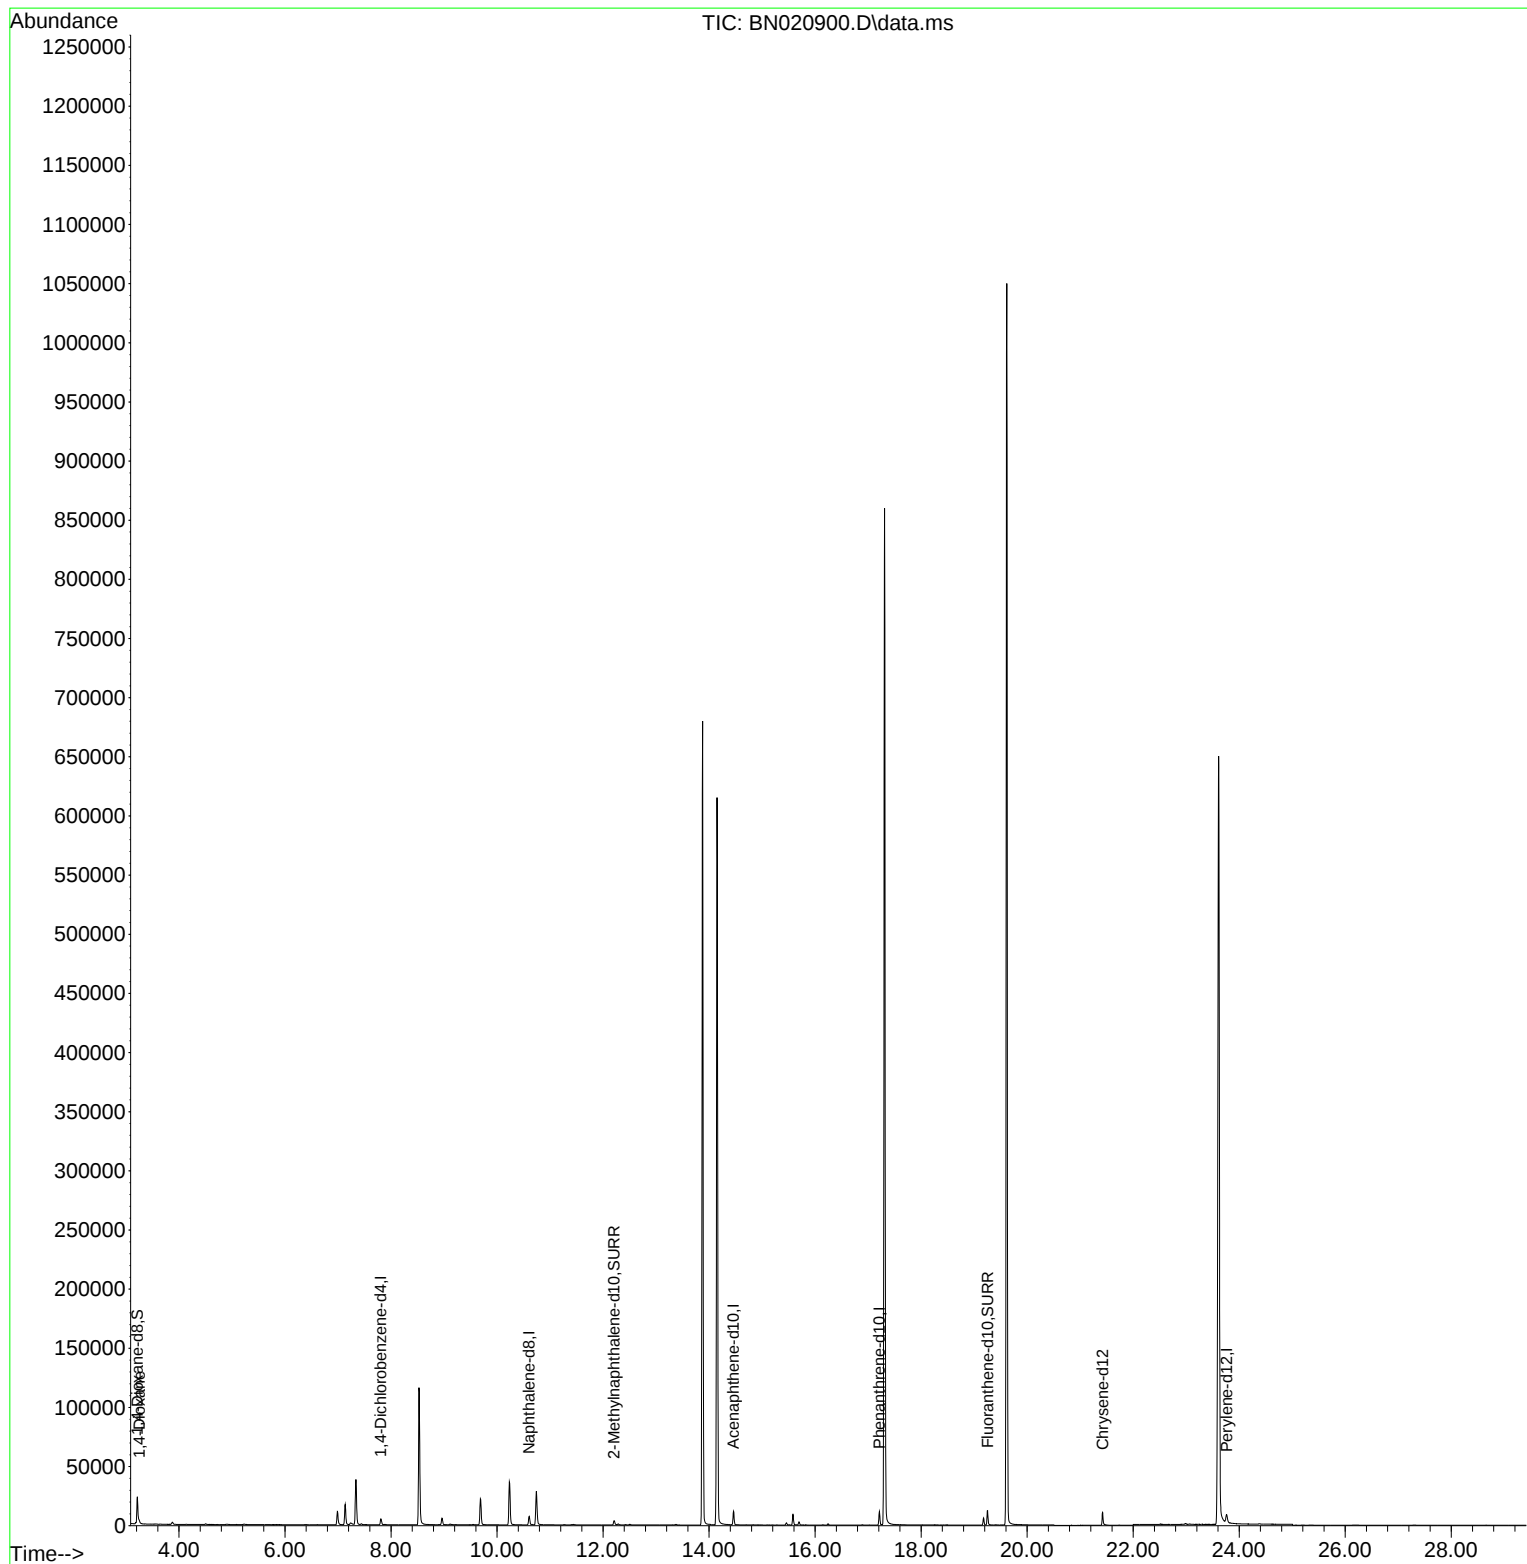

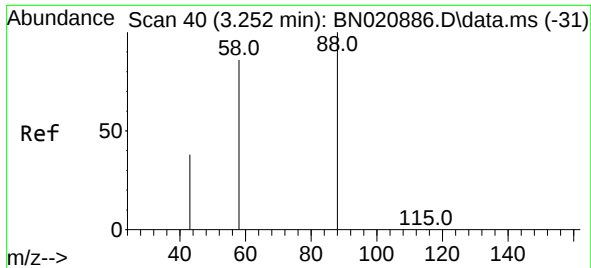

#2
 1,4-Dioxane
 Concen: 0.228 ng/ul
 RT: 3.252 min Scan# 40
 Delta R.T. -0.004 min
 Lab File: BN020900.D
 Acq: 27 Jul 2022 15:38

Instrument :
 BNA_N
 ClientSampleId :
 GBJ18

Tgt Ion: 88	Resp: 816		
Ion Ratio	Lower	Upper	
88 100			
43 38.4	32.5	48.7	
58 45.9	46.2	69.2#	

