




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

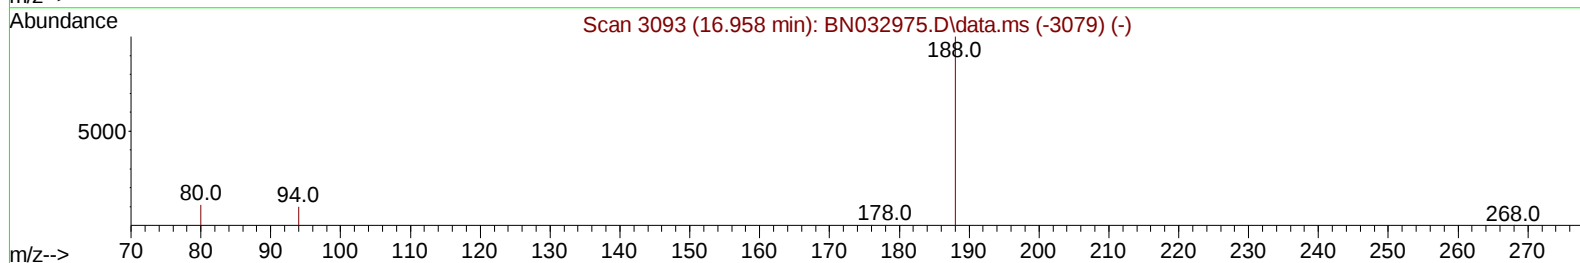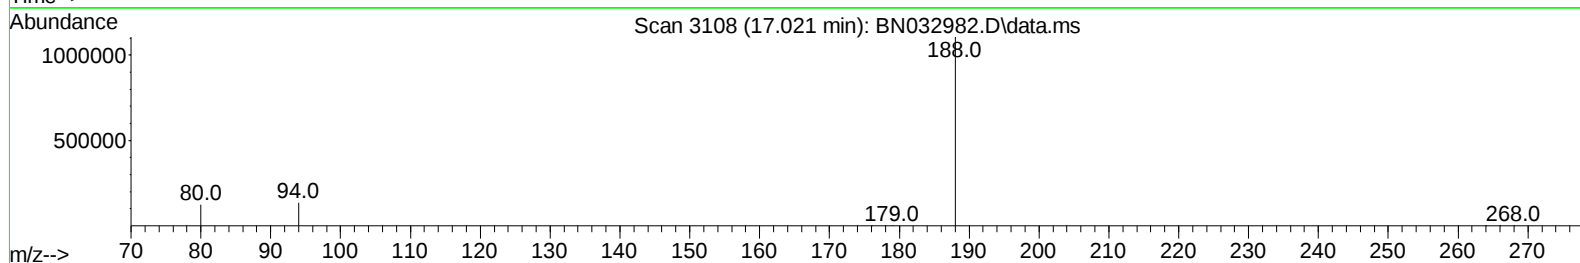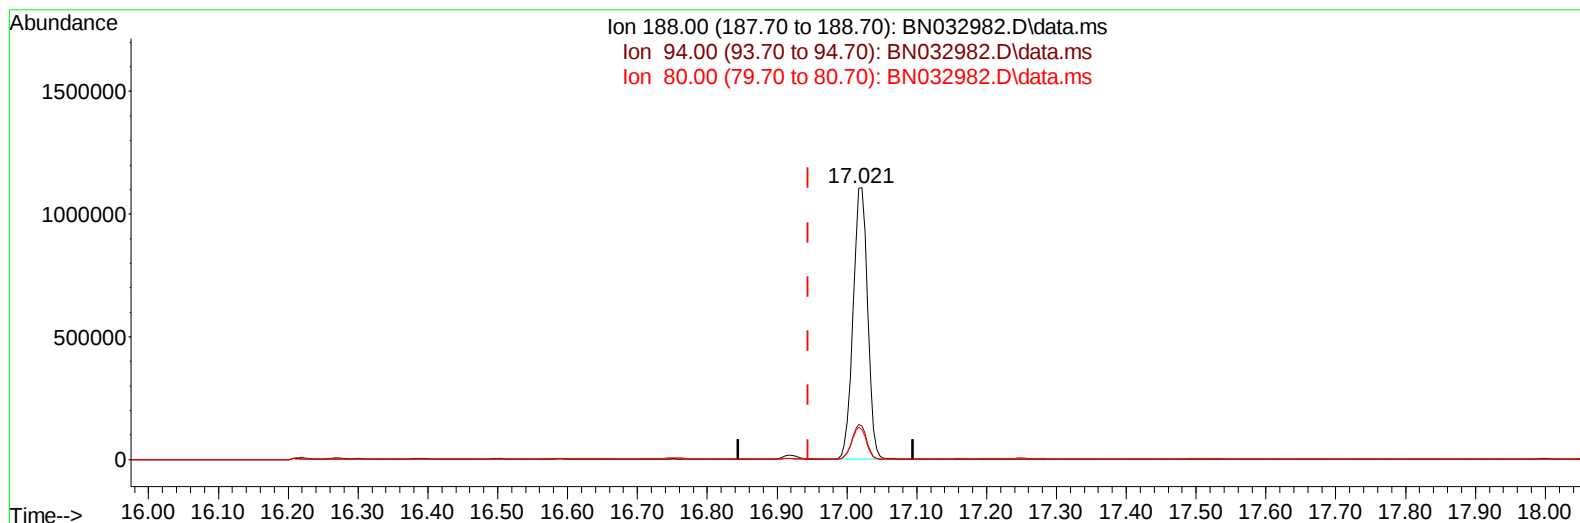

TIC: BN032982.D\data.ms

(13) Phenanthrene-d10 (I)

17.021min (+ 0.076) 0.40 ng/u1

response 1595929

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	12.32
80.00	13.10	11.07
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

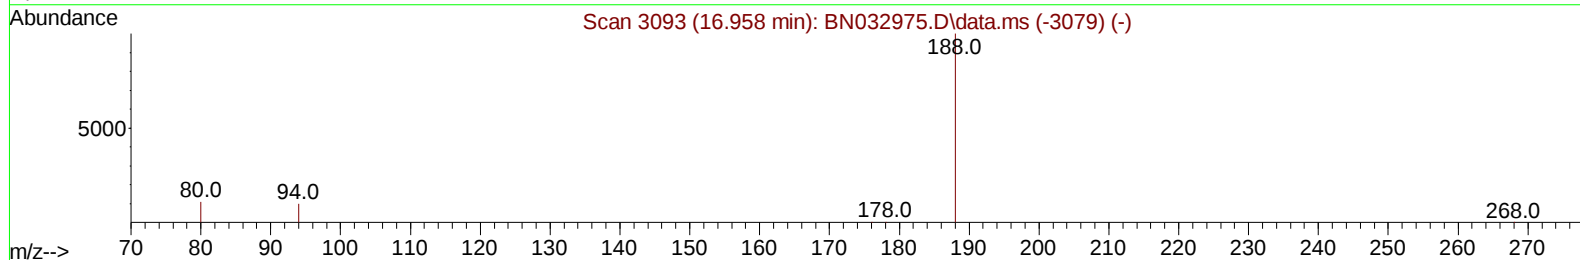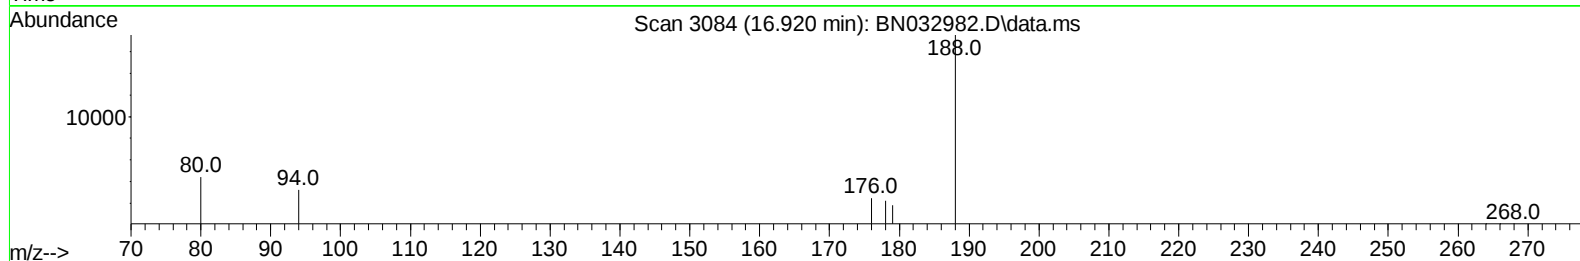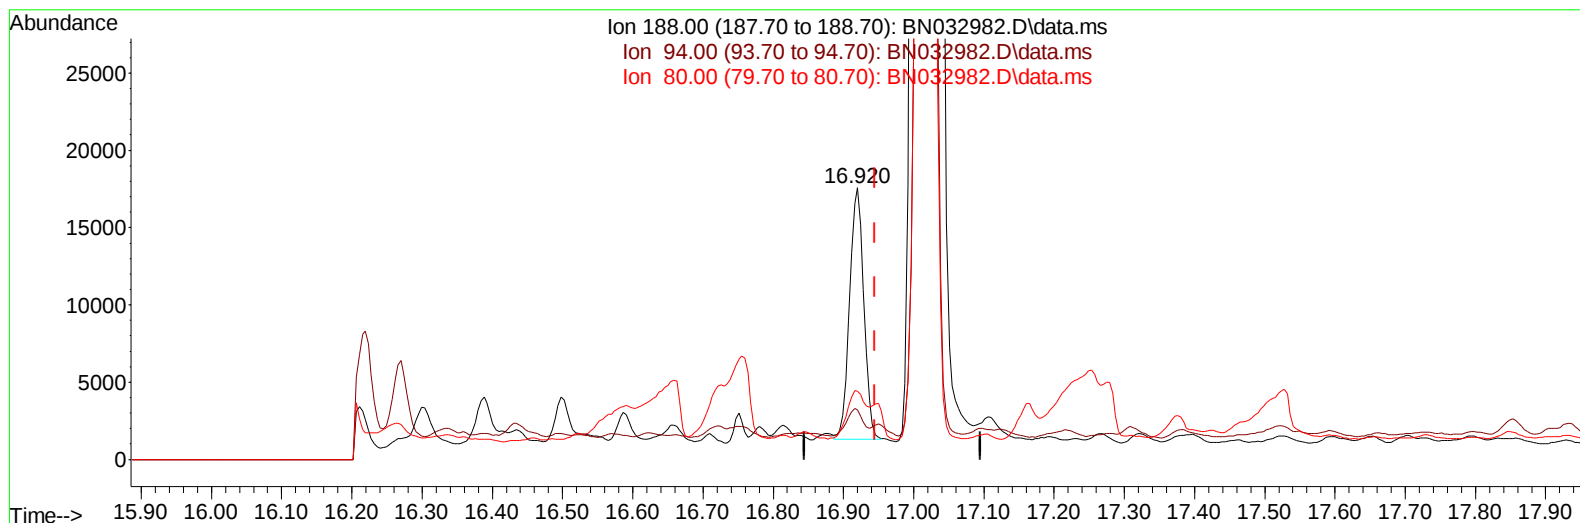

TIC: BN032982.D\data.ms

(13) Phenanthrene-d10 (I)

16.920min (-0.025) 0.40 ng/ul m

response 23019

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	18.31#
80.00	13.10	25.14#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

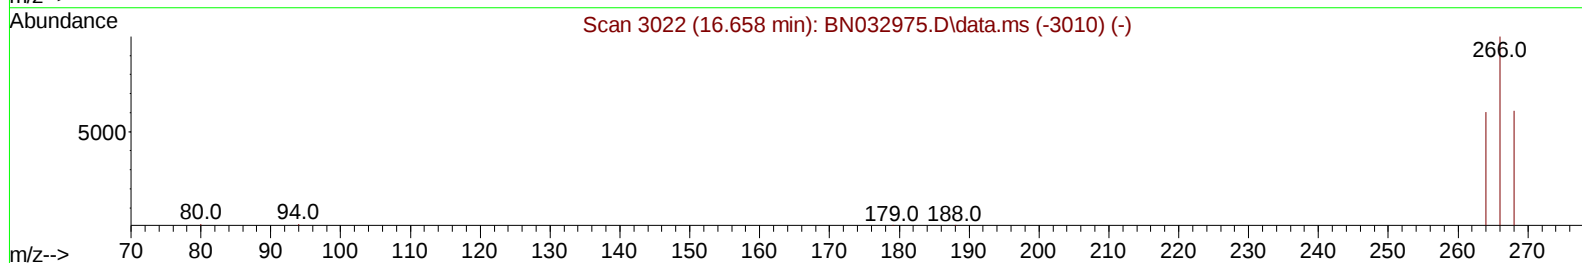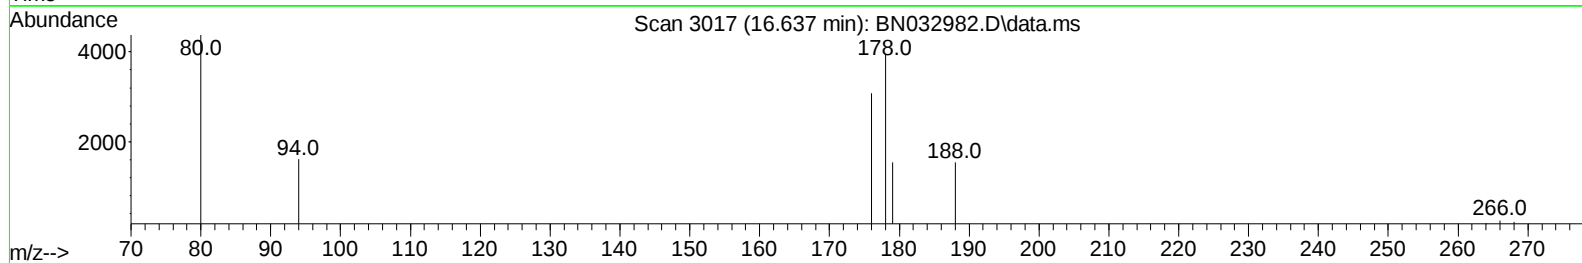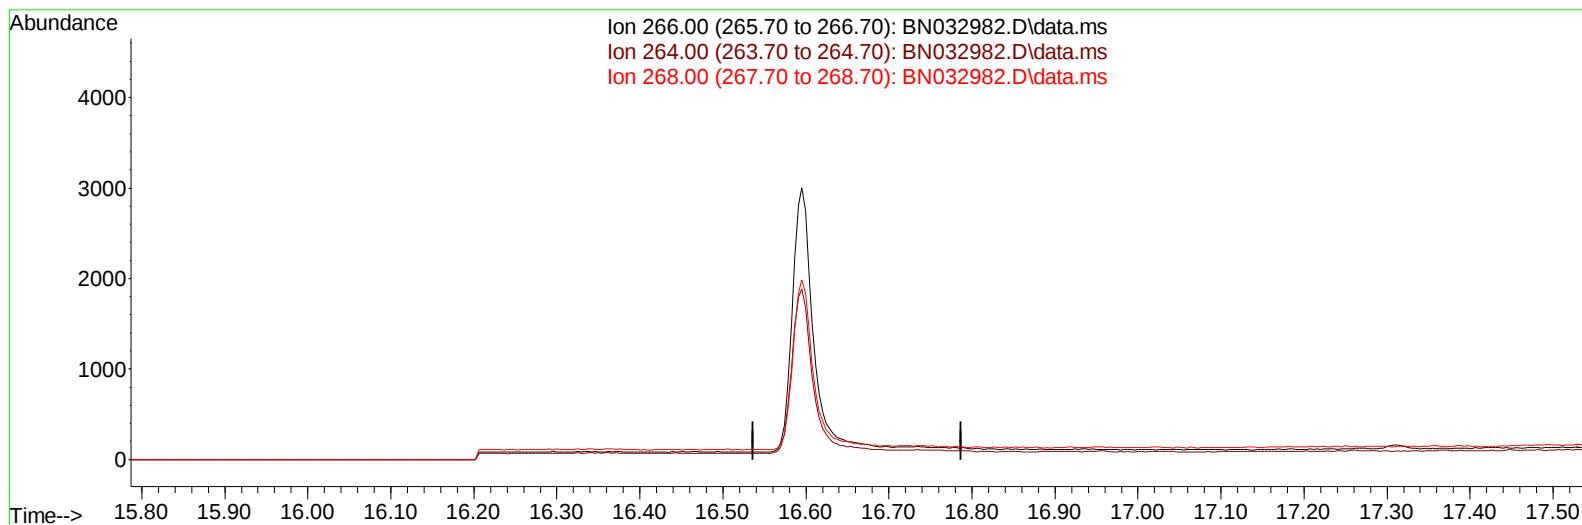

TIC: BN032982.D\data.ms

(14) Pentachlorophenol

16.637min (-16.637) 0.00 ng/u1

response 0

Ion	Exp%	Act%
266.00	100.00	0.00
264.00	61.60	0.00#
268.00	64.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

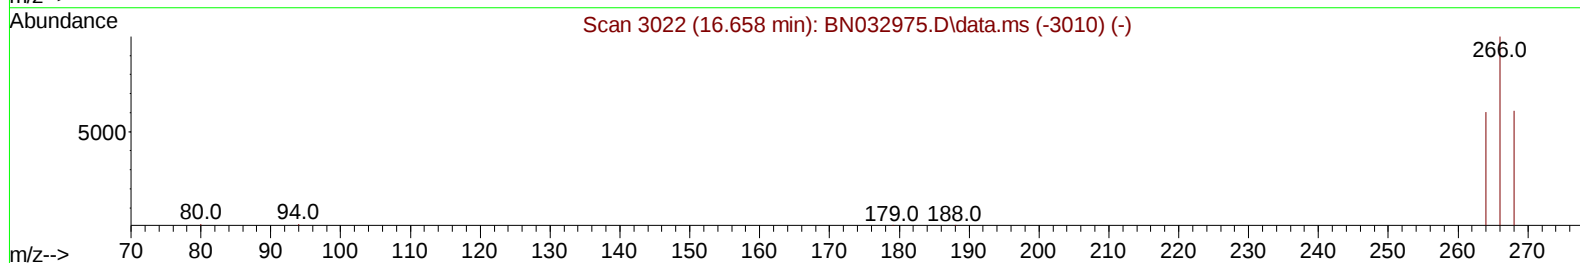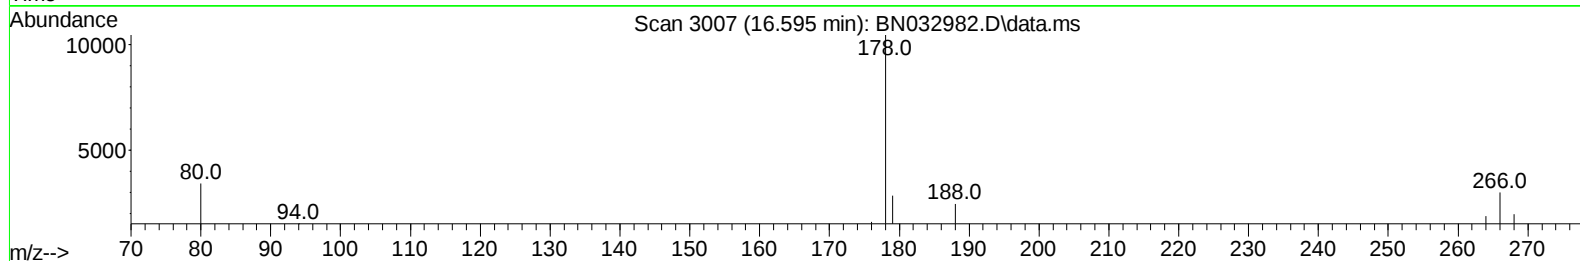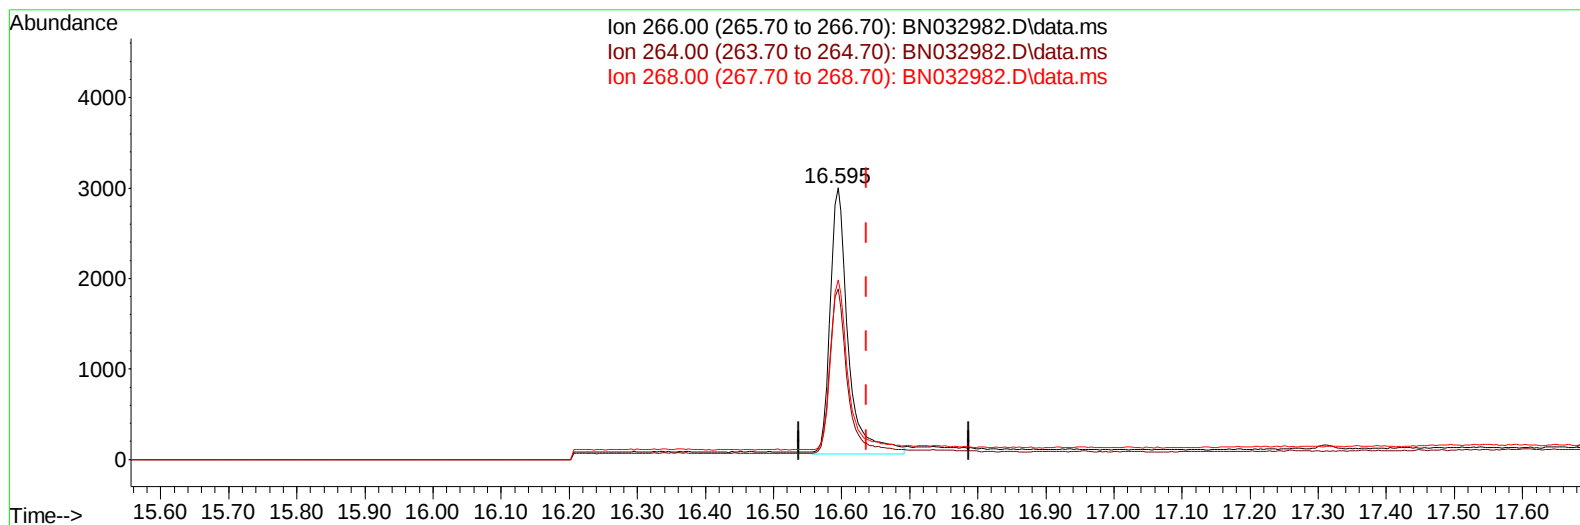

TIC: BN032982.D\data.ms

(14) Pentachlorophenol

16.595min (-0.042) 1.15 ng/ul m

response 5401

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	61.60	0.00#
268.00	64.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

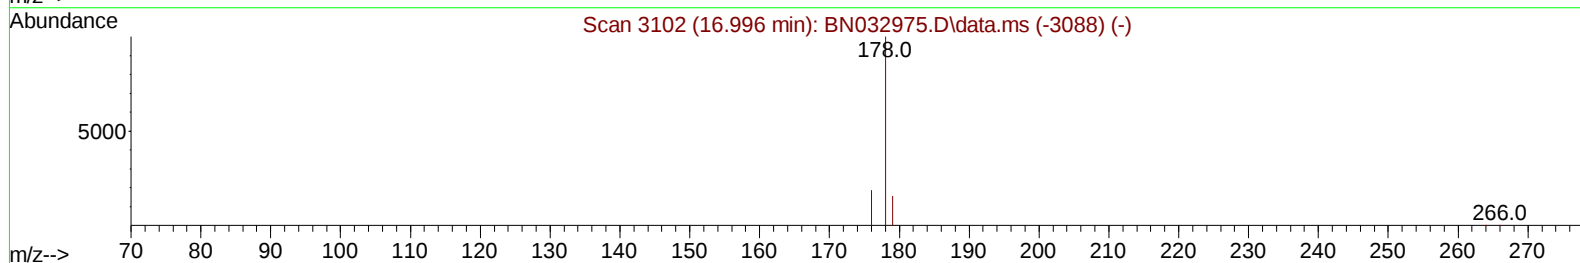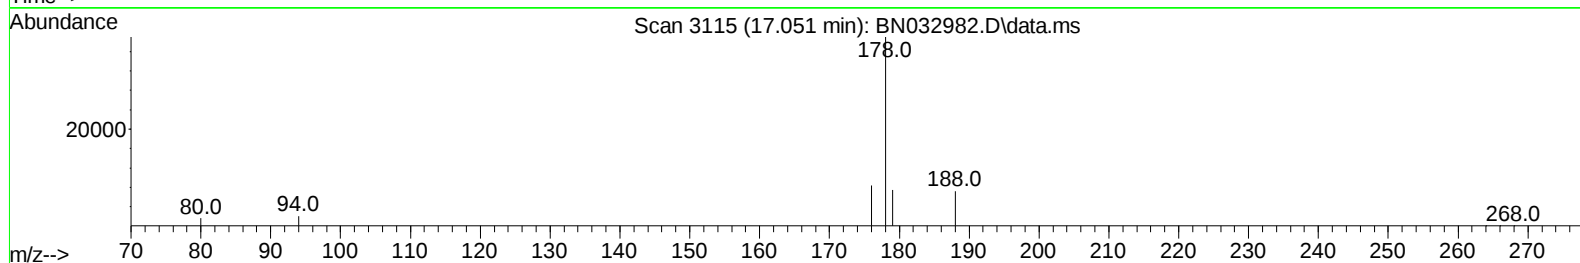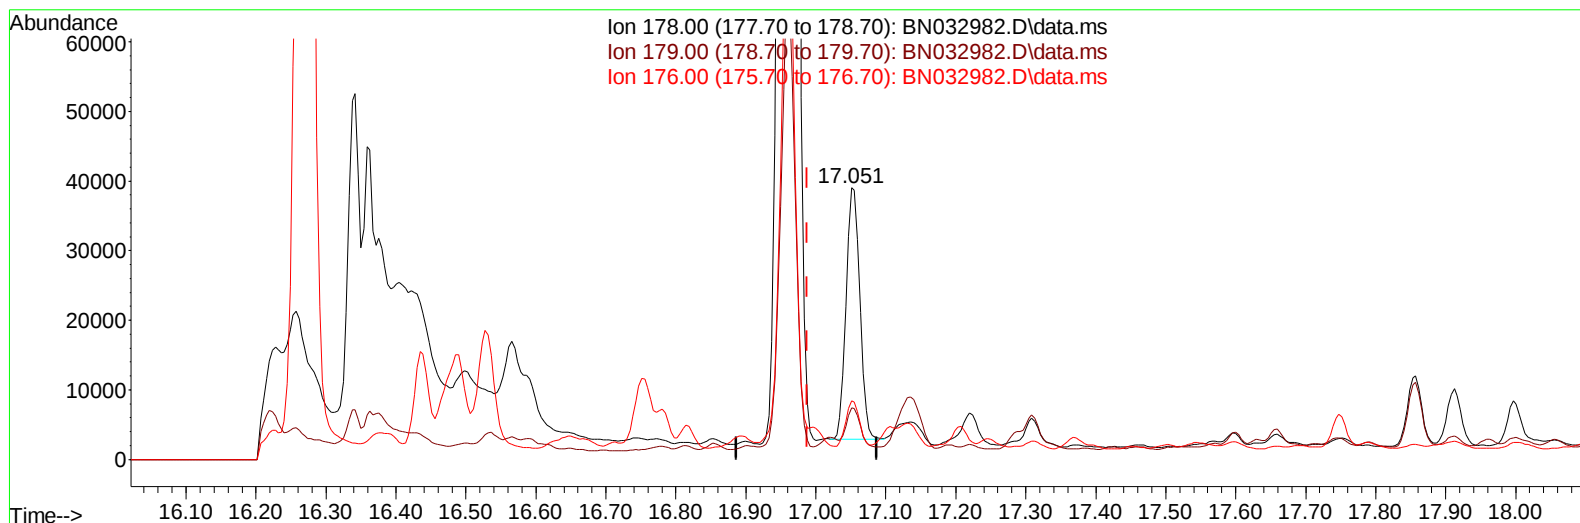

TIC: BN032982.D\data.ms

(15) Phenanthrene

17.051min (+ 0.064) 0.81 ng/u1

response 49810

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.10	19.08
176.00	19.90	21.70
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

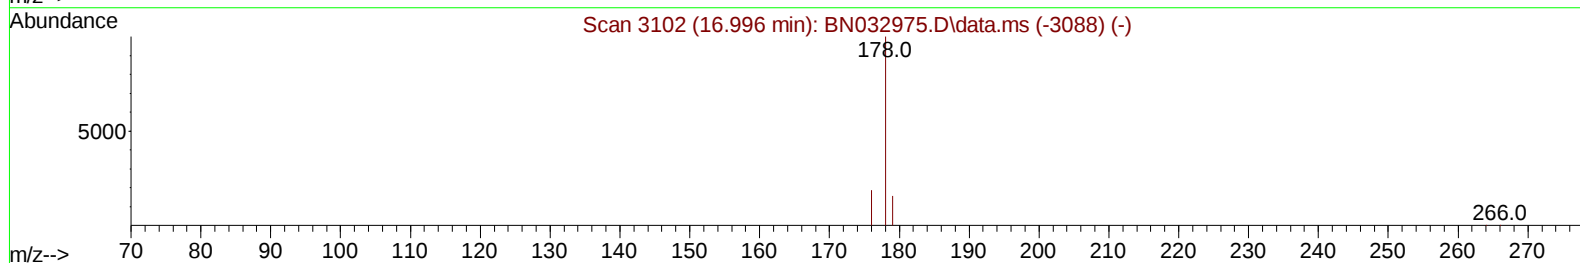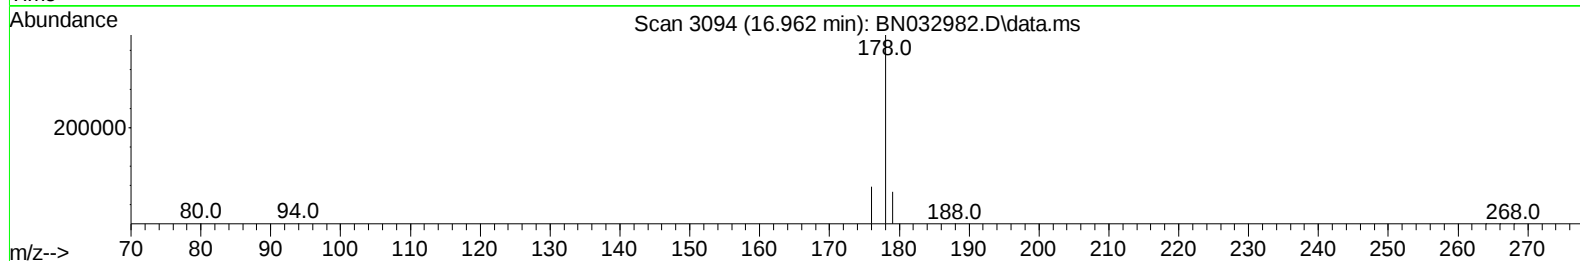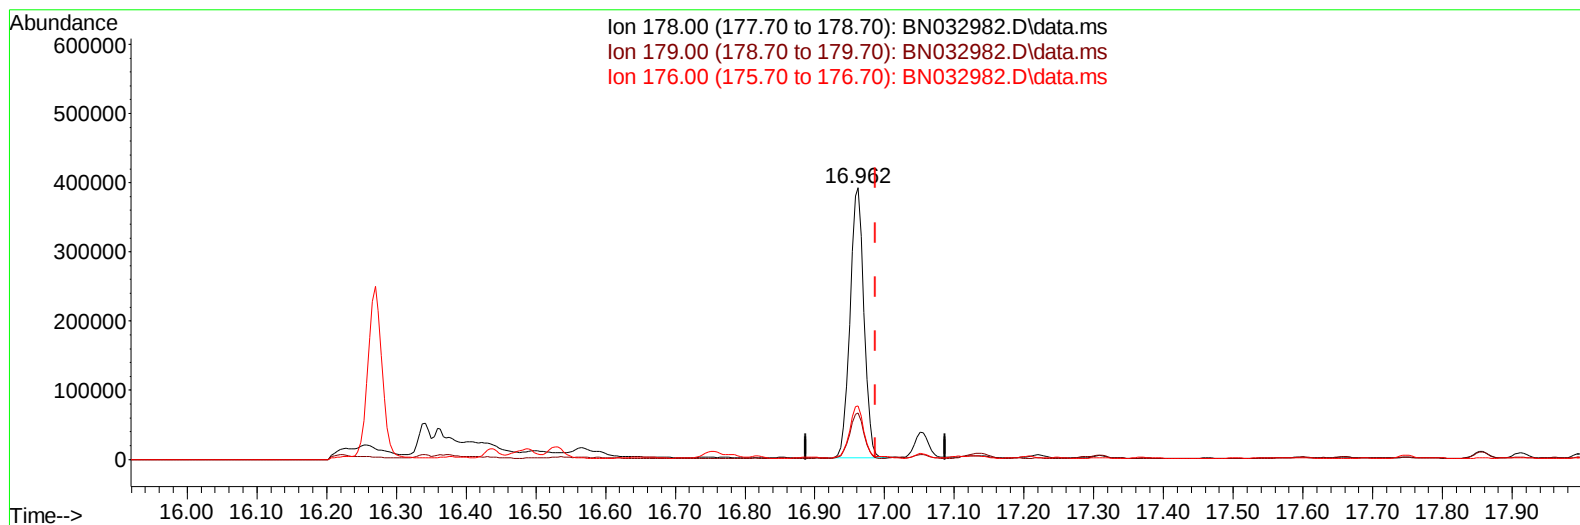

TIC: BN032982.D\data.ms

(15) Phenanthrene

16.962min (-0.025) 8.82 ng/u1 m

response 544815

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.10	17.03
176.00	19.90	19.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

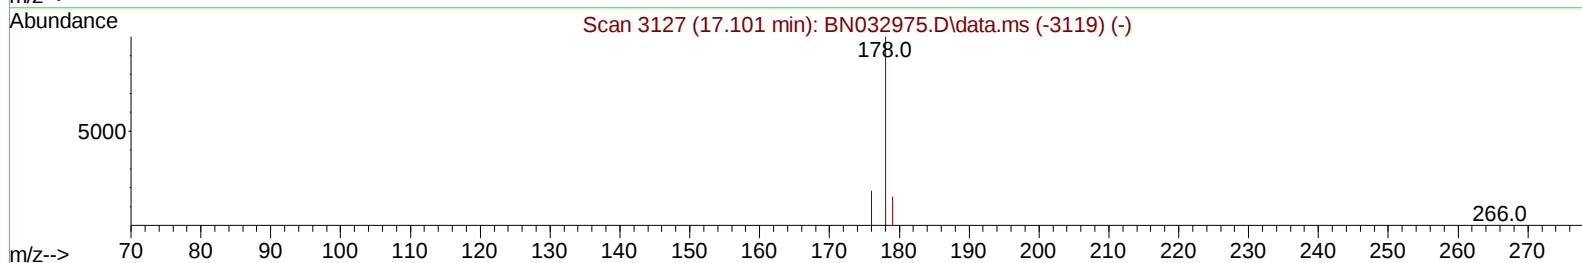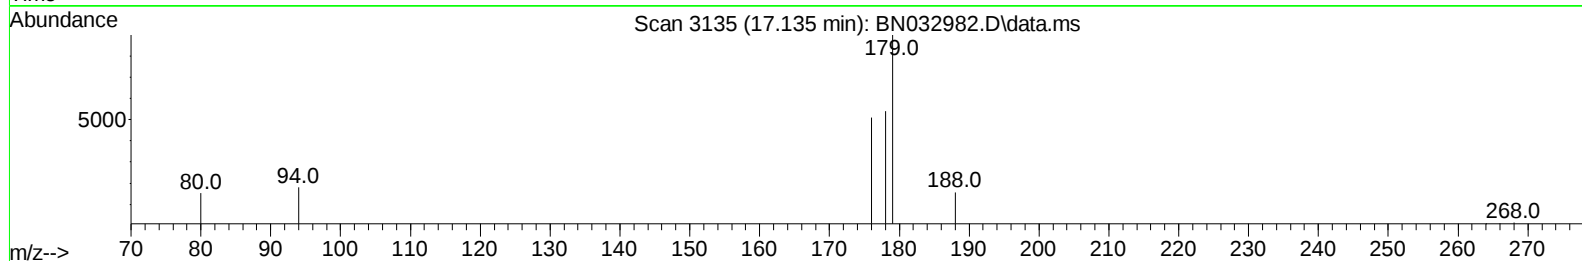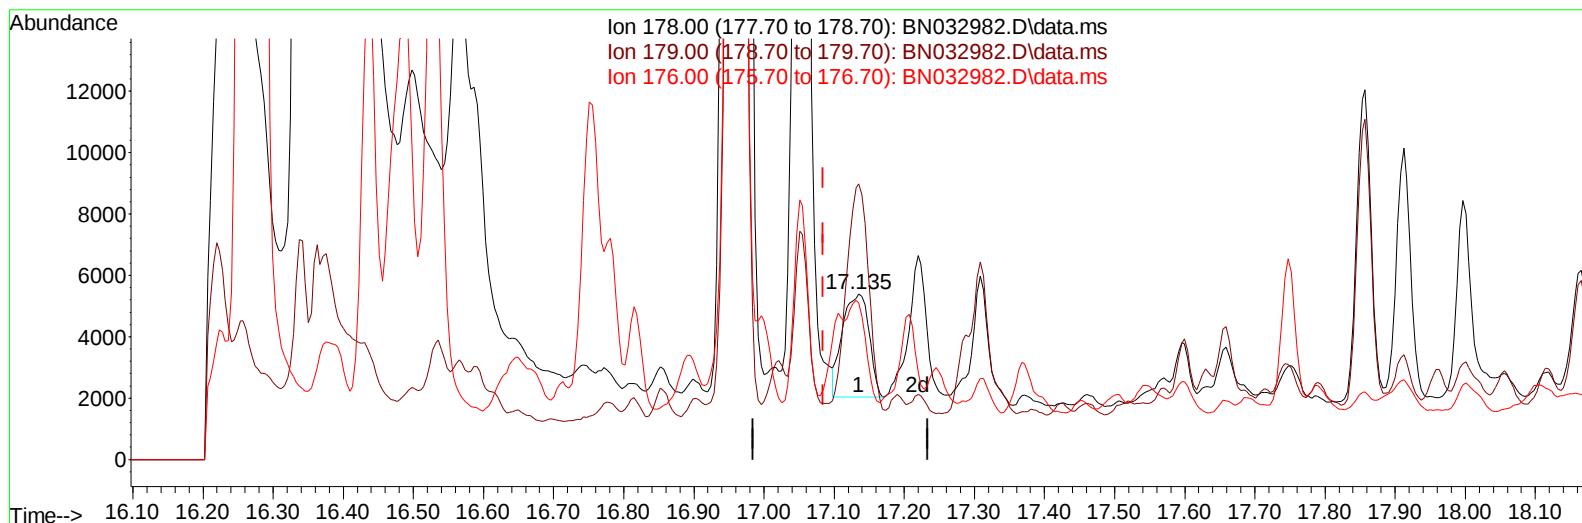

TIC: BN032982.D\data.ms

(16) Anthracene

17.135min (+ 0.051) 0.16 ng/u1

response 8791

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.90	166.66#
176.00	19.80	94.60#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

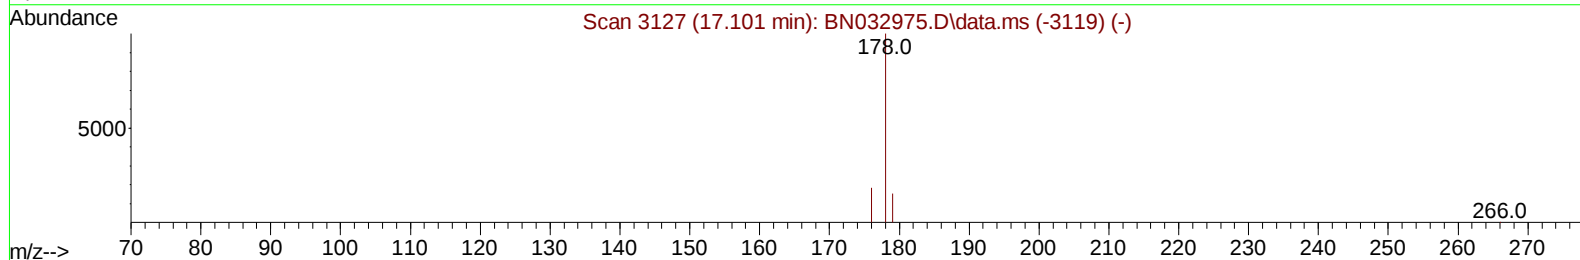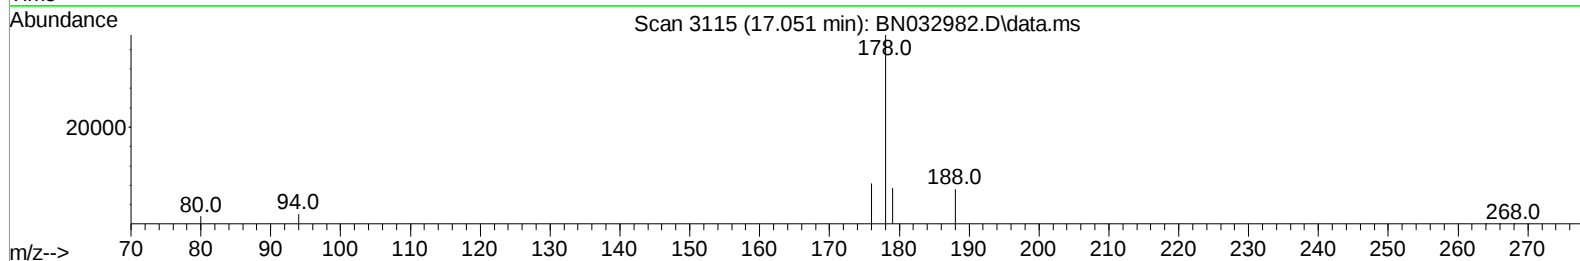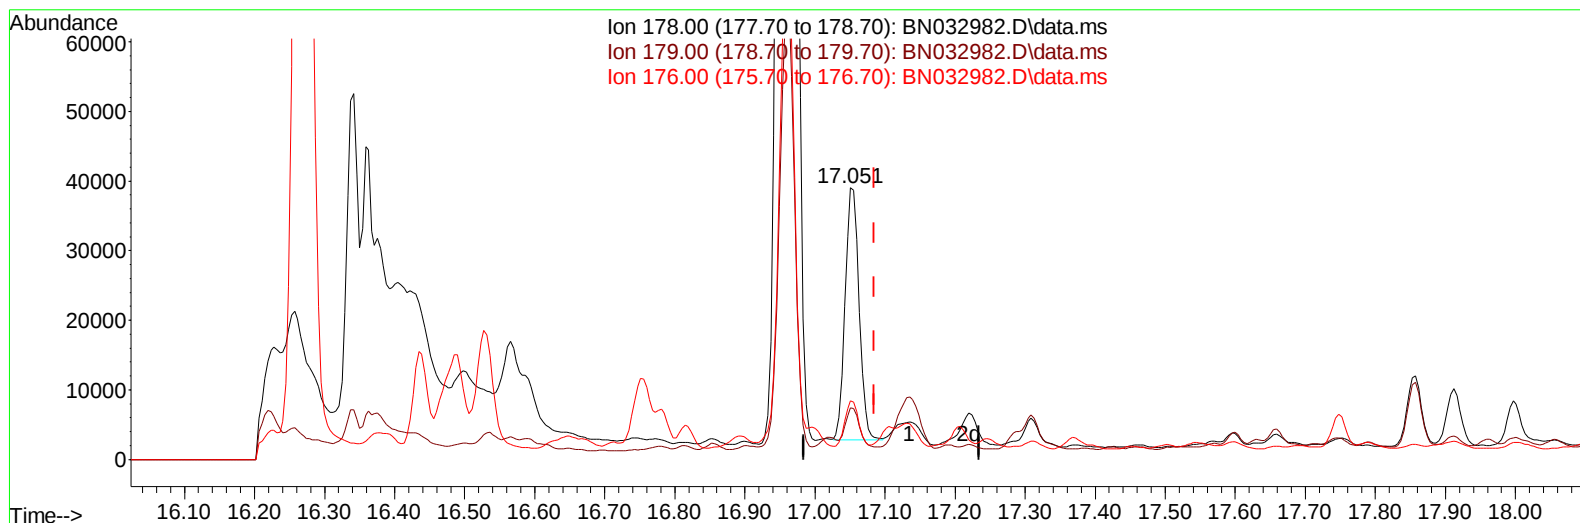

TIC: BN032982.D\data.ms

(16) Anthracene

17.051min (-0.034) 0.90 ng/ul m

response 50021

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.90	19.08
176.00	19.80	21.70
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

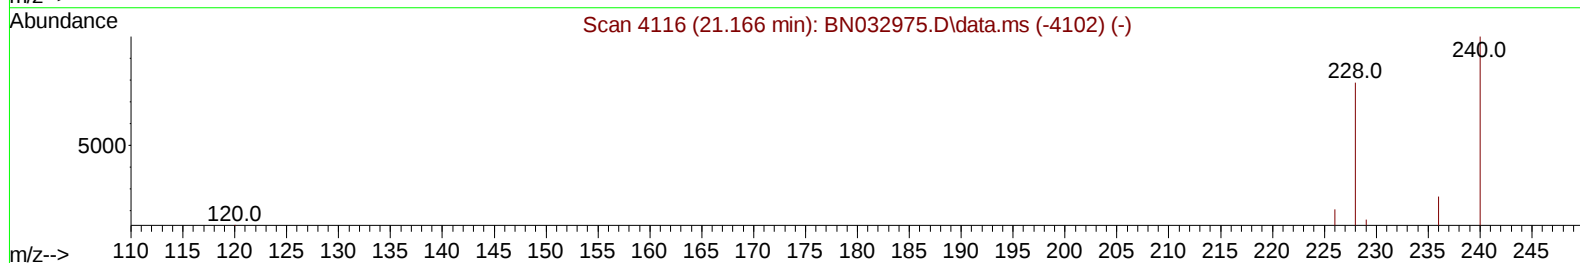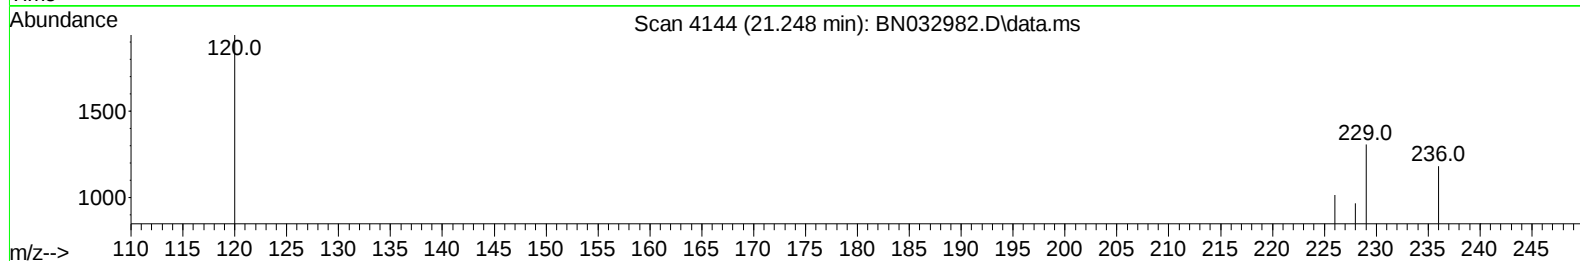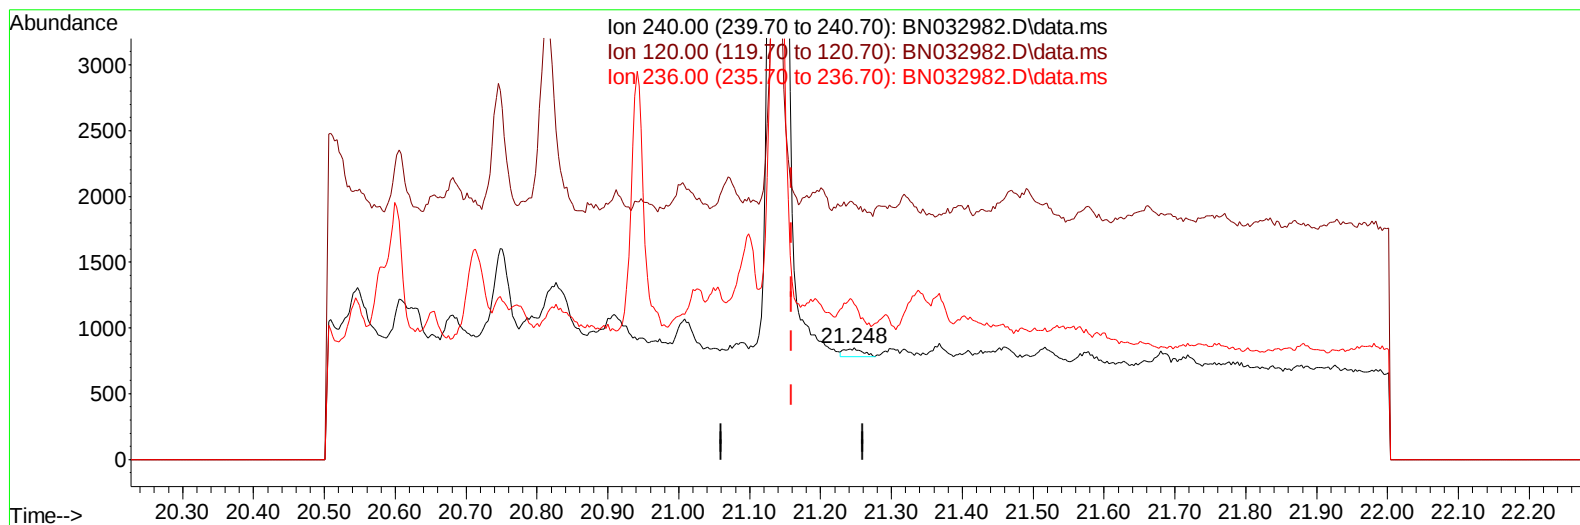

TIC: BN032982.D\data.ms

(17) Chrysene-d12

21.248min (+ 0.088) 0.40 ng/u1

response 109

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	21.40	228.89#
236.00	29.50	139.39#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

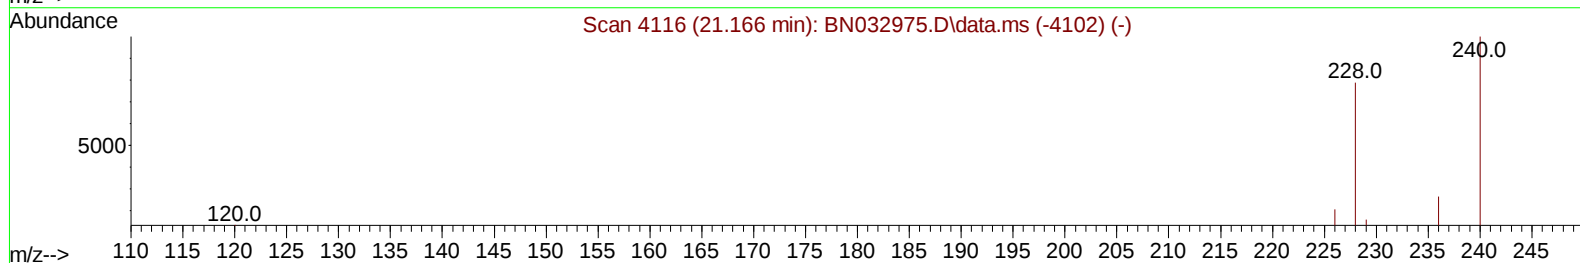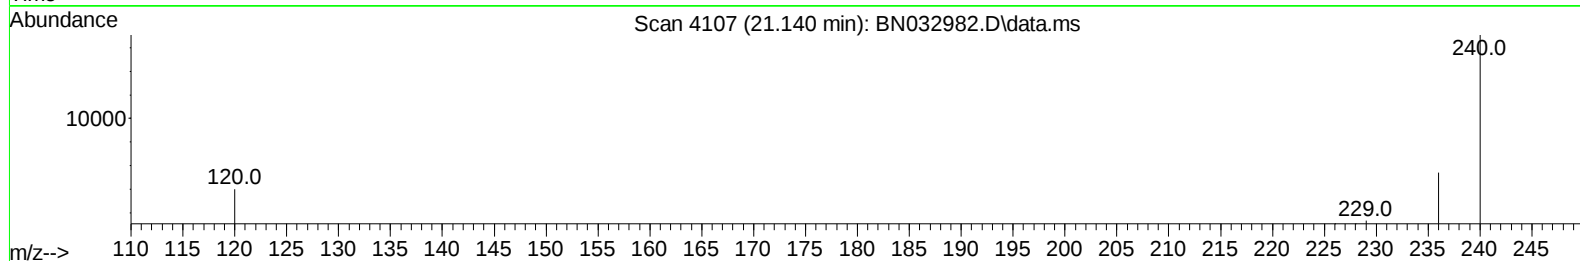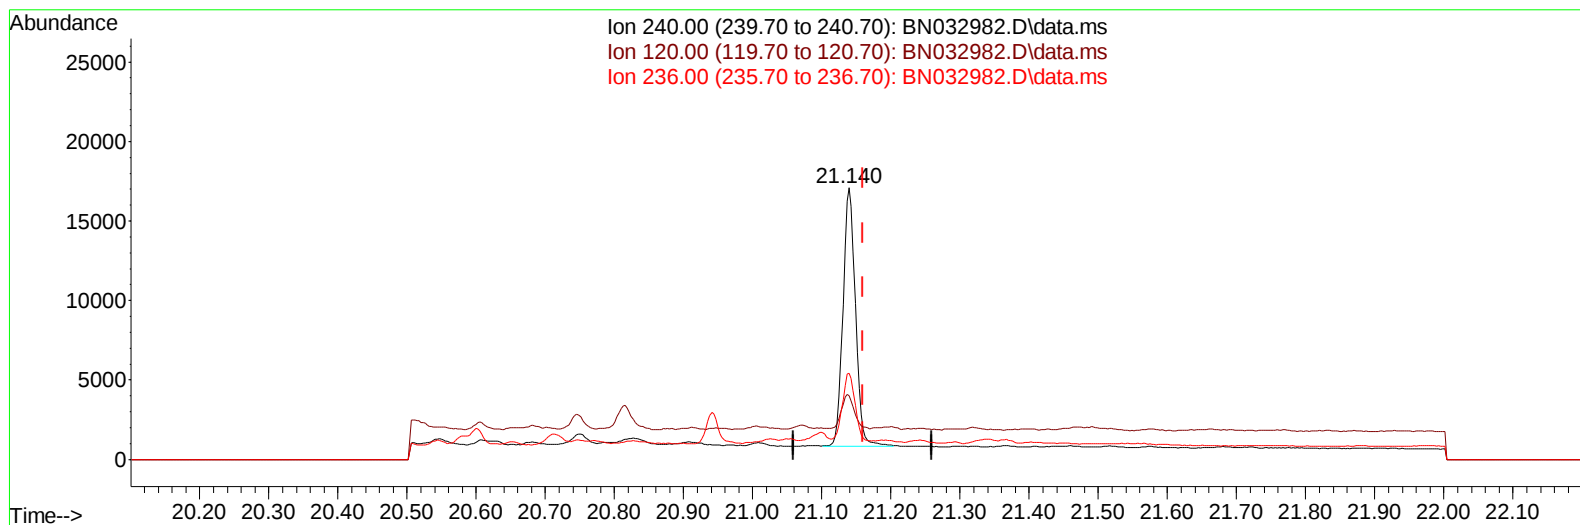

TIC: BN032982.D\data.ms

(17) Chrysene-d12

21.140min (-0.020) 0.40 ng/ul m

response 20355

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	21.40	23.54
236.00	29.50	31.79
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
 Data File : BN032982.D
 Acq On : 25 Jul 2024 21:22
 Operator : MA/JU
 Sample : P3347-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 25 15:43:00 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/30/2024

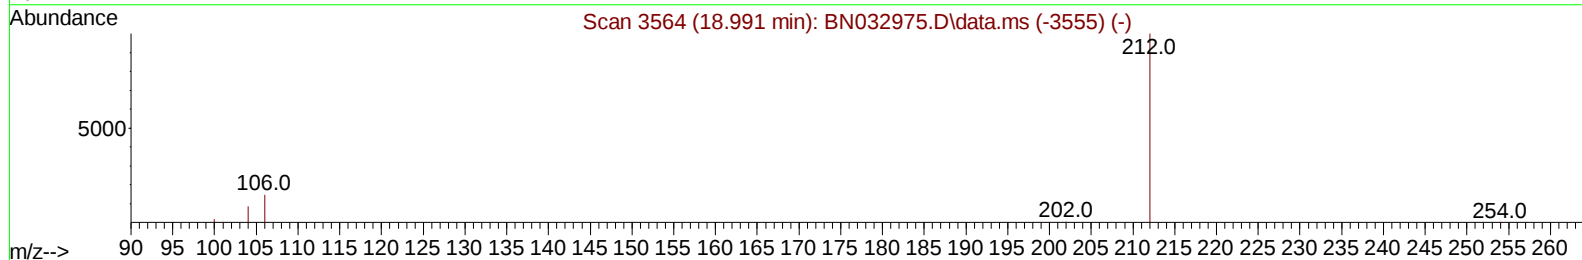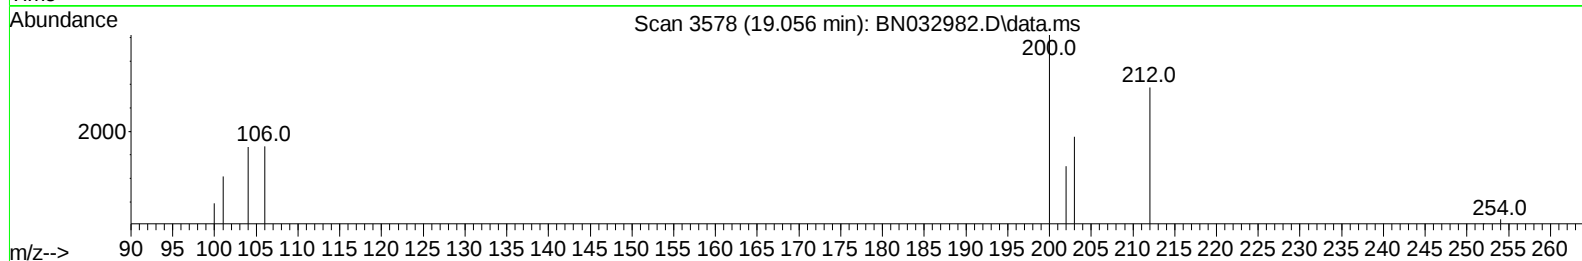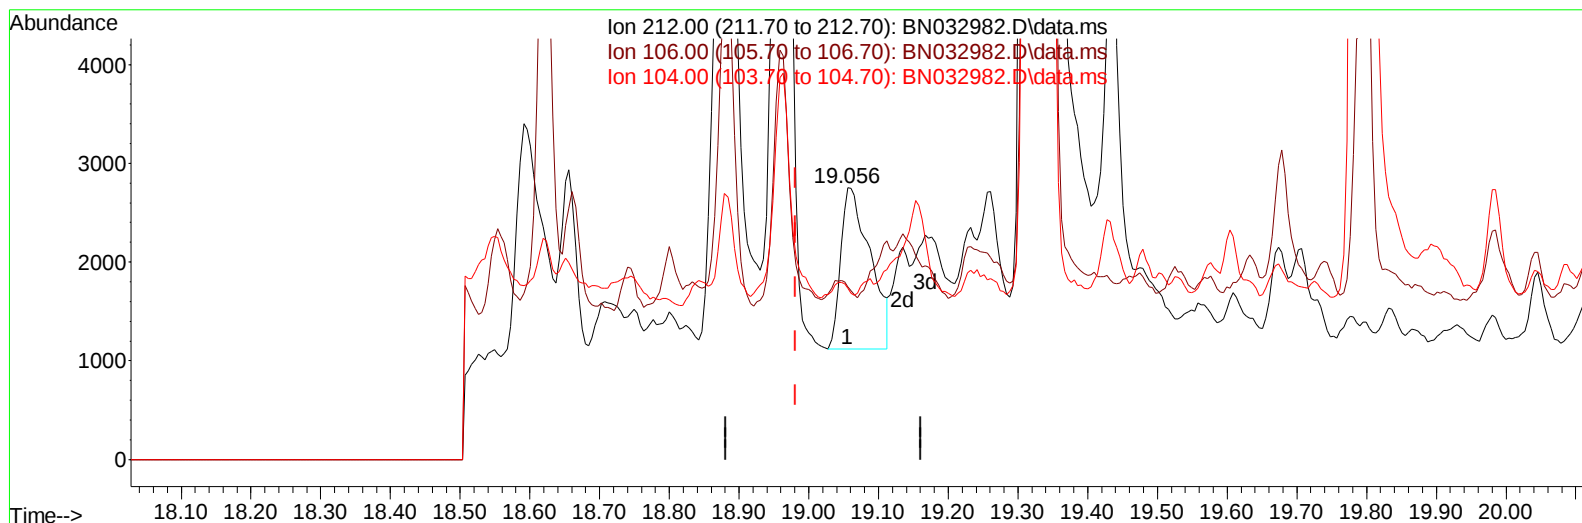

TIC: BN032982.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.056min (+ 0.075) 0.08 ng/u1

response 4808

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	15.00	7.03#
104.00	9.00	5.28#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

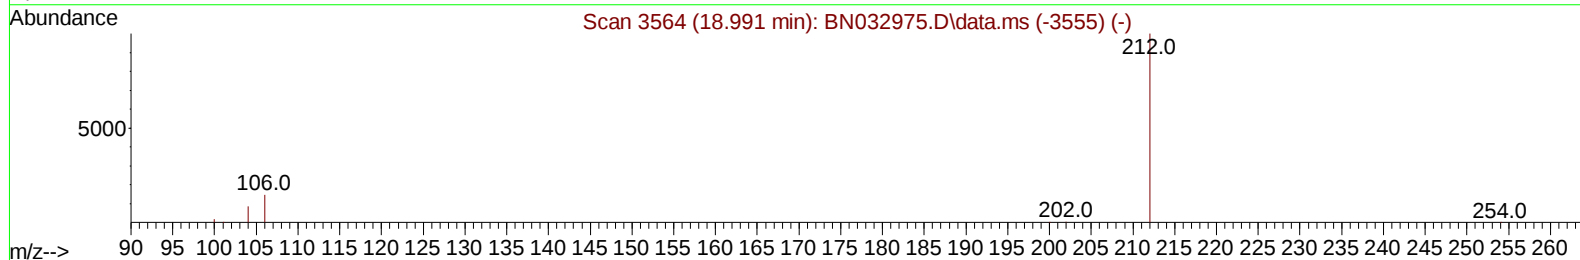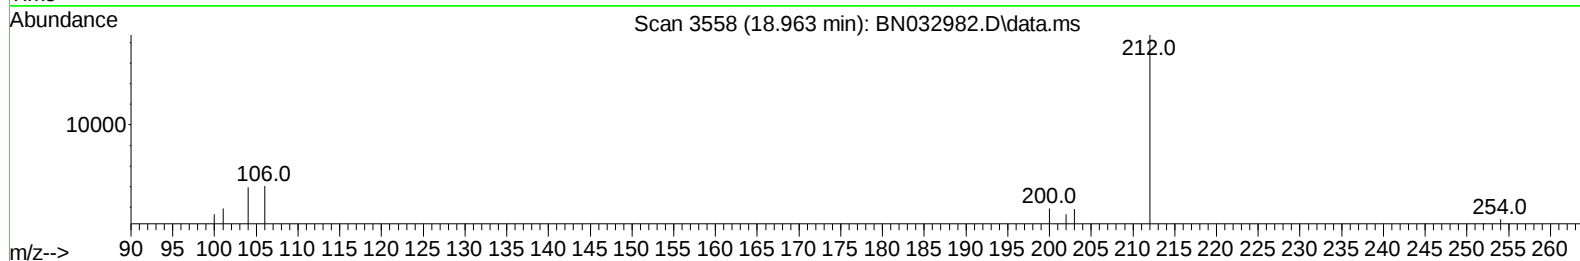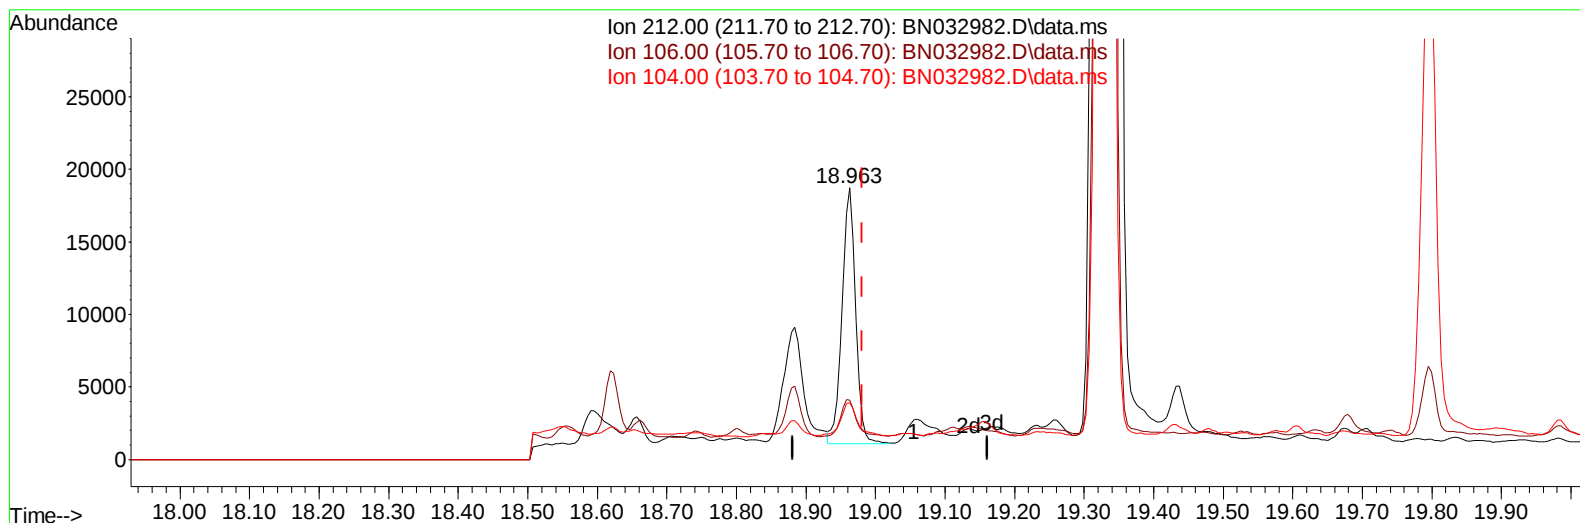

TIC: BN032982.D\data.ms

(18) Fluoranthene-d10 (SURR)

18.963min (-0.018) 0.42 ng/u1 m

response 24123

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	15.00	1.40#
104.00	9.00	1.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

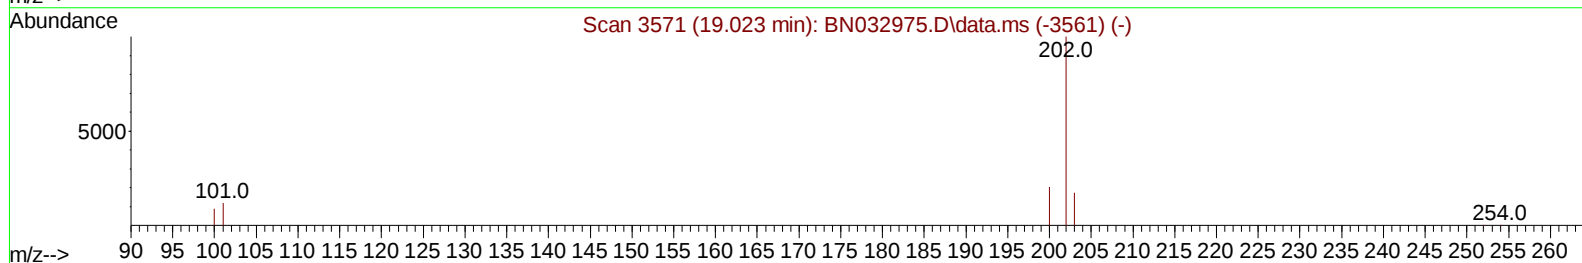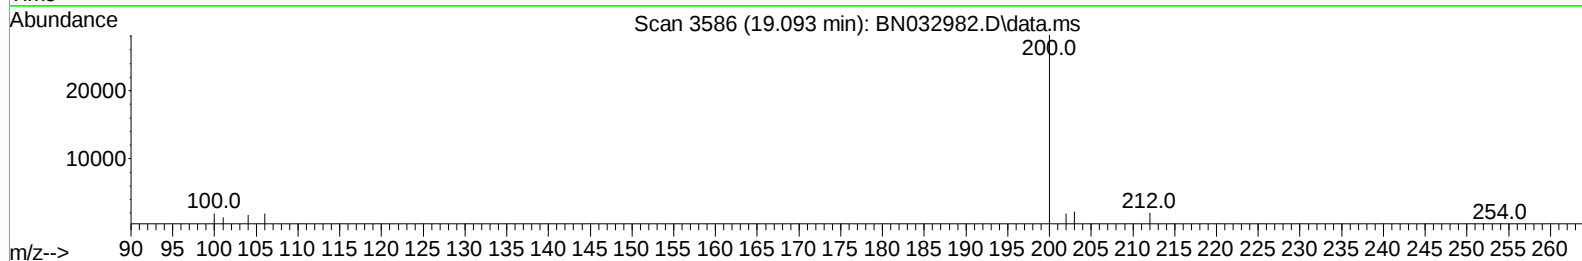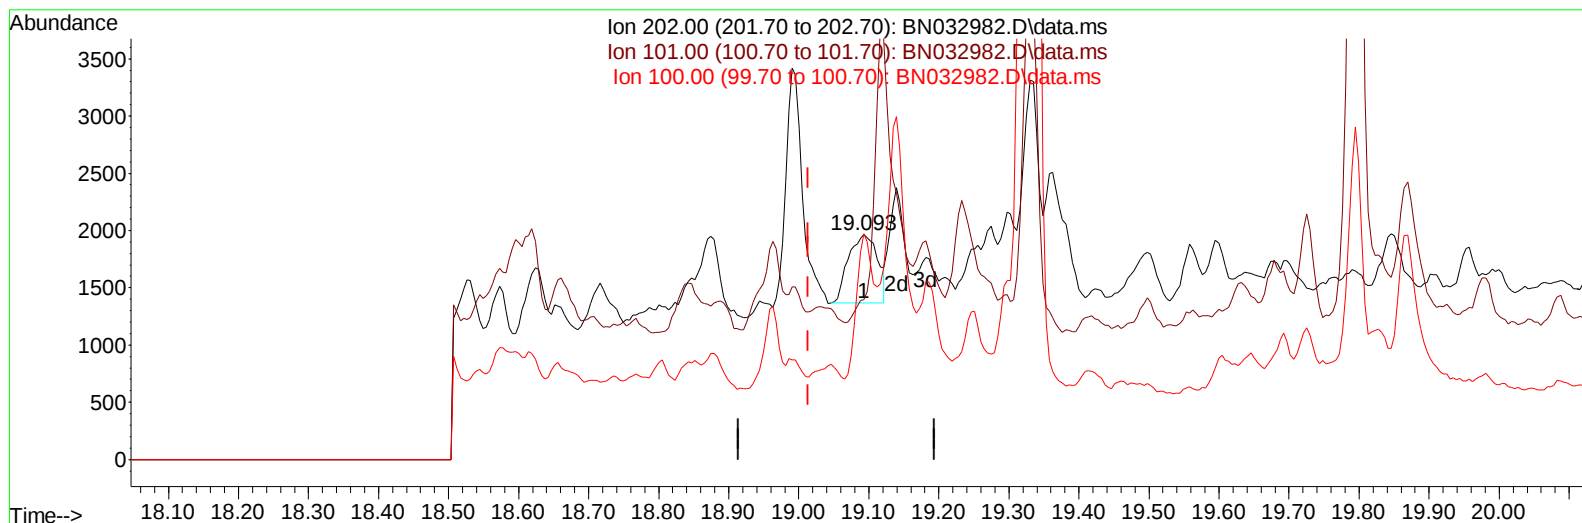

TIC: BN032982.D\data.ms

(19) Fluoranthene (C)

19.093min (+ 0.079) 0.03 ng/u1

response 1720

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.40	71.13#
100.00	10.40	100.46#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
 Data File : BN032982.D
 Acq On : 25 Jul 2024 21:22
 Operator : MA/JU
 Sample : P3347-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 25 15:43:00 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/30/2024

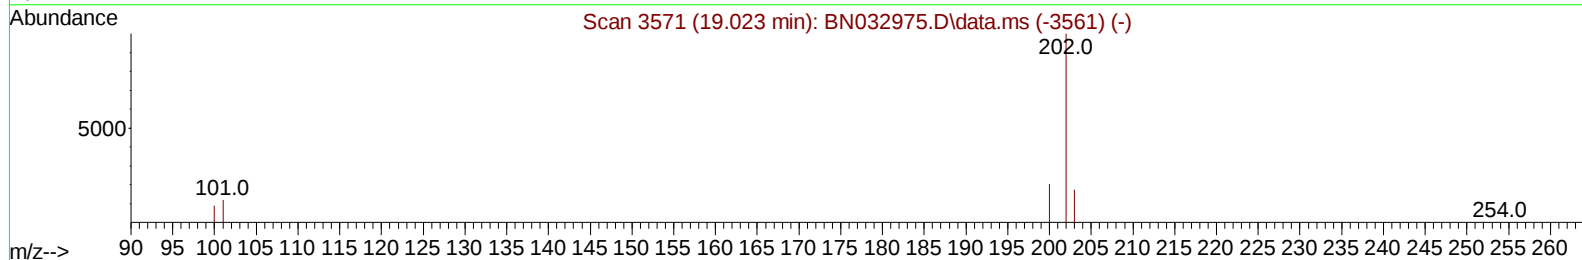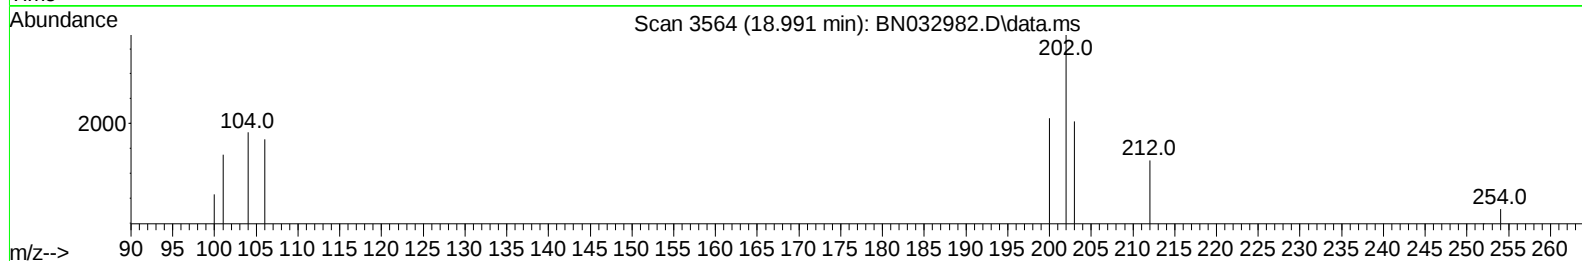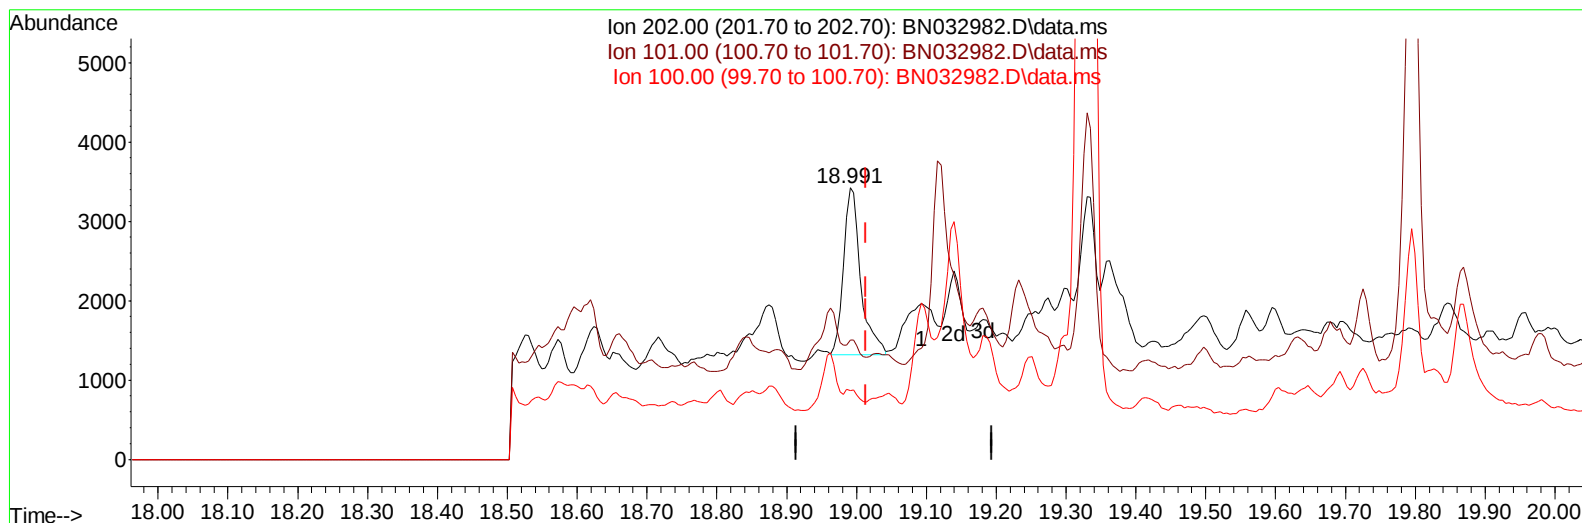

TIC: BN032982.D\data.ms

(19) Fluoranthene (C)

18.991min (-0.023) 0.05 ng/ul m

response 3536

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.40	43.99#
100.00	10.40	25.37#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

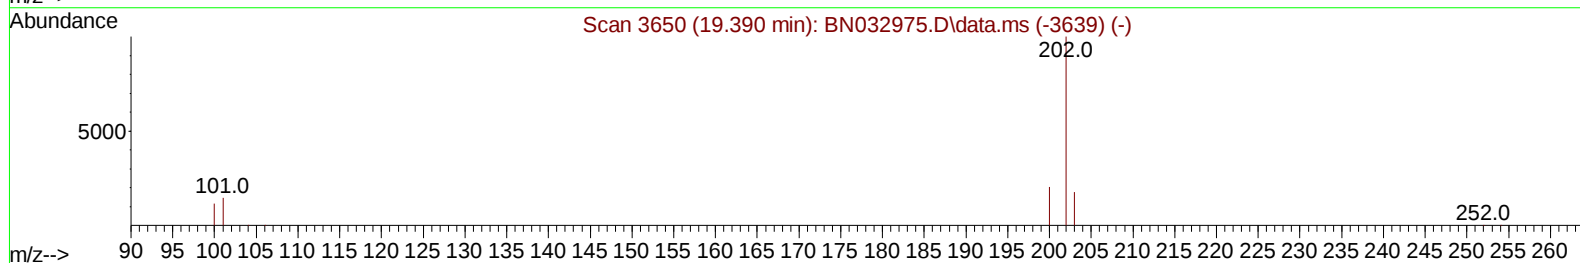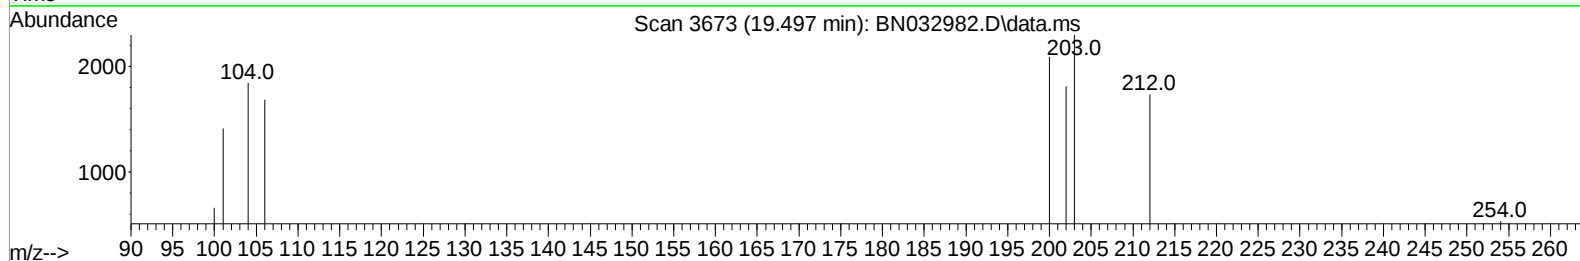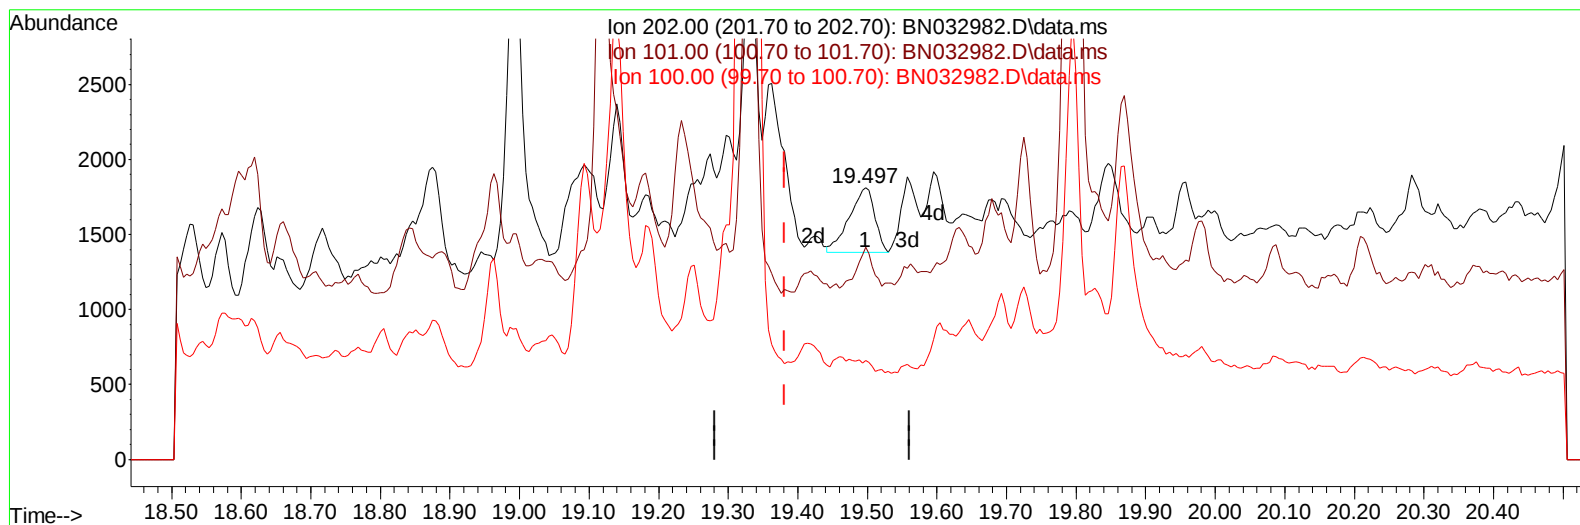

TIC: BN032982.D\data.ms

(20) Pyrene

19.497min (+ 0.116) 0.01 ng/u1

response 1074

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.70	78.07#
100.00	12.40	36.52#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

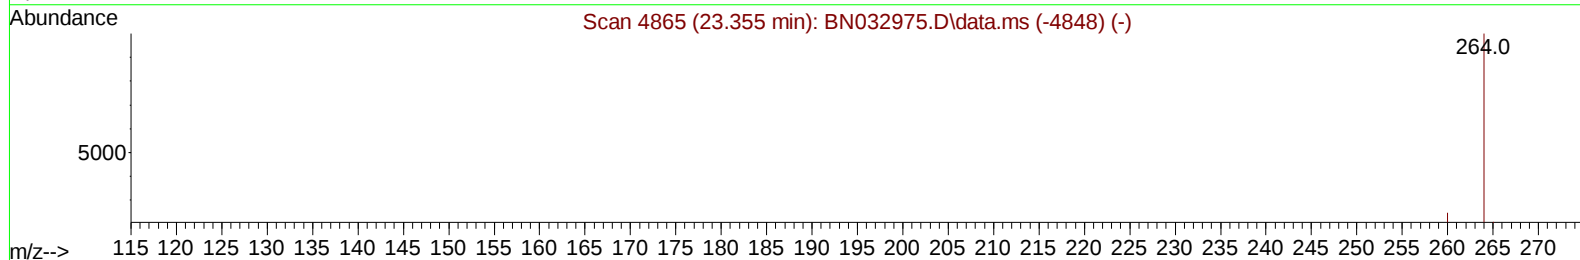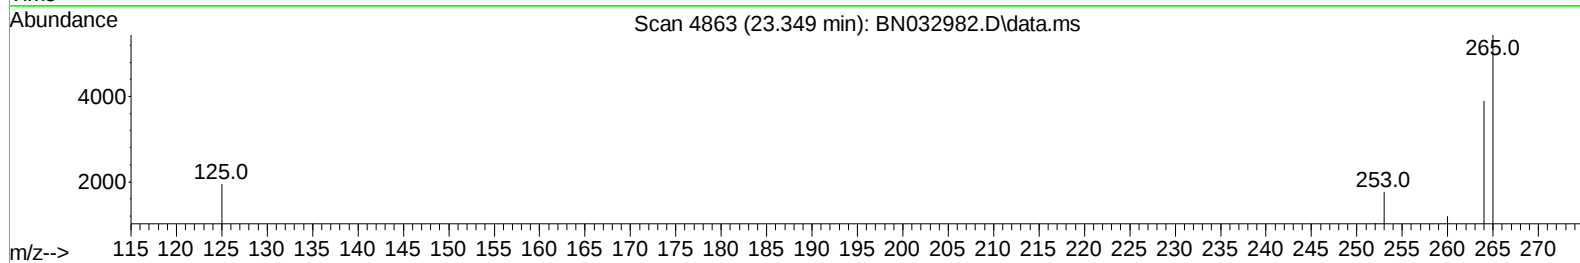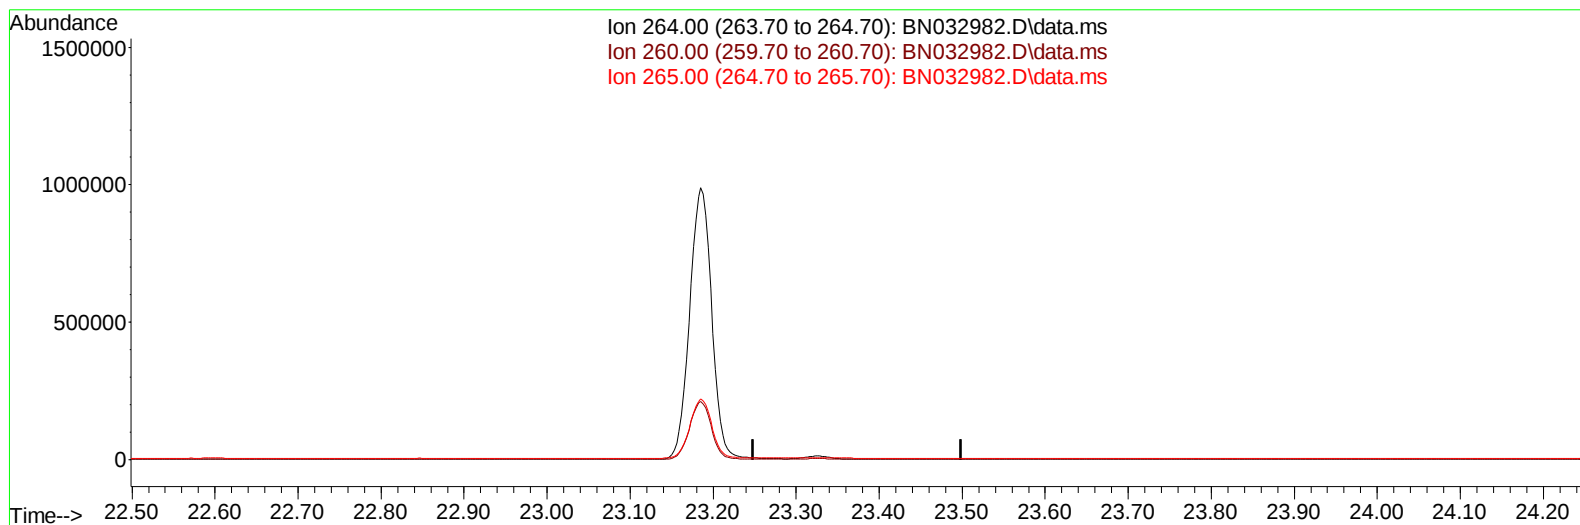

TIC: BN032982.D\data.ms

(23) Perylene-d12 (I)

23.349min (-23.349) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	26.50	0.00#
265.00	80.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

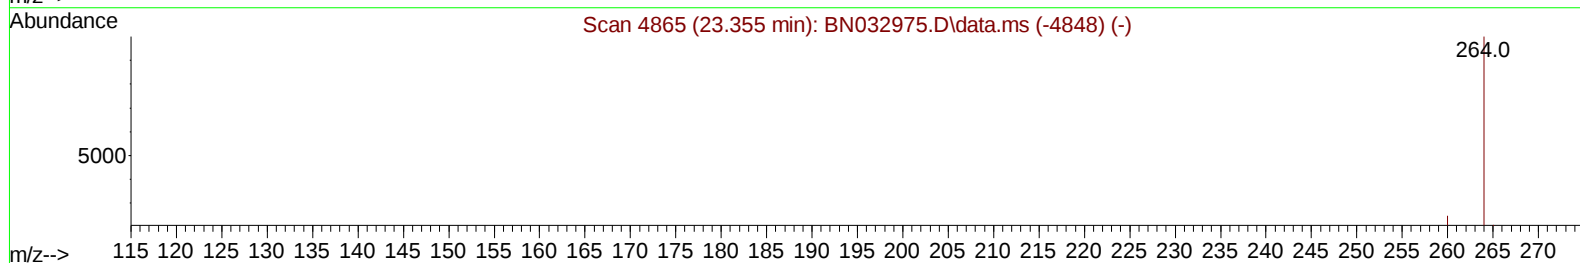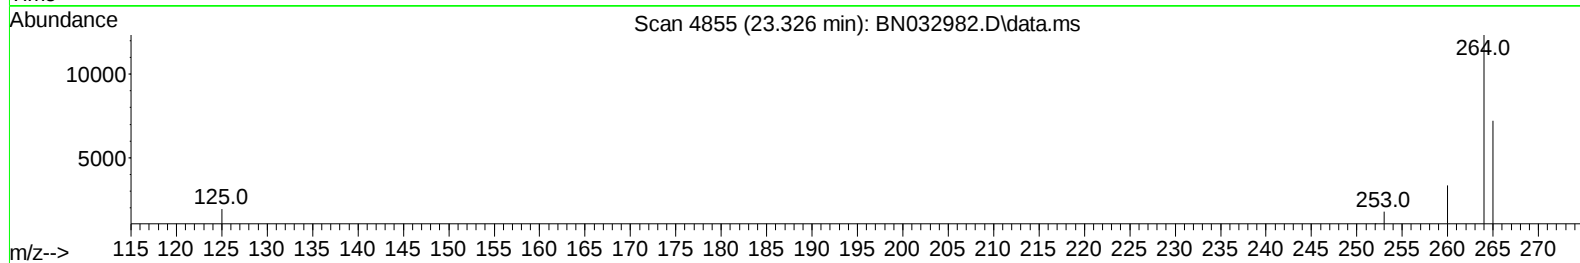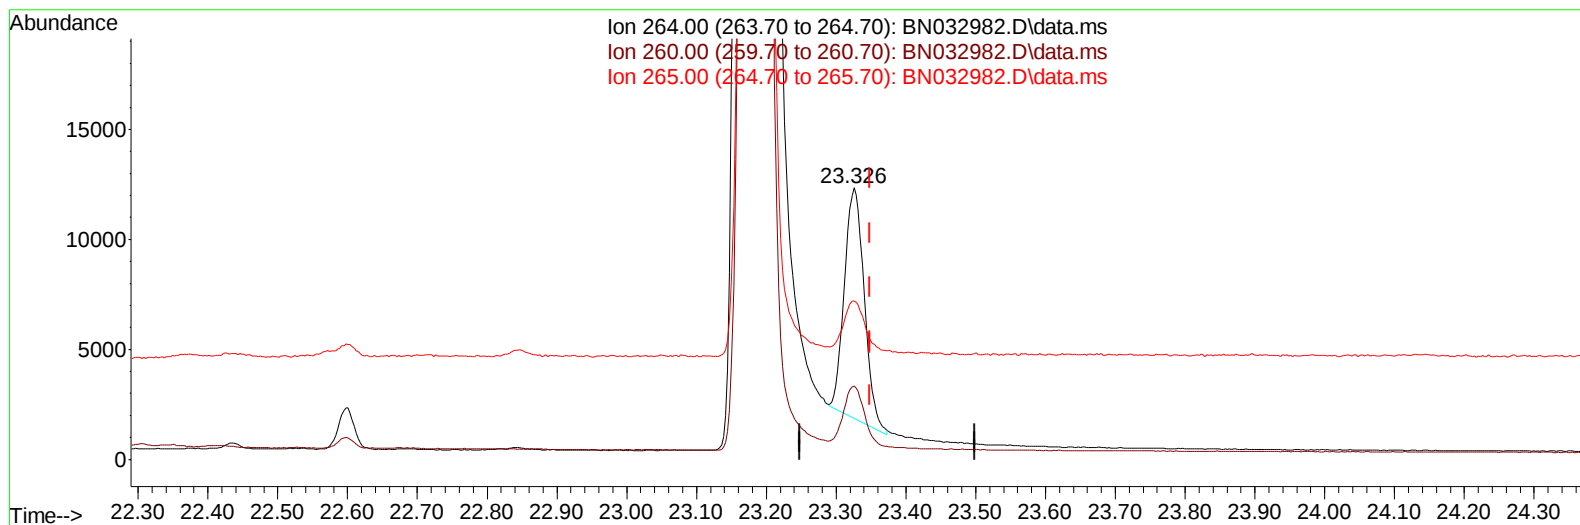

TIC: BN032982.D\data.ms

(23) Perylene-d12 (I)

23.326min (-0.023) 0.40 ng/ul m

response 20521

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.50	27.10
265.00	80.60	58.43#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
 Data File : BN032982.D
 Acq On : 25 Jul 2024 21:22
 Operator : MA/JU
 Sample : P3347-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AW5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/30/2024

Quant Time: Jul 26 01:19:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 25 15:43:00 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.503	152		4438	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.284	136		15481	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.152	164		16993	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	16.920	188		23019m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.140	240		20355m	0.400	ng/ul	-0.02
23) Perylene-d12	23.326	264		20521m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.065	96		22921	4.083	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.868	152		10966	0.434	ng/ul	-0.04
18) Fluoranthene-d10	18.963	212		24123m	0.419	ng/ul	-0.02
Target Compounds							Qvalue
5) Naphthalene	10.394	128	35670692	897.251	ng/ul		95
7) 2-Methylnaphthalene	11.961	142	8520879	316.396	ng/ul		93
8) 1-Methylnaphthalene	12.181	142	6614819	227.128	ng/ul		98
10) Acenaphthylene	13.875	152	267306	3.844	ng/ul		97
11) Acenaphthene	14.231	153	5809745	111.061	ng/ul		96
12) Fluorene	15.217	166	2221204	36.431	ng/ul		97
14) Pentachlorophenol	16.595	266	5401m	1.152	ng/ul		
15) Phenanthrene	16.962	178	544815m	8.824	ng/ul		
16) Anthracene	17.051	178	50021m	0.901	ng/ul		
19) Fluoranthene	18.991	202	3536m	0.053	ng/ul		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032982.D
Acq On : 25 Jul 2024 21:22
Operator : MA/JU
Sample : P3347-03
Misc :
ALS Vial : 17 Sample Multiplier: 3

Instrument :
BNA_N
ClientSampleId :
C0AW5

Manual IntegrationsAPPROVED

Quant Time: Jul 26 01:19:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024

