

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
 Data File : BN032978.D
 Acq On : 25 Jul 2024 18:57
 Operator : MA/JU
 Sample : P3244-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YDZF1

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/30/2024

Quant Time: Jul 26 01:18:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 25 15:43:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.503	152	4304	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.268	136	14071	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.171	164	59561	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	16.920	188	20145m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.143	240	18859m	0.400	ng/ul	-0.02
23) Perylene-d12	23.329	264	20600m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.069	96	19026	3.495	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.868	152	5198	0.226	ng/ul	-0.04
18) Fluoranthene-d10	18.968	212	14608	0.274	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.102	88	3270	0.527	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032978.D
Acq On : 25 Jul 2024 18:57
Operator : MA/JU
Sample : P3244-06
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
YDZF1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024


Quant Time: Jul 26 01:18:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

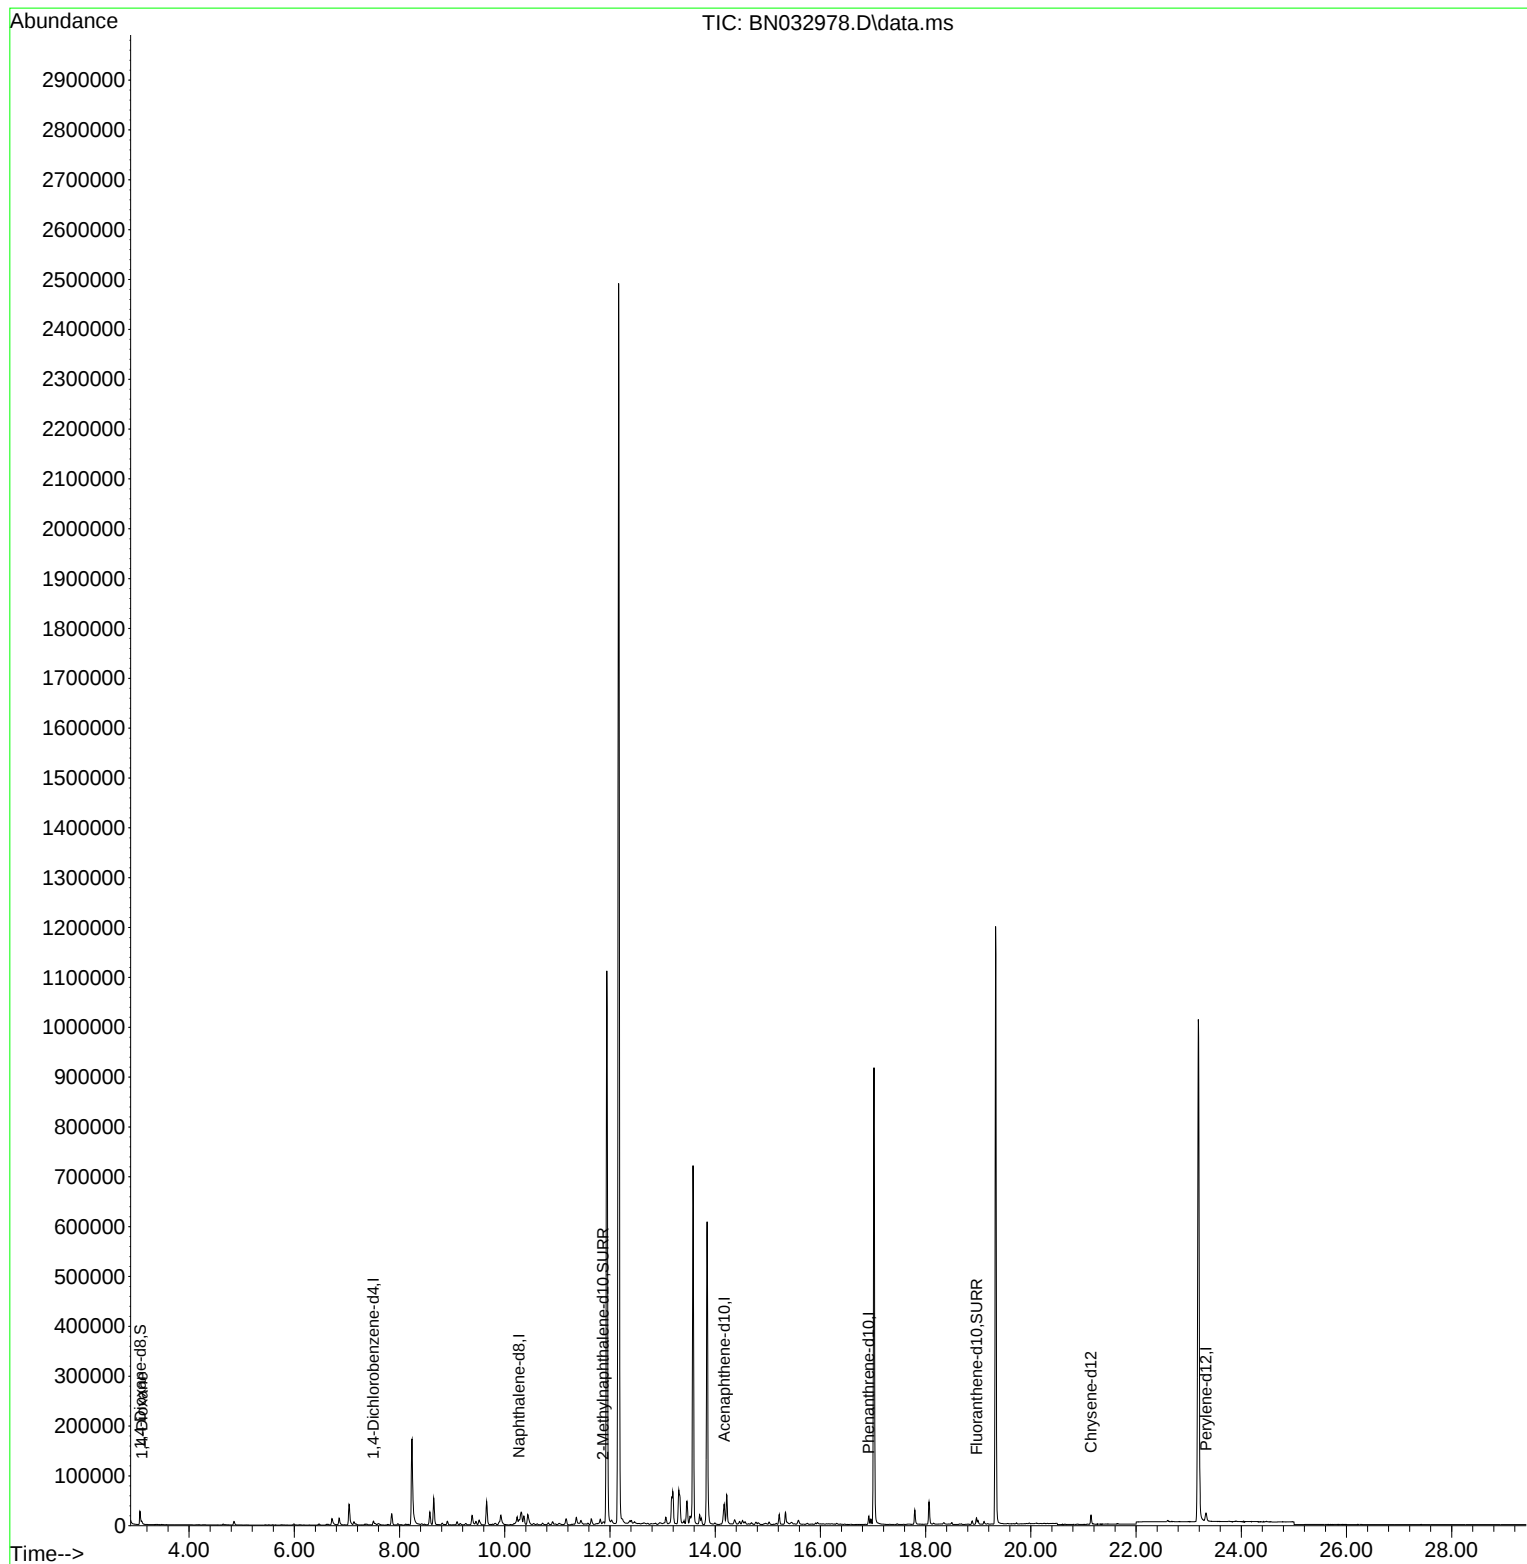

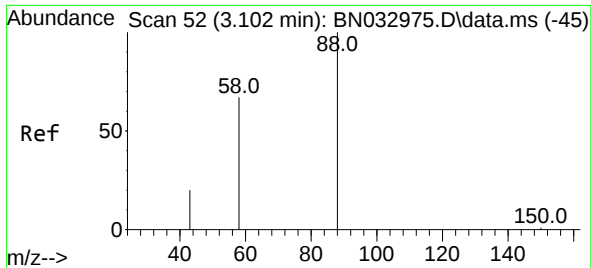

#2
 1,4-Dioxane
 Concen: 0.527 ng/ul
 RT: 3.102 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BN032978.D
 Acq: 25 Jul 2024 18:57

Instrument :
 BNA_N
 ClientSampleId :
 YDZF1

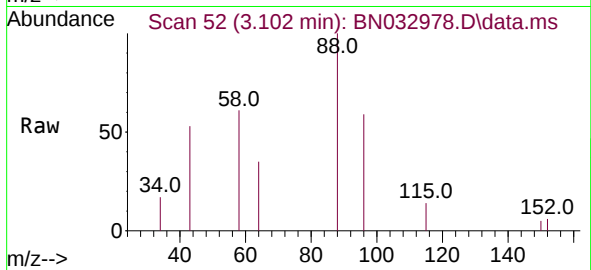

Tgt Ion: 88 Resp: 3270
 Ion Ratio Lower Upper
 88 100
 43 52.7 63.4 95.2
 58 61.4 49.4 74.0

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/30/2024

