

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
 Data File : BN032979.D
 Acq On : 25 Jul 2024 19:33
 Operator : MA/JU
 Sample : P3325-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B34

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/30/2024

Quant Time: Jul 26 01:18:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 25 15:43:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.507	152	3179	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.273	136	10600	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.157	164	7055	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.920	188	14838m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.157	240	14638m	0.400	ng/ul	0.00
23) Perylene-d12	23.334	264	14471m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.064	96	24831	6.175	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.890	152	5028	0.291	ng/ul	-0.02
18) Fluoranthene-d10	18.967	212	14715	0.355	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.098	88	8299	1.810	ng/ul#	70

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072524\
Data File : BN032979.D
Acq On : 25 Jul 2024 19:33
Operator : MA/JU
Sample : P3325-06
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0B34

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/30/2024


Quant Time: Jul 26 01:18:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

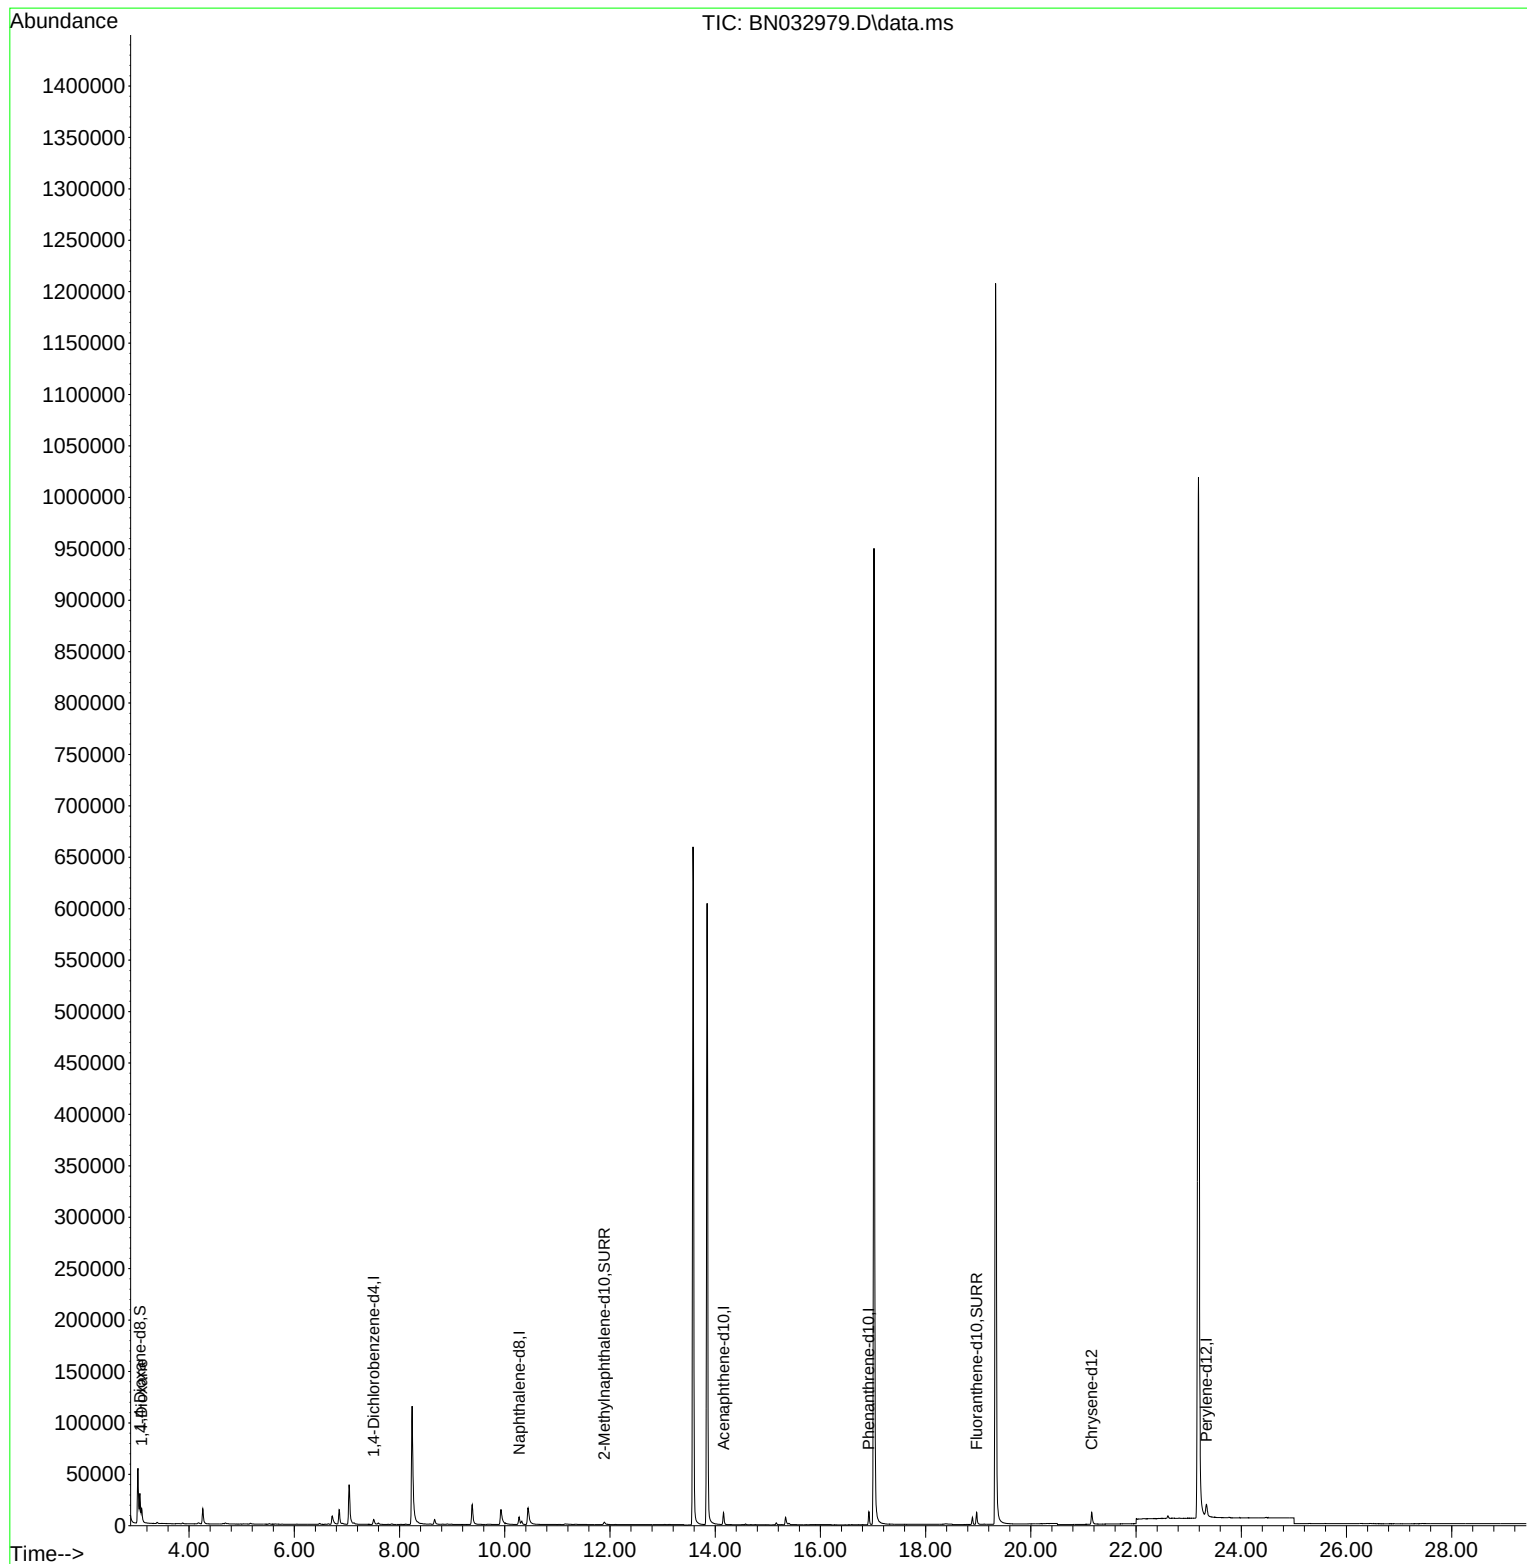

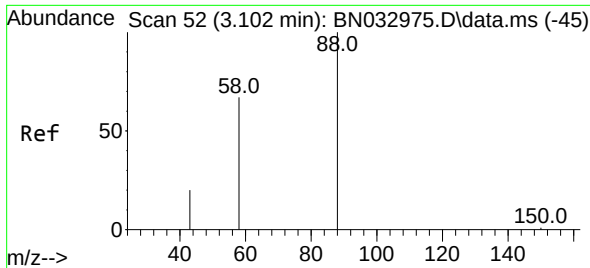

#2
 1,4-Dioxane
 Concen: 1.810 ng/ul
 RT: 3.098 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BN032979.D
 Acq: 25 Jul 2024 19:33

Instrument :
 BNA_N
 ClientSampleId :
 C0B34

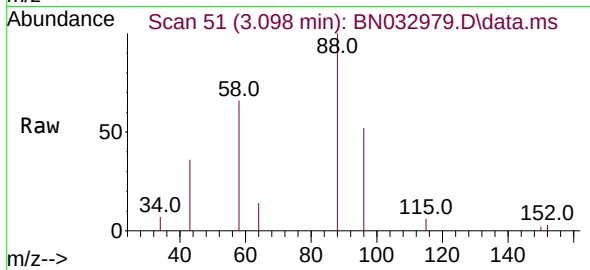

Tgt Ion: 88 Resp: 8299
 Ion Ratio Lower Upper
 88 100
 43 36.5 63.4 95.2
 58 65.5 49.4 74.0

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/30/2024

