




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072624\
Data File : BN033016.D
Acq On : 27 Jul 2024 03:15
Operator : MA/JU
Sample : PB162099BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK099

Manual IntegrationsAPPROVED

Quant Time: Jul 27 03:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

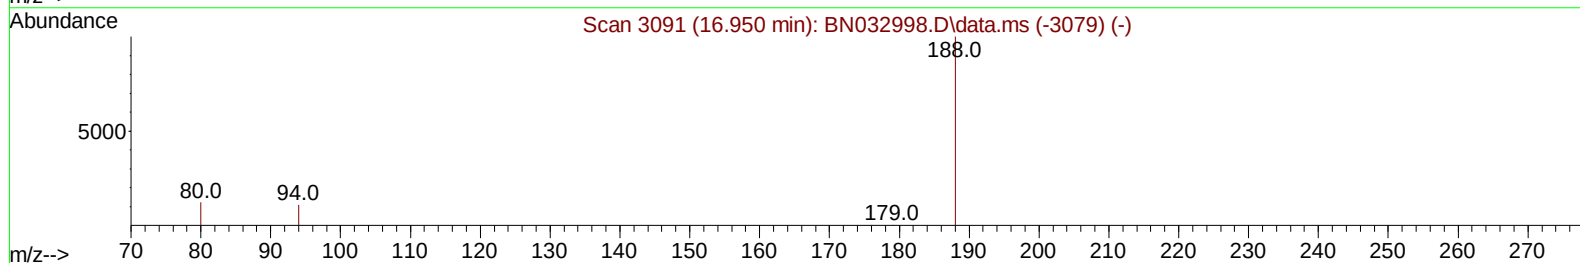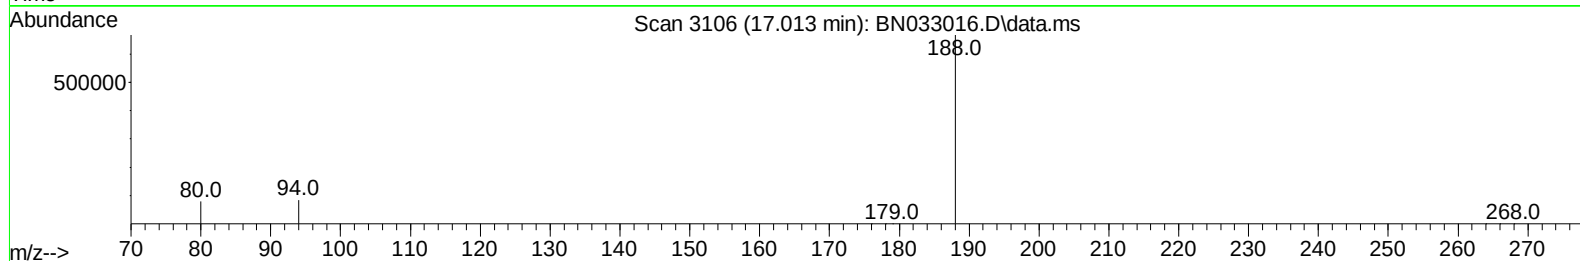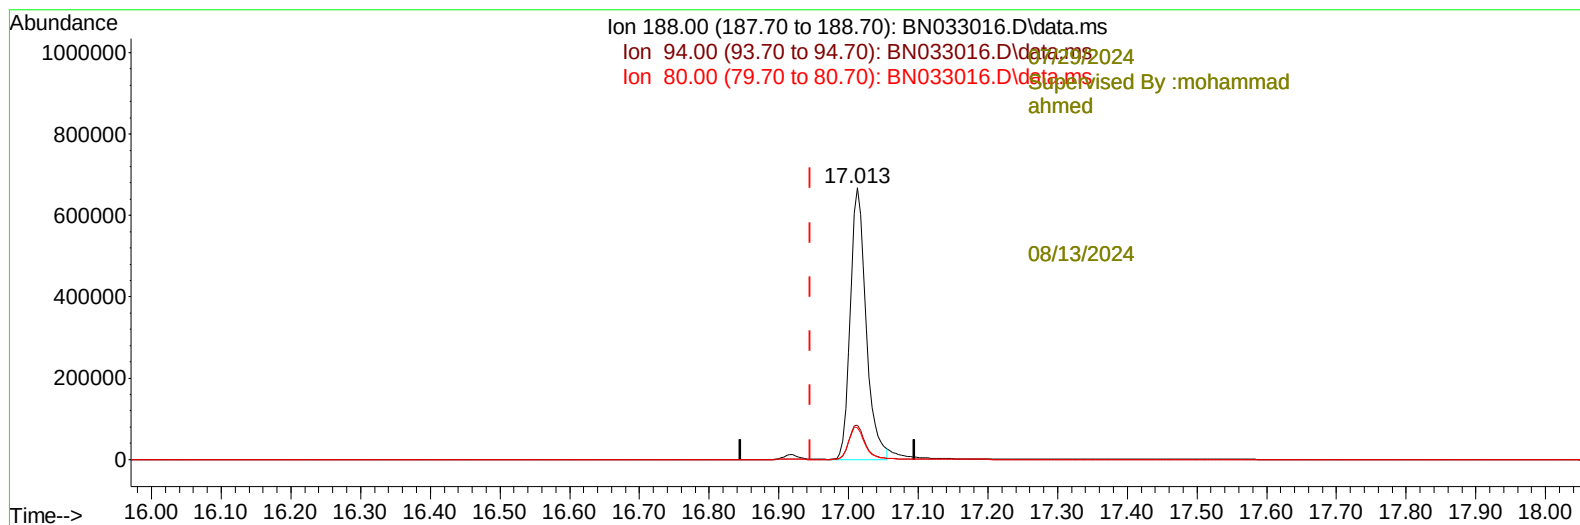

TIC: BN033016.D\data.ms

(13) Phenanthrene-d10 (I)

17.013min (+ 0.068) 0.40 ng/u1

response 1047501

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	12.72
80.00	13.10	11.79
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072624\
Data File : BN033016.D
Acq On : 27 Jul 2024 03:15
Operator : MA/JU
Sample : PB162099BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK099

Manual IntegrationsAPPROVED

Quant Time: Jul 27 03:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

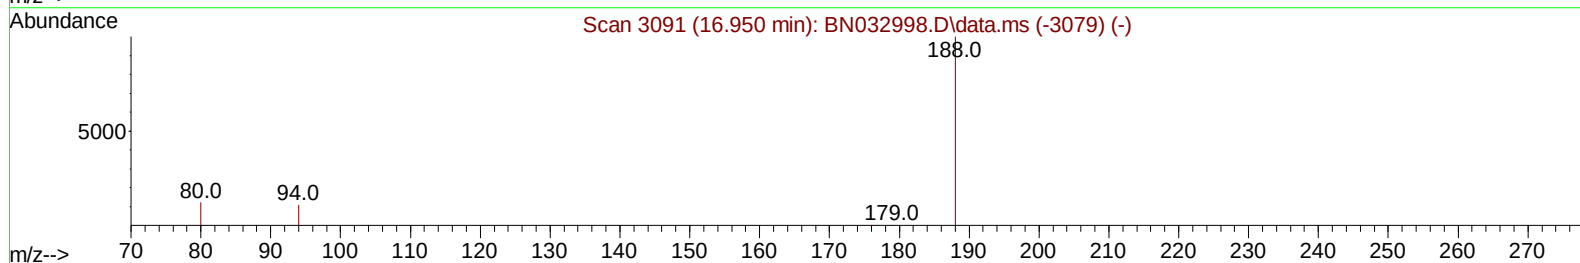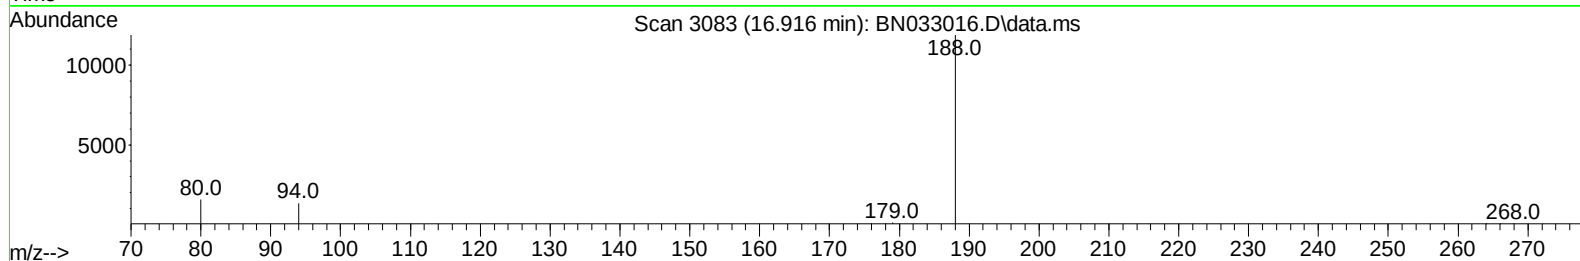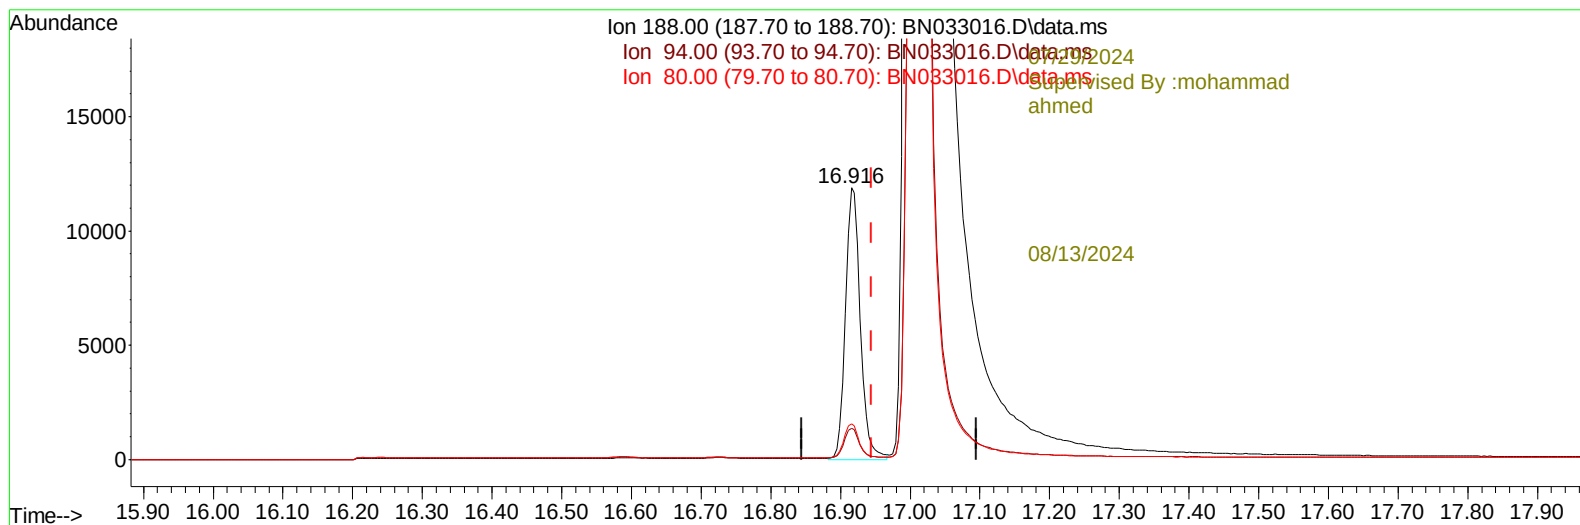

TIC: BN033016.D\data.ms

(13) Phenanthrene-d10 (I)

16.916min (-0.030) 0.40 ng/ul m

response 17554

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	11.38
80.00	13.10	13.17
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072624\
Data File : BN033016.D
Acq On : 27 Jul 2024 03:15
Operator : MA/JU
Sample : PB162099BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK099

Manual IntegrationsAPPROVED

Quant Time: Jul 27 03:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

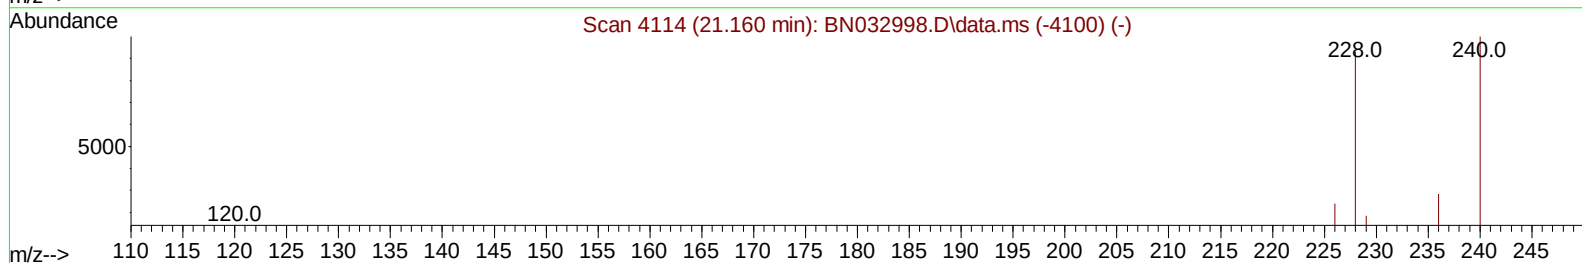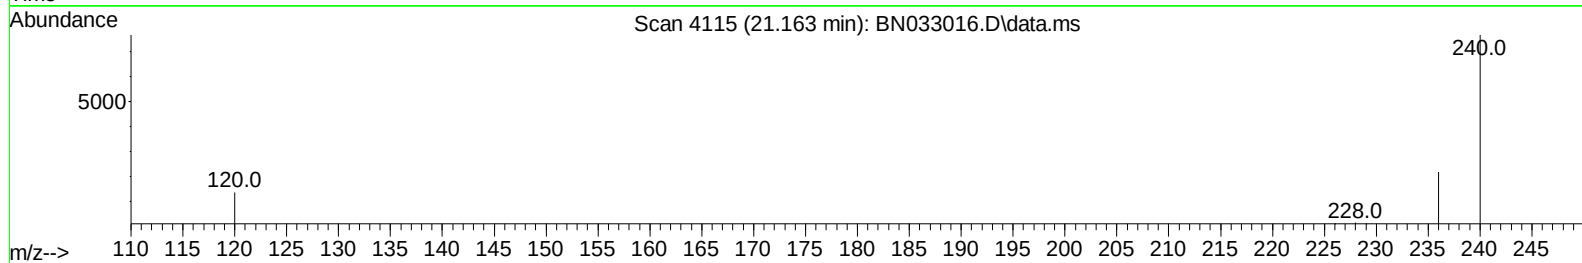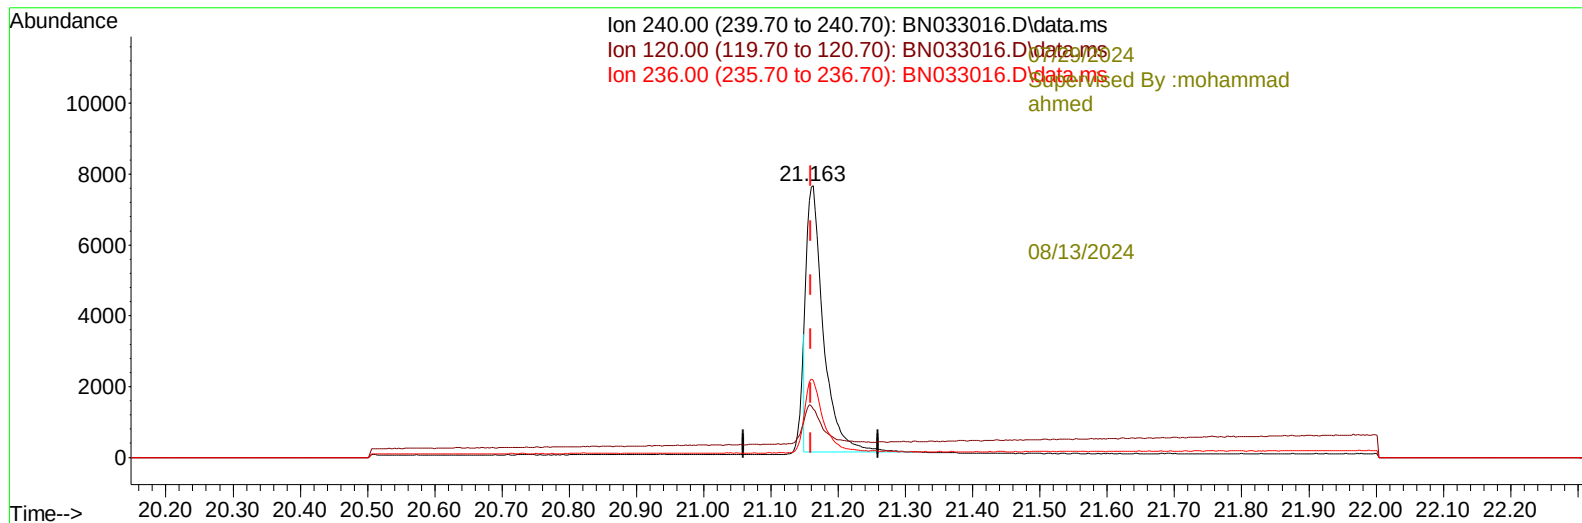

TIC: BN033016.D\data.ms

(17) Chrysene-d12

21.163min (+ 0.003) 0.40 ng/u1

response 13424

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	21.40	17.79
236.00	29.50	28.41
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072624\
Data File : BN033016.D
Acq On : 27 Jul 2024 03:15
Operator : MA/JU
Sample : PB162099BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK099

Manual IntegrationsAPPROVED

Quant Time: Jul 27 03:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

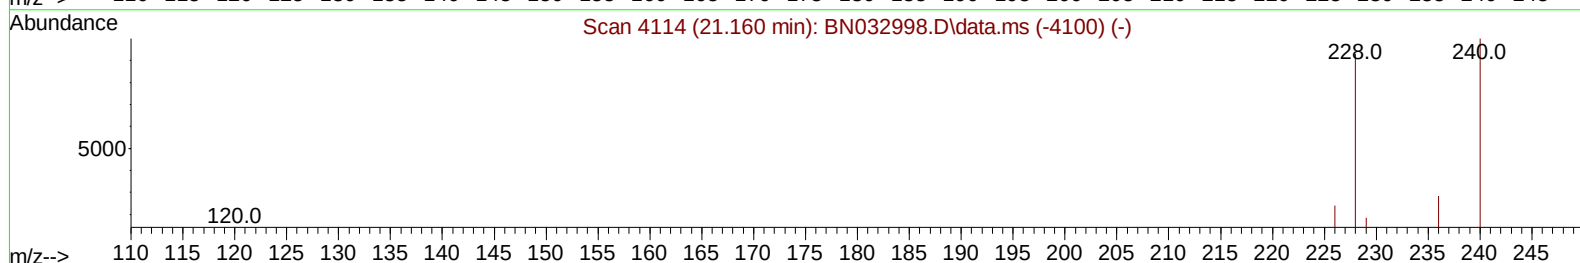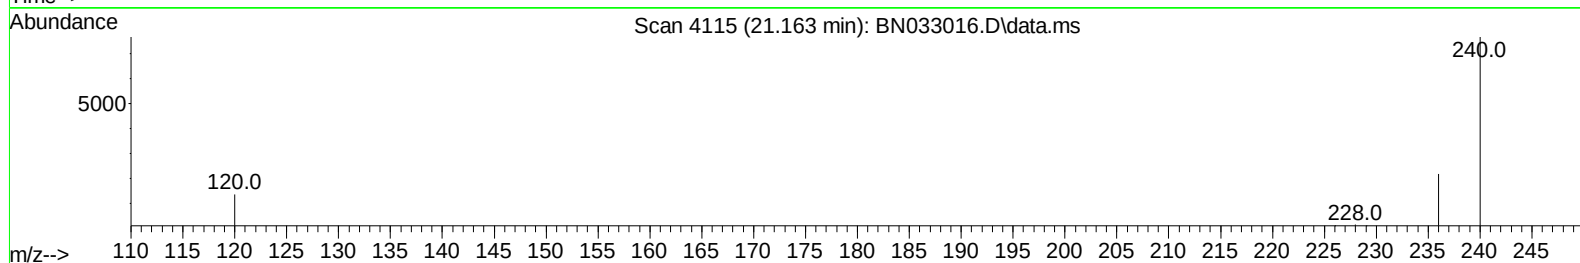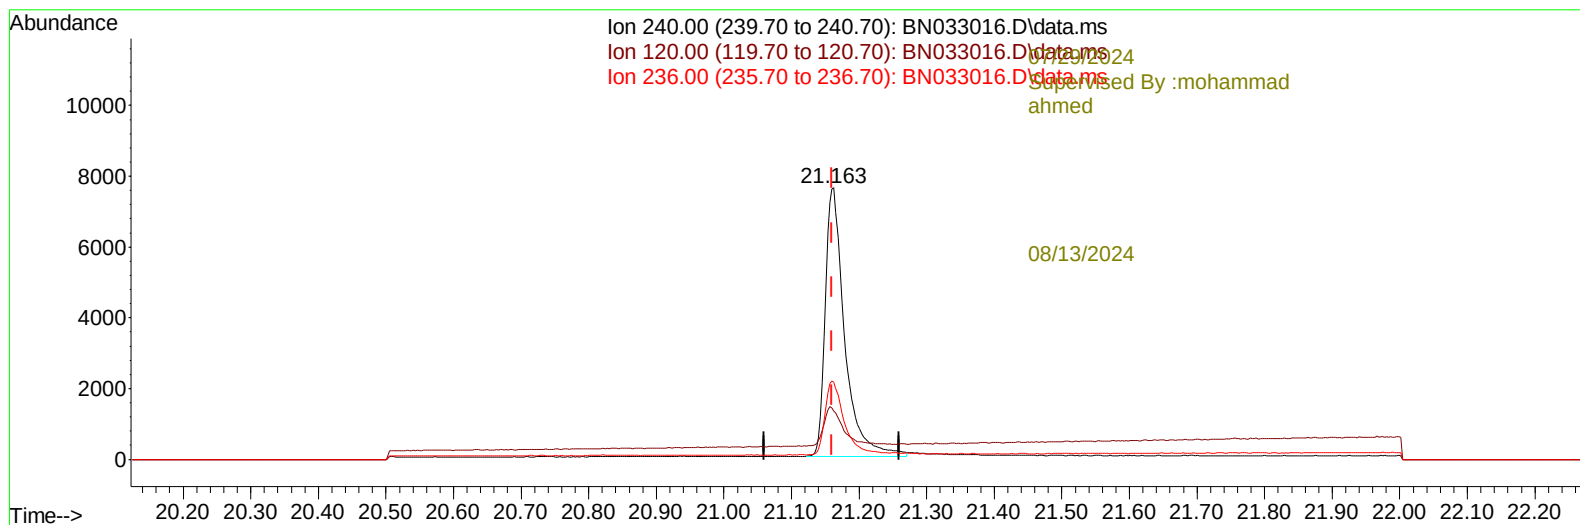

TIC: BN033016.D\data.ms

(17) Chrysene-d12

21.163min (+ 0.003) 0.40 ng/ul m

response 15225

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	21.40	17.79
236.00	29.50	28.41
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072624\
Data File : BN033016.D
Acq On : 27 Jul 2024 03:15
Operator : MA/JU
Sample : PB162099BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK099

Manual IntegrationsAPPROVED

Quant Time: Jul 27 03:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

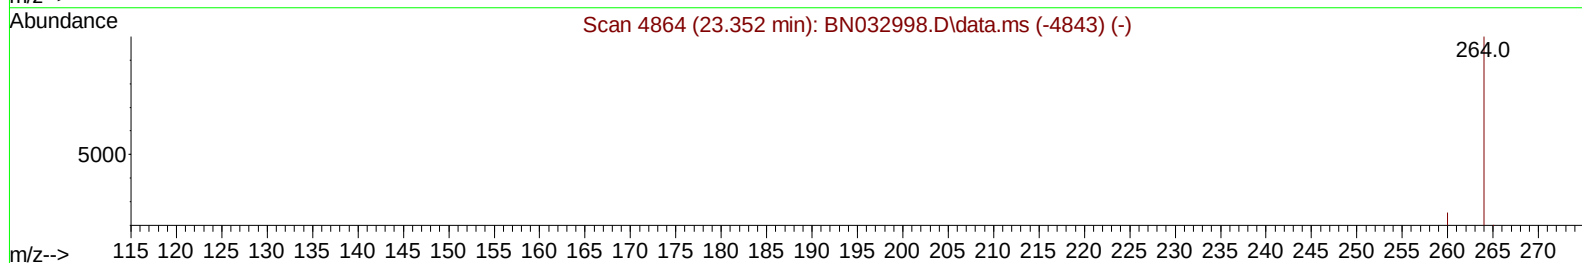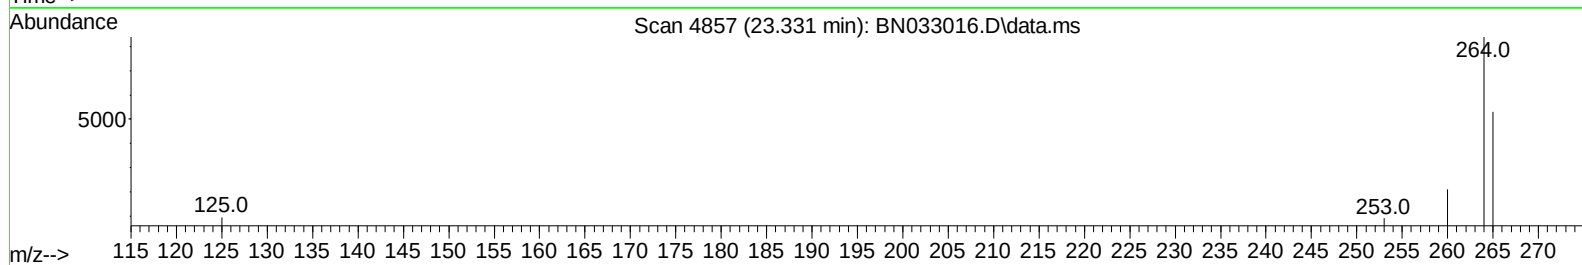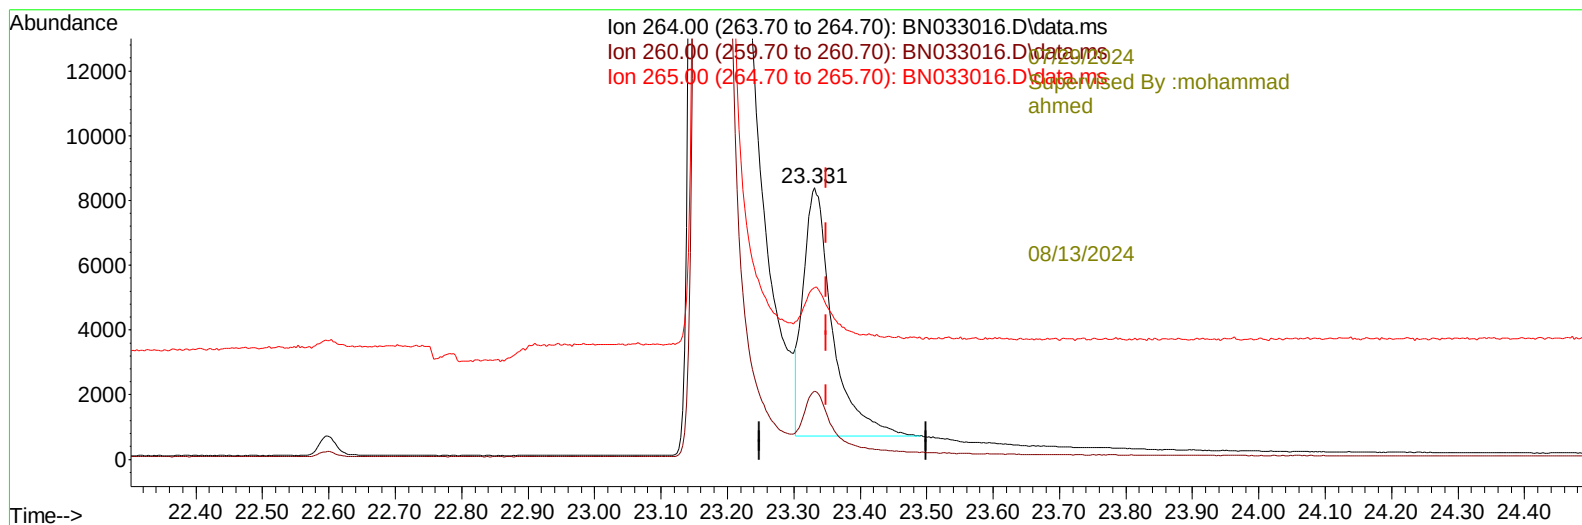

TIC: BN033016.D\data.ms

(23) Perylene-d12 (I)

23.331min (-0.017) 0.40 ng/u1

response 23389

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.50	25.21
265.00	80.60	63.35#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072624\
Data File : BN033016.D
Acq On : 27 Jul 2024 03:15
Operator : MA/JU
Sample : PB162099BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK099

Manual IntegrationsAPPROVED

Quant Time: Jul 27 03:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

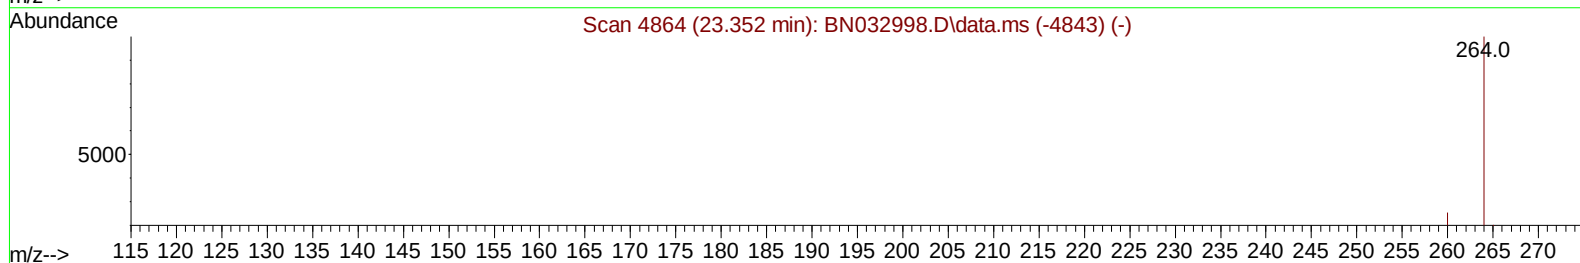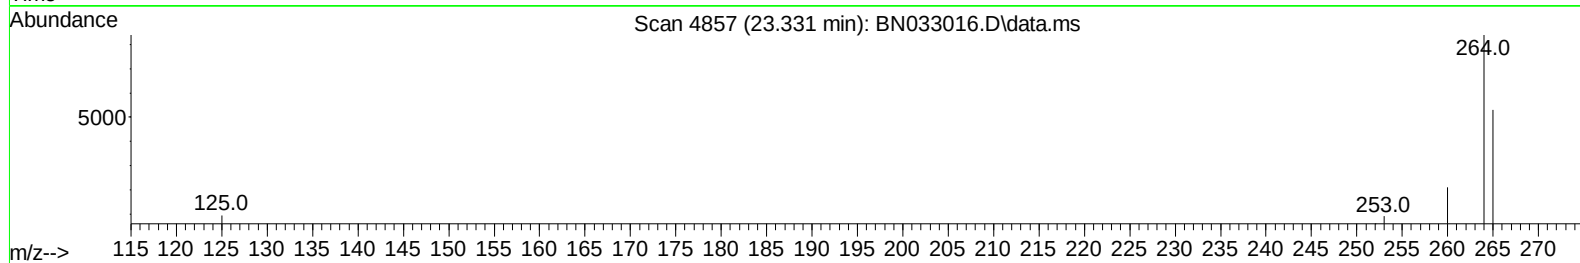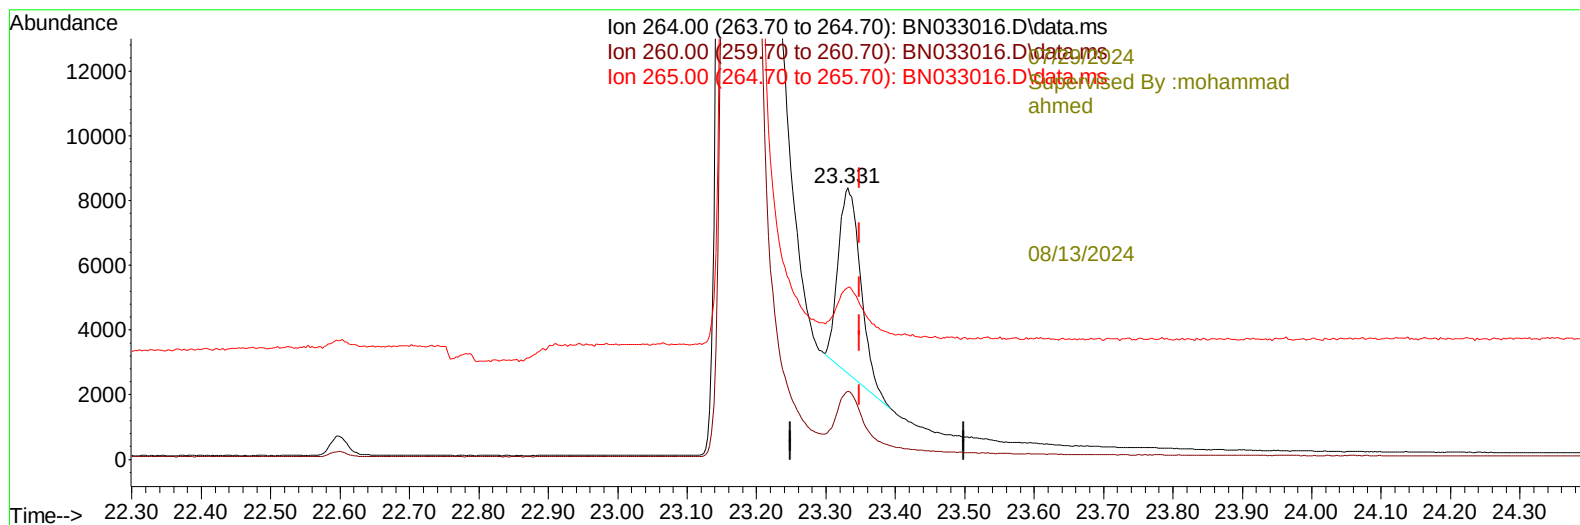

TIC: BN033016.D\data.ms

(23) Perylene-d12 (I)

23.331min (-0.017) 0.40 ng/ul m

response 12838

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.50	25.21
265.00	80.60	63.35#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072624\
 Data File : BN033016.D
 Acq On : 27 Jul 2024 03:15
 Operator : MA/JU
 Sample : PB162099BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK099

Manual IntegrationsAPPROVED

Quant Time: Jul 27 03:42:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 25 15:43:00 2024
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----07/29/2024							
Supervised By :mohammad							
aimed							
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.507	152		3616	0.400	ng/ul	#-0.02
4) Naphthalene-d8	10.267	136		13009	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.152	164		7992	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	16.916	188		17554m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.163	240		15225m	0.400	ng/ul	0.00
23) Perylene-d12	23.331	264		12838m	0.400	ng/ul	-0.02
-----13/2024							
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.060	96		22380	4.893	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.912	152		4725	0.223	ng/ul	0.00
18) Fluoranthene-d10	18.963	212		12717	0.295	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072624\
Data File : BN033016.D
Acq On : 27 Jul 2024 03:15
Operator : MA/JU
Sample : PB162099BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK099

Manual IntegrationsAPPROVED

Quant Time: Jul 27 03:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

