

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072624\
 Data File : BN033006.D
 Acq On : 26 Jul 2024 20:39
 Operator : MA/JU
 Sample : P3244-06RE
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YDZF1RE

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/29/2024
 Supervised By :mohammad ahmed 08/13/2024

Quant Time: Jul 26 23:34:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 25 15:43:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.499	152	5272	0.400	ng/ul	#-0.03
4) Naphthalene-d8	10.262	136	16820	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.166	164	63624	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	16.911	188	25531m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.139	240	21233m	0.400	ng/ul	-0.02
23) Perylene-d12	23.323	264	18745m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.064	96	24451	3.667	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.862	152	6768	0.247	ng/ul	-0.05
18) Fluoranthene-d10	18.963	212	18234	0.303	ng/ul	-0.02
Target Compounds						
2) 1,4-Dioxane	3.098	88	4114	0.541	ng/ul#	Qvalue 76

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072624\
Data File : BN033006.D
Acq On : 26 Jul 2024 20:39
Operator : MA/JU
Sample : P3244-06RE
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
YDZF1RE

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/29/2024
Supervised By :mohammad ahmed 08/13/2024


Quant Time: Jul 26 23:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

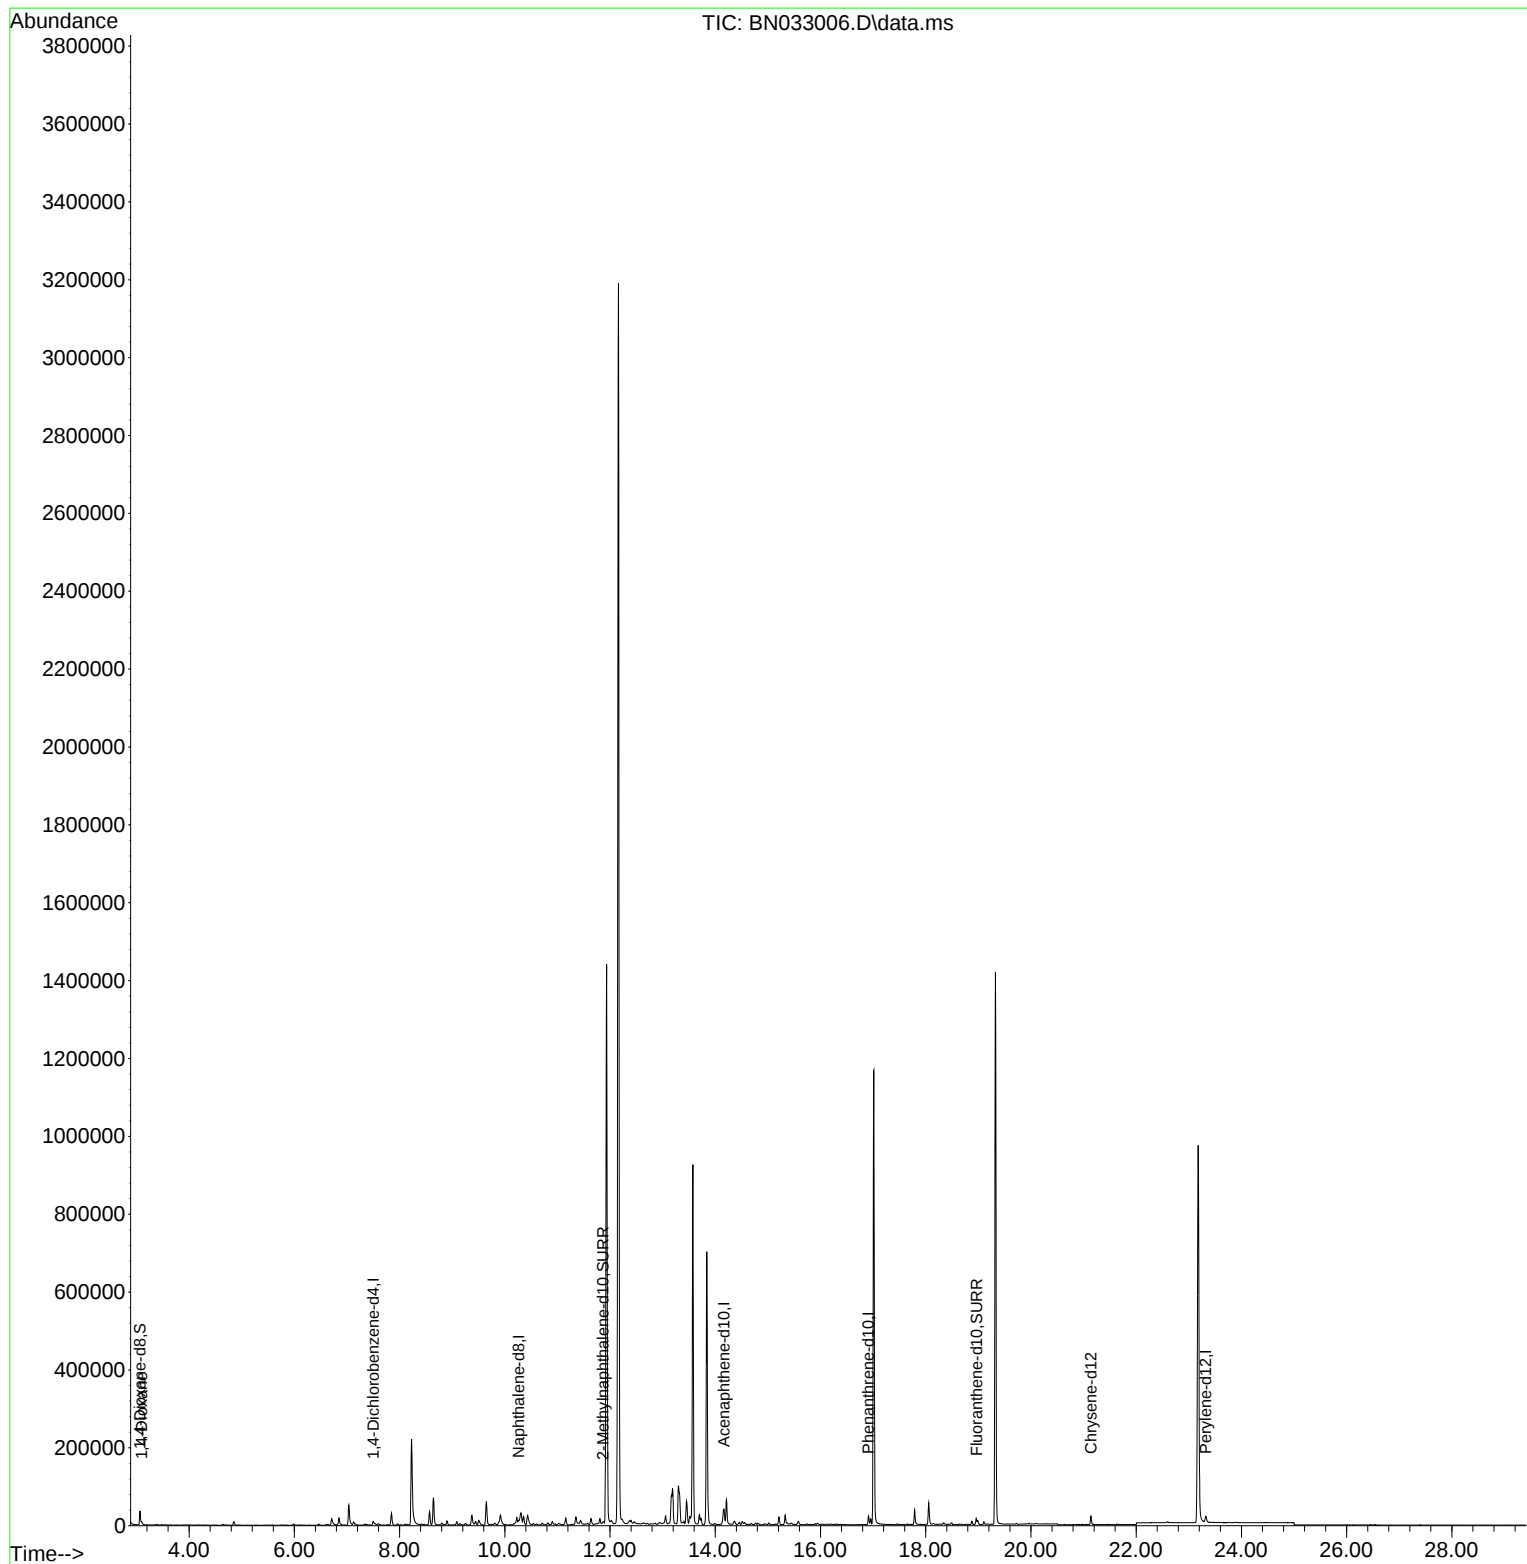

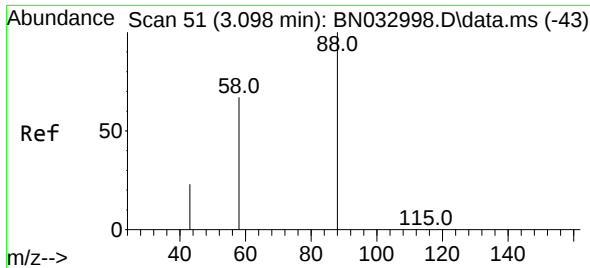

#2
 1,4-Dioxane
 Concen: 0.541 ng/ul
 RT: 3.098 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BN033006.D
 Acq: 26 Jul 2024 20:39

Instrument :
 BNA_N
 ClientSampleId :
 YDZF1RE

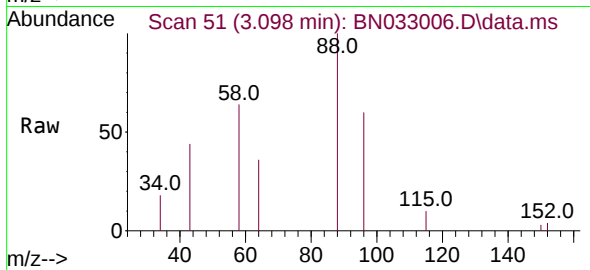

Tgt Ion: 88 Resp: 4114

Ion	Ratio	Lower	Upper
88	100		
43	44.3	63.4	95.2
58	63.7	49.4	74.0

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/29/2024
 Supervised By :mohammad ahmed 08/13/2024

