

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072624\
 Data File : BN033030.D
 Acq On : 27 Jul 2024 12:18
 Operator : MA/JU
 Sample : P3300-24
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1GD4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/29/2024
 Supervised By :mohammad ahmed 08/13/2024

Quant Time: Jul 28 22:58:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 25 15:43:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.507	152	2550	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.262	136	9278	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.148	164	6143	0.400	ng/ul	-0.02
13) Phenanthrene-d10	16.916	188	13253m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.163	240	11468m	0.400	ng/ul	0.00
23) Perylene-d12	23.337	264	8869m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.060	96	15347	4.758	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.895	152	5108	0.337	ng/ul	-0.02
18) Fluoranthene-d10	18.963	212	13159	0.405	ng/ul	-0.02
Target Compounds						Qvalue
5) Naphthalene	10.311	128	1589	0.067	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072624\
Data File : BN033030.D
Acq On : 27 Jul 2024 12:18
Operator : MA/JU
Sample : P3300-24
Misc :
ALS Vial : 44 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E1GD4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/29/2024
Supervised By :mohammad ahmed 08/13/2024


Quant Time: Jul 28 22:58:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 15:43:00 2024
Response via : Initial Calibration

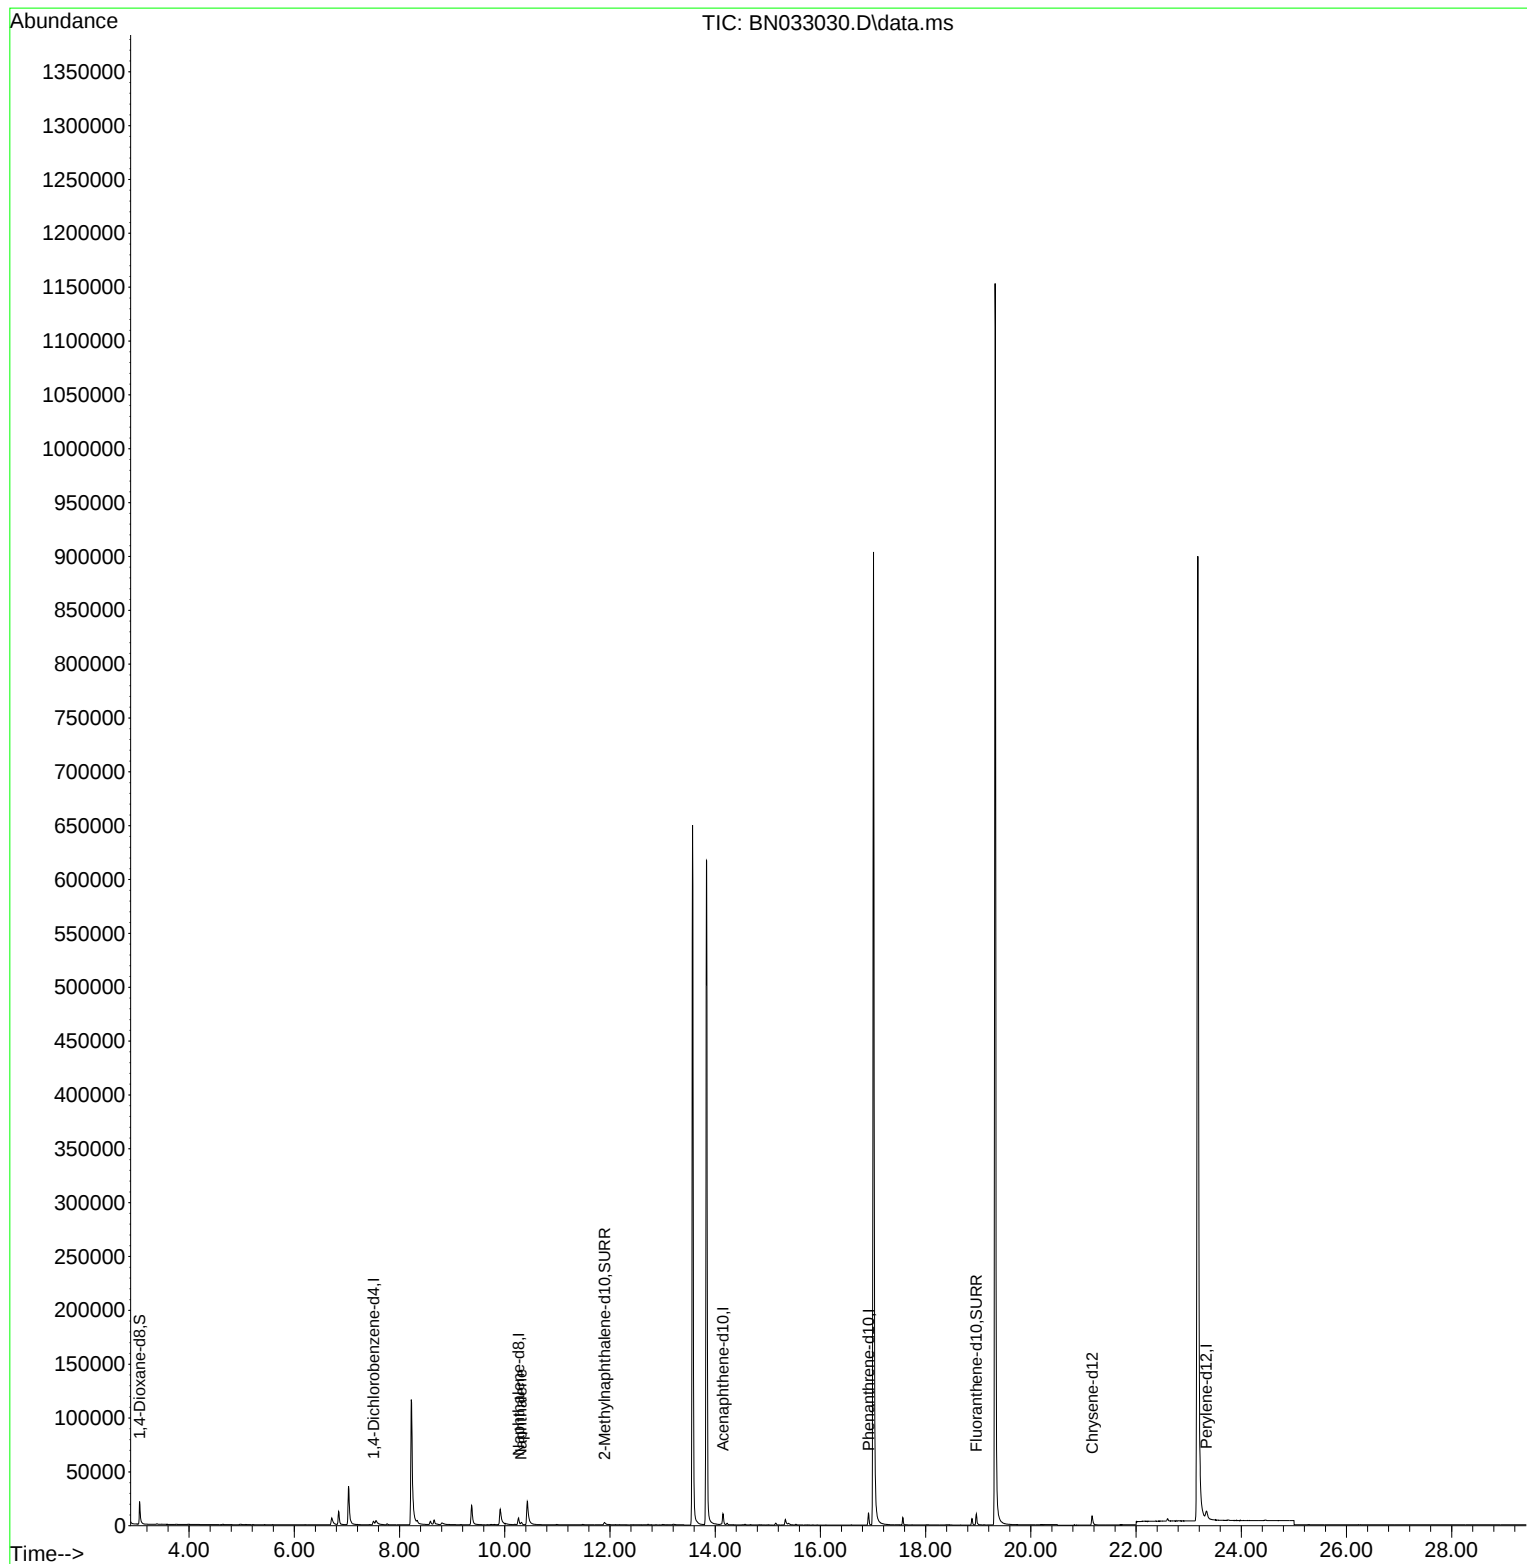

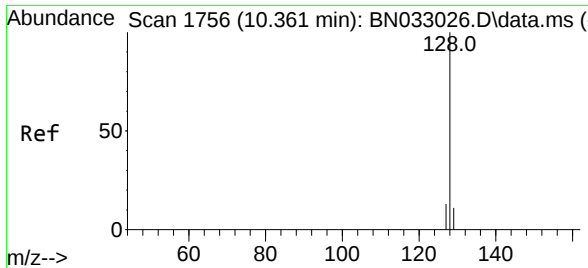

#5
Naphthalene
Concen: 0.067 ng/ul
RT: 10.311 min Scan# 1756
Delta R.T. -0.038 min
Lab File: BN033030.D
Acq: 27 Jul 2024 12:18

Instrument :
BNA_N
ClientSampleId :
E1GD4

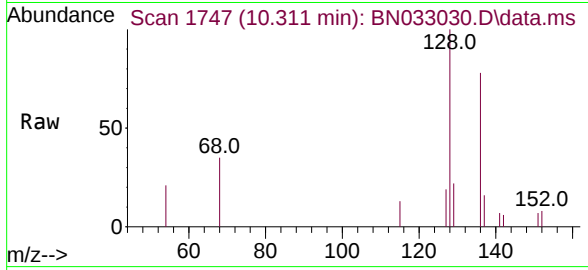

Tgt Ion:128 Resp: 1589

Ion	Ratio	Lower	Upper
128	100		
129	22.2	12.0	18.0
127	18.9	12.7	19.1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/29/2024
Supervised By :mohammad ahmed 08/13/2024

