
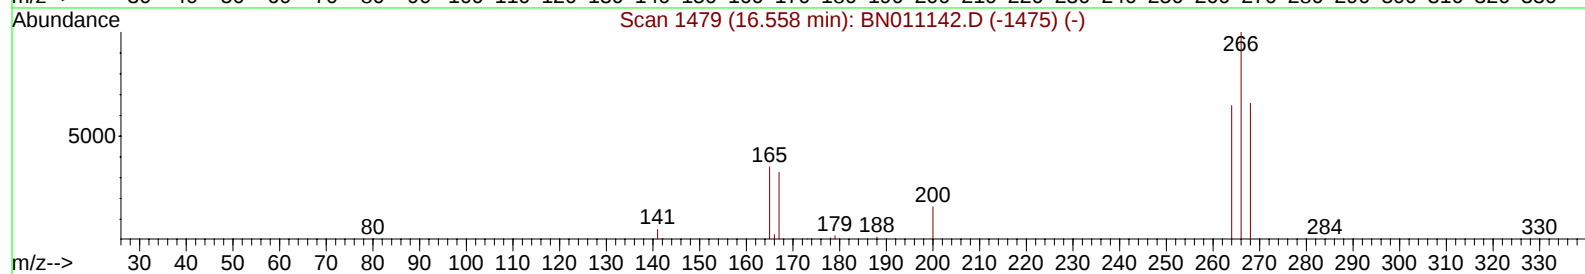
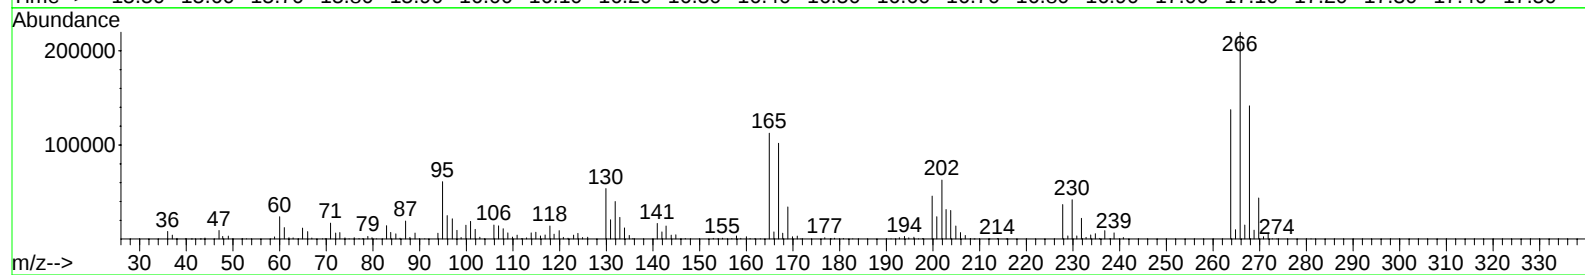


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN072720\
Data File : BN011265.D
Acq On : 27 Jul 2020 08:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 18:56:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN071120.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 27 10:06:24 2020
Response via : Initial Calibration

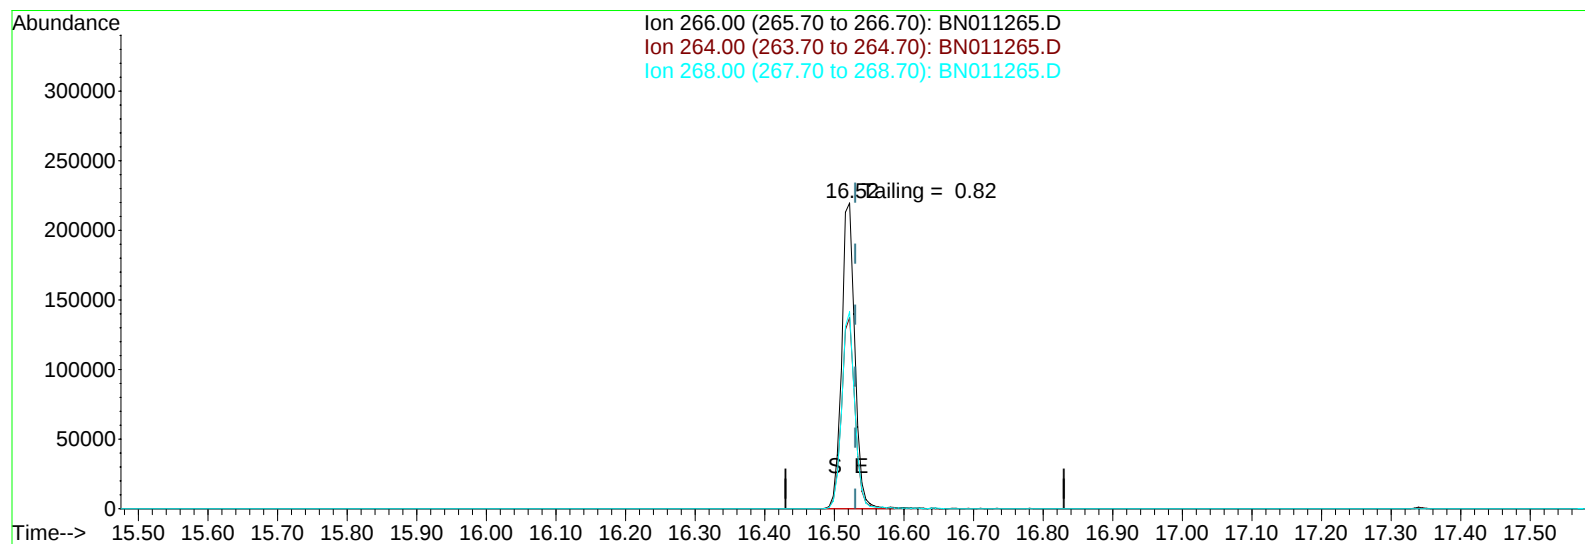

TIC: BN011265.D

(24) Pentachlorophenol

16.522min (-0.008) 2138.55ng

response 287599

Ion	Exp%	Act%
266.00	100	100
264.00	65.60	64.02
268.00	61.10	64.42
0.00	0.00	0.00