


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072720\
 Data File : BN011265.D
 Acq On : 27 Jul 2020 08:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN071120.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 27 10:06:24 2020

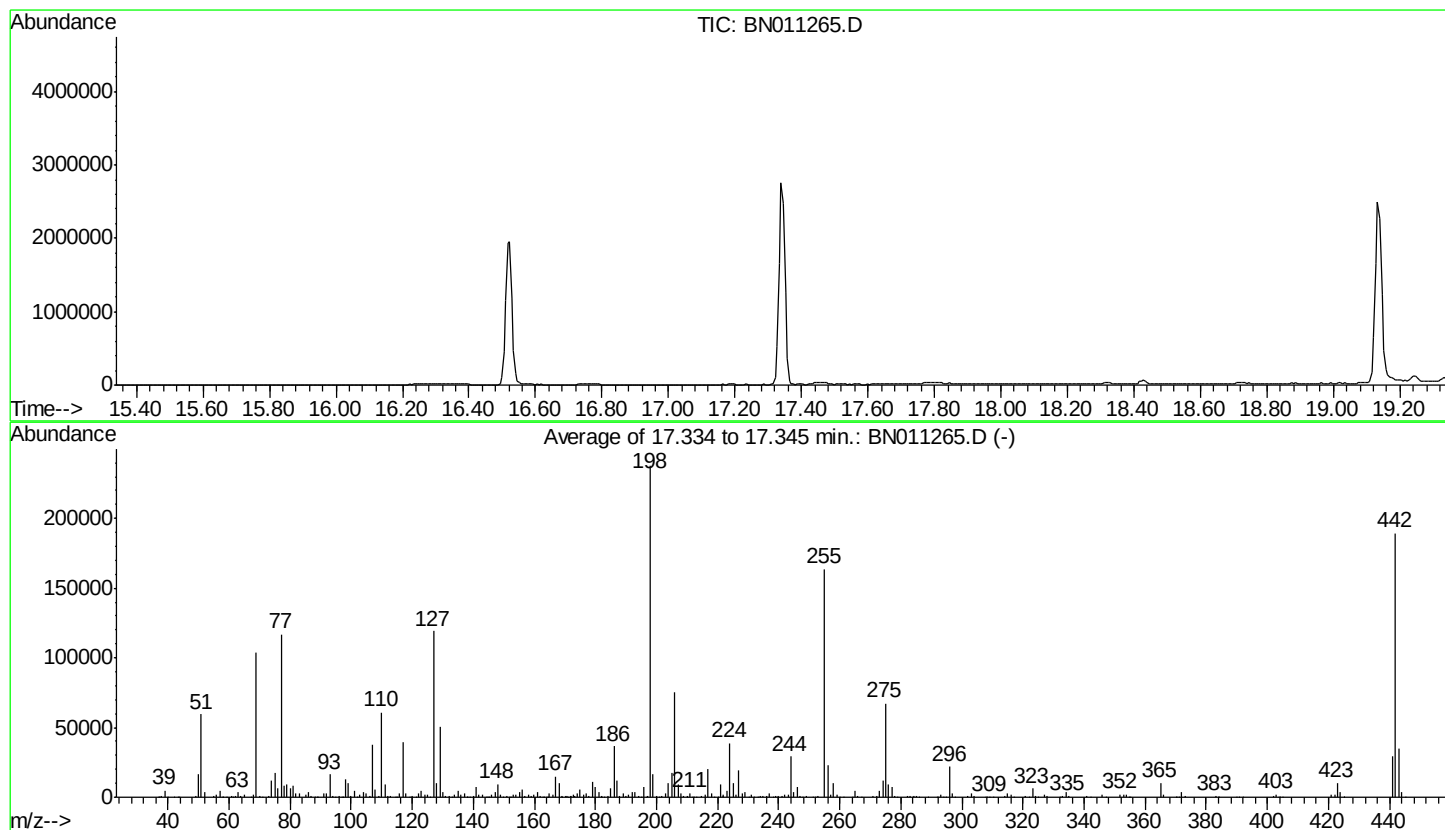

AutoFind: Scans 2439, 2440, 2441; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.0	59354	PASS
68	69	0.00	2	2.0	2067	PASS
69	198	0.00	100	43.6	103689	PASS
70	69	0.00	2	0.7	690	PASS
127	198	10	80	50.1	119298	PASS
197	198	0.00	2	0.5	1103	PASS
198	198	100	100	100.0	237888	PASS
199	198	5	9	6.9	16408	PASS
275	198	10	60	28.2	67170	PASS
365	198	1	100	4.4	10471	PASS
441	198	0.01	100	12.3	29169	PASS
442	198	50	100	79.7	189608	PASS
443	442	15	24	18.4	34940	PASS