
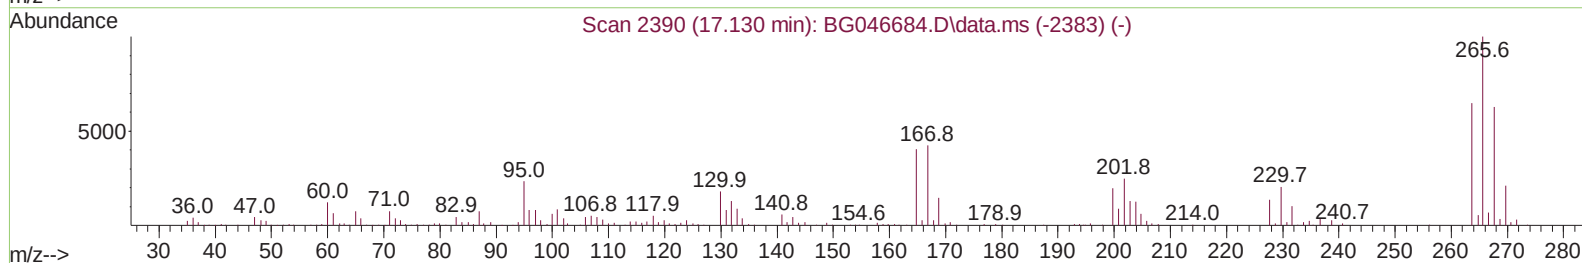
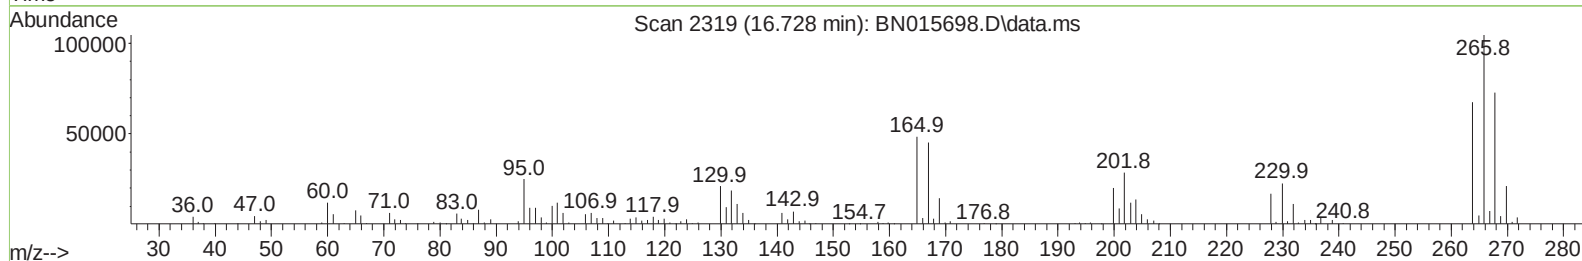


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072721\
Data File : BN015699.D
Acq On : 27 Jul 2021 11:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 13:12:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 06:59:38 2021
Response via : Initial Calibration

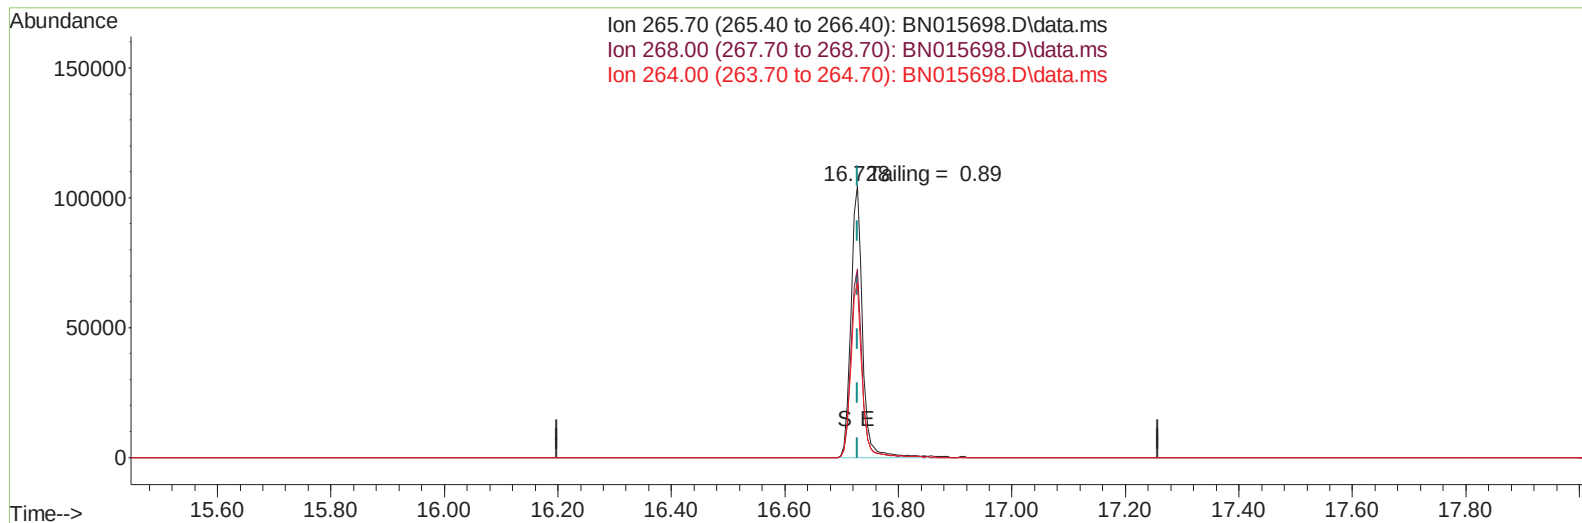

TIC: BN015698.D\data.ms

(70) Pentachlorophenol (C)




16.728min (-0.000) 24781.29 ng

response 149942

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.46
264.00	61.60	64.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072721\
Data File : BN015699.D
Acq On : 27 Jul 2021 11:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 13:12:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 06:59:38 2021
Response via : Initial Calibration

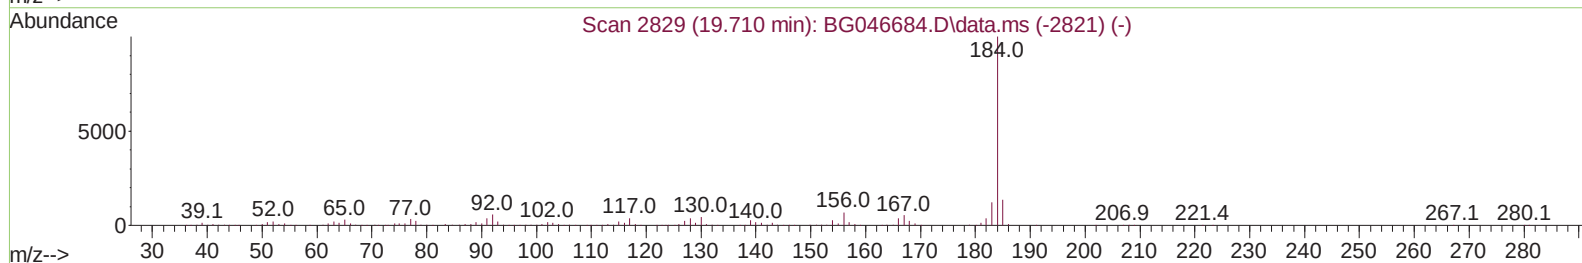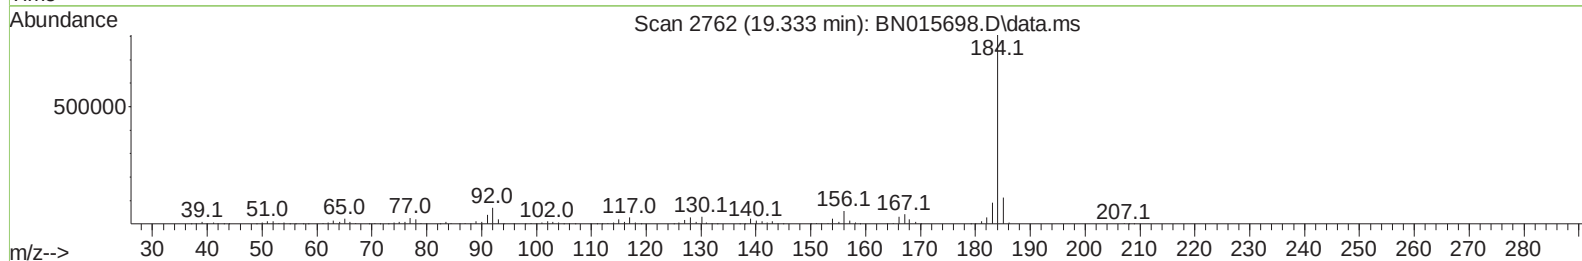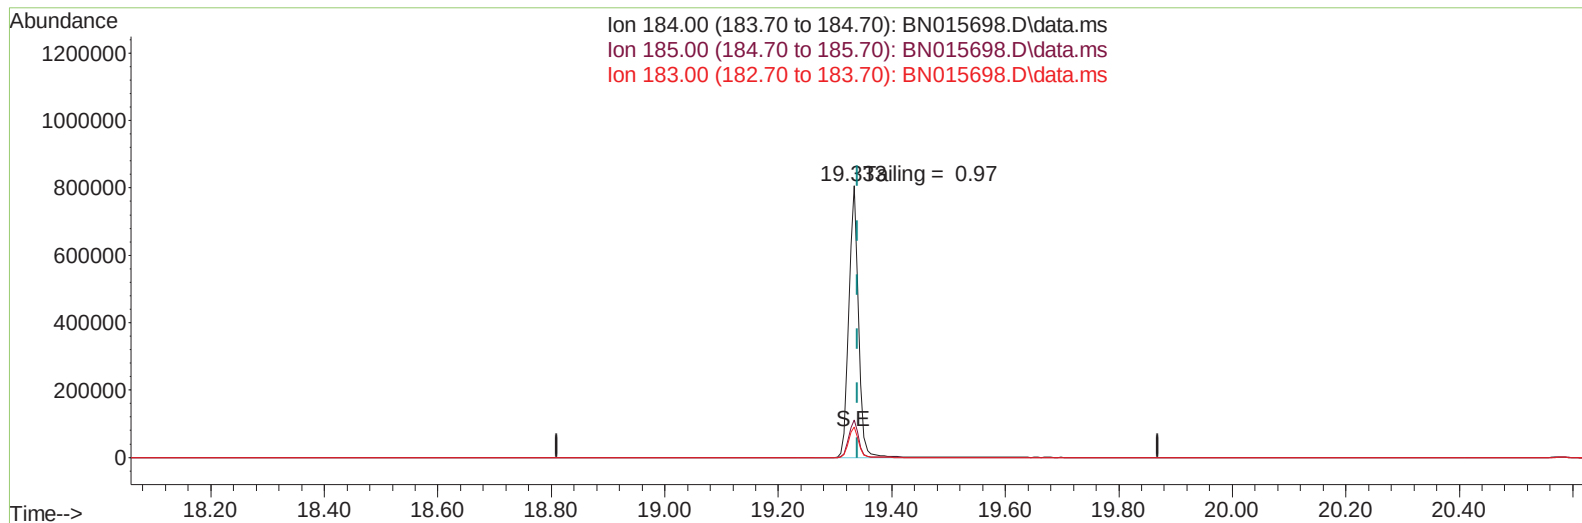

TIC: BN015698.D\data.ms

(77) Benzidine

19.333min (-0.006) 0.00 ng

response 954691

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.82
183.00	13.20	11.23
0.00	0.00	0.00