
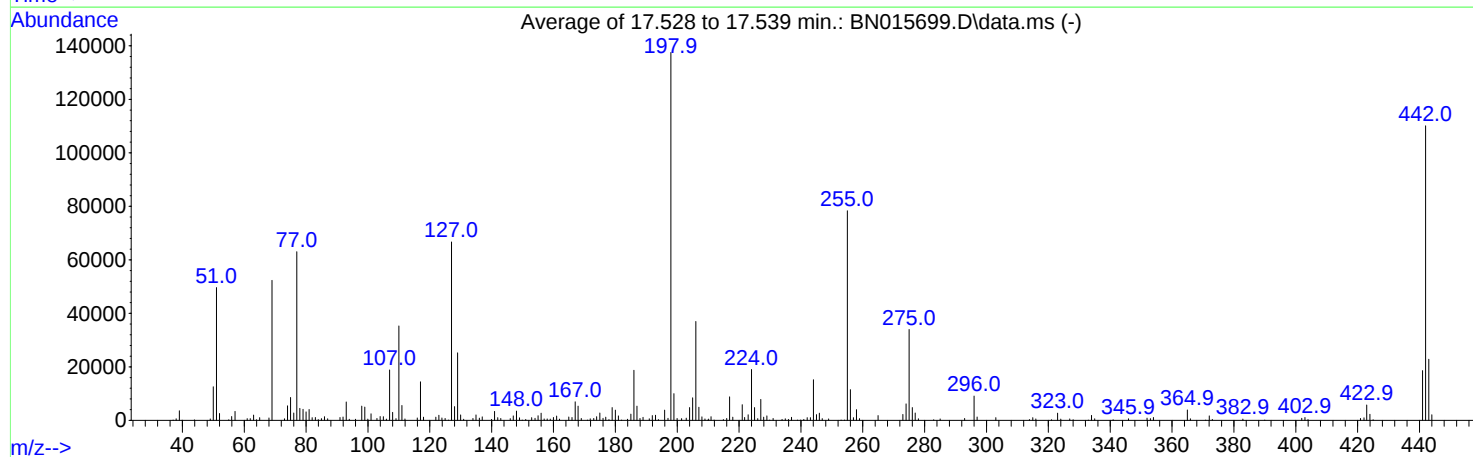


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072721\
 Data File : BN015699.D
 Acq On : 27 Jul 2021 11:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 27 13:51:38 2021

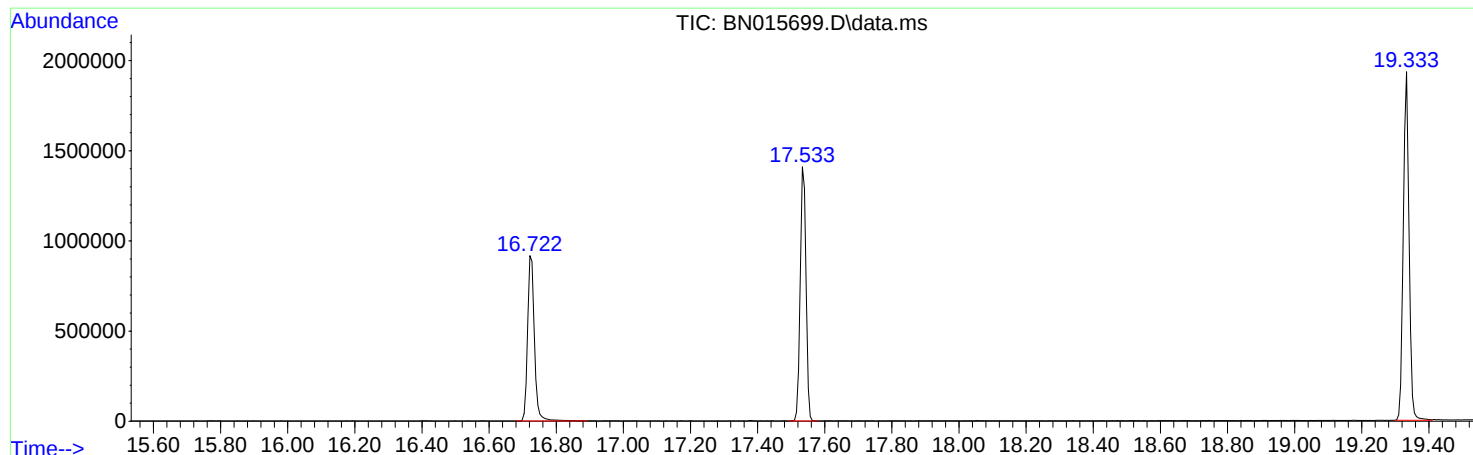




AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	49675	PASS
68	69	0.00	2	1.8	925	PASS
69	198	0.00	100	38.1	52360	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.5	66667	PASS
197	198	0.00	2	0.6	764	PASS
198	198	100	100	100.0	137515	PASS
199	198	5	9	7.3	10017	PASS
275	198	10	60	24.7	34000	PASS
365	198	1	100	2.8	3873	PASS
441	198	0.01	100	13.5	18615	PASS
442	442	50	100	100.0	110136	PASS
443	442	15	24	20.7	22853	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072721\
Data File : BN015699.D
Acq On : 27 Jul 2021 11:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 27 13:12:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 06:59:38 2021
Response via : Initial Calibration

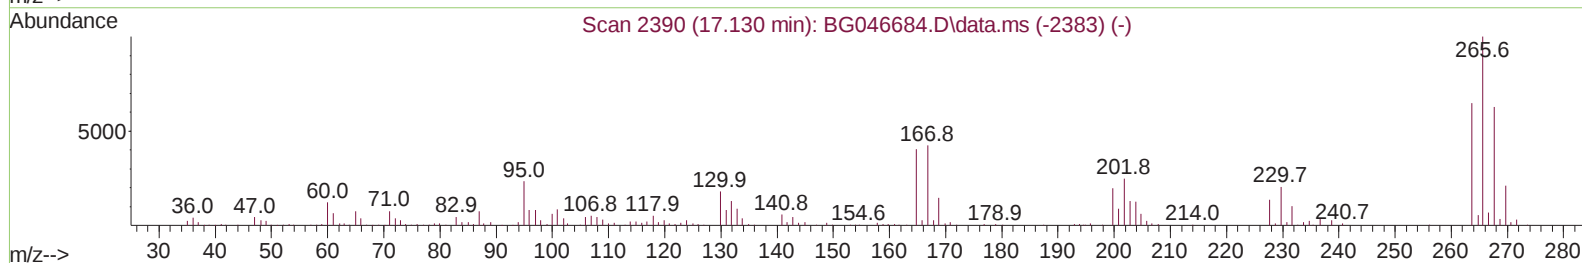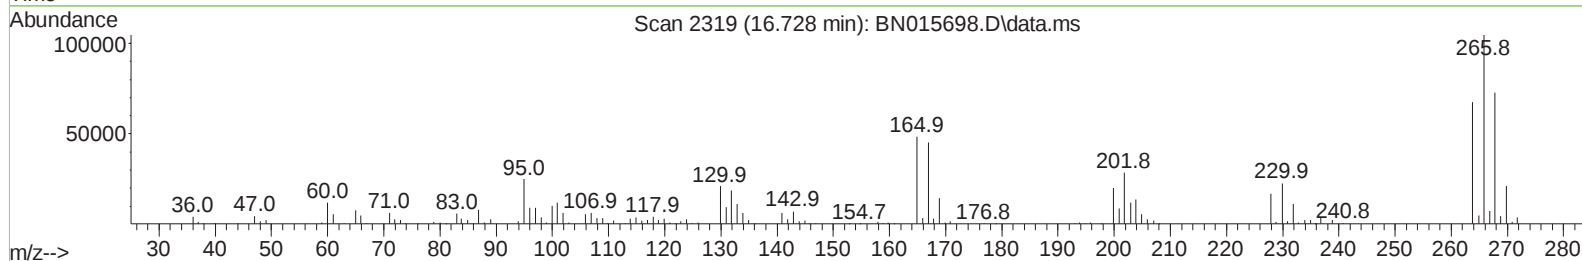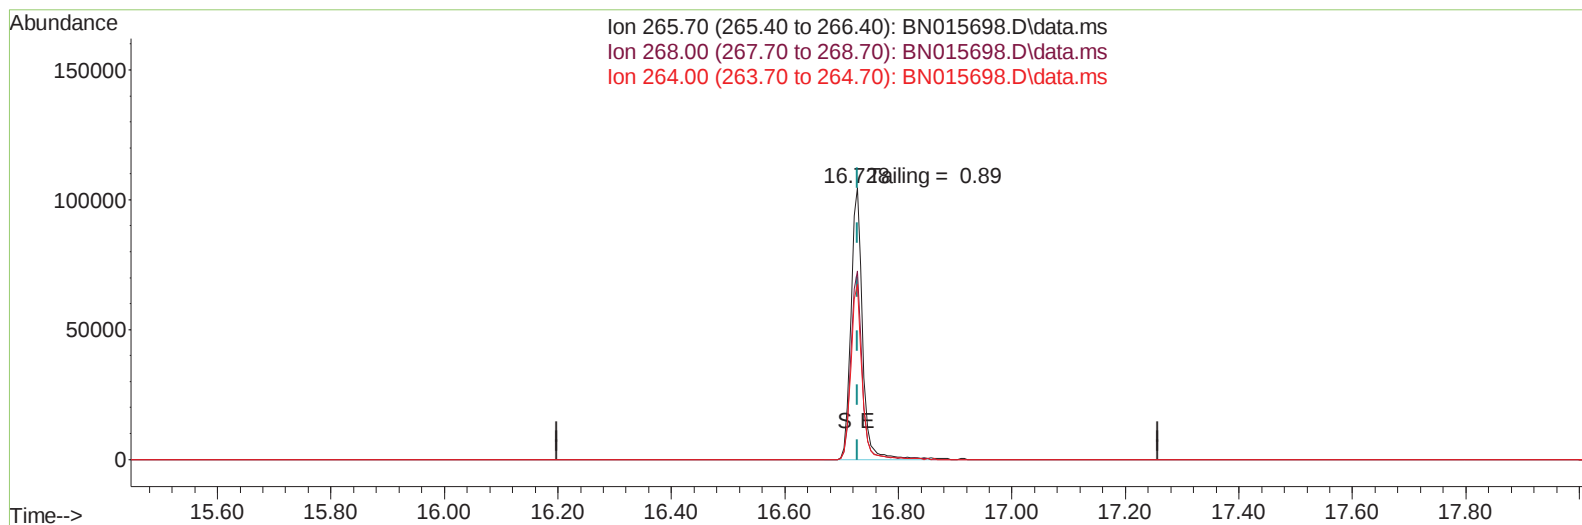

TIC: BN015698.D\data.ms

(70) Pentachloropheno1 (C)

16.728min (-0.000) 24781.29 ng

response 149942

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.46
264.00	61.60	64.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/27/2021	BNA_N	<u>BN015699.D</u>
Compound Name	Response	Retention Time
DDT	477470	20.58
DDD	4179	20.139
DDE	397	19.627
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4576	482046	0.95