

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072820\
 Data File : BN011284.D
 Acq On : 28 Jul 2020 17:31
 Operator : CG/JU
 Sample : L3403-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 W-1

Quant Time: Jul 28 18:02:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN072820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 28 14:38:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	1994	0.40	ng	0.00
7) Naphthalene-d8	10.22	136	7427	0.40	ng	0.00
13) Acenaphthene-d10	14.10	164	5330	0.40	ng	0.00
19) Phenanthrene-d10	16.86	188	10705	0.40	ng	0.00
29) Chrysene-d12	21.09	240	9422	0.40	ng	0.00
36) Perylene-d12	23.22	264	8827	0.40	ng	0.00

System Monitoring Compounds						
4) 2-Fluorophenol	5.15	112	325	0.06	ng	0.00
5) Phenol-d6	6.68	99	268	0.04	ng	0.00
8) Nitrobenzene-d5	8.63	82	1731	0.26	ng	0.00
11) 2-Methylnaphthalene-d10	11.82	152	2599	0.19	ng	0.00
14) 2,4,6-Tribromophenol	15.61	330	330	0.13	ng	0.00
15) 2-Fluorobiphenyl	12.72	172	8109	0.35	ng	0.00
27) Fluoranthene-d10	18.91	212	8902	0.27	ng	0.00
31) Terphenyl-d14	19.52	244	8616	0.30	ng	0.00


Target Compounds				Qvalue		
6) bis(2-Chloroethyl)ether	6.84	93	208	0.039	ng	# 31
16) Acenaphthylene	13.82	152	719	0.026	ng	# 81
20) 4,6-Dinitro-2-methylphenol	15.32	198	44	0.213	ng	# 1
23) Atrazine	16.34	200	422	0.076	ng	# 57
25) Phenanthrene	16.91	178	782	0.022	ng	# 85
26) Anthracene	16.99	178	959	0.033	ng	# 82
28) Fluoranthene	18.94	202	1749	0.044	ng	# 95
30) Pyrene	19.30	202	4156	0.098	ng	# 98
32) Benzo(a)anthracene	21.07	228	1383	0.044	ng	# 71
33) Chrysene	21.12	228	1684	0.048	ng	# 80
34) Bis(2-ethylhexyl)phthalate	21.04	149	7465	0.441	ng	100
35) Indeno(1,2,3-cd)pyrene	25.30	276	1569	0.045	ng	98
37) Benzo(b)fluoranthene	22.60	252	2710	0.077	ng	# 48
38) Benzo(k)fluoranthene	22.60	252	2710	0.070	ng	# 50
39) Benzo(a)pyrene	23.13	252	1706	0.056	ng	# 46
40) Dibenzo(a,h)anthracene	25.31	278	697	0.022	ng	# 1
41) Benzo(a,h,i)perylene	25.93	276	1966	0.056	ng	# 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072820\
Data File : BN011284.D
Acq On : 28 Jul 2020 17:31
Operator : CG/JU
Sample : L3403-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
W-1

Quant Time: Jul 28 18:02:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN072820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 28 14:38:05 2020
Response via : Initial Calibration

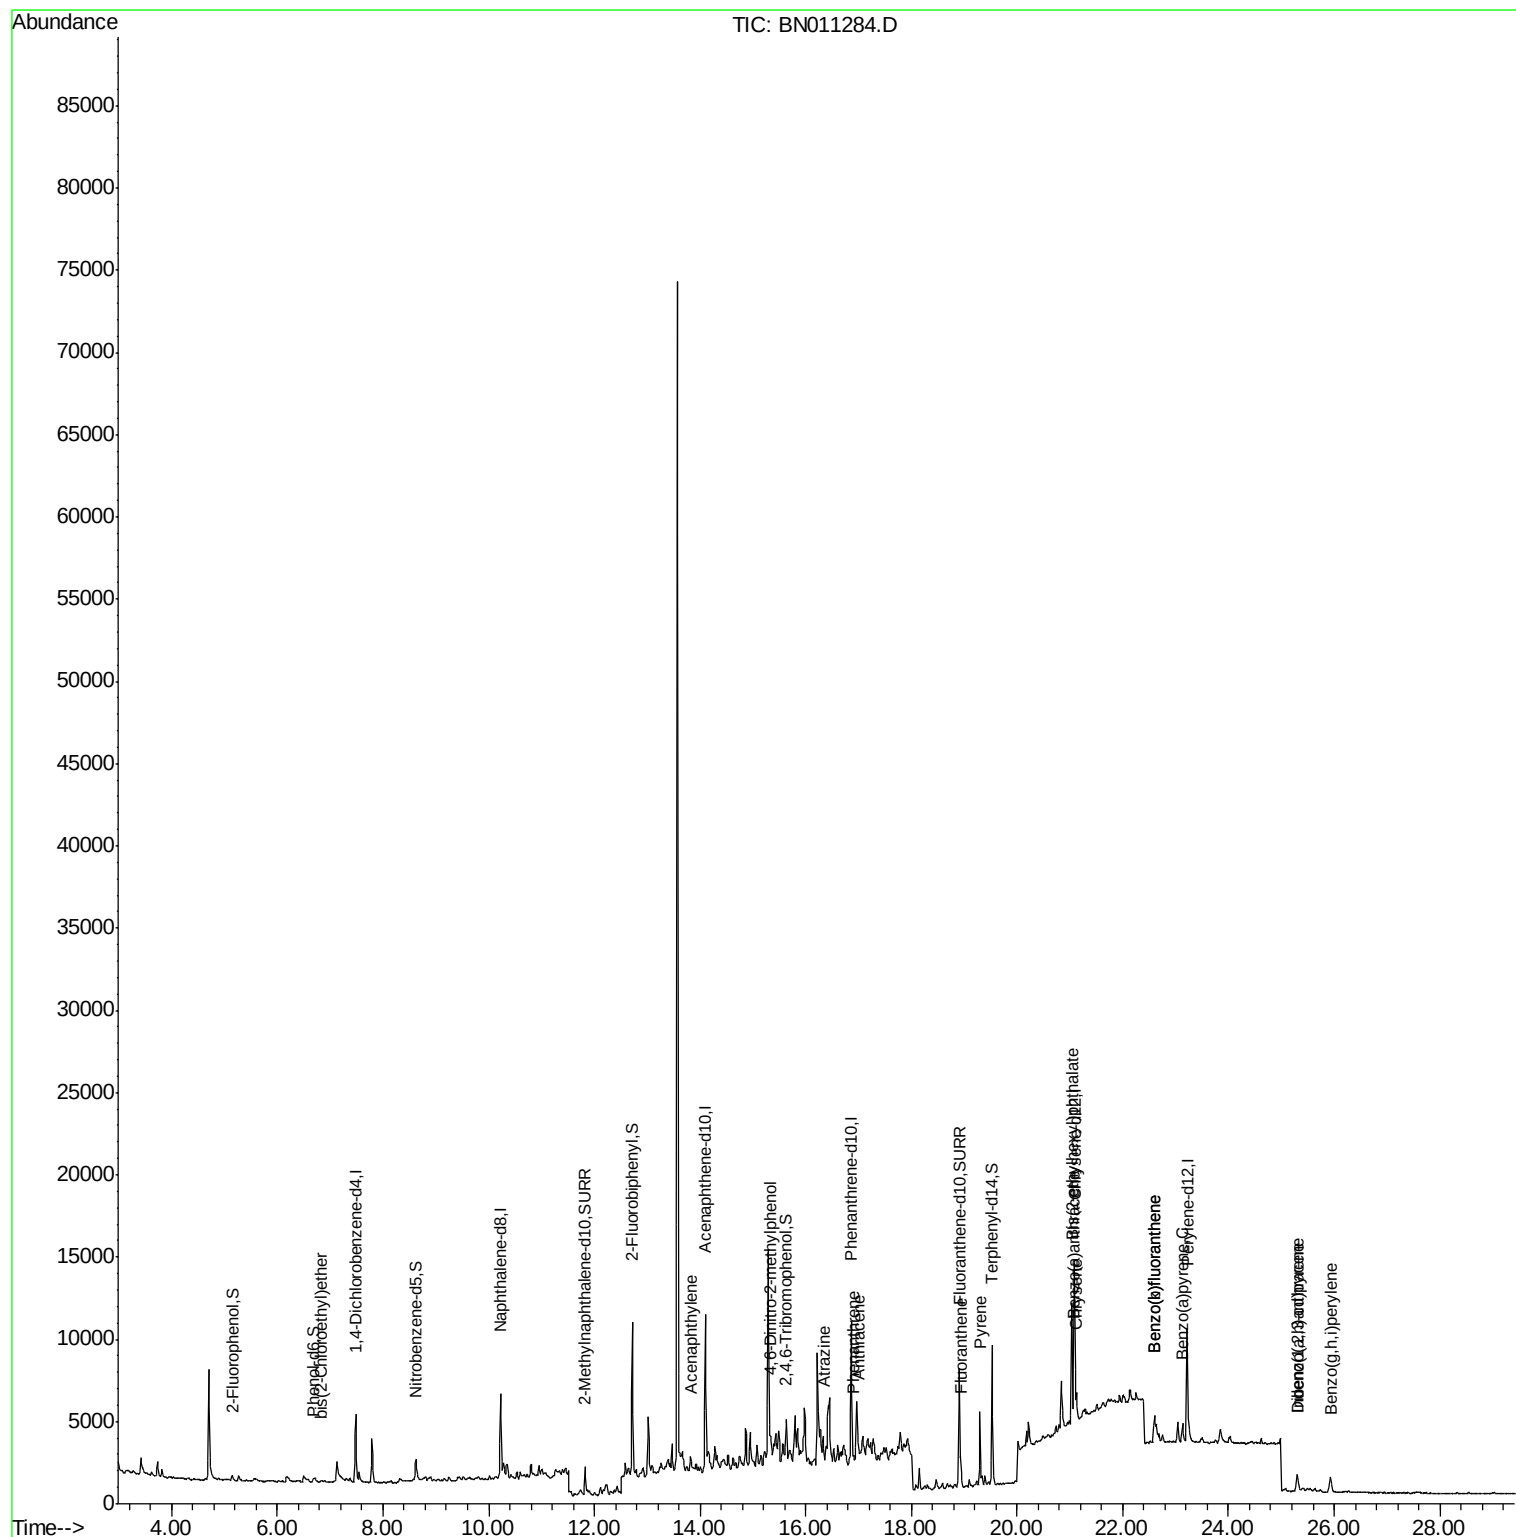

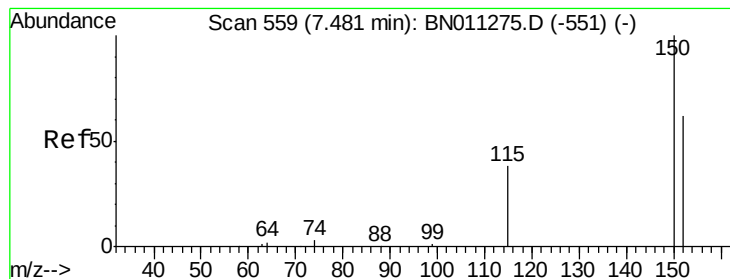


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.48 min Scan# 559
Delta R.T. 0.00 min
Lab File: BN011284.D
Acq: 28 Jul 2020 17:31

Instrument :
BNA_N
ClientSampled :
W-1

Tot Ion:152 Resp: 1994
Ion Ratio Lower Upper
152 100
150 155.4 126.5 189.7
115 62.2 51.9 77.9




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

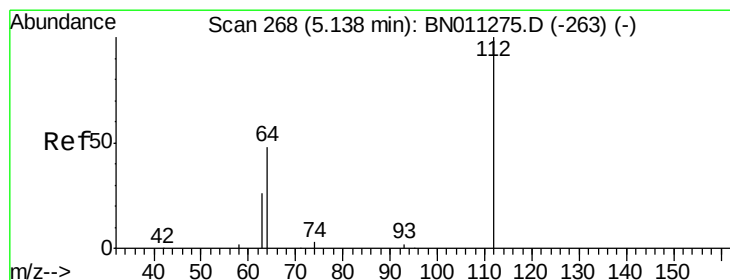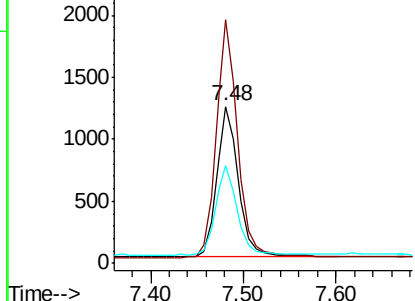



#4


2-Fluorophenol
Concen: 0.062 ng
RT: 5.15 min Scan# 269
Delta R.T. 0.01 min
Lab File: BN011284.D
Acq: 28 Jul 2020 17:31

Tgt Ion:112 Resp: 325
Ion Ratio Lower Upper
112 100
64 47.4 35.8 53.6
63 27.1 19.3 28.9



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

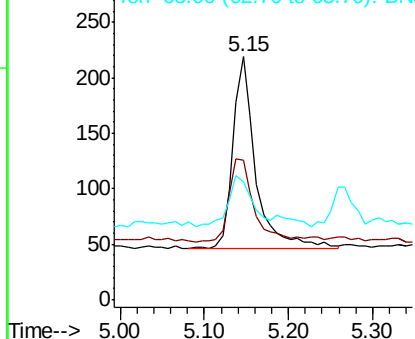

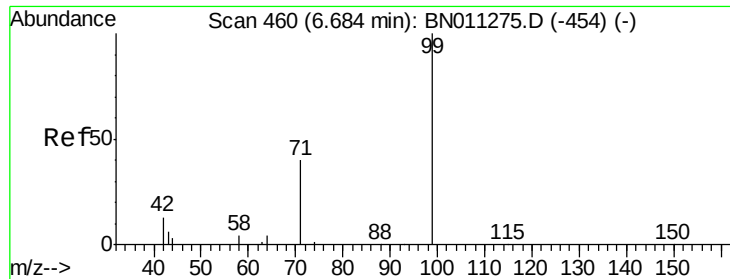

#5

Phenol-d6

Concen: 0.042 ng

RT: 6.68 min Scan# 460

Delta R.T. 0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31

Instrument :

BNA_N

ClientSampleId :

W-1


Tot Ion: 99 Resp: 268

Ion Ratio Lower Upper

99 100

42 6.7 11.2 16.8#

71 48.5 30.6 45.8#





Abundance Ion 99.00 (98.70 to 99.70): BN011284.D (-454) (-)

Ion 42.00 (41.70 to 42.70): BN011284.D (-454) (-)

Ion 71.00 (70.70 to 71.70): BN011284.D (-454) (-)

6.68

Time-->

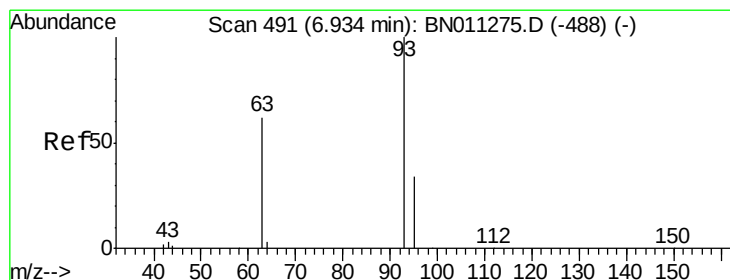

#6

bis(2-Chloroethyl)ether

Concen: 0.039 ng

RT: 6.84 min Scan# 479

Delta R.T. -0.10 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31


Tgt Ion: 93 Resp: 208

Ion Ratio Lower Upper

93 100

63 0.0 47.8 71.6#

95 4.3 27.1 40.7#




Abundance Ion 93.00 (92.70 to 93.70): BN011284.D (-488) (-)


Ion 63.00 (62.70 to 63.70): BN011284.D (-488) (-)

Ion 95.00 (94.70 to 95.70): BN011284.D (-488) (-)

6.84

Time-->

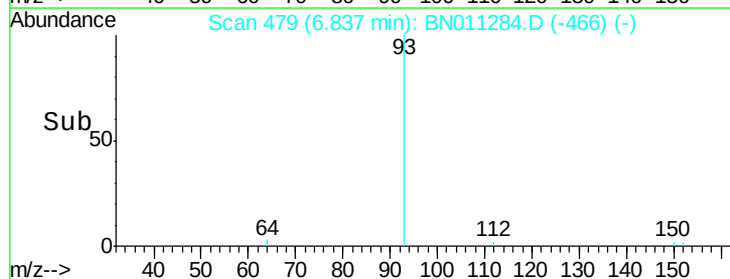



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.22 min Scan# 813

Delta R.T. -0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31

Instrument :

BNA_N

ClientSampleId :

W-1

Tot Ion:136 Resp: 7427


Ion Ratio Lower Upper

136 100

137 11.8 9.9 14.9

54 6.0 4.8 7.2

68 6.4 4.9 7.3



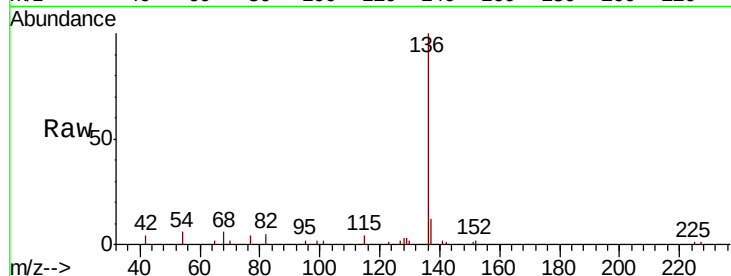


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

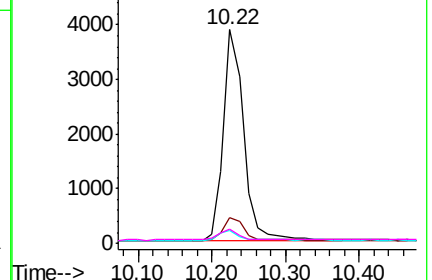

#8

Nitrobenzene-d5

Concen: 0.261 ng

RT: 8.63 min Scan# 687

Delta R.T. 0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31


Tgt Ion: 82 Resp: 1731

Ion Ratio Lower Upper

82 100

128 48.5 40.1 60.1



54 33.2 29.0 43.6




Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC

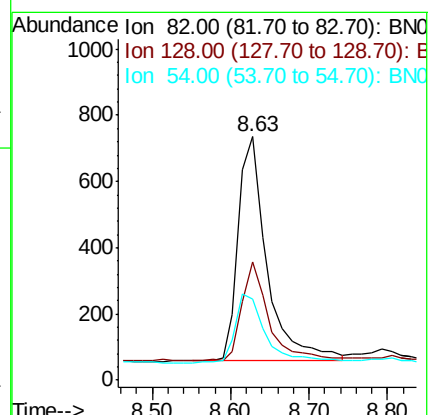

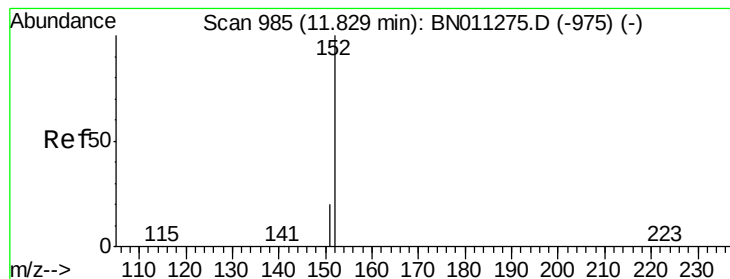

#11

2-Methylnaphthalene-d10

Concen: 0.192 ng

RT: 11.82 min Scan# 984

Delta R.T. -0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31

Instrument :

BNA_N

ClientSampleId :


W-1

Tot Ion:152 Resp: 2599

Ion Ratio Lower Upper

152 100

151 20.9 16.6 24.8



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

11.82

1500



1000

500

0

Time-->

11.80 11.90

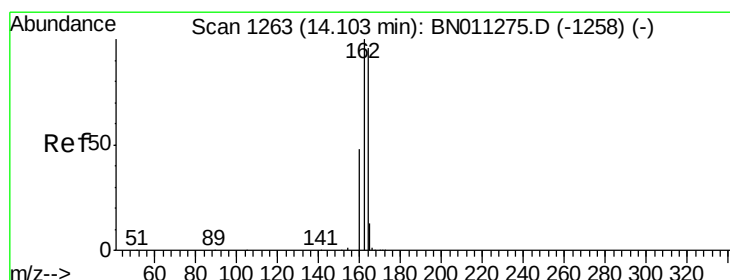

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.10 min Scan# 1263

Delta R.T. 0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31


Tgt Ion:164 Resp: 5330

Ion Ratio Lower Upper

164 100

162 104.5 83.6 125.4

160 54.0 41.2 61.8



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

14.10

5000

4000

3000


2000


1000

0

Time-->

14.00 14.10 14.20









#14
2,4,6-Tribromophenol
Concen: 0.134 ng
RT: 15.61 min Scan# 1382
Delta R.T. 0.00 min
Lab File: BN011284.D
Acq: 28 Jul 2020 17:31

Instrument :
BNA_N
ClientSampled :
W-1

Tot Ion:330 Resp: 330
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 103.0 34.2 51.2#

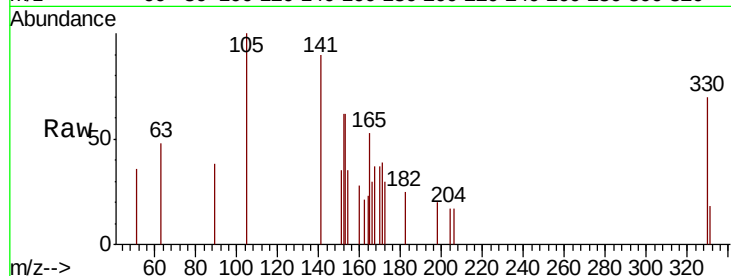


Abundance Ion 330.00 (329.70 to 330.70): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E


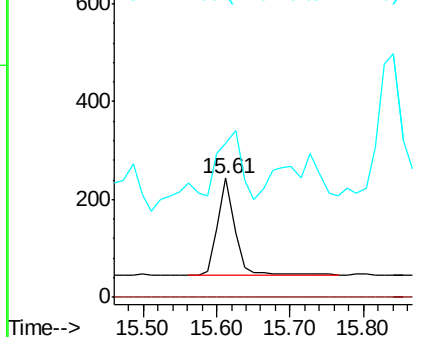



#15
2-Fluorobiphenyl
Concen: 0.352 ng
RT: 12.72 min Scan# 1154
Delta R.T. 0.00 min
Lab File: BN011284.D
Acq: 28 Jul 2020 17:31

Tgt Ion:172 Resp: 8109
Ion Ratio Lower Upper
172 100
171 35.0 30.6 46.0
170 23.4 21.0 31.4



Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

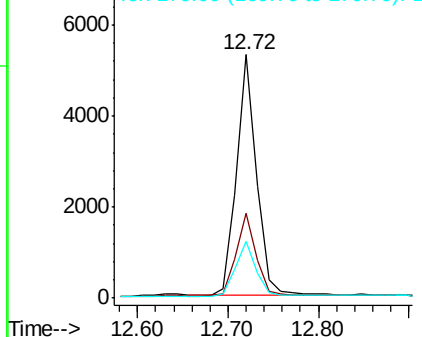



#16

Acenaphthylene

Concen: 0.026 ng

RT: 13.82 min Scan# 1241

Delta R.T. 0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31

Instrument :

BNA_N

ClientSampleId :

W-1


Tot Ion:152 Resp: 719

Ion Ratio Lower Upper

152 100

151 30.7 15.8 23.8#




153 17.0 10.2 15.4#

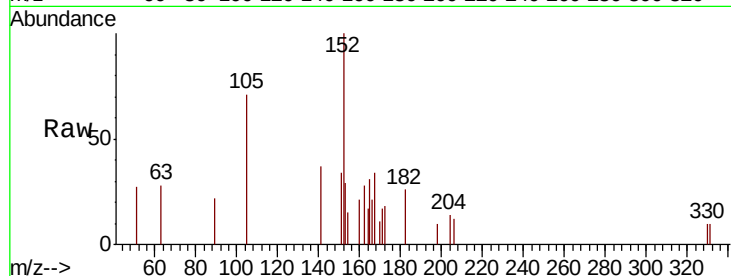

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

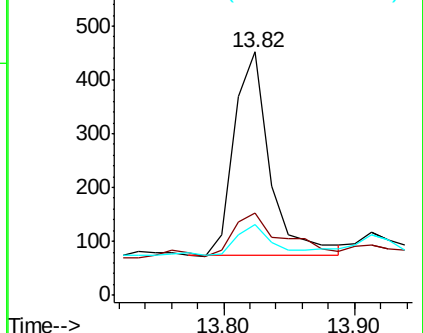

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.86 min Scan# 1483

Delta R.T. -0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31


Tgt Ion:188 Resp: 10705

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0



80 8.4 7.4 11.0




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

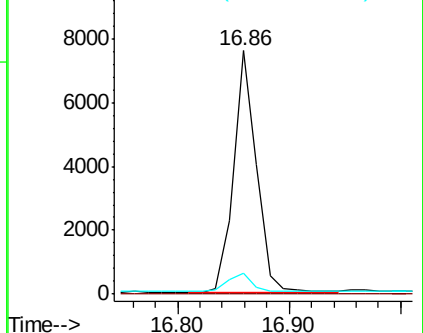

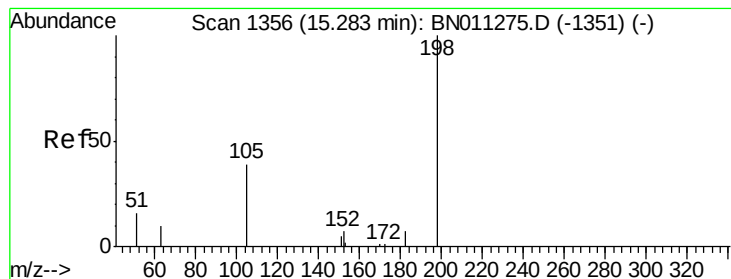

#20

4,6-Dinitro-2-methylphenol

Concen: 0.213 ng

RT: 15.32 min Scan# 1359

Delta R.T. 0.04 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31

Instrument :

BNA_N

ClientSampled :

W-1


Tot Ion:198 Resp: 44

Ion Ratio Lower Upper

198 100

51 195.7 49.0 73.6#




105 302.9 53.8 80.6#



Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BNO

Ion 105.00 (104.70 to 105.70): E

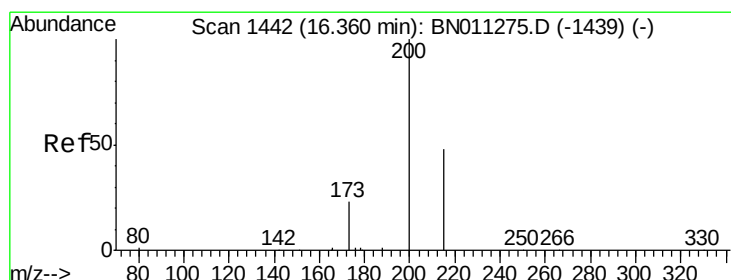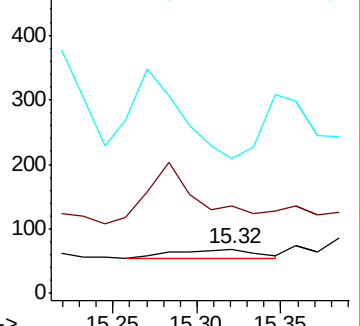

#23

Atrazine

Concen: 0.076 ng

RT: 16.34 min Scan# 1440

Delta R.T. -0.02 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31


Tgt Ion:200 Resp: 422

Ion Ratio Lower Upper

200 100

173 76.1 22.0 33.0#



215 40.4 41.1 61.7#




Abundance Ion 200.00 (199.70 to 200.70): E

Ion 173.00 (172.70 to 173.70): E

Ion 215.00 (214.70 to 215.70): E

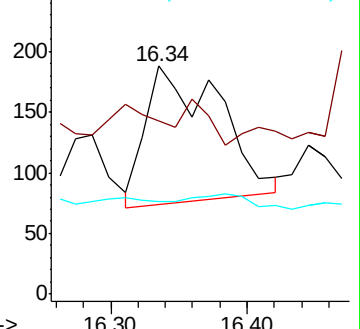



#25

Phenanthrene

Concen: 0.022 ng

RT: 16.91 min Scan# 1487

Delta R.T. 0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31

Instrument :

BNA_N

ClientSampleId :

W-1


Tot Ion:178 Resp: 782

Ion Ratio Lower Upper

178 100

176 8.8 14.9 22.3#




179 12.1 12.2 18.4#

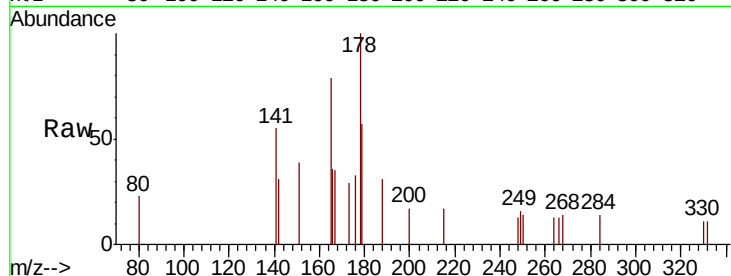

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

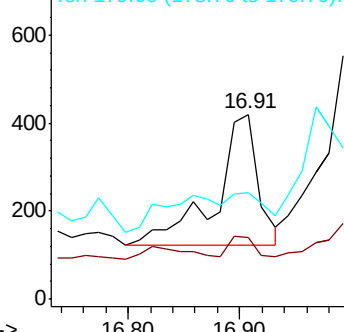

#26

Anthracene

Concen: 0.033 ng

RT: 16.99 min Scan# 1494

Delta R.T. 0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31


Tgt Ion:178 Resp: 959

Ion Ratio Lower Upper

178 100

176 19.9 15.0 22.6



179 0.0 12.1 18.1#




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E




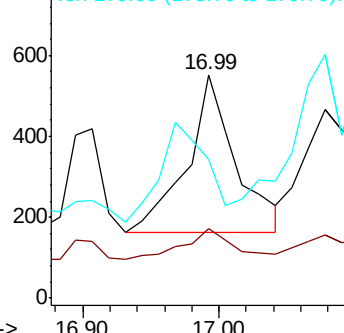


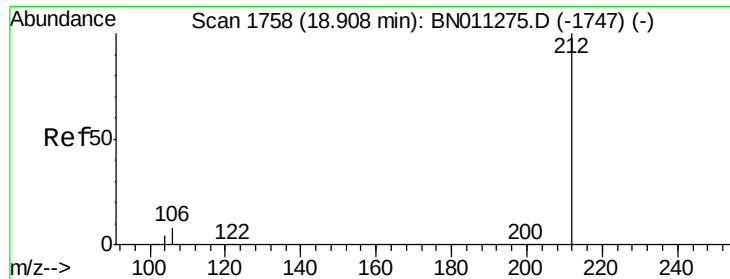

#27
 Fluoranthene-d10
 Concen: 0.272 ng
 RT: 18.91 min Scan# 1758
 Delta R.T. 0.00 min
 Lab File: BN011284.D
 Acq: 28 Jul 2020 17:31




Instrument :
 BNA_N
 ClientSampleId :
 W-1


Tot Ion:212 Resp: 8902
 Ion Ratio Lower Upper
 212 100
 106 9.2 6.9 10.3
 104 6.1 4.2 6.2

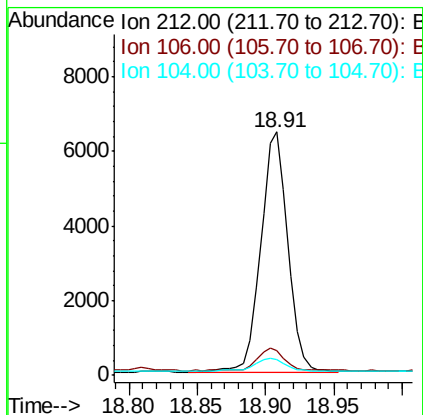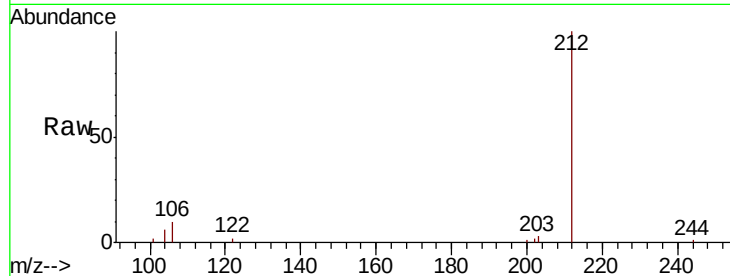

#28
 Fluoranthene
 Concen: 0.044 ng
 RT: 18.94 min Scan# 1764
 Delta R.T. 0.00 min
 Lab File: BN011284.D
 Acq: 28 Jul 2020 17:31

Tgt Ion:202 Resp: 1749
 Ion Ratio Lower Upper
 202 100
 101 9.7 5.9 8.9#
 203 18.9 13.7 20.5

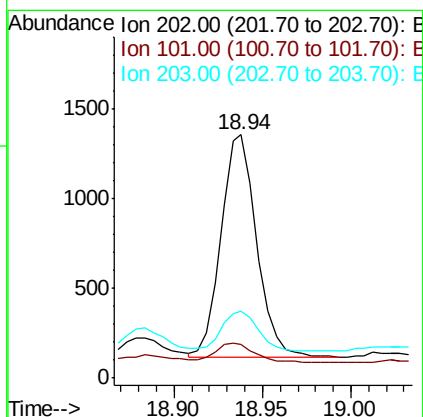



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.09 min Scan# 2081

Delta R.T. -0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31

Instrument :

BNA_N

ClientSampleId :

W-1


Tot Ion:240 Resp: 9422

Ion Ratio Lower Upper

240 100

120 7.6 5.8 8.8




236 27.6 22.7 34.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

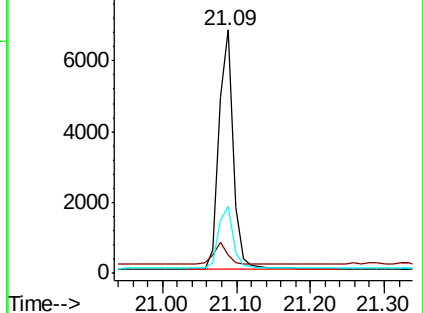

#30

Pyrene

Concen: 0.098 ng

RT: 19.30 min Scan# 1837

Delta R.T. -0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31


Tgt Ion:202 Resp: 4156

Ion Ratio Lower Upper

202 100

200 21.4 16.3 24.5



203 17.1 14.1 21.1




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

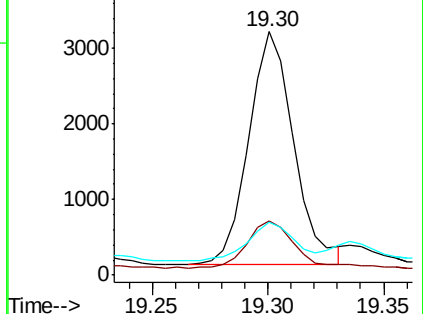



#31

Terphenyl-d14

Concen: 0.302 ng

RT: 19.52 min Scan# 1882

Delta R.T. -0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31

Instrument :

BNA_N

ClientSampleId :

W-1


Tot Ion:244 Resp: 8616

Ion Ratio Lower Upper

244 100

212 9.4 7.6 11.4




122 11.5 7.5 11.3#

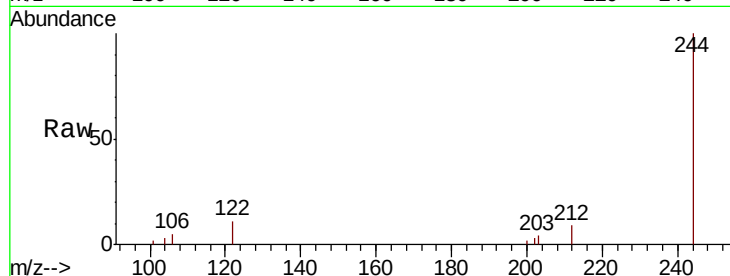

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

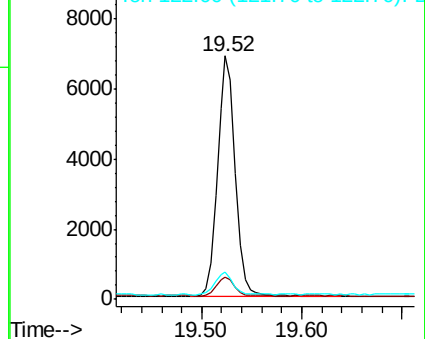

#32

Benzo(a)anthracene

Concen: 0.044 ng

RT: 21.07 min Scan# 2079

Delta R.T. 0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31


Tgt Ion:228 Resp: 1383

Ion Ratio Lower Upper

228 100

226 39.8 21.6 32.4#



229 35.7 16.0 24.0#




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

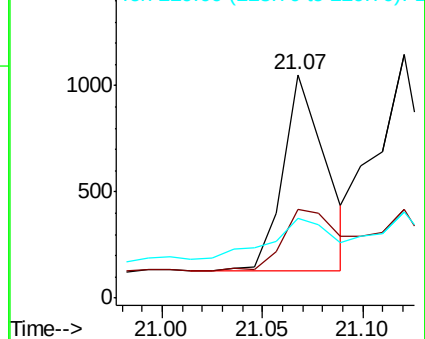



#33

Chrysene

Concen: 0.048 ng

RT: 21.12 min Scan# 2084

Delta R.T. 0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31

Instrument :

BNA_N

ClientSampled :

W-1


Tot Ion:228 Resp: 1684

Ion Ratio Lower Upper

228 100

226 36.6 24.3 36.5#




229 35.6 15.9 23.9#



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

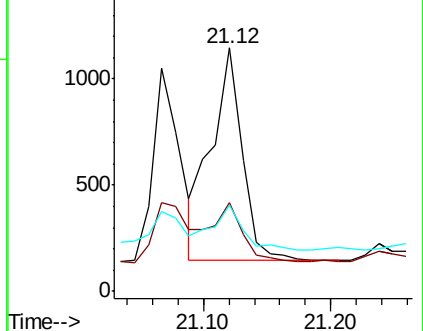

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.441 ng

RT: 21.04 min Scan# 2076

Delta R.T. 0.01 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31


Tgt Ion:149 Resp: 7465

Ion Ratio Lower Upper

149 100

167 27.2 21.7 32.5



279 4.3 3.9 5.9




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E




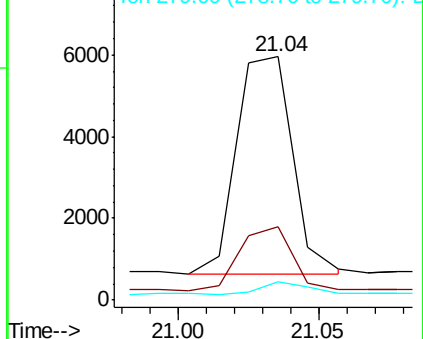




#35
 Indeno(1,2,3-cd)pyrene
 Concen: 0.045 ng
 RT: 25.30 min Scan# 3050
 Delta R.T. -0.00 min
 Lab File: BN011284.D
 Acq: 28 Jul 2020 17:31




Instrument :
 BNA_N
 ClientSampleId :
 W-1


Tot Ion:276 Resp: 1569
 Ion Ratio Lower Upper
 276 100
 138 17.5 13.6 20.4
 277 25.6 19.7 29.5

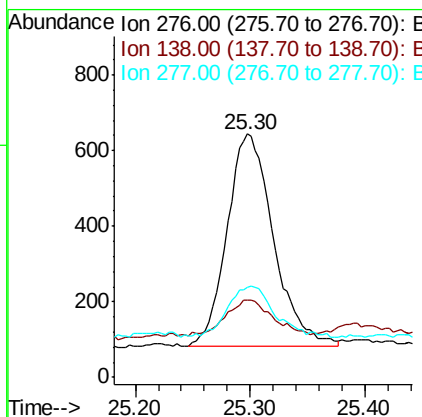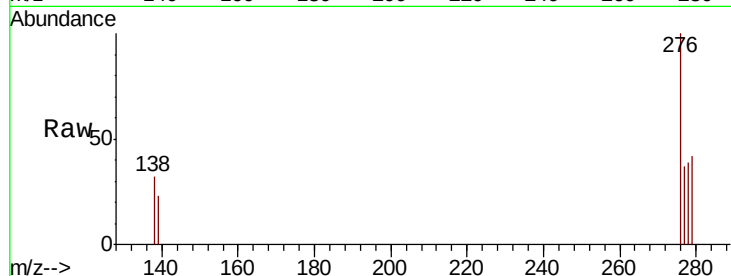

#36
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.22 min Scan# 2442
 Delta R.T. -0.00 min
 Lab File: BN011284.D
 Acq: 28 Jul 2020 17:31

Tgt Ion:264 Resp: 8827
 Ion Ratio Lower Upper
 264 100
 260 25.8 20.1 30.1
 265 64.6 70.7 106.1#



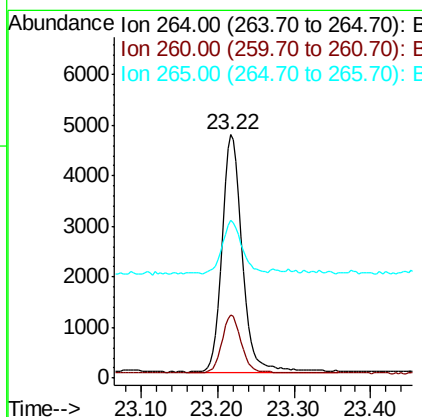



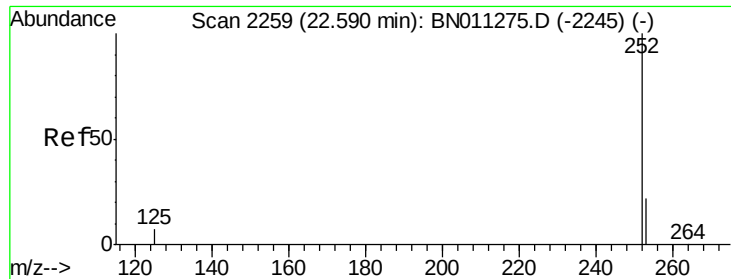

#37
Benzo(b)fluoranthene
Concen: 0.077 ng
RT: 22.60 min Scan# 2261
Delta R.T. 0.01 min
Lab File: BN011284.D
Acq: 28 Jul 2020 17:31




Instrument :
BNA_N
ClientSampleId :
W-1


Tot Ion:252 Resp: 2710
Ion Ratio Lower Upper
252 100
253 54.4 23.1 34.7#
125 35.9 9.4 14.2#

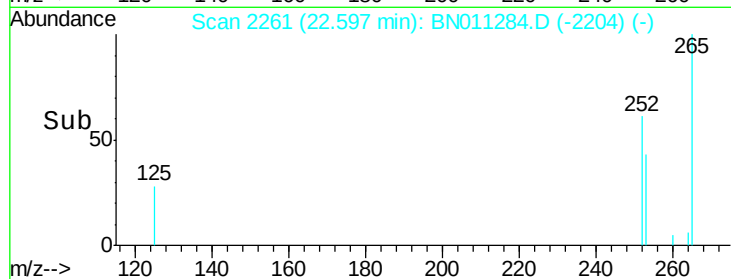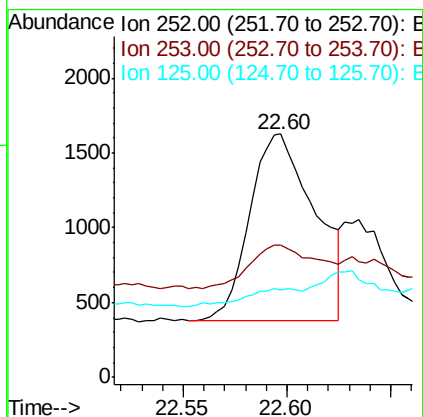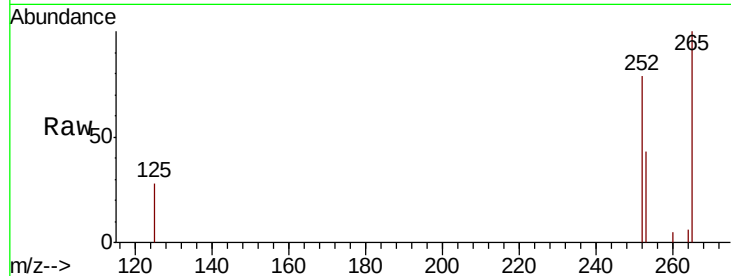

#38
Benzo(k)fluoranthene
Concen: 0.070 ng
RT: 22.60 min Scan# 2261
Delta R.T. -0.03 min
Lab File: BN011284.D
Acq: 28 Jul 2020 17:31

Tgt Ion:252 Resp: 2710
Ion Ratio Lower Upper
252 100
253 54.4 22.9 34.3#
125 35.9 11.3 16.9#

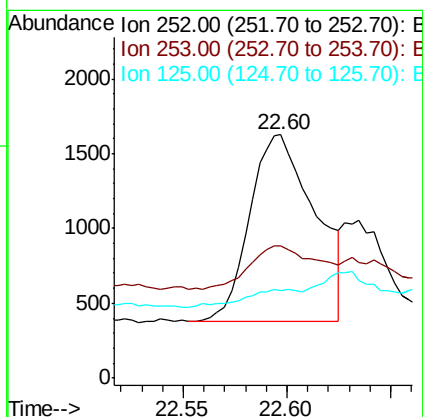

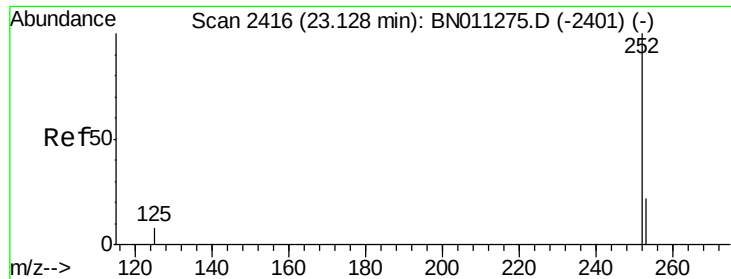

#39

Benzo(a)pyrene

Concen: 0.056 ng

RT: 23.13 min Scan# 2416

Delta R.T. 0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31

Instrument :

BNA_N

ClientSampleId :

W-1


Tot Ion:252 Resp: 1706

Ion Ratio Lower Upper

252 100

253 61.5 26.6 39.8#




125 43.0 12.7 19.1#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

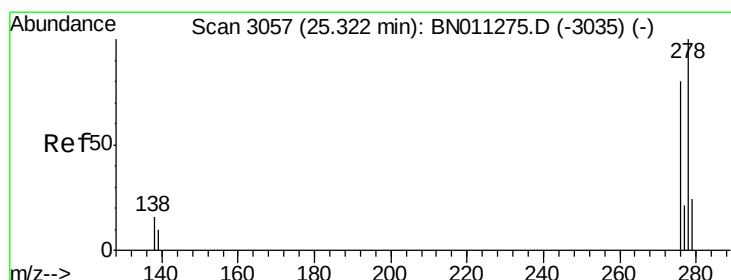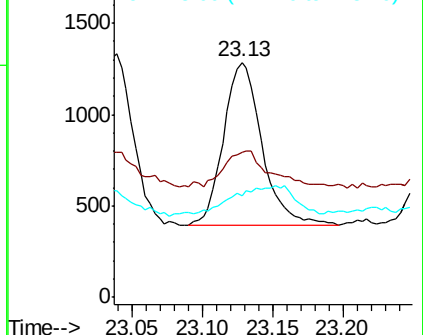

#40

Dibenzo(a,h)anthracene

Concen: 0.022 ng

RT: 25.31 min Scan# 3055

Delta R.T. -0.01 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31


Tgt Ion:278 Resp: 697

Ion Ratio Lower Upper

278 100

139 50.5 12.4 18.6#



279 92.4 25.8 38.6#

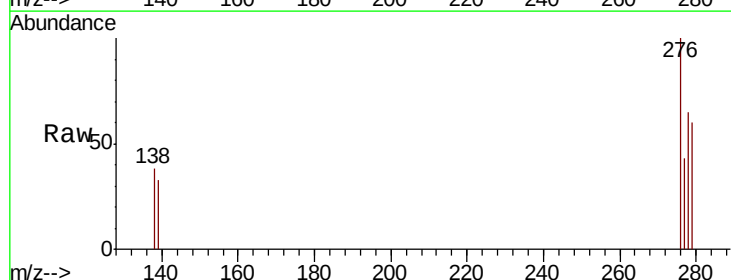


Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

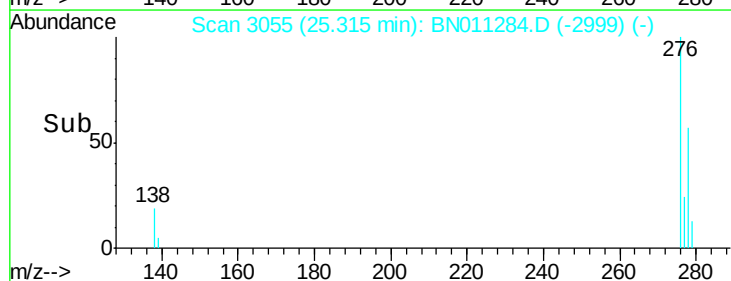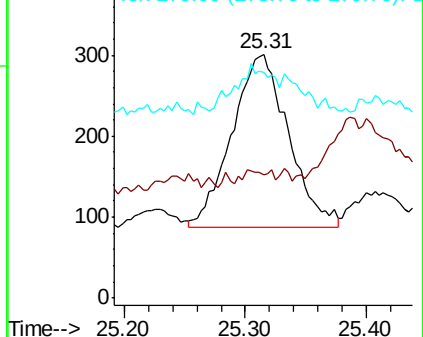

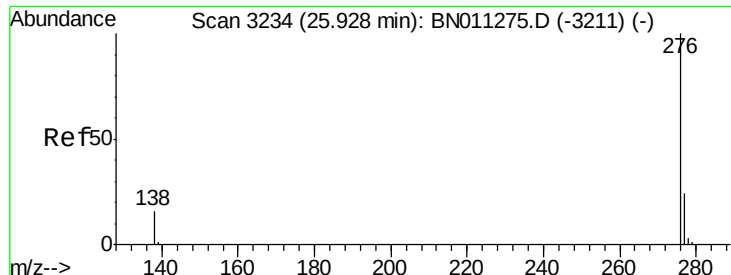

#41

Benzo(a,h,i)perylene

Concen: 0.056 ng

RT: 25.93 min Scan# 3234

Delta R.T. -0.00 min

Lab File: BN011284.D

Acq: 28 Jul 2020 17:31

Instrument :

BNA_N

ClientSampleId :

W-1

Tot Ion:276 Resp: 1966

Ion Ratio Lower Upper

276 100

277 33.8 21.0 31.6#

138 30.5 15.0 22.6#

