
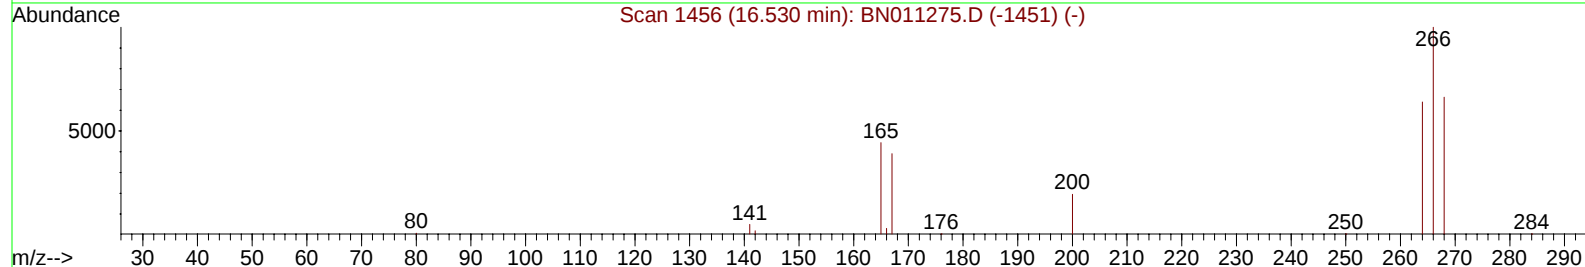
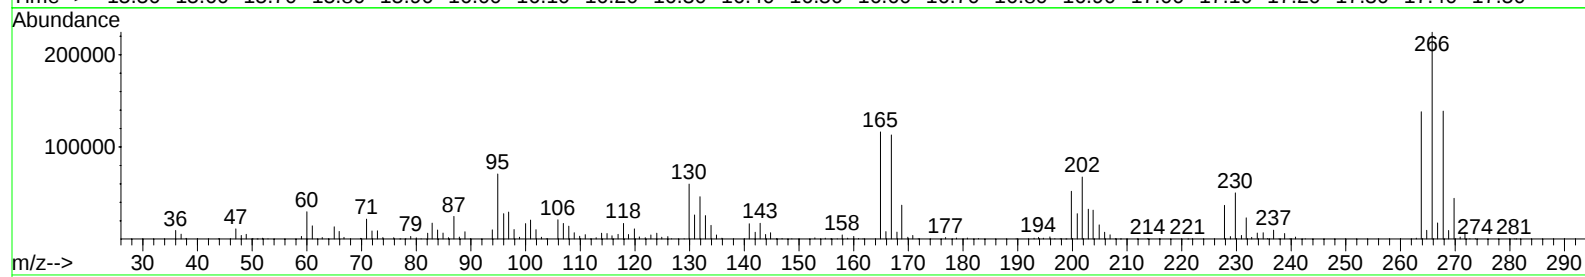


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072820\
Data File : BN011271.D
Acq On : 28 Jul 2020 09:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 28 18:16:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN072820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 28 14:38:05 2020
Response via : Initial Calibration

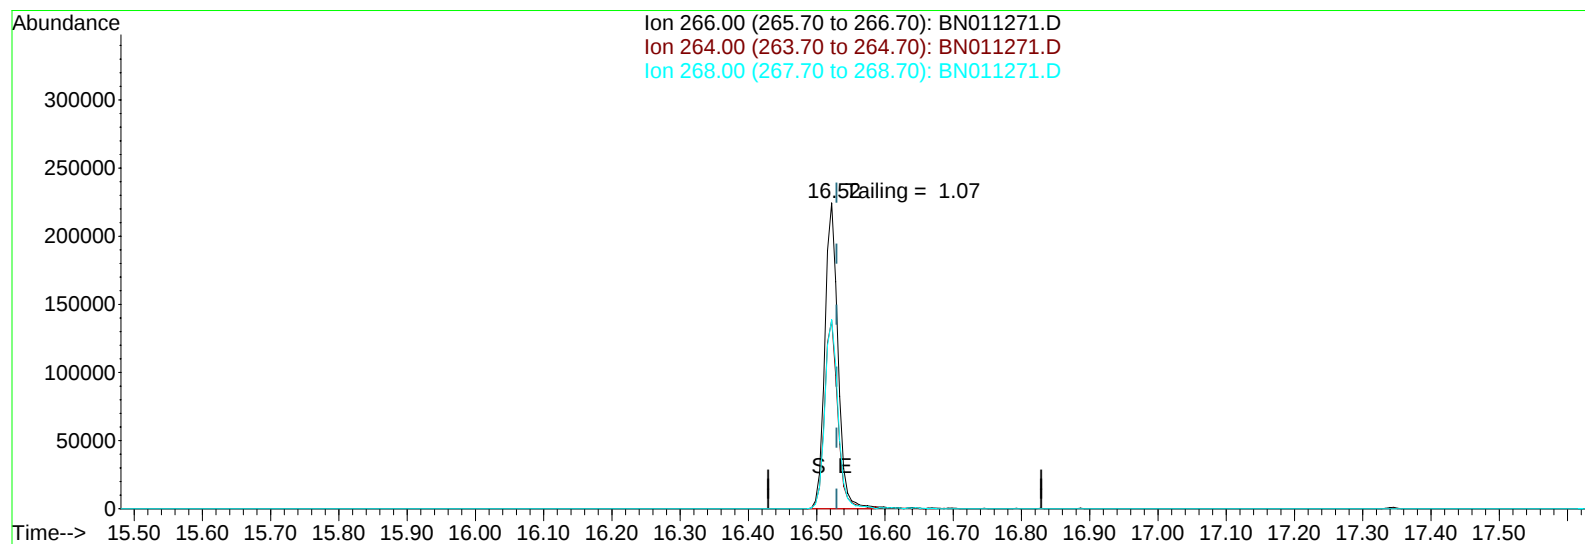

(24) Pentachlorophenol

16.522min (-0.007) 0.00ng

response 300349

Ion	Exp%	Act%
266.00	100	100
264.00	63.90	62.07
268.00	69.40	62.13
0.00	0.00	0.00