


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072820\
 Data File : BN011271.D
 Acq On : 28 Jul 2020 09:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 28 14:38:05 2020

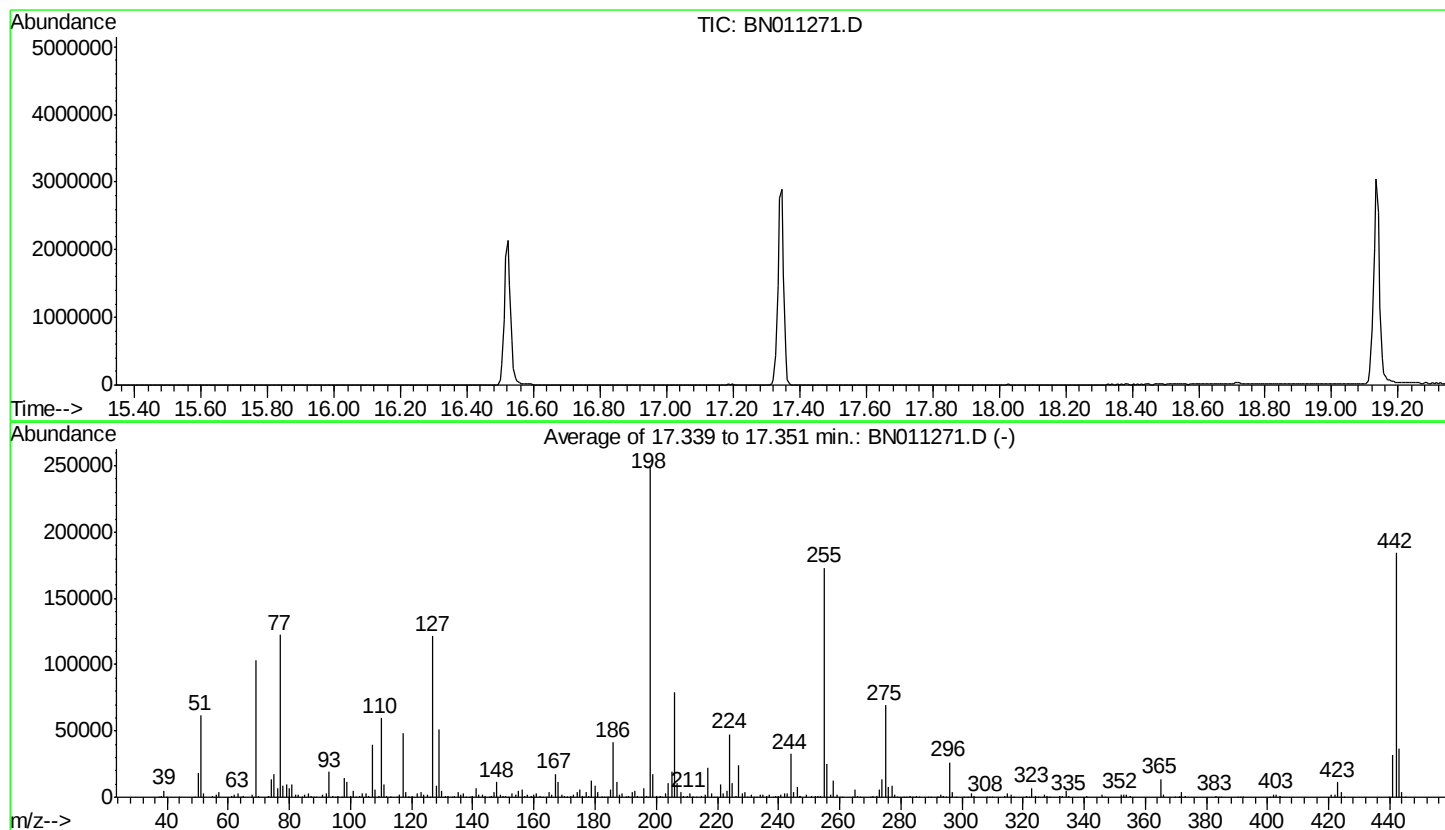

AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.7	61656	PASS
68	69	0.00	2	1.7	1810	PASS
69	198	0.00	100	41.4	103448	PASS
70	69	0.00	2	0.7	756	PASS
127	198	10	80	48.6	121506	PASS
197	198	0.00	2	0.2	544	PASS
198	198	100	100	100.0	250112	PASS
199	198	5	9	7.0	17557	PASS
275	198	10	60	27.7	69274	PASS
365	198	1	100	5.5	13779	PASS
441	198	0.01	100	12.8	31938	PASS
442	198	50	100	73.6	184042	PASS
443	442	15	24	19.8	36477	PASS