
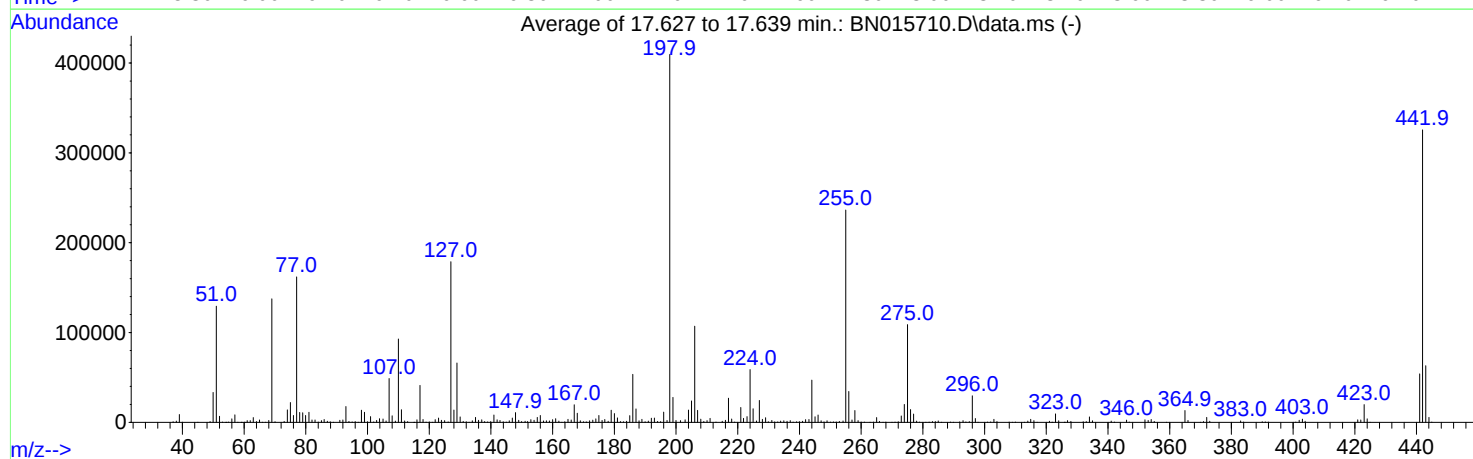


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072921\
 Data File : BN015710.D
 Acq On : 29 Jul 2021 16:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 30 02:33:42 2021

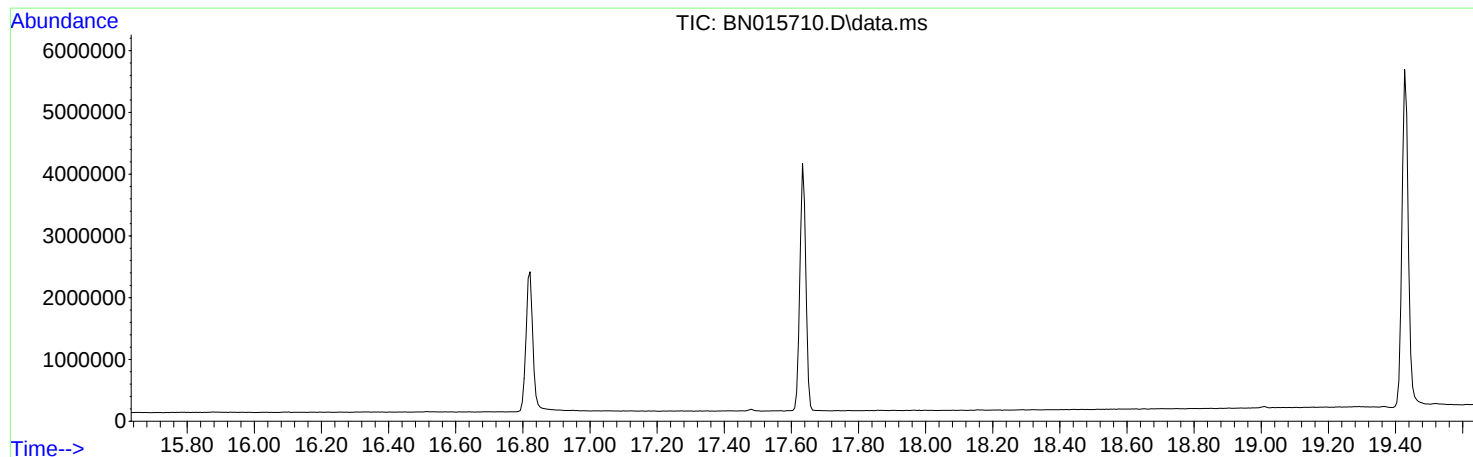




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	129398	PASS
68	69	0.00	2	1.6	2150	PASS
69	198	0.00	100	33.6	137525	PASS
70	69	0.00	2	0.5	651	PASS
127	198	10	80	43.7	178860	PASS
197	198	0.00	2	0.5	2124	PASS
198	198	100	100	100.0	409493	PASS
199	198	5	9	6.8	27803	PASS
275	198	10	60	26.6	108773	PASS
365	198	1	100	3.2	13221	PASS
441	198	0.01	100	13.2	53907	PASS
442	442	50	100	100.0	325675	PASS
443	442	15	24	19.4	63043	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072921\
 Data File : BN015710.D
 Acq On : 29 Jul 2021 16:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 30 07:20:23 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 30 07:20:03 2021
 Response via : Initial Calibration

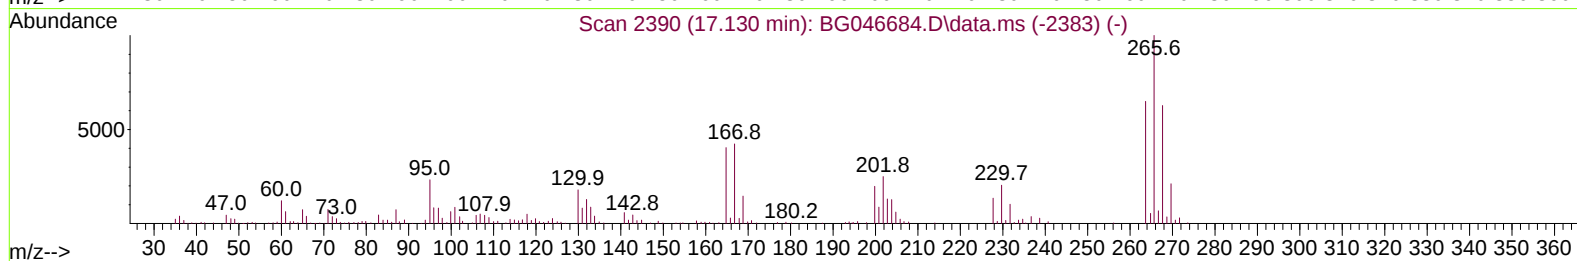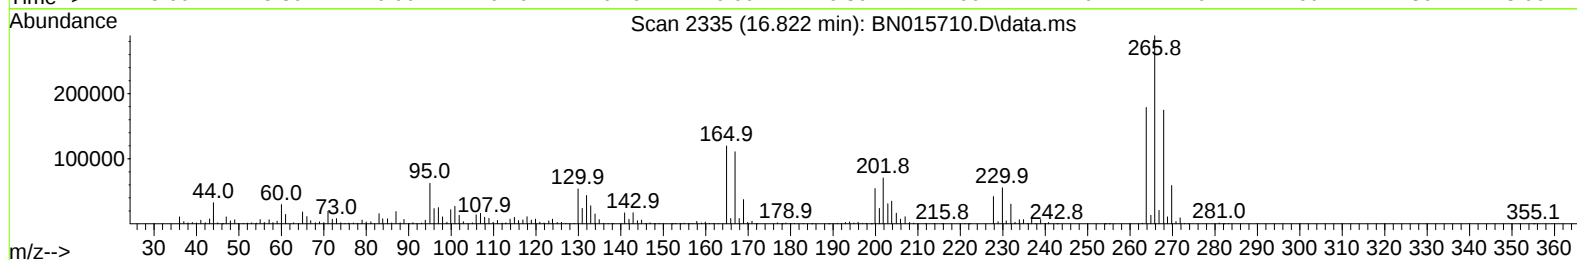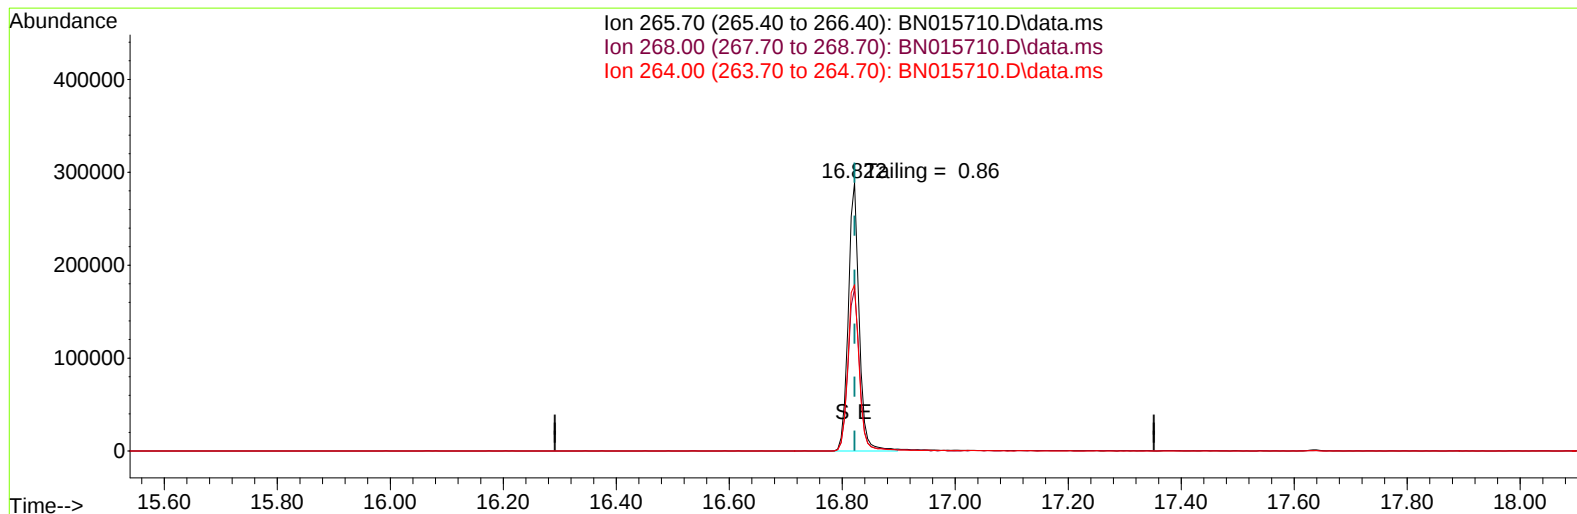

TIC: BN015710.D\data.ms

(70) Pentachlorophenol (C)

16.822min (0.000) 20050.28 ng




response 392115

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.48
264.00	61.60	61.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072921\
 Data File : BN015710.D
 Acq On : 29 Jul 2021 16:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 30 07:20:23 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 30 07:20:03 2021
 Response via : Initial Calibration

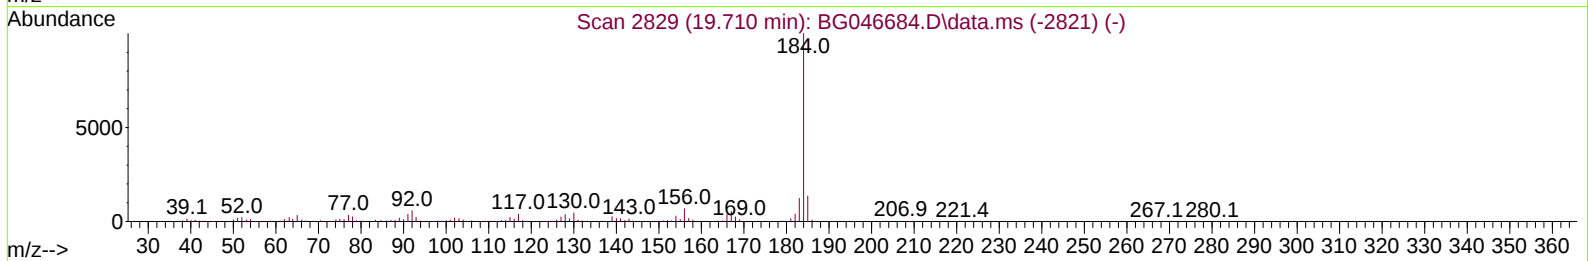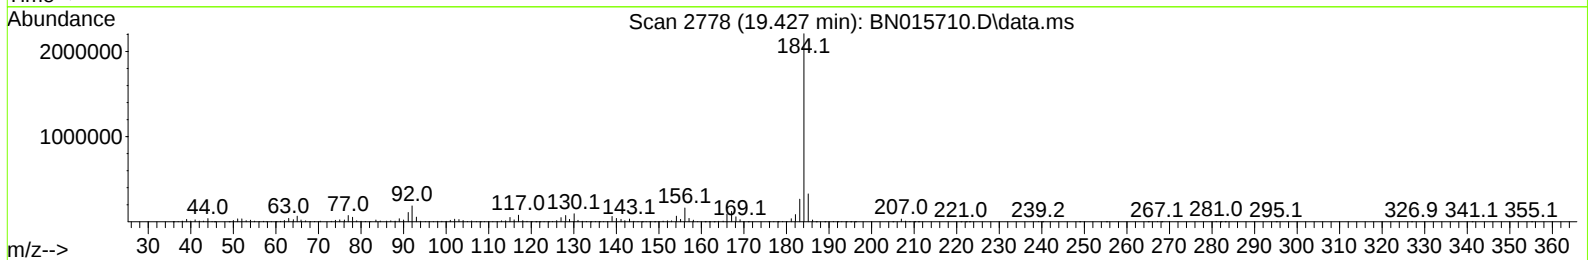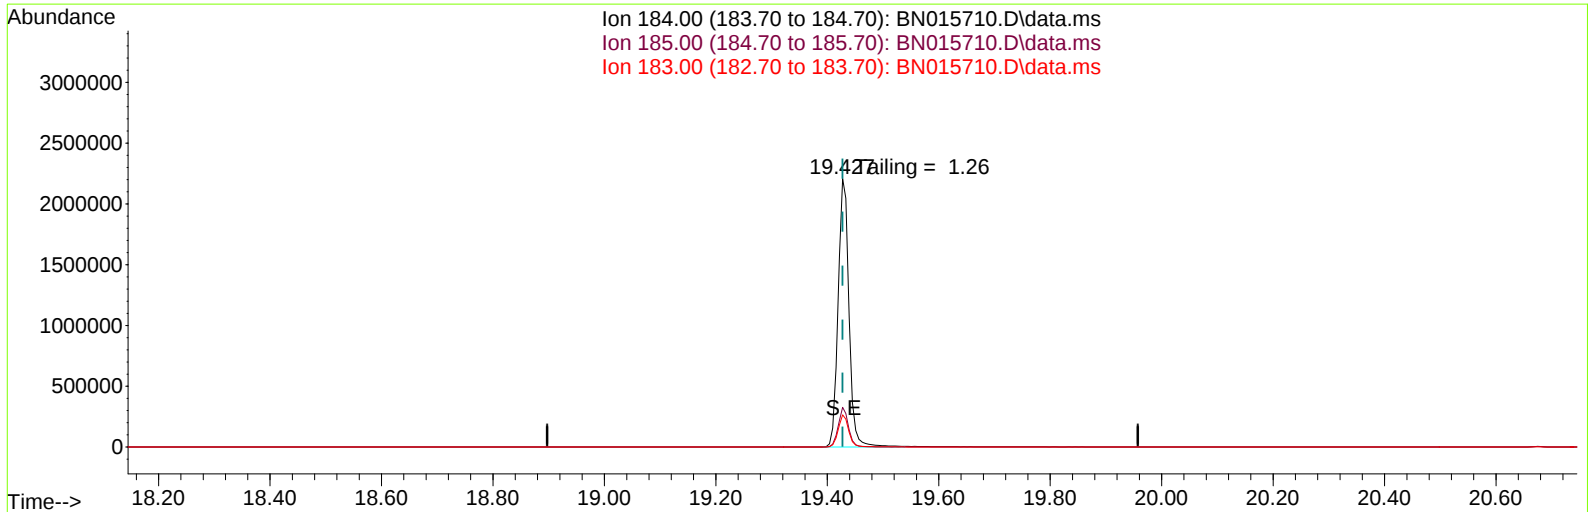

TIC: BN015710.D\data.ms

(77) Benzidine

19.427min (0.000) 919906.44 ng

response 3034141

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.83
183.00	13.20	12.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/29/2021	BNA_N	<u>BN015710.D</u>
Compound Name	Response	Retention Time
DDT	1237959	20.674
DDD	6015	20.286
DDE	1498	19.721
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7513	1245472	0.60

Instrument :
BNA_N
ClientSampleId :
DFTPP