

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072922\
 Data File : BN020918.D
 Acq On : 29 Jul 2022 12:34
 Operator : CG/JU
 Sample : N3890-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YBEA6

Quant Time: Jul 29 17:30:47 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 25 18:06:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.808	152	2429	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.606	136	8658	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.460	164	5499	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	11717	0.400	ng/ul	0.00
17) Chrysene-d12	21.422	240	9134	0.400	ng/ul	0.00
23) Perylene-d12	23.760	264	9082	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.214	96	13569	4.649	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.212	152	4120	0.313	ng/ul	0.00
18) Fluoranthene-d10	19.253	212	10635	0.365	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.252	88	2837	0.946	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072922\
Data File : BN020918.D
Acq On : 29 Jul 2022 12:34
Operator : CG/JU
Sample : N3890-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YBEA6

Quant Time: Jul 29 17:30:47 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 25 18:06:54 2022
Response via : Initial Calibration

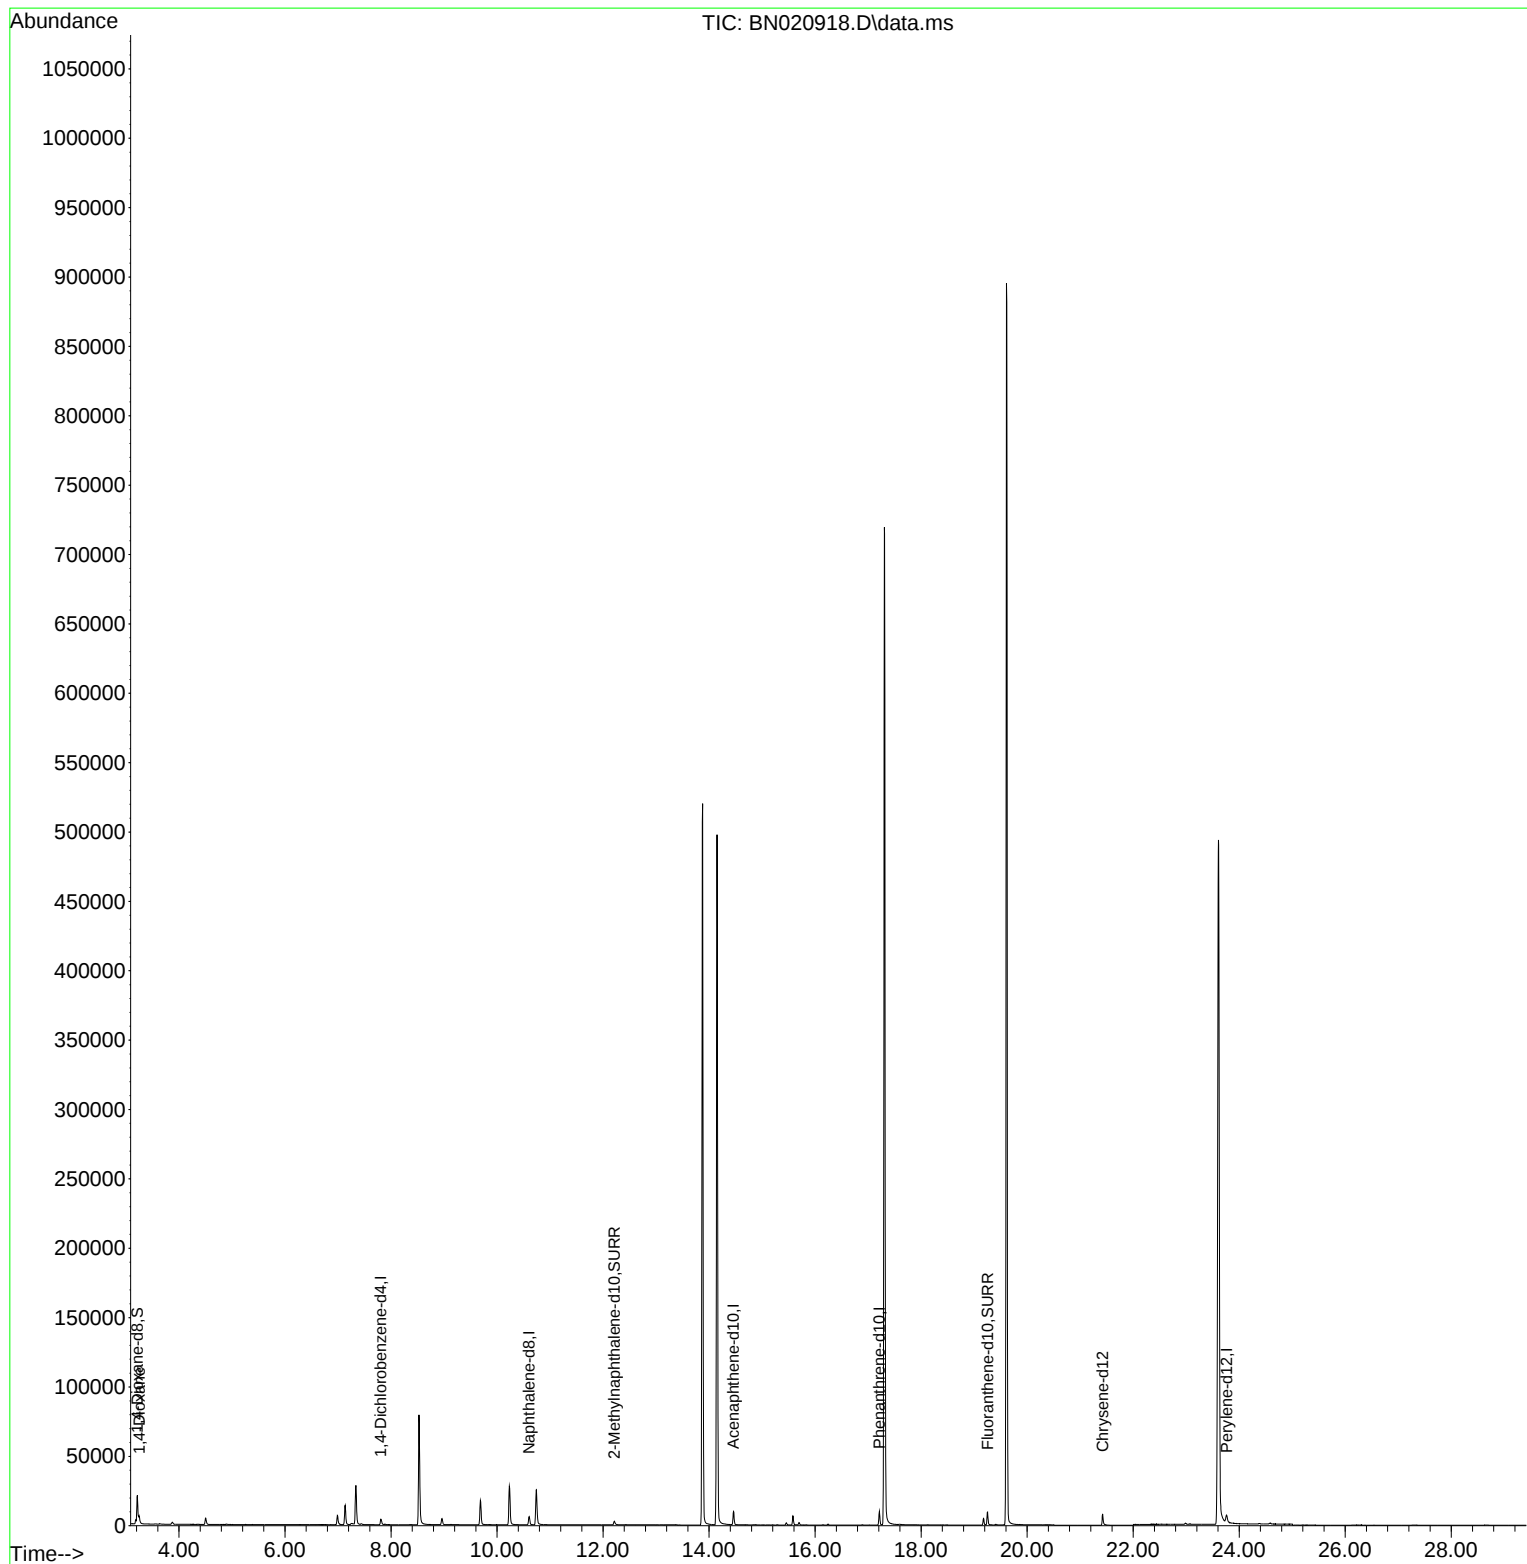

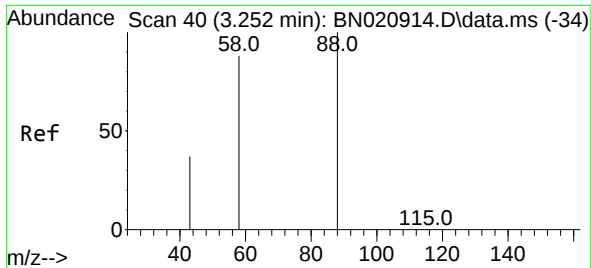

#2
 1,4-Dioxane
 Concen: 0.946 ng/ul
 RT: 3.252 min Scan# 40
 Delta R.T. -0.004 min
 Lab File: BN020918.D
 Acq: 29 Jul 2022 12:34

Instrument :
 BNA_N
 ClientSampleId :
 YBEA6

Tgt Ion: 88 Resp: 2837

Ion	Ratio	Lower	Upper
88	100		
43	36.6	32.5	48.7
58	69.8	46.2	69.2#

