
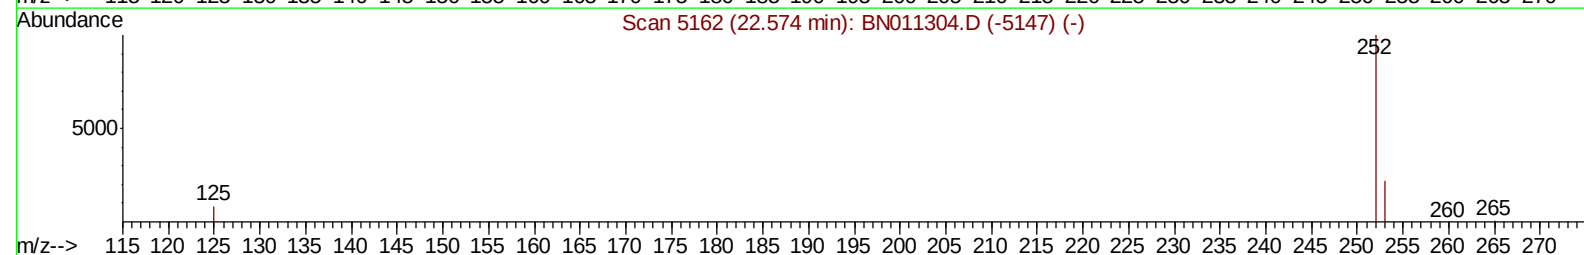
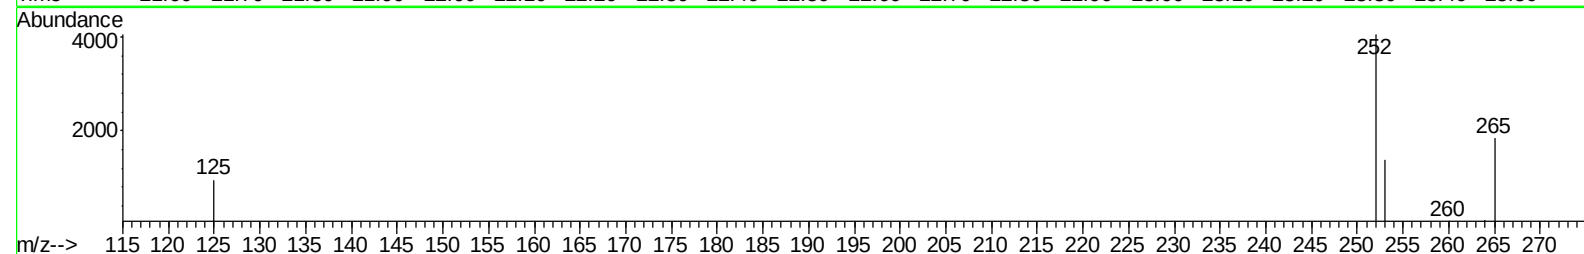


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN073020\
Data File : BN011308.D
Acq On : 30 Jul 2020 21:05
Operator : CG/JU
Sample : L3388-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Jul 31 03:00:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 31 02:58:38 2020
Response via : Initial Calibration

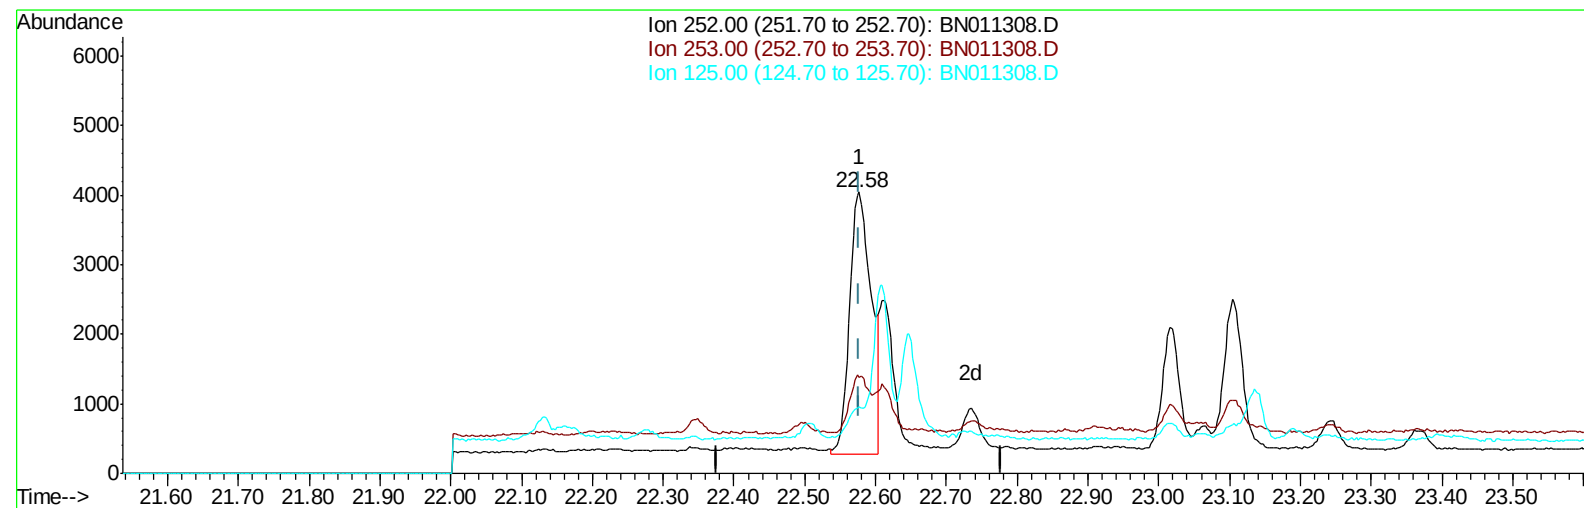

TIC: BN011308.D

(21) Benzo(b)fluoranthene

22.577min (-0.000) 0.21ng/ul m

response 7956

Ion	Exp%	Act%
252.00	100	100
253.00	25.90	34.16
125.00	12.10	23.54
0.00	0.00	0.00