
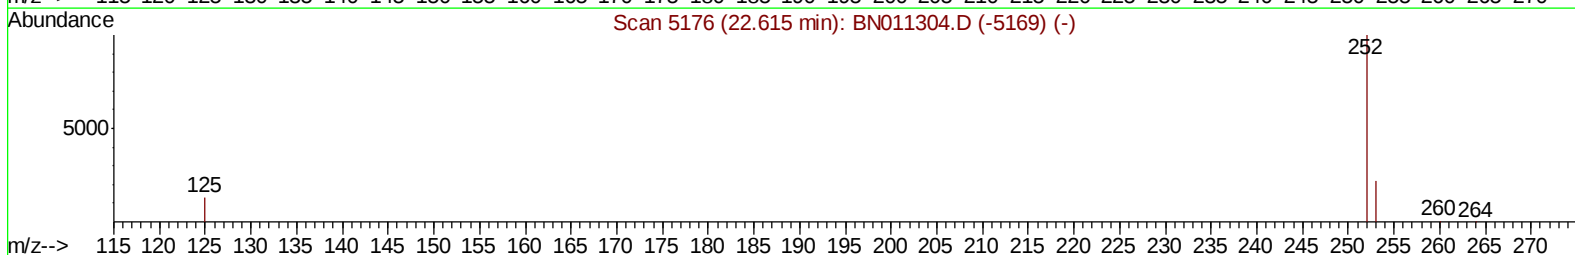
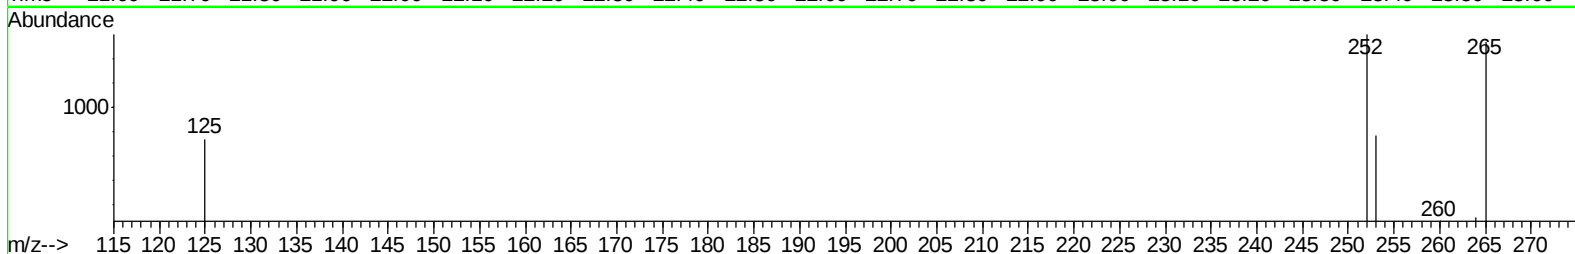


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN073020\
Data File : BN011315.D
Acq On : 31 Jul 2020 01:16
Operator : CG/JU
Sample : L3388-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Jul 31 03:52:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 31 02:58:38 2020
Response via : Initial Calibration

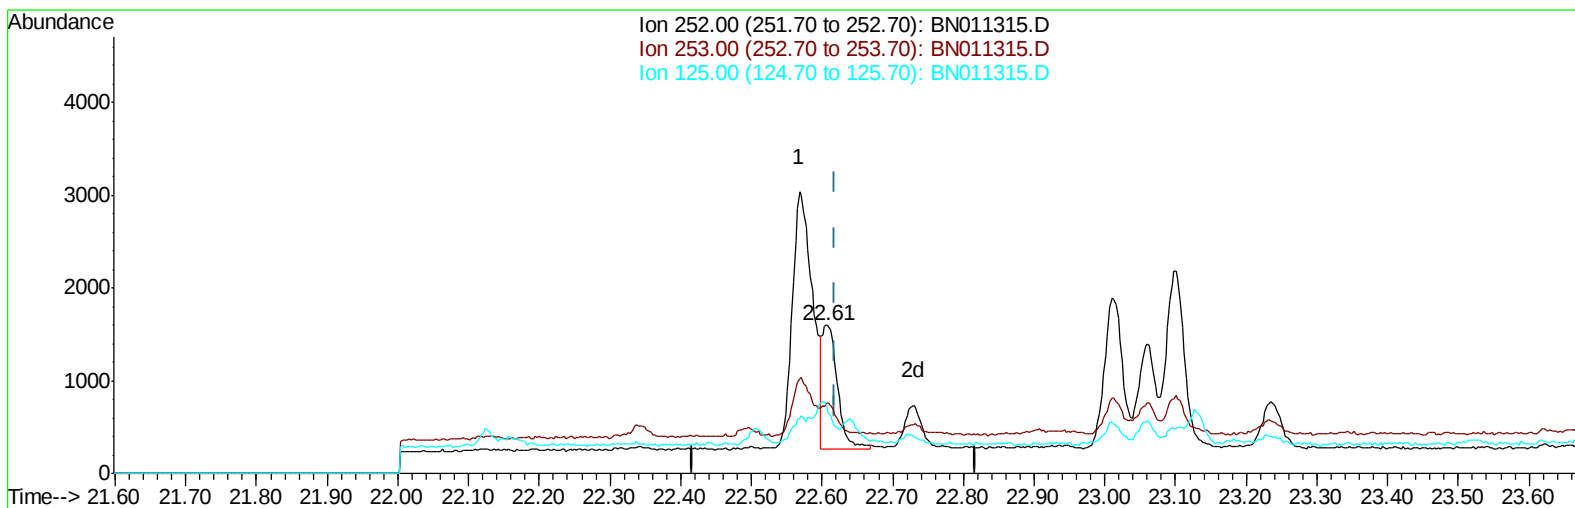

TIC: BN011315.D

(22) Benzo(k)fluoranthene

22.606min (-0.012) 0.06ng/ul m

response 1996

Ion	Exp%	Act%
252.00	100	100
253.00	26.70	47.75#
125.00	15.70	46.25#
0.00	0.00	0.00