
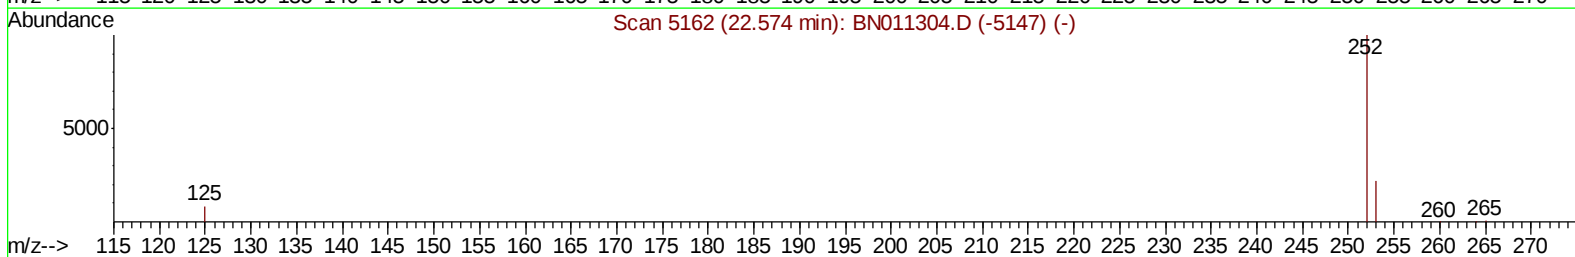
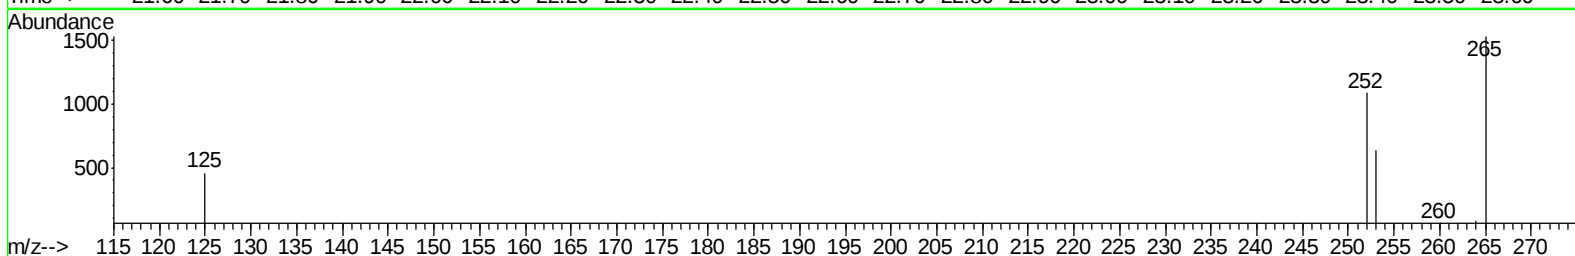


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN073020\
 Data File : BN011317.D
 Acq On : 31 Jul 2020 02:28
 Operator : CG/JU
 Sample : L3388-20
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Quant Time: Jul 31 04:10:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 31 02:58:38 2020
 Response via : Initial Calibration

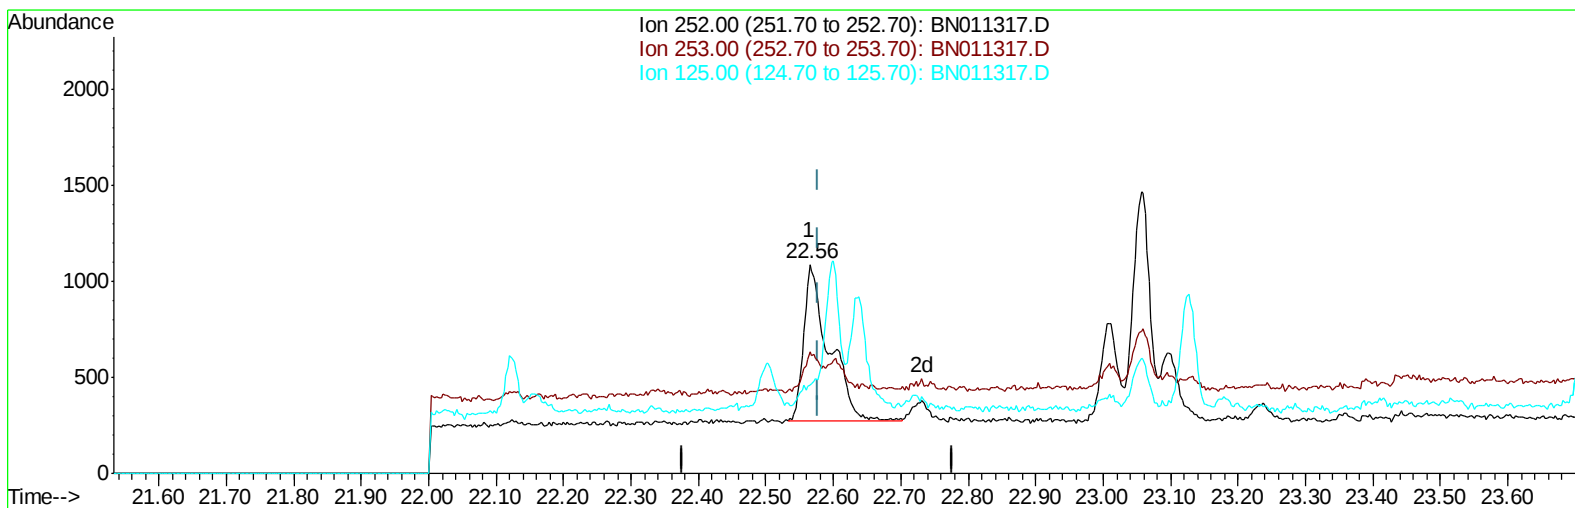

TIC: BN011317.D

(21) Benzo(b)fluoranthene
 22.565min (-0.012) 0.07ng/ul
 response 2174

Ion	Exp%	Act%
252.00	100	100
253.00	25.90	58.31#
125.00	12.10	42.15#
0.00	0.00	0.00