

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN073020\
 Data File : BN011313.D
 Acq On : 31 Jul 2020 00:05
 Operator : CG/JU
 Sample : L3388-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Quant Time: Jul 31 03:49:21 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 31 02:58:38 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	931	0.40	ng/ul	0.00
2) Naphthalene-d8	10.21	136	3734	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.10	164	2463	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.85	188	5841	0.40	ng/ul	0.00
16) Chrysene-d12	21.07	240	5730	0.40	ng/ul	0.00
20) Perylene-d12	23.19	264	7049	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.81	152	1807	0.19	ng/ul	0.00
14) Fluoranthene-d10	18.89	212	5752	0.20	ng/ul	0.00
Target Compounds						
15) Fluoranthene	18.93	202	511	0.021	ng/ul	Ovalue 63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN073020\
Data File : BN011313.D
Acq On : 31 Jul 2020 00:05
Operator : CG/JU
Sample : L3388-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD4

Quant Time: Jul 31 03:49:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 31 02:58:38 2020
Response via : Initial Calibration

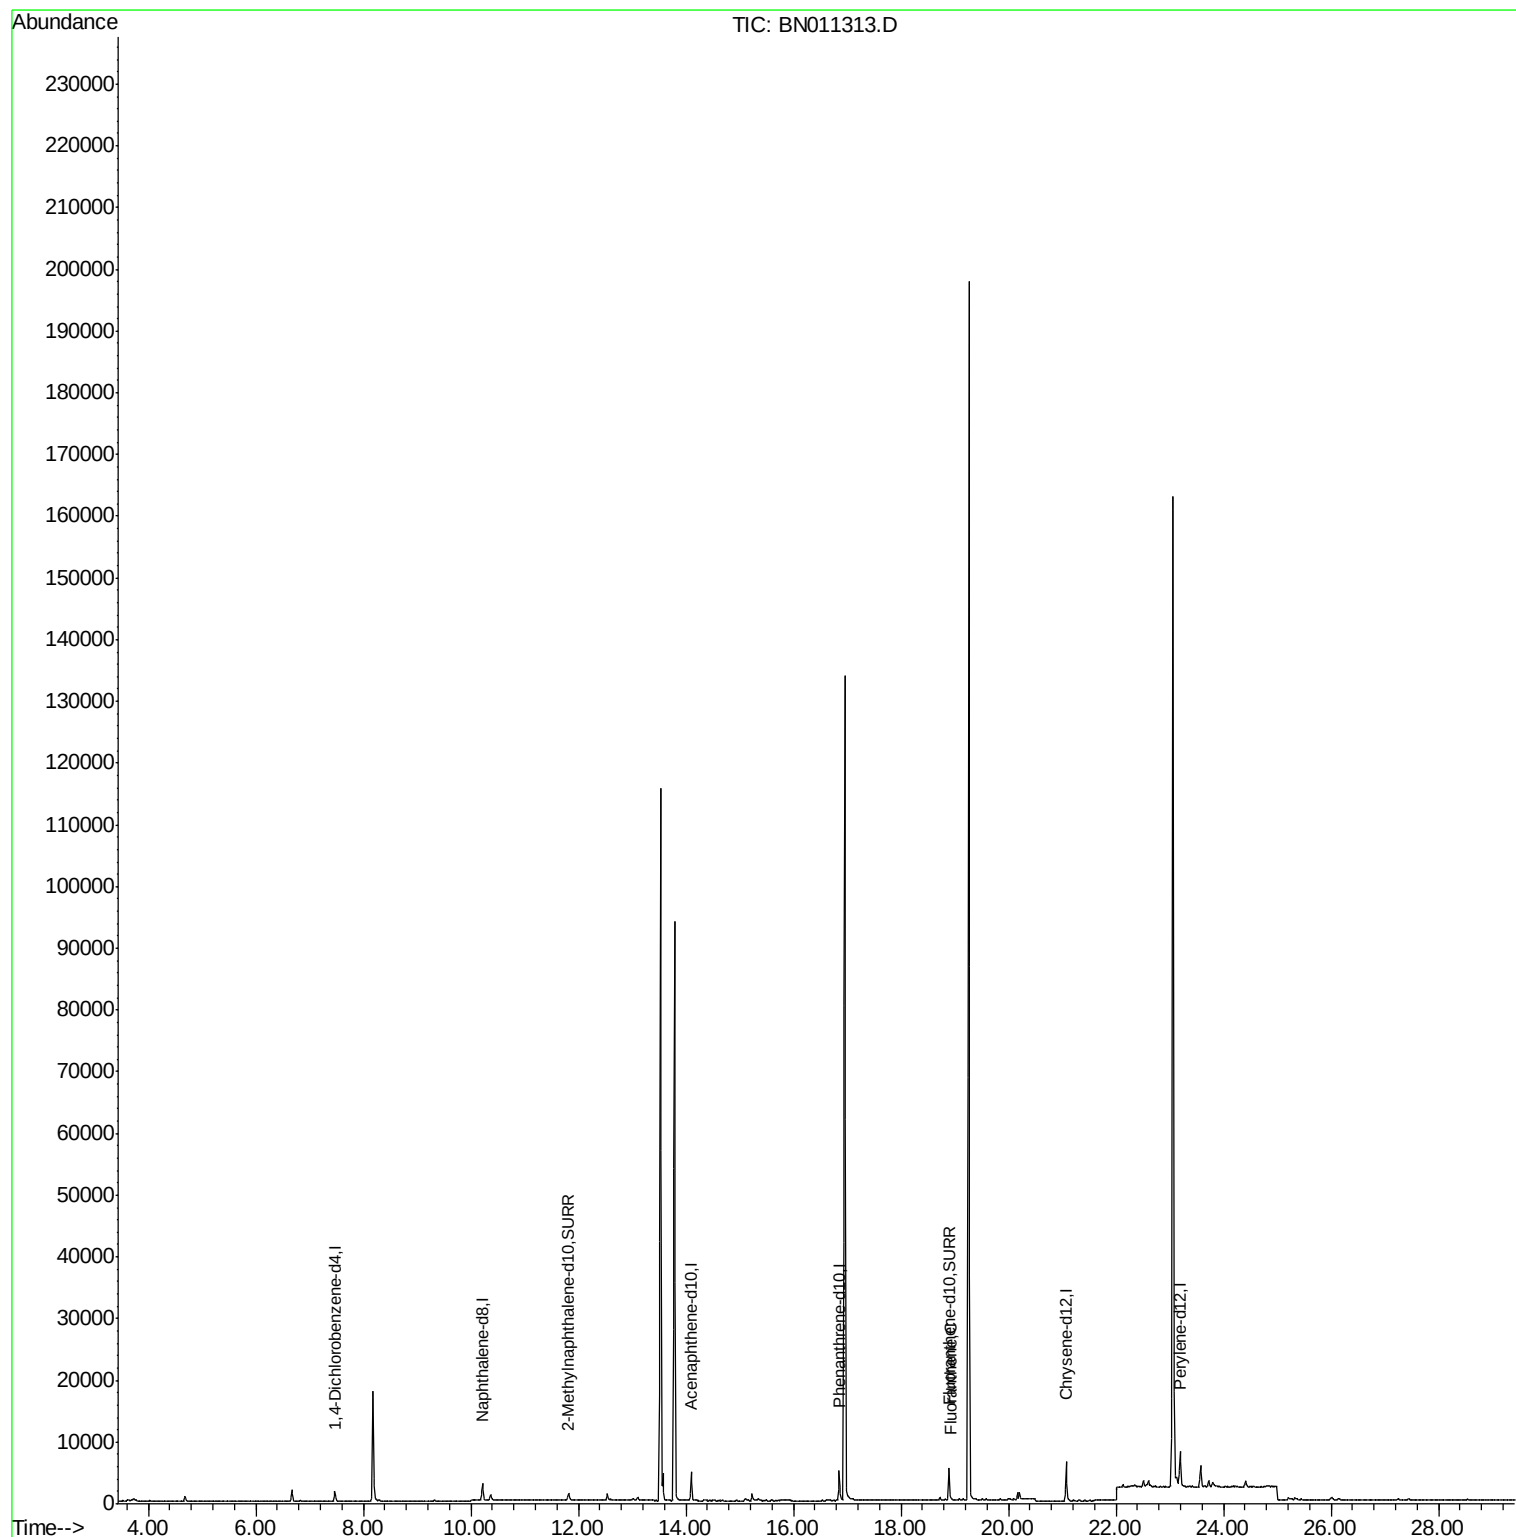

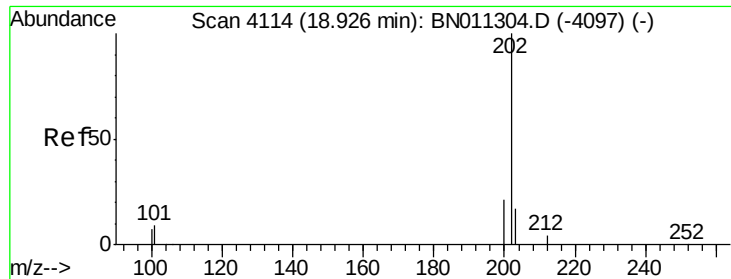

#15
 Fluoranthene
 Concen: 0.021 ng/ul
 RT: 18.93 min Scan# 4114
 Delta R.T. -0.00 min
 Lab File: BN011313.D
 Acq: 31 Jul 2020 00:05

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Tot Ion	Ratio	Lower	Upper
202	100		
101	21.4	0.0	28.2
100	19.7	0.0	26.8

