
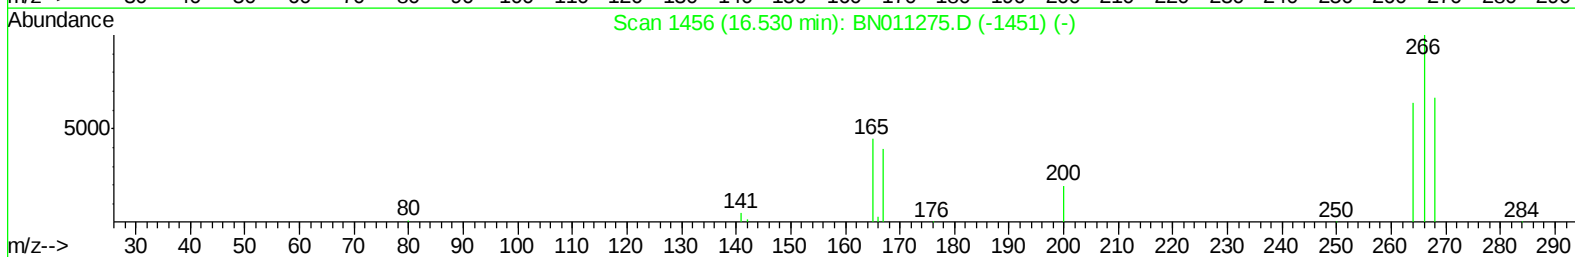
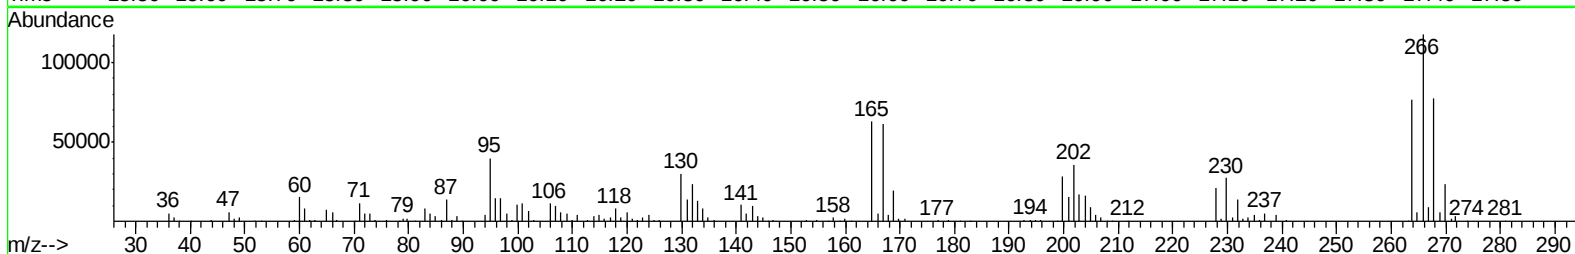


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN073120\
Data File : BN011321.D
Acq On : 31 Jul 2020 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 00:16:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN072820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 31 12:17:46 2020
Response via : Initial Calibration

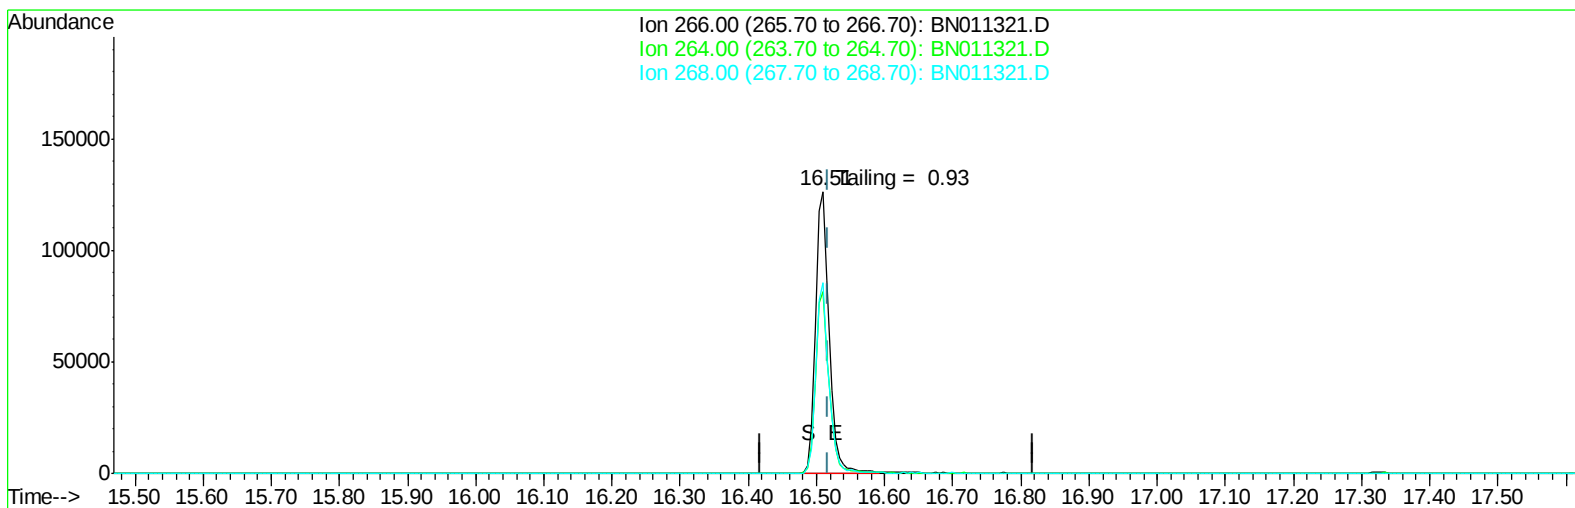

TIC: BN011321.D

(24) Pentachlorophenol

16.510min (-0.008) 0.00ng

response 175191

Ion	Exp%	Act%
266.00	100	100
264.00	63.90	64.29
268.00	69.40	64.58
0.00	0.00	0.00