


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073120\
 Data File : BN011321.D
 Acq On : 31 Jul 2020 10:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 31 12:17:46 2020

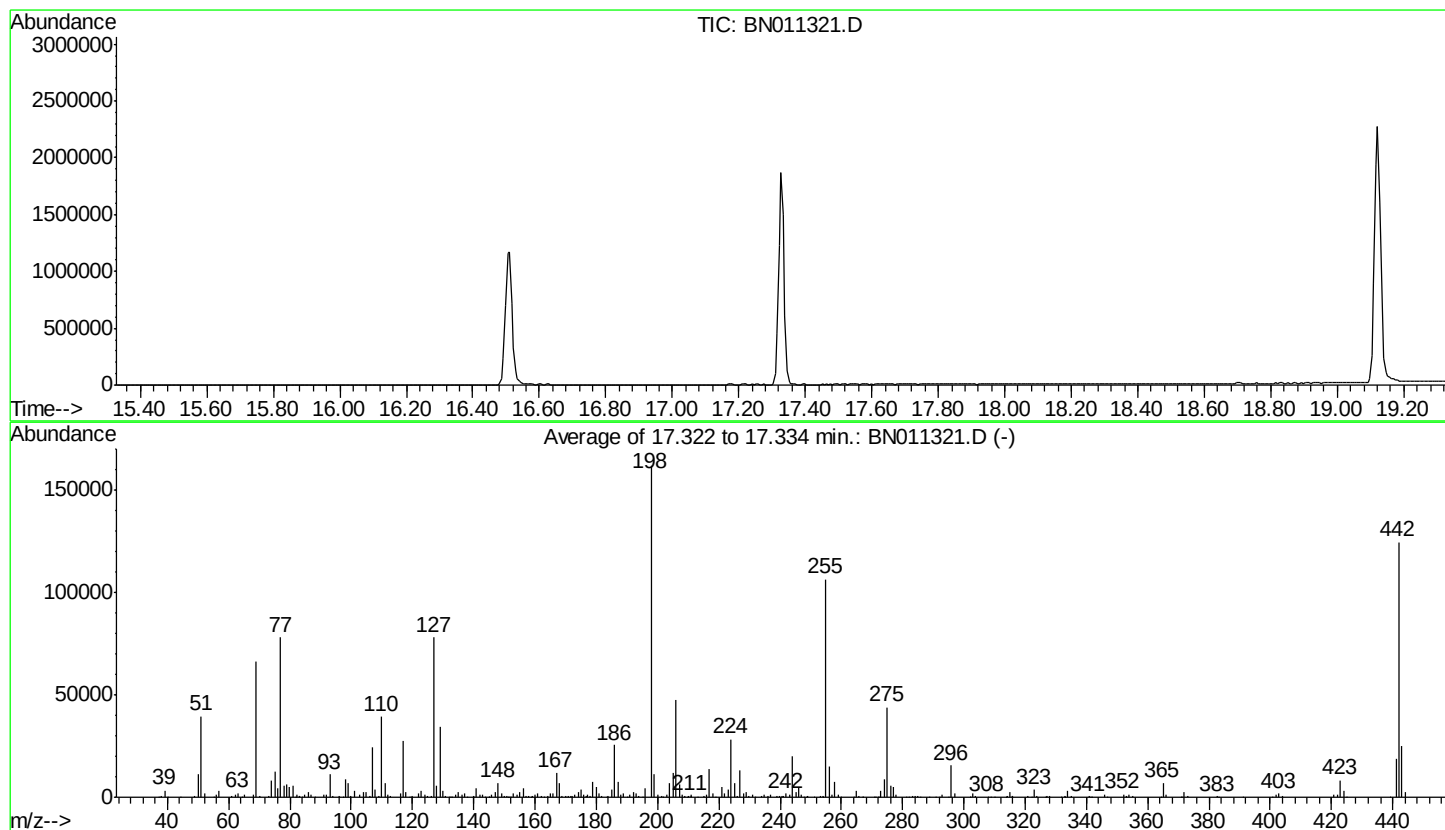

AutoFind: Scans 2437, 2438, 2439; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.5	39645	PASS
68	69	0.00	2	1.9	1264	PASS
69	198	0.00	100	41.1	66528	PASS
70	69	0.00	2	0.7	454	PASS
127	198	10	80	48.2	78157	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	162048	PASS
199	198	5	9	7.1	11446	PASS
275	198	10	60	27.0	43826	PASS
365	198	1	100	4.4	7134	PASS
441	198	0.01	100	11.8	19066	PASS
442	198	50	100	76.8	124520	PASS
443	442	15	24	19.9	24760	PASS