

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073121\
 Data File : BN015732.D
 Acq On : 31 Jul 2021 11:50
 Operator : CG/JU
 Sample : PB137923BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB137923BL

Quant Time: Aug 02 04:26:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 02 04:24:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.790	152	42172	0.400	ng	0.00
7) Naphthalene-d8	10.571	136	187824	0.400	ng	# 0.00
13) Acenaphthene-d10	14.421	164	96868	0.400	ng	0.00
19) Phenanthrene-d10	17.164	188	181355	0.400	ng	# 0.00
29) Chrysene-d12	21.376	240	161821	0.400	ng	# 0.00
35) Perylene-d12	23.714	264	165070	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.411	112	40563	0.358	ng	0.03
5) Phenol-d6	6.960	99	45407	0.331	ng	0.00
8) Nitrobenzene-d5	8.937	82	39721	0.337	ng	0.00
11) 2-Methylnaphthalene-d10	12.163	152	108675	0.384	ng	0.00
14) 2,4,6-Tribromophenol	15.905	330	10420	0.249	ng	-0.01
15) 2-Fluorobiphenyl	13.038	172	140392	0.379	ng	-0.01
27) Fluoranthene-d10	19.207	212	180361	0.377	ng	0.00
31) Terphenyl-d14	19.813	244	159617	0.405	ng	0.00
Target Compounds						
						Qvalue
6) bis(2-Chloroethyl)ether	7.237	93	26	0.000	ng	# 22
9) Naphthalene	10.622	128	373	0.001	ng	# 41
10) Hexachlorobutadiene	10.914	225	8	0.000	ng	# 1
12) 2-Methylnaphthalene	12.234	142	150	0.000	ng	# 61
16) Acenaphthylene	14.129	152	73	0.000	ng	# 84
17) Acenaphthene	14.472	154	46	0.000	ng	# 1
18) Fluorene	15.461	166	136	0.000	ng	# 80
20) 4,6-Dinitro-2-methylph...	15.525	198	3	0.000	ng	# 1
21) 4-Bromophenyl-phenylether	16.360	248	6	0.000	ng	# 15
22) Hexachlorobenzene	16.482	284	9	0.000	ng	# 1
23) Atrazine	16.628	200	11	0.000	ng	# 1
24) Pentachlorophenol	16.823	266	107	0.002	ng	90
25) Phenanthrene	17.237	178	1592	0.003	ng	# 1
26) Anthracene	17.297	178	91	0.000	ng	# 56
28) Fluoranthene	19.237	202	174	0.000	ng	# 64
30) Pyrene	19.599	202	199	0.000	ng	93
32) Benzo(a)anthracene	21.365	228	598	0.001	ng	# 80
33) Chrysene	21.365	228	572	0.001	ng	# 78
34) Bis(2-ethylhexyl)phtha...	21.302	149	1601	0.006	ng	# 91
36) Indeno(1,2,3-cd)pyrene	26.110	276	42	0.000	ng	# 69
37) Benzo(b)fluoranthene	23.009	252	100	0.000	ng	# 1
38) Benzo(k)fluoranthene	23.043	252	588	0.001	ng	# 1
39) Benzo(a)pyrene	23.611	252	21	0.000	ng	# 1
40) Dibenzo(a,h)anthracene	26.141	278	120	0.000	ng	# 1
41) Benzo(g,h,i)perylene	26.842	276	35	0.000	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073121\
Data File : BN015732.D
Acq On : 31 Jul 2021 11:50
Operator : CG/JU
Sample : PB137923BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB137923BL

Quant Time: Aug 02 04:26:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 02 04:24:05 2021
Response via : Initial Calibration




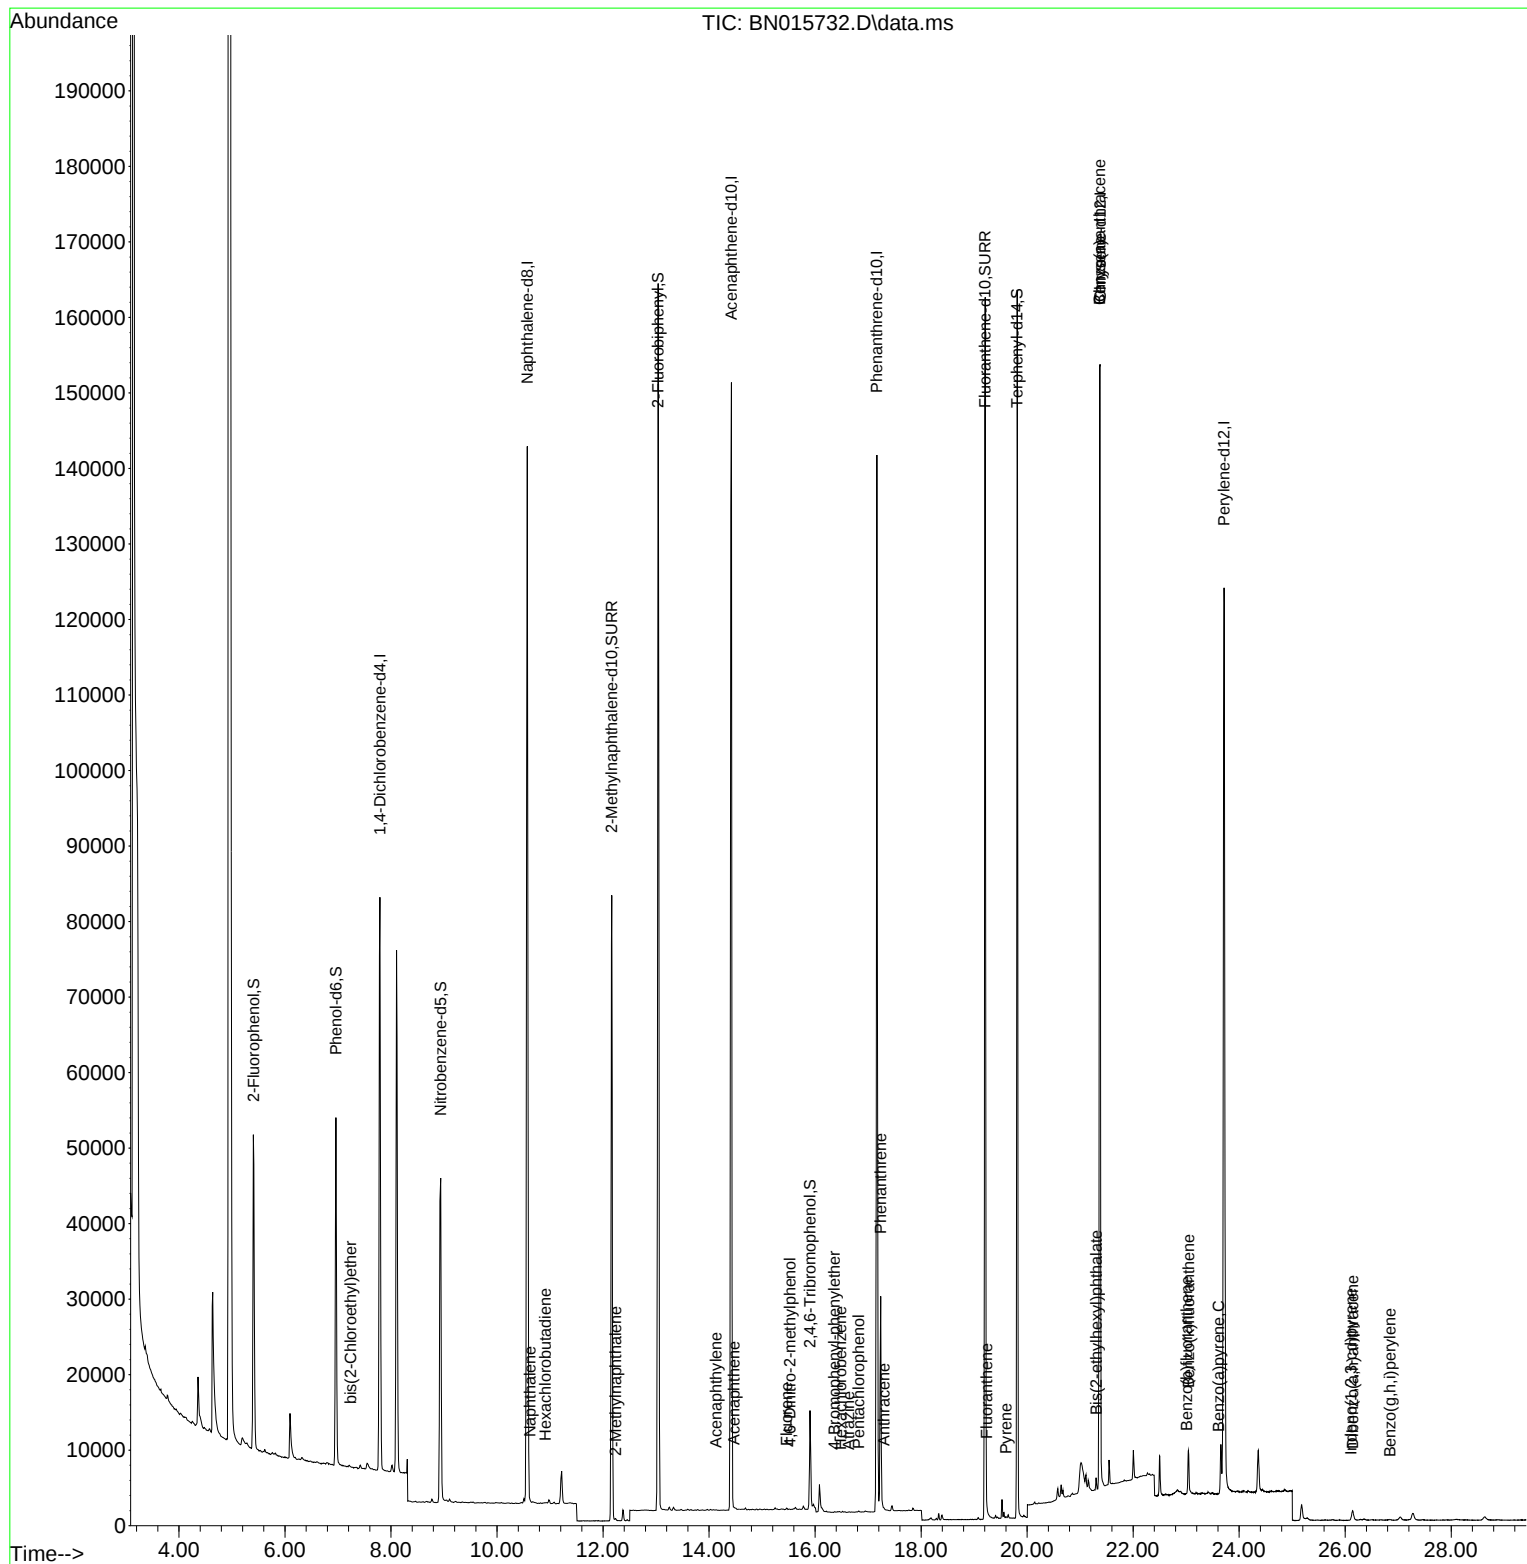




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.790 min Scan# 511
Delta R.T. -0.000 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50




Instrument :
BNA_N
ClientSampleId :
PB137923BL


Tgt Ion:152 Resp: 42172
Ion Ratio Lower Upper
152 100
150 153.5 123.9 185.9
115 57.6 47.8 71.6



#4
2-Fluorophenol
Concen: 0.358 ng
RT: 5.411 min Scan# 253
Delta R.T. 0.028 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50

Tgt Ion:112 Resp: 40563
Ion Ratio Lower Upper
112 100
64 51.6 42.1 63.1
63 26.8 21.9 32.9


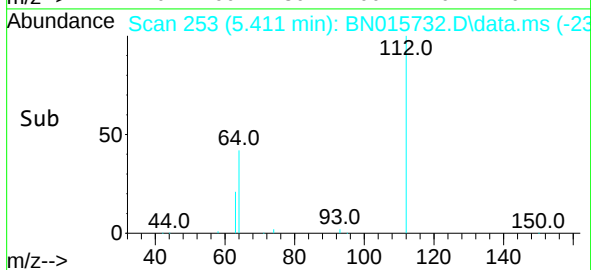

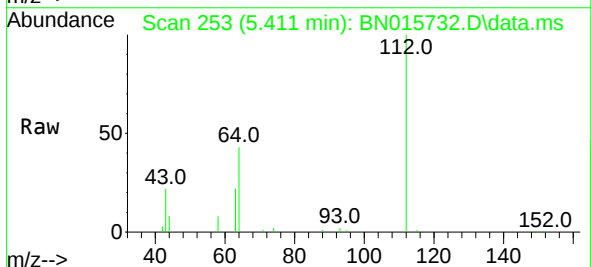




#5
Phenol-d6
Concen: 0.331 ng
RT: 6.960 min Scan# 421
Delta R.T. 0.009 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50




Instrument :
BNA_N
ClientSampleId :
PB137923BL


Tgt Ion:	99	Resp:	45407
Ion	Ratio	Lower	Upper
99	100		
42	15.0	12.9	19.3
71	29.5	23.8	35.6

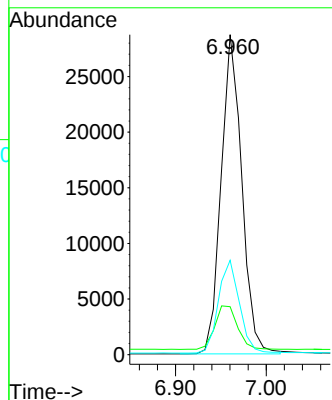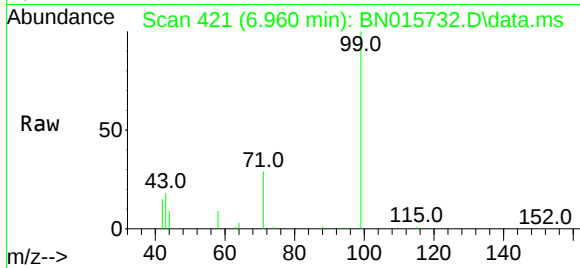

#6
bis(2-Chloroethyl)ether
Concen: 0.000 ng
RT: 7.237 min Scan# 451
Delta R.T. 0.019 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50

Tgt Ion:	93	Resp:	26
Ion	Ratio	Lower	Upper
93	100		
63	0.0	58.6	87.8#
95	0.0	26.9	40.3#


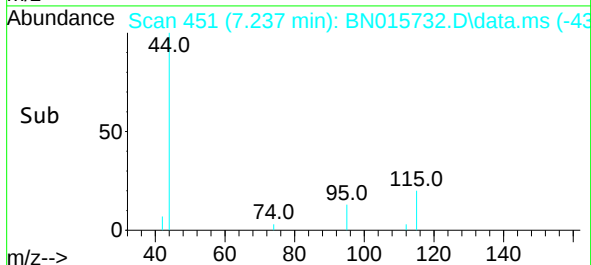
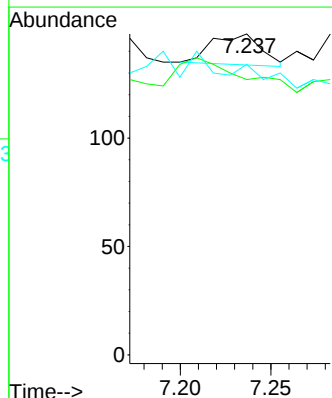
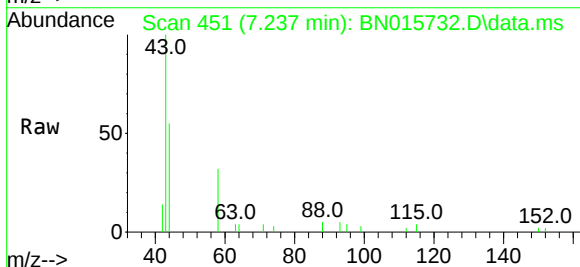




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.571 min Scan# 746
Delta R.T. 0.000 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50




Instrument :
BNA_N
ClientSampleId :
PB137923BL


Tgt Ion:136	Resp:	187824
Ion Ratio	Lower	Upper
136	100	
137	11.0	8.7 13.1
54	5.0	5.5 8.3#
68	4.2	4.5 6.7#

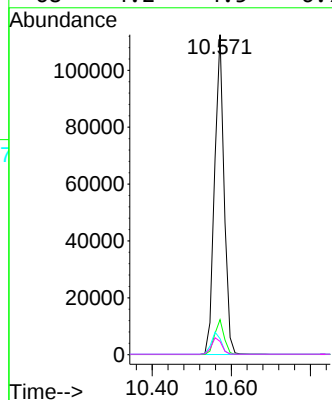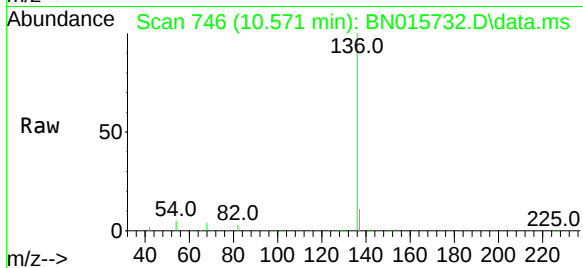

#8
Nitrobenzene-d5
Concen: 0.337 ng
RT: 8.937 min Scan# 617
Delta R.T. 0.000 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50

Tgt Ion: 82	Resp:	39721
Ion Ratio	Lower	Upper
82	100	
128	46.9	33.2 49.8
54	44.4	38.4 57.6



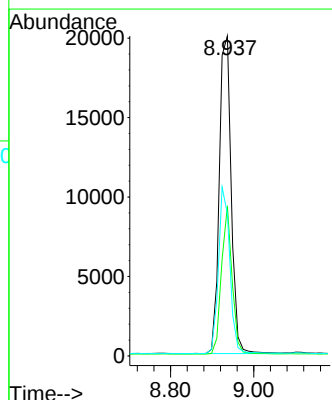
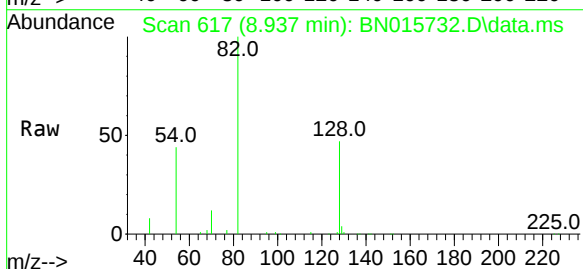




#9
Naphthalene
Concen: 0.001 ng
RT: 10.622 min Scan# 750
Delta R.T. 0.000 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50




Instrument :
BNA_N
ClientSampleId :
PB137923BL


Tgt Ion:128 Resp: 373
Ion Ratio Lower Upper
128 100
129 39.2 8.9 13.3#
127 31.3 10.4 15.6#



#10
Hexachlorobutadiene
Concen: 0.000 ng
RT: 10.914 min Scan# 773
Delta R.T. 0.000 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50

Tgt Ion:225 Resp: 8
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 200.0 51.0 76.4#


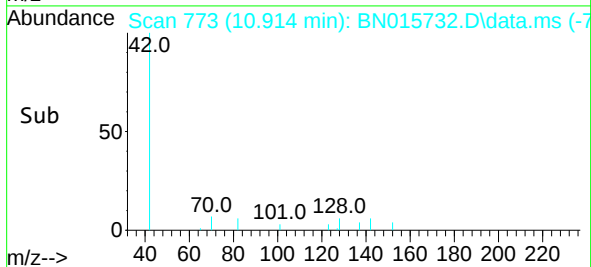

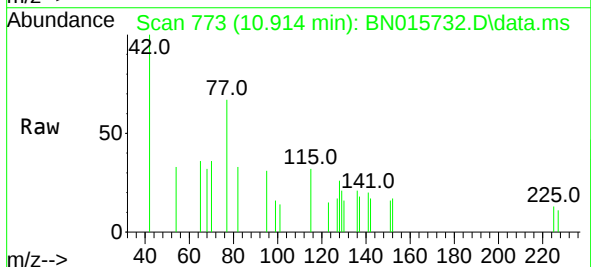


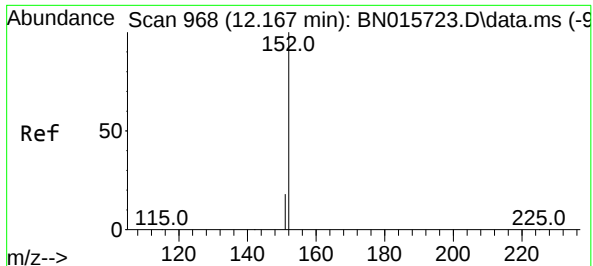

#11
2-Methylnaphthalene-d10
Concen: 0.384 ng
RT: 12.163 min Scan# 967
Delta R.T. -0.004 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50




Instrument :
BNA_N
ClientSampleId :
PB137923BL


Tgt Ion:152 Resp: 108675
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.4

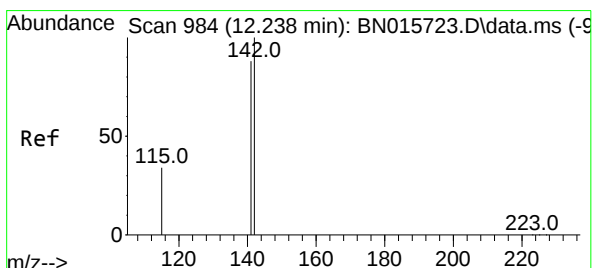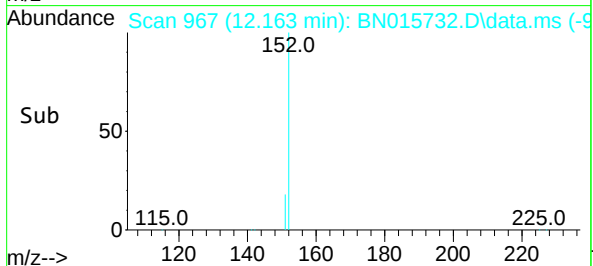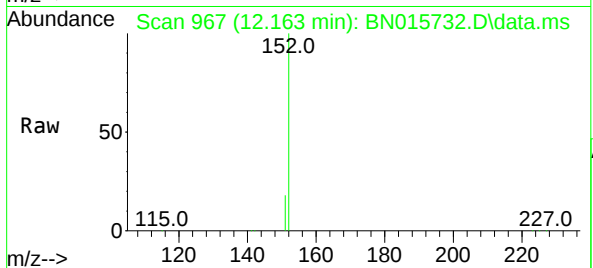

#12
2-Methylnaphthalene
Concen: 0.000 ng
RT: 12.234 min Scan# 983
Delta R.T. -0.004 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50

Tgt Ion:142 Resp: 150
Ion Ratio Lower Upper
142 100
141 94.7 70.5 105.7
115 103.5 27.3 40.9#


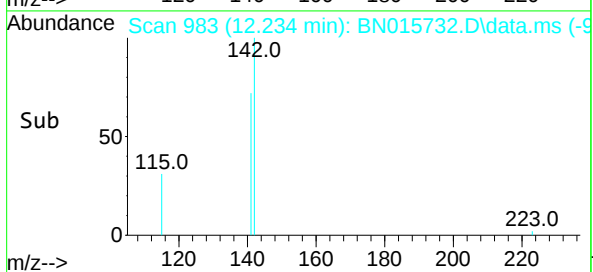

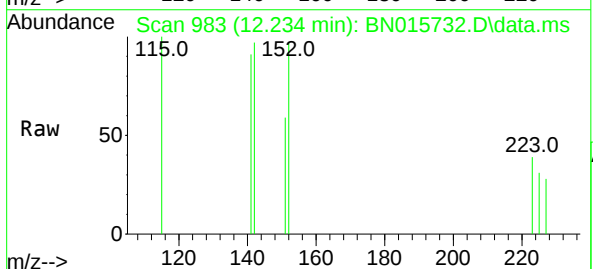




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.421 min Scan# 1195
Delta R.T. -0.000 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50




Instrument :
BNA_N
ClientSampleId :
PB137923BL


Tgt Ion:164 Resp: 96868
Ion Ratio Lower Upper
164 100
162 98.4 79.8 119.6
160 43.3 35.8 53.6

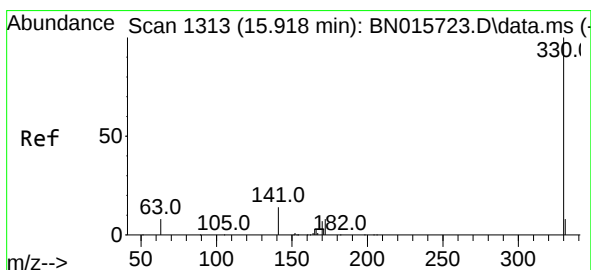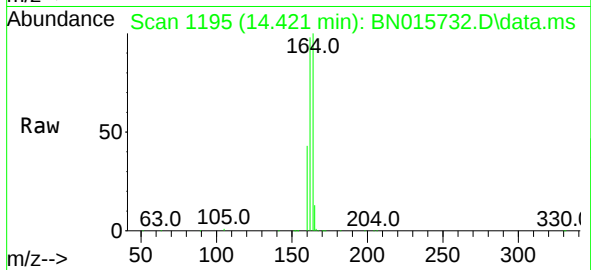

#14
2,4,6-Tribromophenol
Concen: 0.249 ng
RT: 15.905 min Scan# 1312
Delta R.T. -0.013 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50

Tgt Ion:330 Resp: 10420
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.3 28.8 43.2


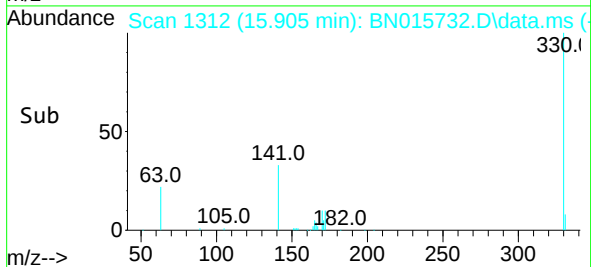

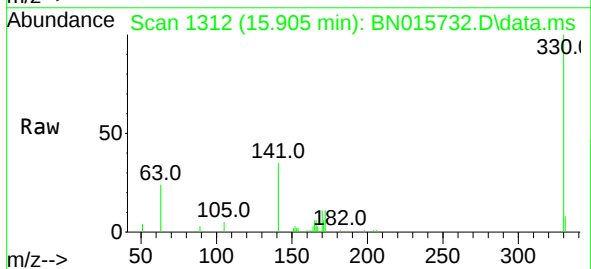


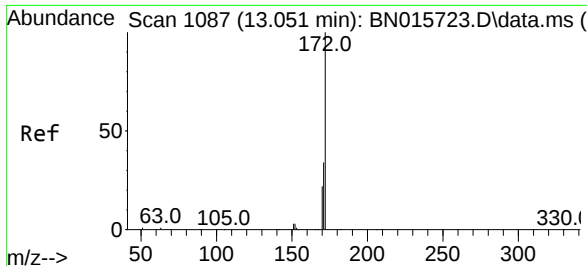

#15
2-Fluorobiphenyl
Concen: 0.379 ng
RT: 13.038 min Scan# 1086
Delta R.T. -0.013 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50




Instrument :
BNA_N
ClientSampleId :
PB137923BL


Tgt Ion:172 Resp: 140392
Ion Ratio Lower Upper
172 100
171 35.0 26.9 40.3
170 23.8 17.4 26.0

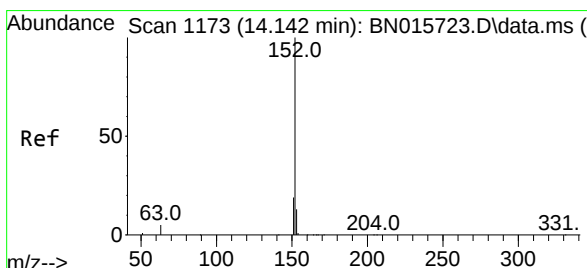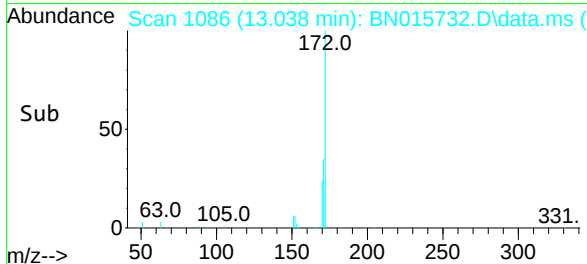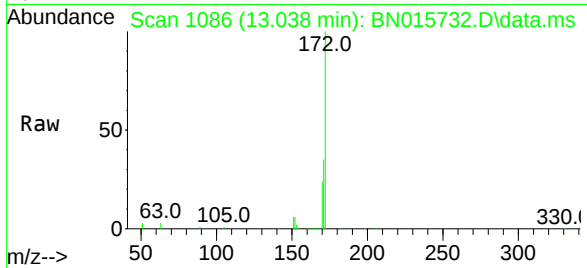

#16
Acenaphthylene
Concen: 0.000 ng
RT: 14.129 min Scan# 1172
Delta R.T. -0.013 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50

Tgt Ion:152 Resp: 73
Ion Ratio Lower Upper
152 100
151 30.1 15.7 23.5#
153 11.0 10.4 15.6


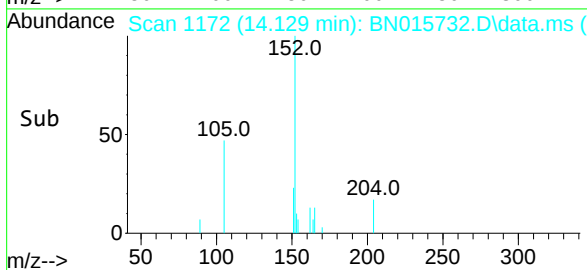

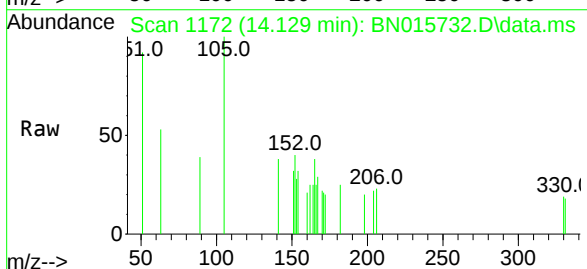


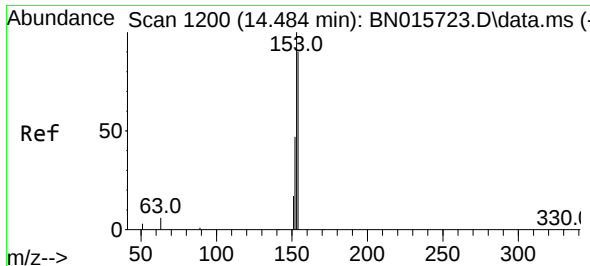

#17
Acenaphthene
Concen: 0.000 ng
RT: 14.472 min Scan# 1199
Delta R.T. -0.012 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50




Instrument :
BNA_N
ClientSampled :
PB137923BL


Tgt Ion:154 Resp: 46
Ion Ratio Lower Upper
154 100
153 217.4 89.7 134.5#
152 150.0 43.8 65.6#

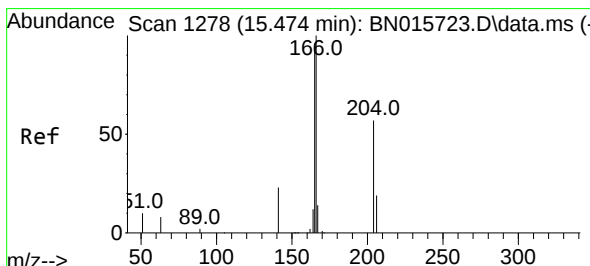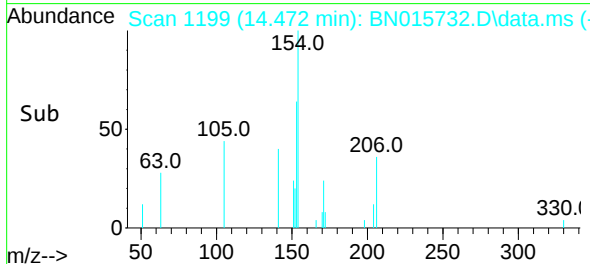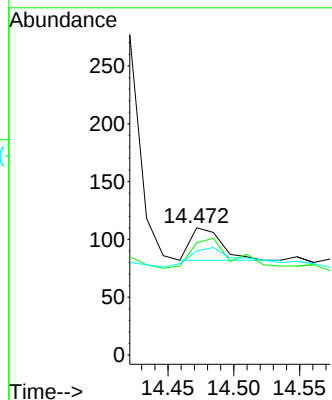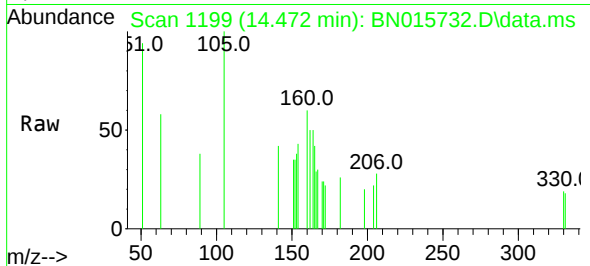

#18
Fluorene
Concen: 0.000 ng
RT: 15.461 min Scan# 1277
Delta R.T. -0.013 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50

Tgt Ion:166 Resp: 136
Ion Ratio Lower Upper
166 100
165 114.0 78.1 117.1
167 30.9 10.8 16.2#


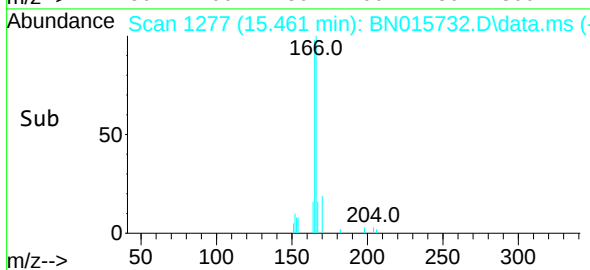
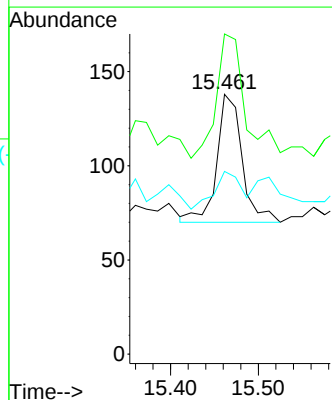
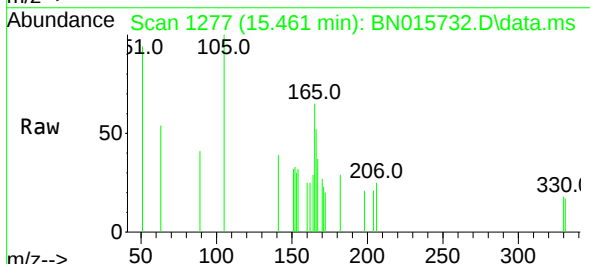




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.164 min Scan# 1415
Delta R.T. 0.001 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50




Instrument :
BNA_N
ClientSampleId :
PB137923BL


Tgt Ion:188 Resp: 181355
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.8 10.2 15.4#



#20
4,6-Dinitro-2-methylphenol
Concen: 0.000 ng
RT: 15.525 min Scan# 1282
Delta R.T. -0.025 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50

Tgt Ion:198 Resp: 3
Ion Ratio Lower Upper
198 100
182 138.9 9.4 14.0#
77 0.0 0.0 0.0


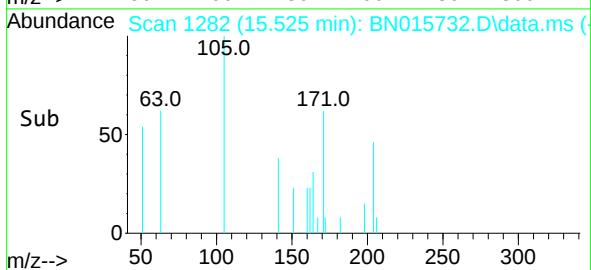

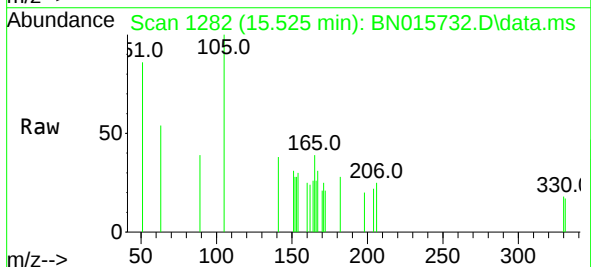


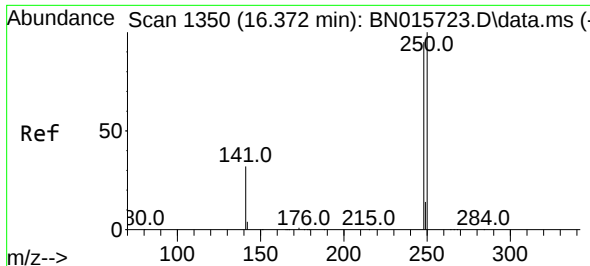

#21
4-Bromophenyl-phenylether
Concen: 0.000 ng
RT: 16.360 min Scan# 1349
Delta R.T. -0.012 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50




Instrument :
BNA_N
ClientSampleId :
PB137923BL


Tgt Ion:248 Resp: 6
Ion Ratio Lower Upper
248 100
250 111.8 83.9 125.9
141 221.6 26.9 40.3#

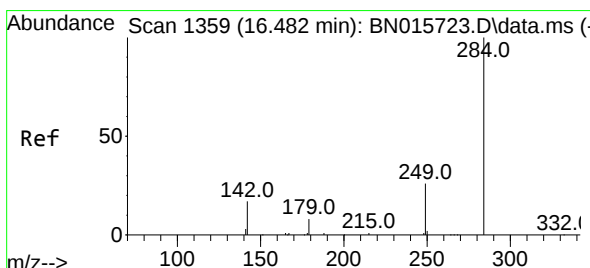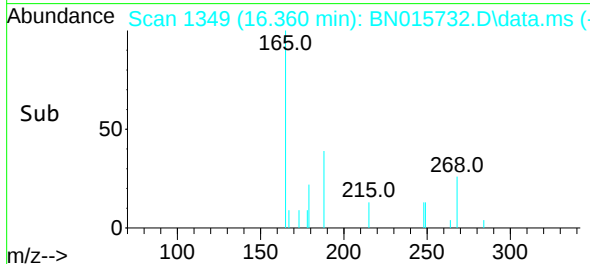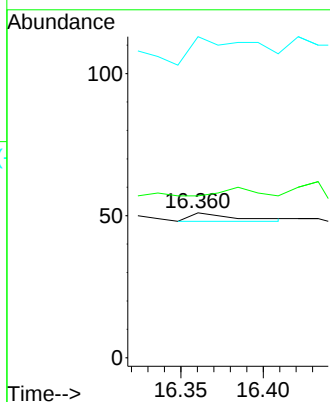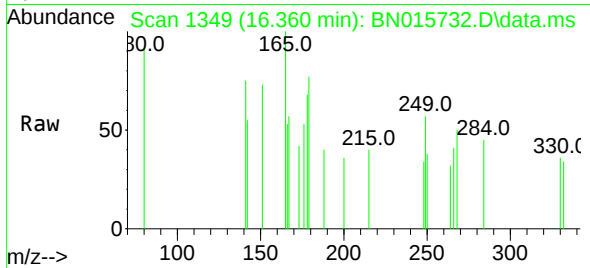

#22
Hexachlorobenzene
Concen: 0.000 ng
RT: 16.482 min Scan# 1359
Delta R.T. 0.000 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50

Tgt Ion:284 Resp: 9
Ion Ratio Lower Upper
284 100
142 0.0 29.4 44.0#
249 222.2 23.8 35.6#

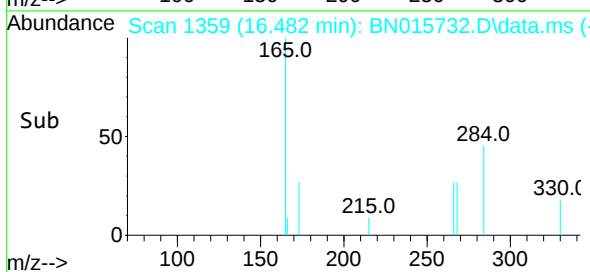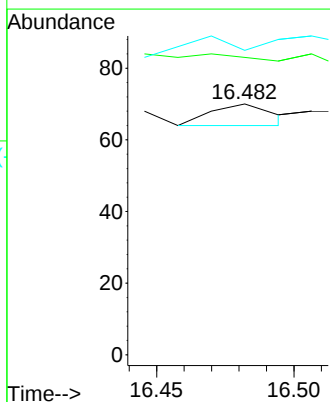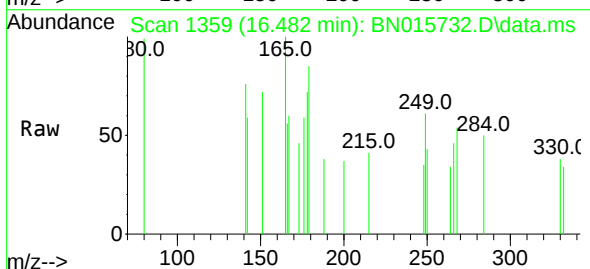



#23

Atrazine

Concen: 0.000 ng

RT: 16.628 min Scan# 1371

Delta R.T. -0.012 min

Lab File: BN015732.D

Acq: 31 Jul 2021 11:50





Tgt Ion:	200	Resp:	11
Ion Ratio	Lower	Upper	
200	100		
173	105.2	18.9	28.3#
215	100.0	38.1	57.1#

Instrument :

BNA_N

ClientSampleId :

PB137923BL

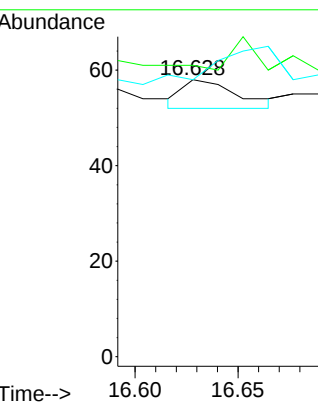

#24

Pentachlorophenol

Concen: 0.002 ng




RT: 16.823 min Scan# 1387


Delta R.T. -0.000 min

Lab File: BN015732.D

Acq: 31 Jul 2021 11:50

Tgt Ion:	266	Resp:	107
Ion Ratio	Lower	Upper	
266	100		
264	57.0	50.2	75.2
268	54.2	51.1	76.7


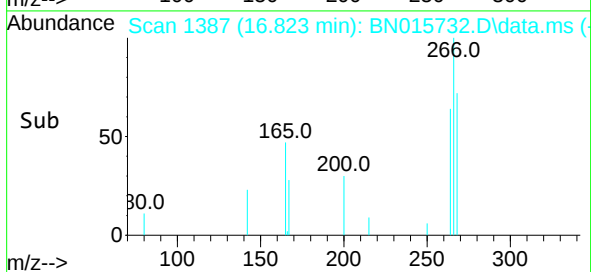
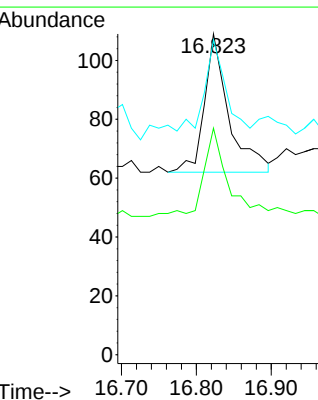



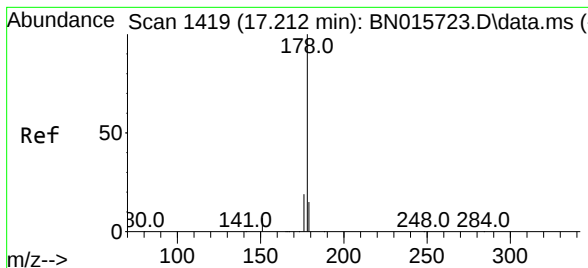

#25
Phenanthrene
Concen: 0.003 ng
RT: 17.237 min Scan# 1421
Delta R.T. 0.024 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50




Instrument :
BNA_N
ClientSampleId :
PB137923BL


Tgt Ion:178 Resp: 1592
Ion Ratio Lower Upper
178 100
176 0.0 15.3 22.9#
179 870.0 12.4 18.6#

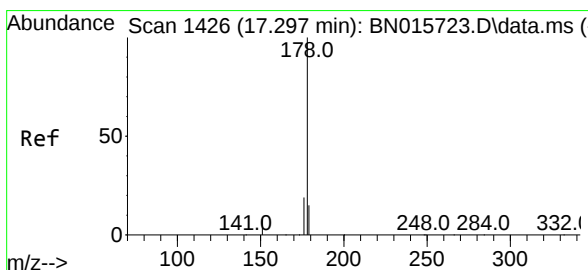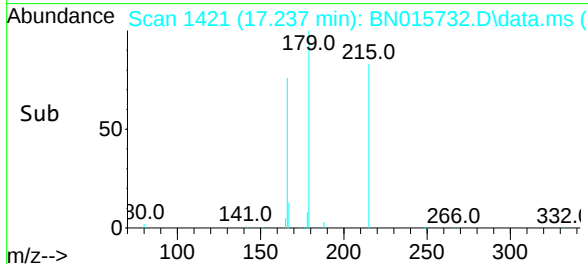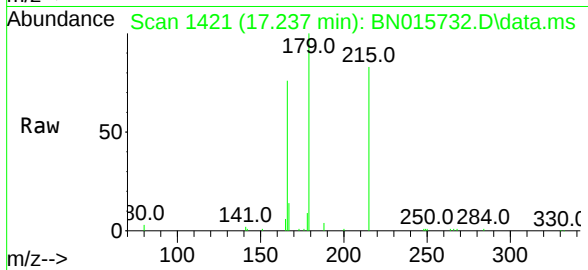

#26
Anthracene
Concen: 0.000 ng
RT: 17.297 min Scan# 1426
Delta R.T. 0.000 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50

Tgt Ion:178 Resp: 91
Ion Ratio Lower Upper
178 100
176 40.7 14.6 22.0#
179 0.0 12.2 18.4#


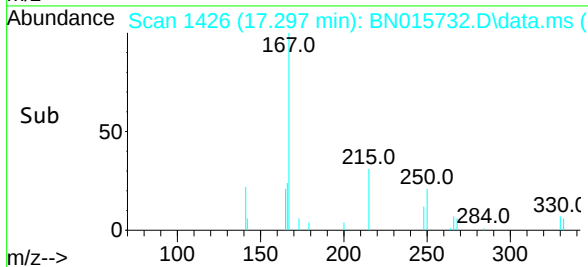

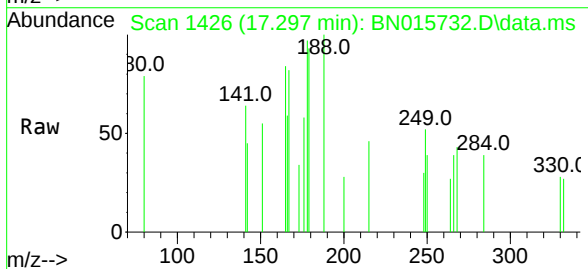




#27
Fluoranthene-d10
Concen: 0.377 ng
RT: 19.207 min Scan# 1725
Delta R.T. -0.005 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50




Instrument :
BNA_N
ClientSampleId :
PB137923BL


Tgt Ion:212 Resp: 180361
Ion Ratio Lower Upper
212 100
106 13.2 10.6 16.0
104 7.3 5.9 8.9

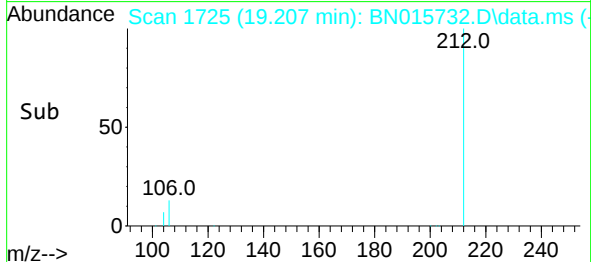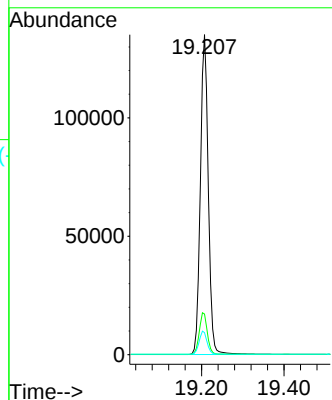

#28
Fluoranthene
Concen: 0.000 ng
RT: 19.237 min Scan# 1731
Delta R.T. -0.005 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50

Tgt Ion:202 Resp: 174
Ion Ratio Lower Upper
202 100
101 0.0 9.0 13.6#
203 0.0 13.8 20.8#

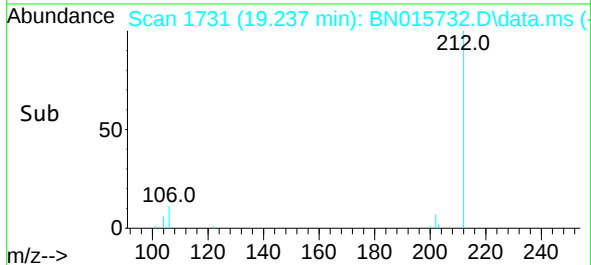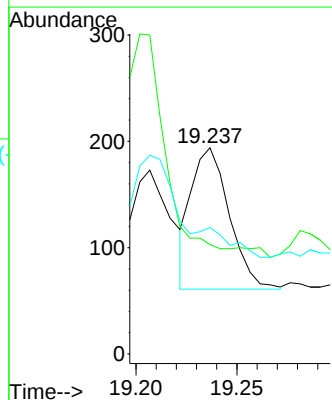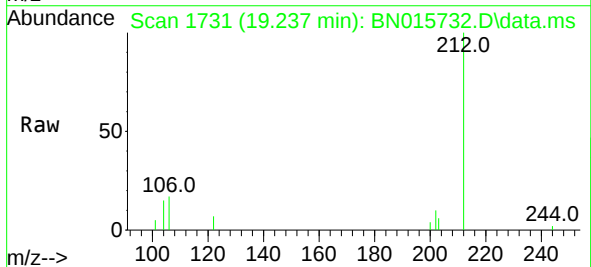



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.376 min Scan# 2015

Delta R.T. 0.000 min

Lab File: BN015732.D

Acq: 31 Jul 2021 11:50





Tgt Ion:240 Resp: 161821

Ion Ratio Lower Upper

240 100

120 5.5 7.4 11.0#

236 25.0 20.9 31.3

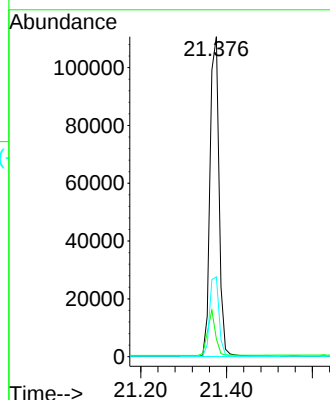

#30

Pyrene

Concen: 0.000 ng

RT: 19.599 min Scan# 1804

Delta R.T. -0.005 min

Lab File: BN015732.D

Acq: 31 Jul 2021 11:50




Tgt Ion:202 Resp: 199


Ion Ratio Lower Upper

202 100

200 24.1 16.5 24.7

203 20.1 14.0 21.0


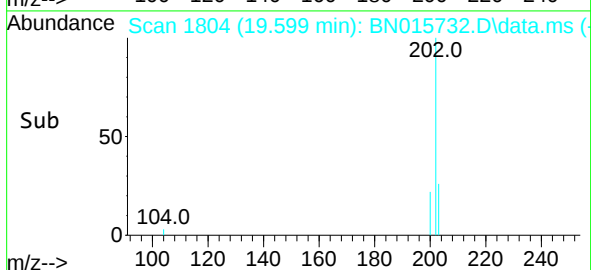
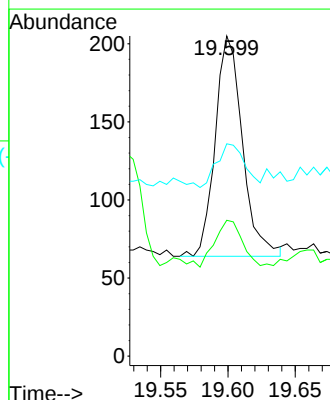





#31
 Terphenyl-d14
 Concen: 0.405 ng
 RT: 19.813 min Scan# 1847
 Delta R.T. -0.005 min
 Lab File: BN015732.D
 Acq: 31 Jul 2021 11:50




Instrument :
 BNA_N
 ClientSampleId :
 PB137923BL


Tgt Ion:244	Resp:	159617
Ion Ratio	Lower	Upper
244	100	
212	7.3	5.9 8.9
122	11.9	9.6 14.4

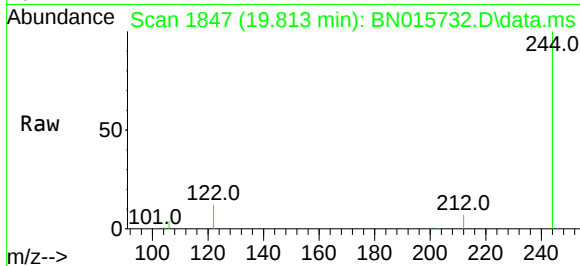

#32
 Benzo(a)anthracene
 Concen: 0.001 ng
 RT: 21.365 min Scan# 2014
 Delta R.T. 0.010 min
 Lab File: BN015732.D
 Acq: 31 Jul 2021 11:50

Tgt Ion:228	Resp:	598
Ion Ratio	Lower	Upper
228	100	
226	26.4	21.9 32.9
229	39.8	15.4 23.0#


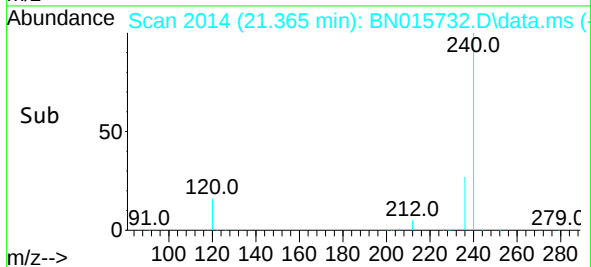
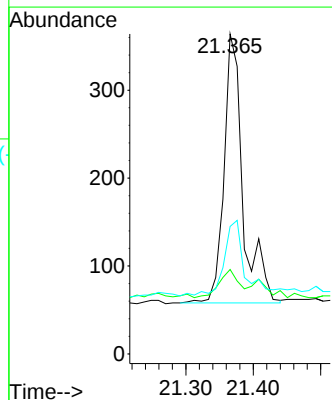
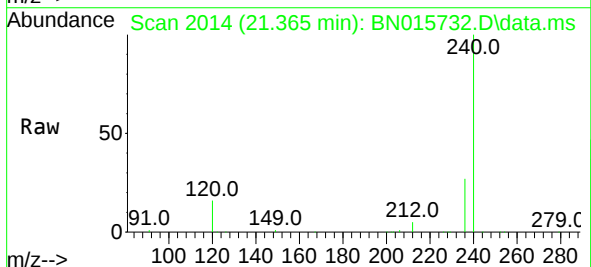


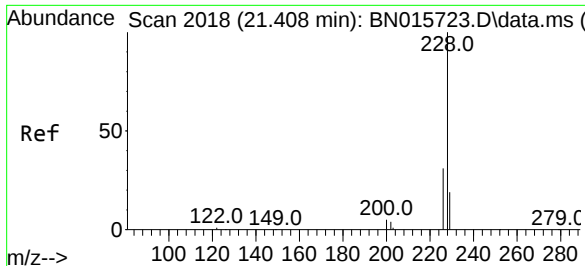

#33
Chrysene
Concen: 0.001 ng
RT: 21.365 min Scan# 2014
Delta R.T. -0.043 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50




Instrument :
BNA_N
ClientSampleId :
PB137923BL


Tgt Ion:228 Resp: 572
Ion Ratio Lower Upper
228 100
226 26.4 24.3 36.5
229 39.8 15.3 22.9#

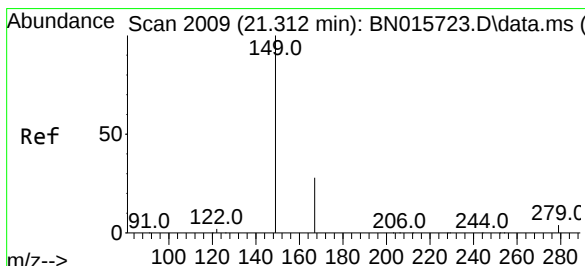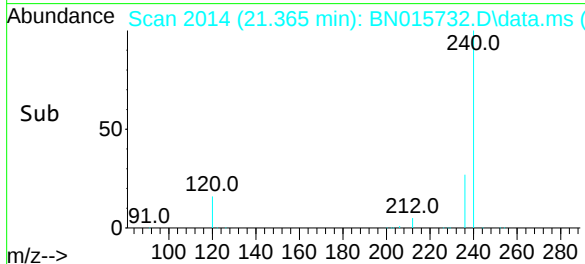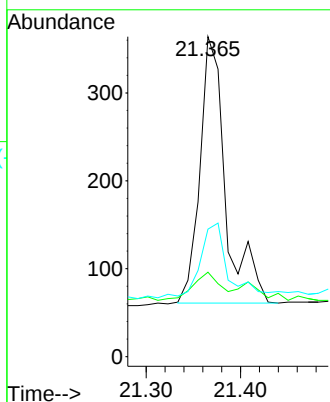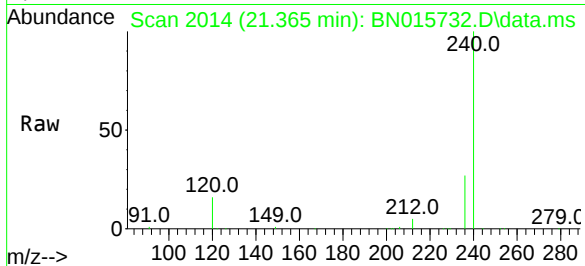

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.006 ng
RT: 21.302 min Scan# 2008
Delta R.T. -0.010 min
Lab File: BN015732.D
Acq: 31 Jul 2021 11:50


Tgt Ion:149 Resp: 1601
Ion Ratio Lower Upper
149 100
167 21.8 21.5 32.3
279 5.6 3.2 4.8#

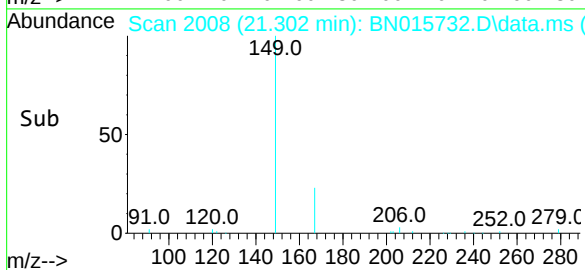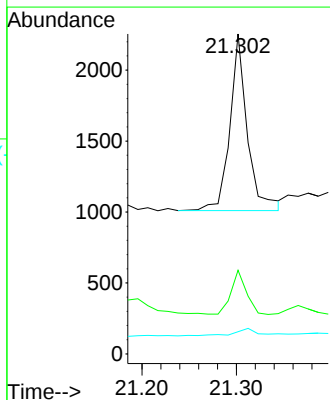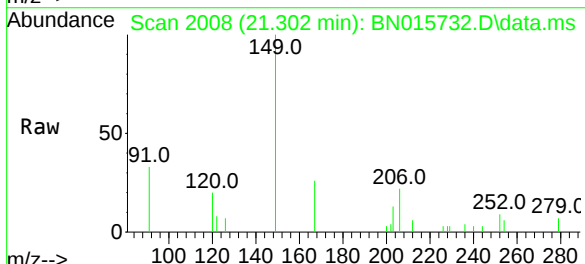






#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.714 min Scan# 2494
 Delta R.T. -0.006 min
 Lab File: BN015732.D
 Acq: 31 Jul 2021 11:50

Instrument :
 BNA_N
 ClientSampleId :
 PB137923BL







Tgt Ion:264 Resp: 165070
 Ion Ratio Lower Upper
 264 100
 260 24.6 19.4 29.2
 265 24.2 19.9 29.9



#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.000 ng
 RT: 26.110 min Scan# 3194
 Delta R.T. -0.017 min
 Lab File: BN015732.D
 Acq: 31 Jul 2021 11:50

Tgt Ion:276 Resp: 42
 Ion Ratio Lower Upper
 276 100
 138 0.0 20.6 30.8#
 277 31.0 20.1 30.1#

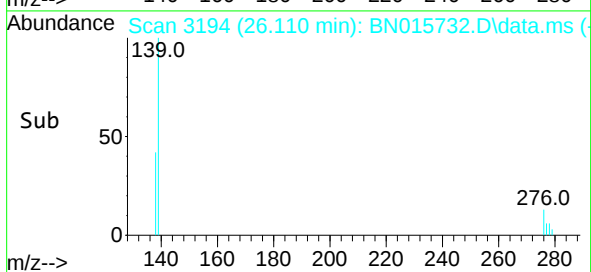



#37

Benzo(b)fluoranthene

Concen: 0.000 ng

RT: 23.009 min Scan# 2288

Delta R.T. -0.003 min

Lab File: BN015732.D

Acq: 31 Jul 2021 11:50





Tgt Ion:252	Resp:	100
Ion Ratio	Lower	Upper
252	100	
253	167.3	18.1 27.1#
125	138.9	8.3 12.5#

Instrument :

BNA_N

ClientSampleId :

PB137923BL

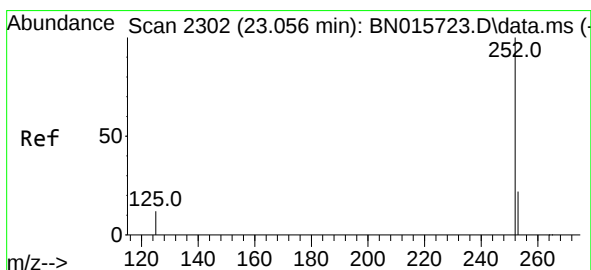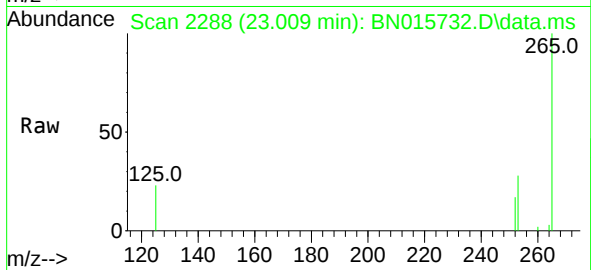

#38

Benzo(k)fluoranthene

Concen: 0.001 ng




RT: 23.043 min Scan# 2298


Delta R.T. -0.014 min

Lab File: BN015732.D

Acq: 31 Jul 2021 11:50

Tgt Ion:252	Resp:	588
Ion Ratio	Lower	Upper
252	100	
253	189.5	18.1 27.1#
125	663.4	10.4 15.6#

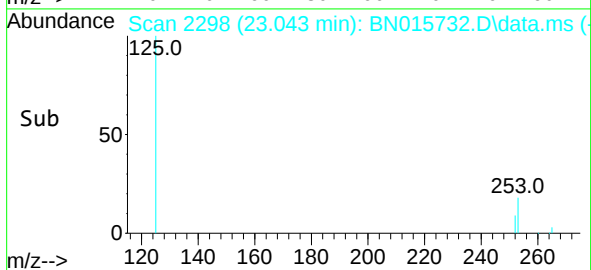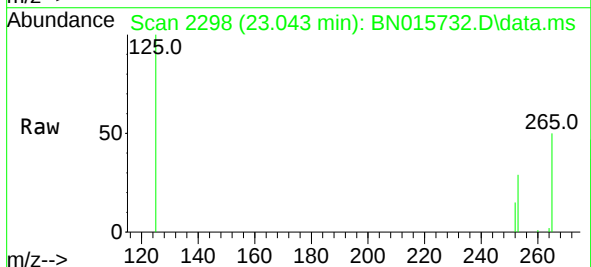



#39

Benzo(a)pyrene

Concen: 0.000 ng

RT: 23.611 min Scan# 2464

Delta R.T. -0.007 min

Lab File: BN015732.D

Acq: 31 Jul 2021 11:50





Tgt Ion:252	Resp:	21
Ion Ratio	Lower	Upper
252	100	
253	172.2	18.1 27.1#
125	140.6	9.2 13.8#

Instrument :

BNA_N

ClientSampleId :

PB137923BL



#40

Dibenzo(a,h)anthracene

Concen: 0.000 ng




RT: 26.141 min Scan# 3203


Delta R.T. -0.007 min

Lab File: BN015732.D

Acq: 31 Jul 2021 11:50

Tgt Ion:278	Resp:	120
Ion Ratio	Lower	Upper
278	100	
139	967.0	16.0 24.0#
279	246.6	19.2 28.8#

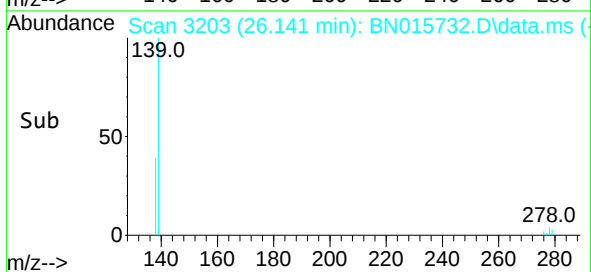

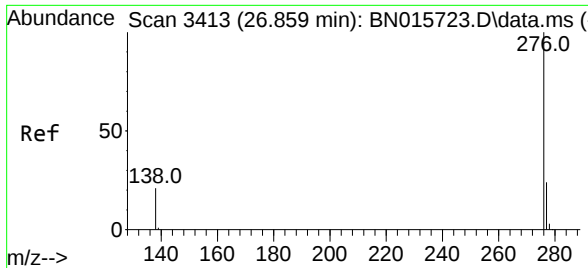

#41
 Benzo(g,h,i)perylene
 Concen: 0.000 ng
 RT: 26.842 min Scan# 3408
 Delta R.T. -0.017 min
 Lab File: BN015732.D
 Acq: 31 Jul 2021 11:50

Instrument :
 BNA_N
 ClientSampleId :
 PB137923BL

Tgt Ion:	276	Resp:	35
Ion Ratio	Lower	Upper	
276	100		
277	127.3	19.2	28.8#
138	185.7	16.8	25.2#

