

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073121\
 Data File : BN015750.D
 Acq On : 01 Aug 2021 01:23
 Operator : CG/JU
 Sample : PB137774BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB137774BL

Quant Time: Aug 02 04:31:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 02 04:24:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.790	152	40830	0.400	ng	0.00
7) Naphthalene-d8	10.571	136	177186	0.400	ng	0.00
13) Acenaphthene-d10	14.421	164	89301	0.400	ng	0.00
19) Phenanthrene-d10	17.164	188	167463	0.400	ng	0.00
29) Chrysene-d12	21.365	240	143178	0.400	ng	#-0.01
35) Perylene-d12	23.710	264	146298	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.383	112	36217	0.330	ng	0.00
5) Phenol-d6	6.951	99	41478	0.313	ng	0.00
8) Nitrobenzene-d5	8.936	82	37302	0.335	ng	0.00
11) 2-Methylnaphthalene-d10	12.163	152	107477	0.403	ng	0.00
14) 2,4,6-Tribromophenol	15.905	330	8396	0.218	ng	-0.01
15) 2-Fluorobiphenyl	13.038	172	135281	0.396	ng	-0.01
27) Fluoranthene-d10	19.207	212	181429	0.411	ng	0.00
31) Terphenyl-d14	19.812	244	155176	0.445	ng	0.00
Target Compounds						
						Qvalue
6) bis(2-Chloroethyl)ether	7.227	93	37	0.000	ng	# 58
9) Naphthalene	10.622	128	374	0.001	ng	# 47
10) Hexachlorobutadiene	10.926	225	10	0.000	ng	# 18
12) 2-Methylnaphthalene	12.234	142	163	0.001	ng	# 61
16) Acenaphthylene	14.129	152	78	0.000	ng	# 70
17) Acenaphthene	14.472	154	48	0.000	ng	# 70
18) Fluorene	15.474	166	63	0.000	ng	# 76
20) 4,6-Dinitro-2-methylph...	15.537	198	6	0.000	ng	# 1
21) 4-Bromophenyl-phenylether	16.360	248	16	0.000	ng	# 34
22) Hexachlorobenzene	16.482	284	18	0.000	ng	# 1
23) Atrazine	16.811	200	2612	0.035	ng	# 44
24) Pentachlorophenol	16.823	266	14347	0.354	ng	100
25) Phenanthrene	17.212	178	376	0.001	ng	# 81
26) Anthracene	17.297	178	156	0.000	ng	# 82
28) Fluoranthene	19.237	202	473	0.001	ng	# 88
30) Pyrene	19.599	202	467	0.001	ng	# 94
32) Benzo(a)anthracene	21.355	228	943	0.002	ng	# 86
33) Chrysene	21.408	228	641	0.001	ng	# 84
34) Bis(2-ethylhexyl)phtha...	21.302	149	1372	0.006	ng	# 95
36) Indeno(1,2,3-cd)pyrene	26.113	276	762	0.001	ng	# 71
37) Benzo(b)fluoranthene	22.998	252	737	0.002	ng	# 1
38) Benzo(k)fluoranthene	23.046	252	1173	0.002	ng	# 1
39) Benzo(a)pyrene	23.604	252	398	0.001	ng	# 1
40) Dibenzo(a,h)anthracene	26.127	278	663	0.001	ng	# 1
41) Benzo(g,h,i)perylene	26.839	276	646	0.001	ng	# 25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073121\
Data File : BN015750.D
Acq On : 01 Aug 2021 01:23
Operator : CG/JU
Sample : PB137774BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB137774BL

Quant Time: Aug 02 04:31:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 02 04:24:05 2021
Response via : Initial Calibration




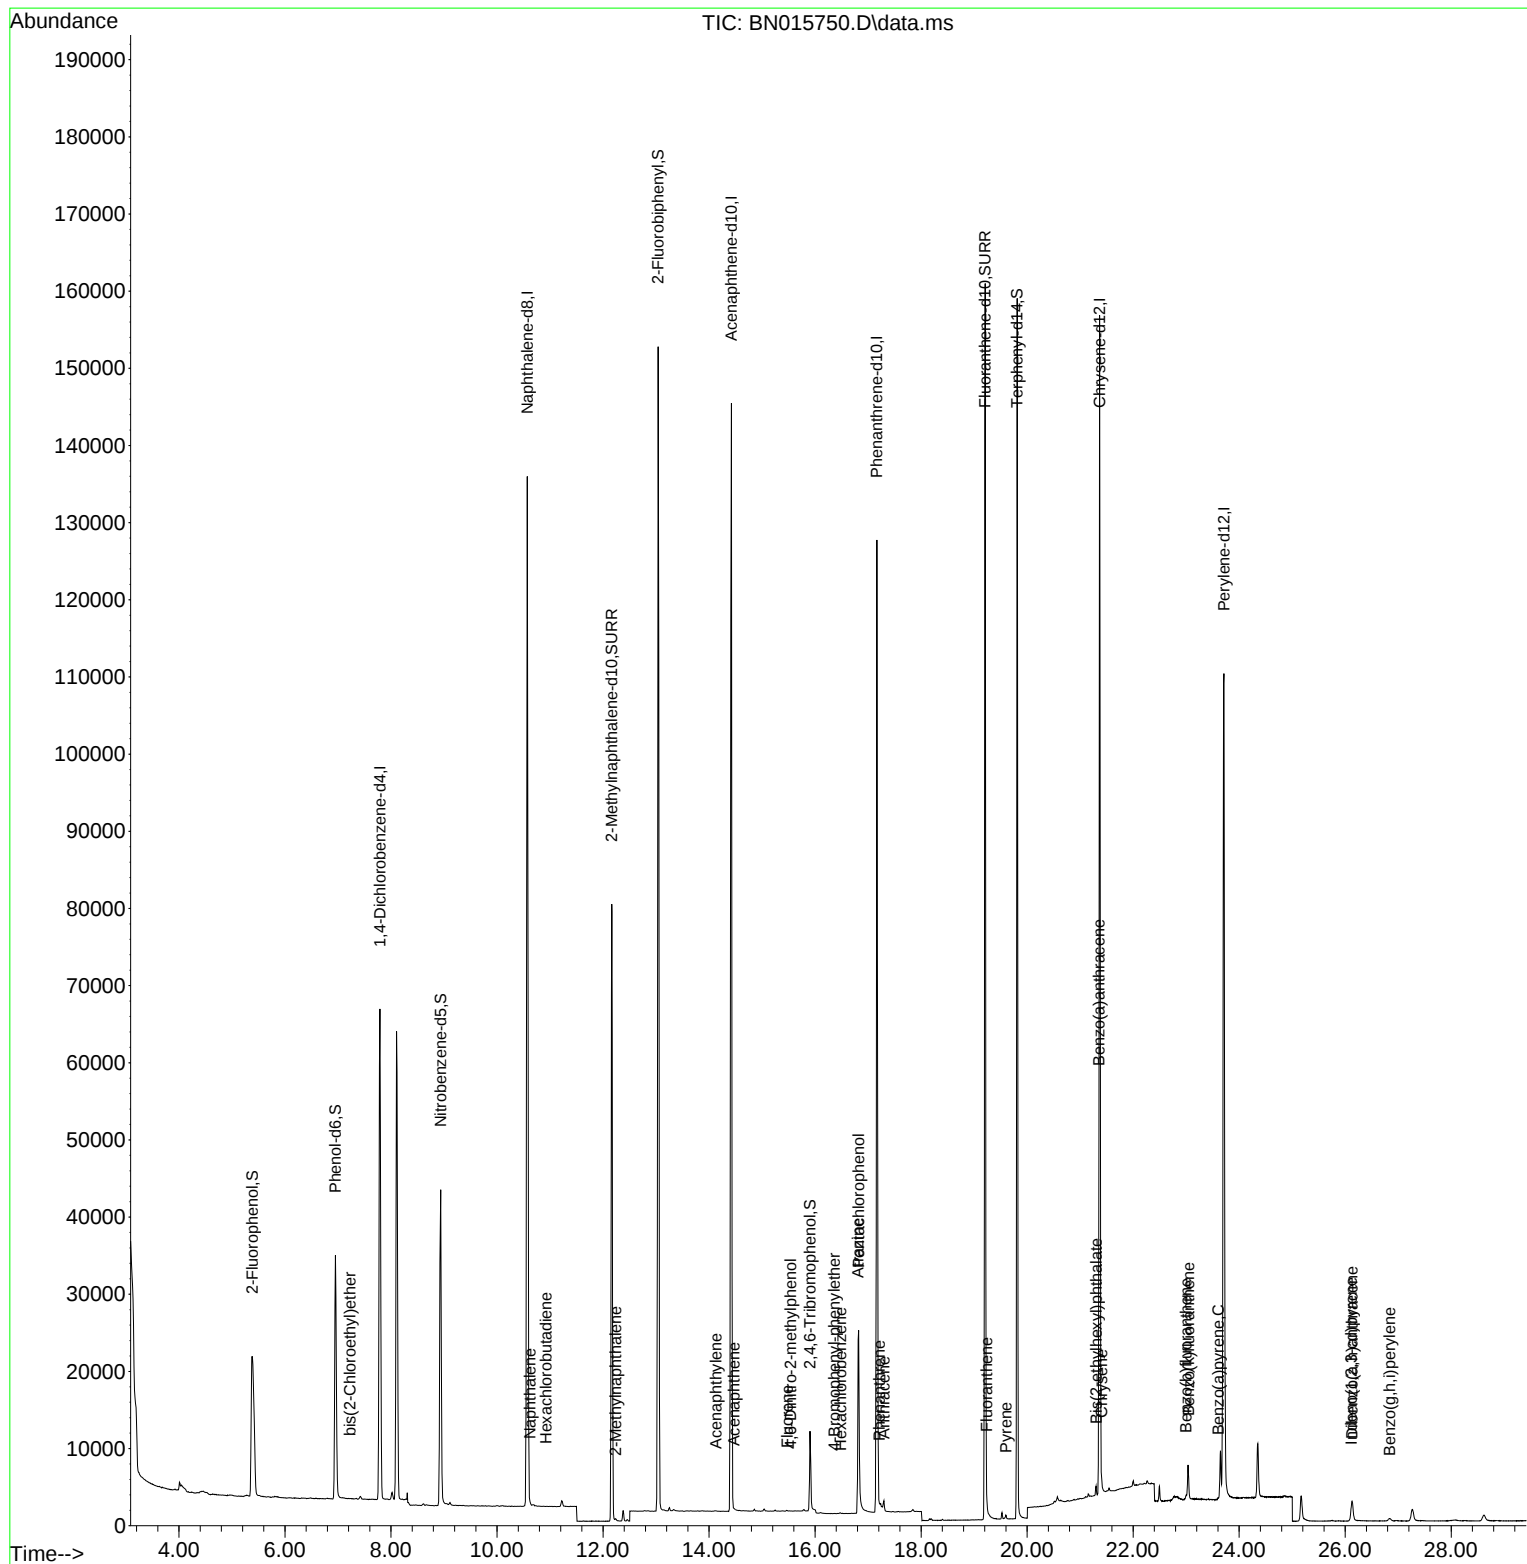




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.790 min Scan# 511
Delta R.T. -0.000 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:152 Resp: 40830
Ion Ratio Lower Upper
152 100
150 153.8 123.9 185.9
115 58.6 47.8 71.6



#4
2-Fluorophenol
Concen: 0.330 ng
RT: 5.383 min Scan# 250
Delta R.T. 0.000 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:112 Resp: 36217
Ion Ratio Lower Upper
112 100
64 52.4 42.1 63.1
63 27.6 21.9 32.9



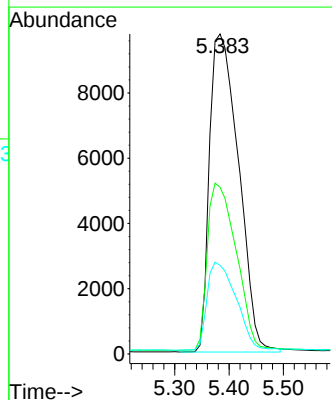





#5
Phenol-d6
Concen: 0.313 ng
RT: 6.951 min Scan# 420
Delta R.T. 0.000 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:	99	Resp:	41478
Ion	Ratio	Lower	Upper
99	100		
42	15.5	12.9	19.3
71	29.6	23.8	35.6

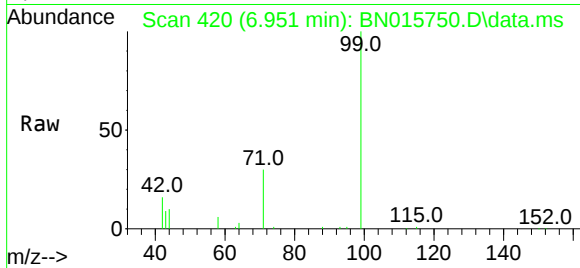

#6
bis(2-Chloroethyl)ether
Concen: 0.000 ng
RT: 7.227 min Scan# 450
Delta R.T. 0.009 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:	93	Resp:	37
Ion	Ratio	Lower	Upper
93	100		
63	105.4	58.6	87.8#
95	62.2	26.9	40.3#



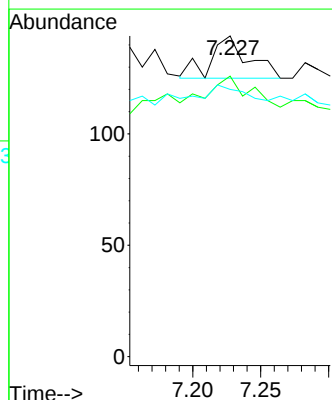
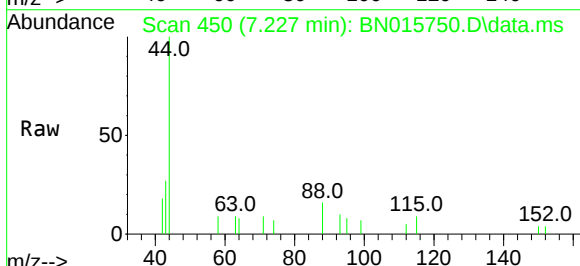




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.571 min Scan# 746
Delta R.T. 0.000 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:	136	Resp:	177186
Ion Ratio	Lower	Upper	
136	100		
137	10.9	8.7	13.1
54	5.9	5.5	8.3
68	4.7	4.5	6.7

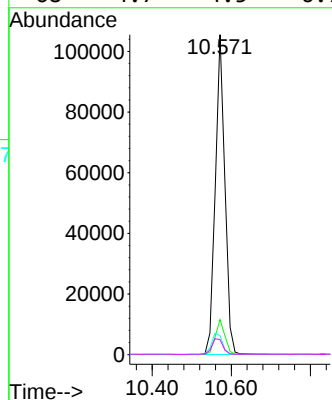

#8
Nitrobenzene-d5
Concen: 0.335 ng
RT: 8.936 min Scan# 617
Delta R.T. 0.000 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:	82	Resp:	37302
Ion Ratio	Lower	Upper	
82	100		
128	42.7	33.2	49.8
54	47.1	38.4	57.6



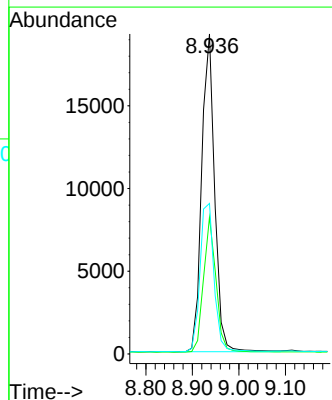





#9
Naphthalene
Concen: 0.001 ng
RT: 10.622 min Scan# 750
Delta R.T. 0.000 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:128 Resp: 374
Ion Ratio Lower Upper
128 100
129 35.5 8.9 13.3#
127 30.5 10.4 15.6#



#10
Hexachlorobutadiene
Concen: 0.000 ng
RT: 10.926 min Scan# 774
Delta R.T. 0.013 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:225 Resp: 10
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 0.0 51.0 76.4#







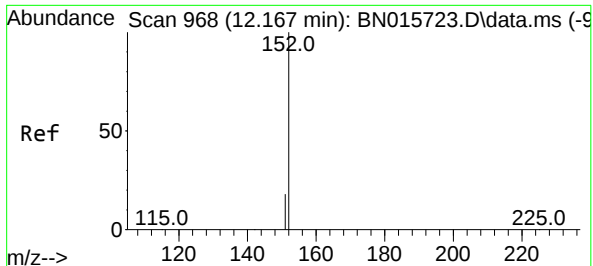

#11
2-Methylnaphthalene-d10
Concen: 0.403 ng
RT: 12.163 min Scan# 967
Delta R.T. -0.004 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:152 Resp: 107477
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.4

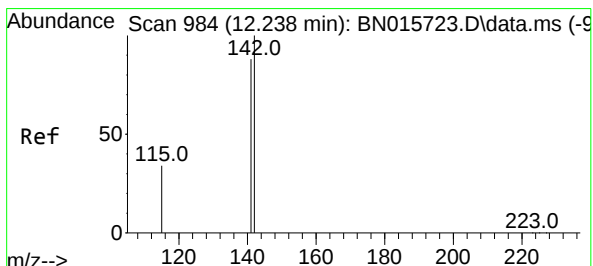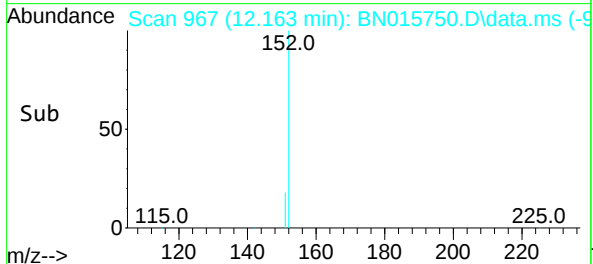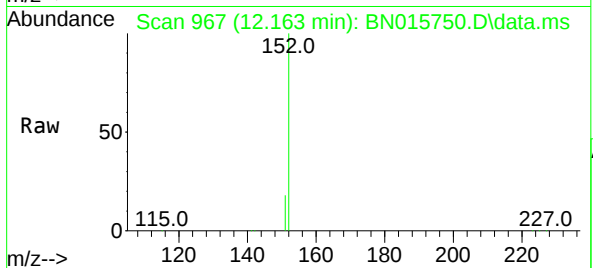

#12
2-Methylnaphthalene
Concen: 0.001 ng
RT: 12.234 min Scan# 983
Delta R.T. -0.004 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:142 Resp: 163
Ion Ratio Lower Upper
142 100
141 96.4 70.5 105.7
115 101.2 27.3 40.9#


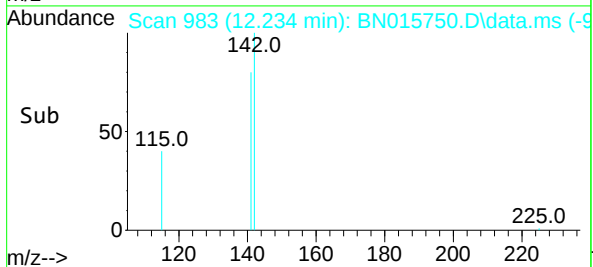

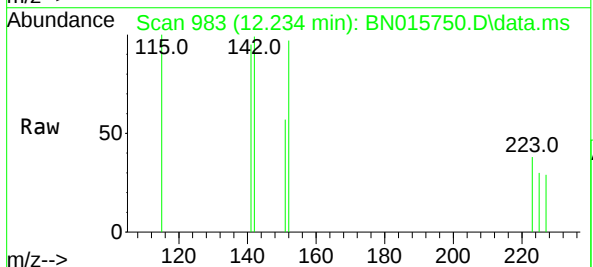




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.421 min Scan# 1195
Delta R.T. -0.000 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:164 Resp: 89301
Ion Ratio Lower Upper
164 100
162 99.2 79.8 119.6
160 44.4 35.8 53.6



#14
2,4,6-Tribromophenol
Concen: 0.218 ng
RT: 15.905 min Scan# 1312
Delta R.T. -0.013 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:330 Resp: 8396
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 34.9 28.8 43.2







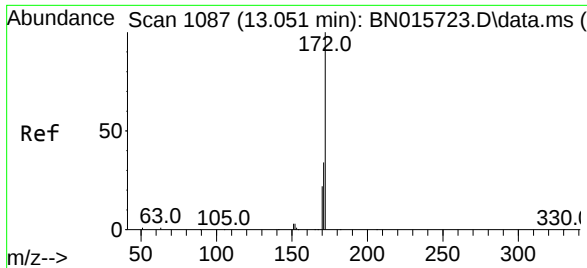

#15
2-Fluorobiphenyl
Concen: 0.396 ng
RT: 13.038 min Scan# 1086
Delta R.T. -0.013 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:172 Resp: 135281
Ion Ratio Lower Upper
172 100
171 35.4 26.9 40.3
170 24.2 17.4 26.0

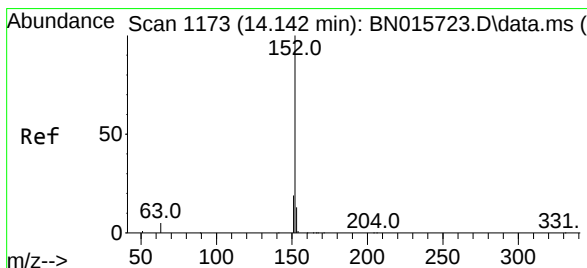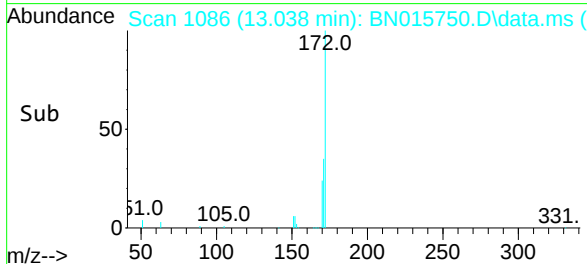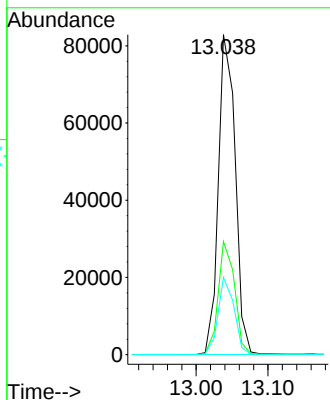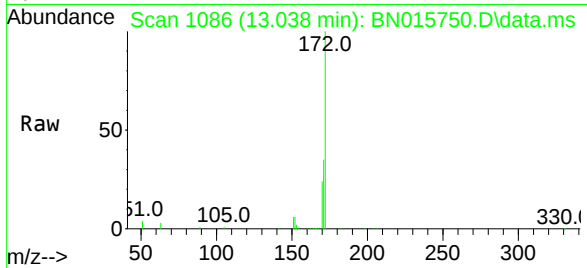

#16
Acenaphthylene
Concen: 0.000 ng
RT: 14.129 min Scan# 1172
Delta R.T. -0.013 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:152 Resp: 78
Ion Ratio Lower Upper
152 100
151 38.5 15.7 23.5#
153 17.9 10.4 15.6#


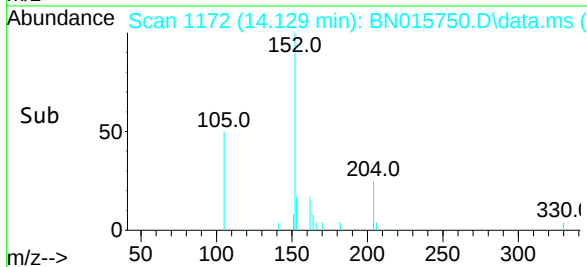
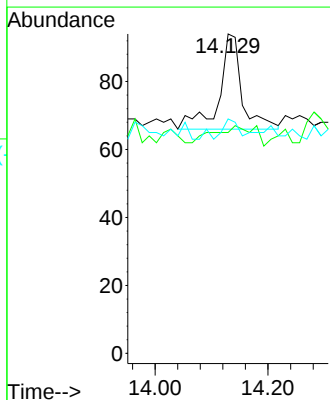
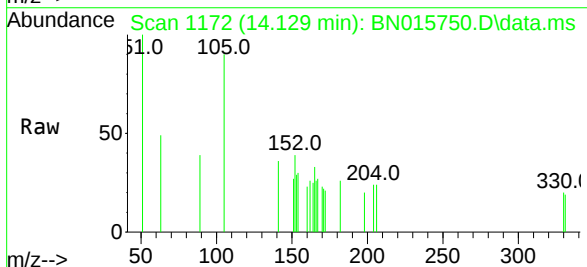


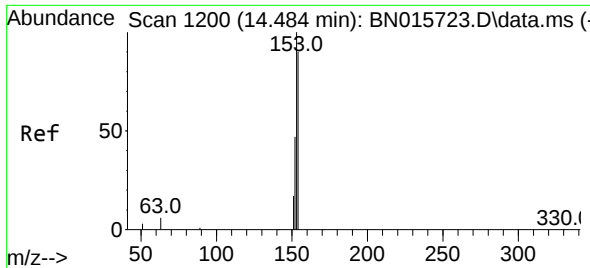

#17
Acenaphthene
Concen: 0.000 ng
RT: 14.472 min Scan# 1199
Delta R.T. -0.012 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:154 Resp: 48
Ion Ratio Lower Upper
154 100
153 77.1 89.7 134.5#
152 37.5 43.8 65.6#

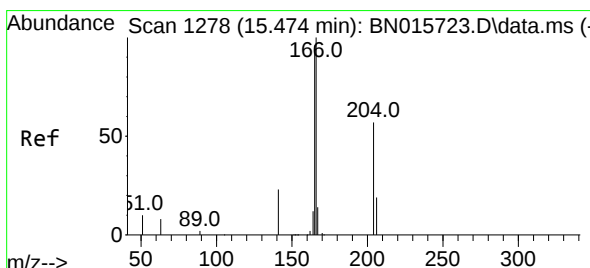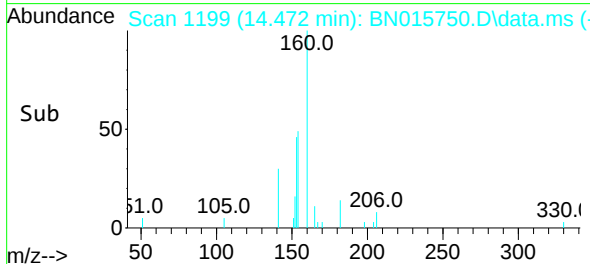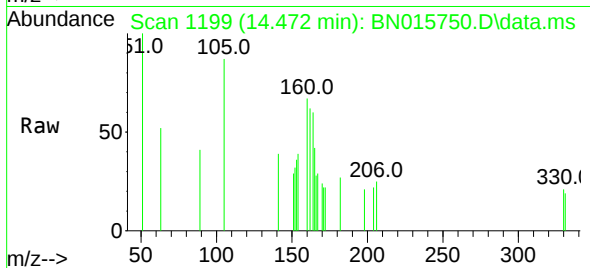

#18
Fluorene
Concen: 0.000 ng
RT: 15.474 min Scan# 1278
Delta R.T. 0.000 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:166 Resp: 63
Ion Ratio Lower Upper
166 100
165 122.2 78.1 117.1#
167 20.6 10.8 16.2#


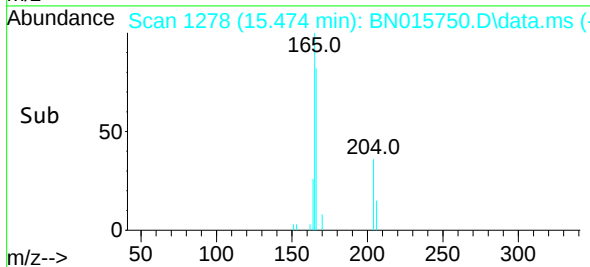

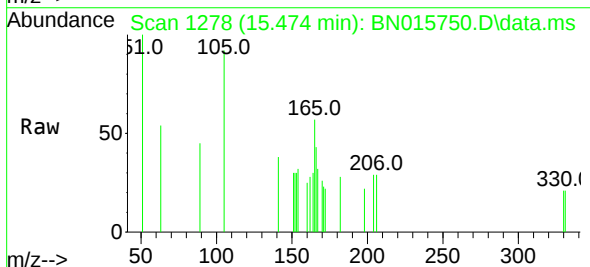




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.164 min Scan# 1415
Delta R.T. 0.001 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:188 Resp: 167463
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.3 10.2 15.4

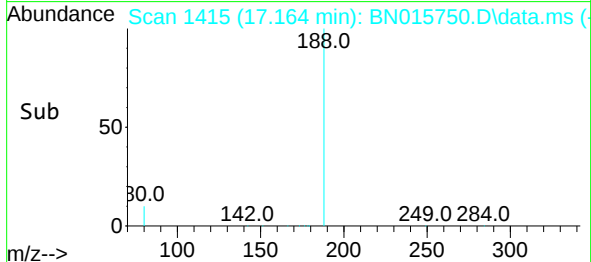

#20
4,6-Dinitro-2-methylphenol
Concen: 0.000 ng
RT: 15.537 min Scan# 1283
Delta R.T. -0.013 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:198 Resp: 6
Ion Ratio Lower Upper
198 100
182 125.5 9.4 14.0#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.000 ng
RT: 16.360 min Scan# 1349
Delta R.T. -0.012 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:248 Resp: 16
Ion Ratio Lower Upper
248 100
250 115.1 83.9 125.9
141 171.7 26.9 40.3#



#22
Hexachlorobenzene
Concen: 0.000 ng
RT: 16.482 min Scan# 1359
Delta R.T. 0.000 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:284 Resp: 18
Ion Ratio Lower Upper
284 100
142 144.4 29.4 44.0#
249 94.4 23.8 35.6#

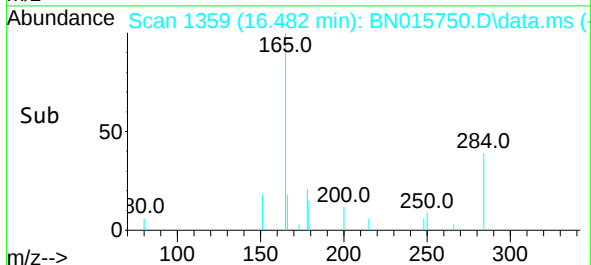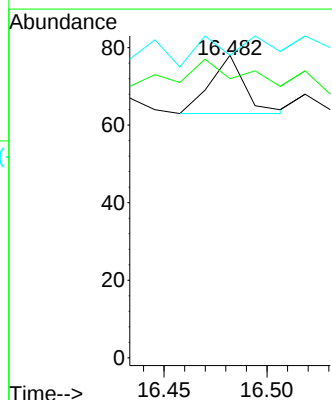

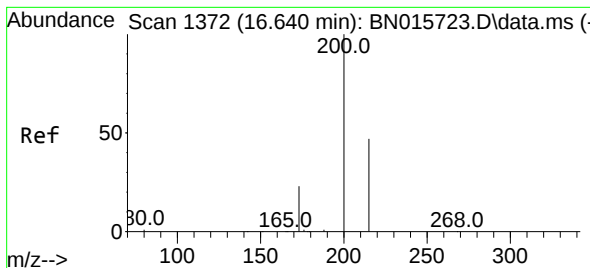

#23

Atrazine

Concen: 0.035 ng

RT: 16.811 min Scan# 1386

Delta R.T. 0.171 min

Lab File: BN015750.D

Acq: 01 Aug 2021 01:23

Tgt Ion:200 Resp: 2612

Ion Ratio Lower Upper

200 100

173 4.3 18.9 28.3#





215 4.4 38.1 57.1#

Instrument :

BNA_N

ClientSampleId :

PB137774BL

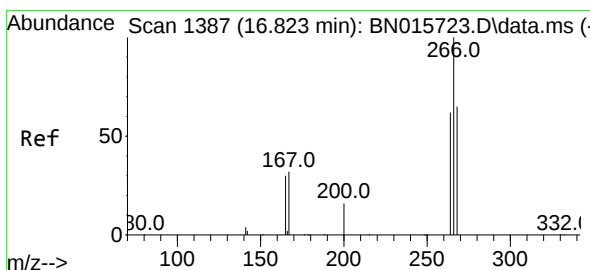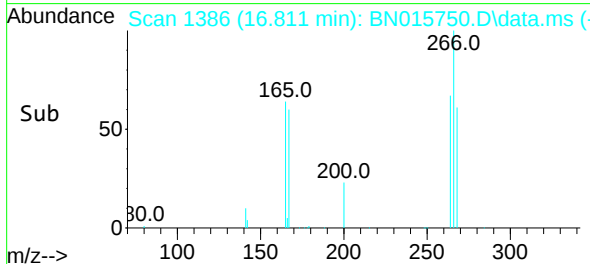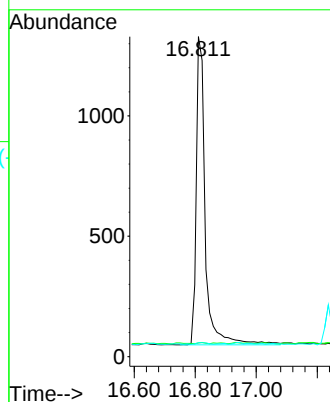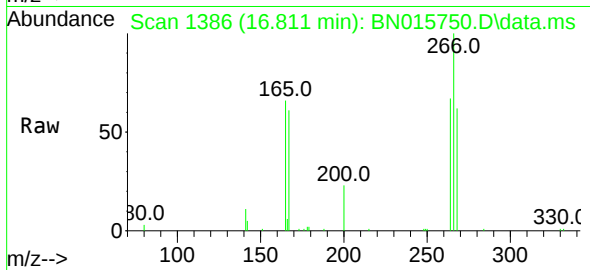

#24

Pentachlorophenol

Concen: 0.354 ng

RT: 16.823 min Scan# 1387

Delta R.T. -0.000 min

Lab File: BN015750.D

Acq: 01 Aug 2021 01:23




Tgt Ion:266 Resp: 14347


Ion Ratio Lower Upper

266 100

264 62.2 50.2 75.2

268 64.1 51.1 76.7


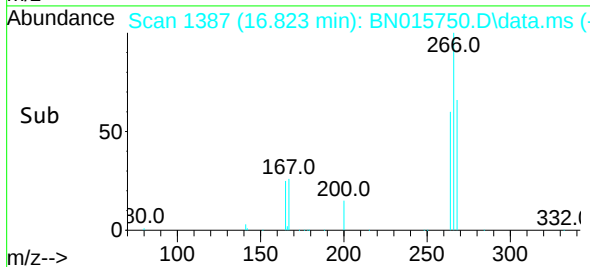
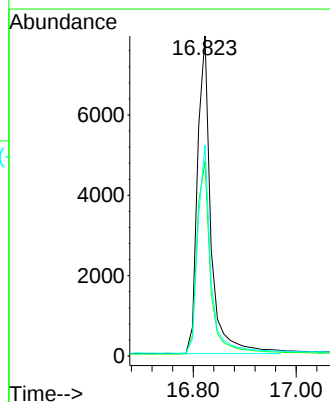
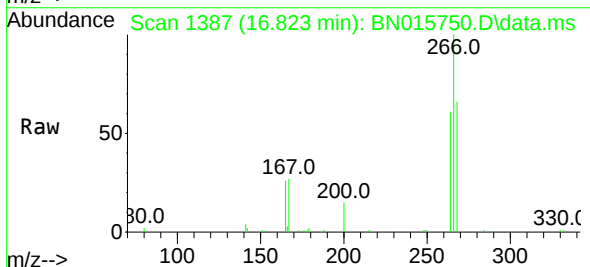




#25
Phenanthrene
Concen: 0.001 ng
RT: 17.212 min Scan# 1419
Delta R.T. 0.000 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:178 Resp: 376
Ion Ratio Lower Upper
178 100
176 17.3 15.3 22.9
179 0.0 12.4 18.6#



#26
Anthracene
Concen: 0.000 ng
RT: 17.297 min Scan# 1426
Delta R.T. 0.000 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:178 Resp: 156
Ion Ratio Lower Upper
178 100
176 26.9 14.6 22.0#
179 21.8 12.2 18.4#







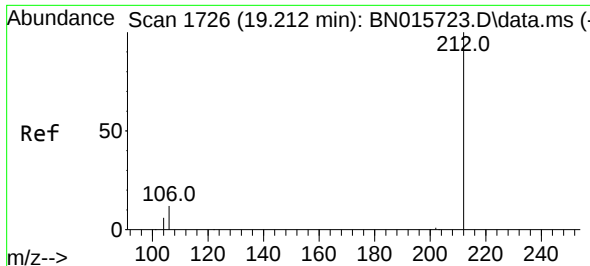

#27
Fluoranthene-d10
Concen: 0.411 ng
RT: 19.207 min Scan# 1725
Delta R.T. -0.005 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:212 Resp: 181429
Ion Ratio Lower Upper
212 100
106 13.4 10.6 16.0
104 7.3 5.9 8.9

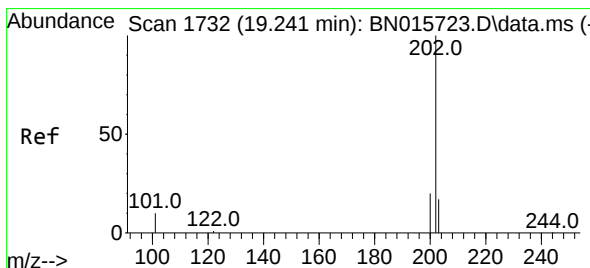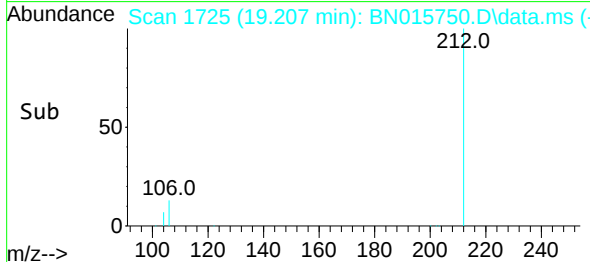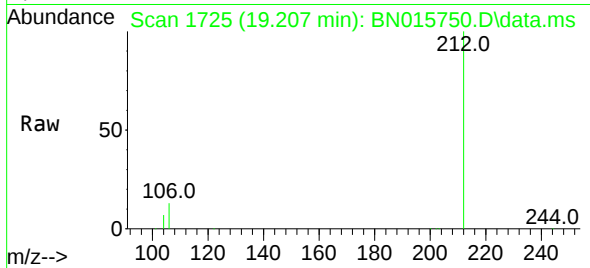

#28
Fluoranthene
Concen: 0.001 ng
RT: 19.237 min Scan# 1731
Delta R.T. -0.005 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:202 Resp: 473
Ion Ratio Lower Upper
202 100
101 0.0 9.0 13.6#
203 16.9 13.8 20.8


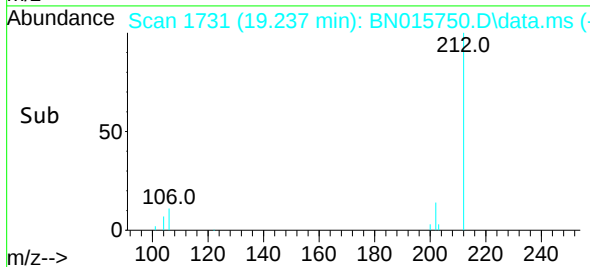

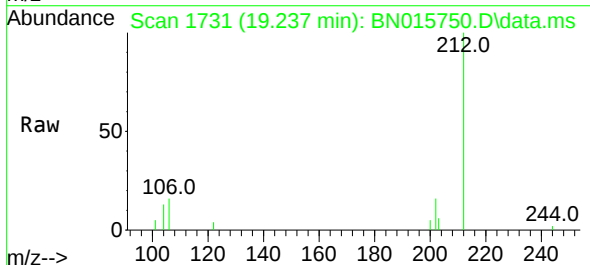




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.365 min Scan# 2014
Delta R.T. -0.011 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:240 Resp: 143178
Ion Ratio Lower Upper
240 100
120 12.1 7.4 11.0#
236 26.4 20.9 31.3

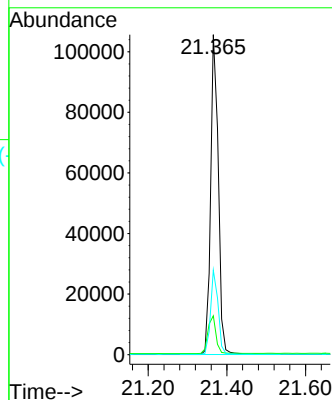

#30
Pyrene
Concen: 0.001 ng
RT: 19.599 min Scan# 1804
Delta R.T. -0.005 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:202 Resp: 467
Ion Ratio Lower Upper
202 100
200 23.8 16.5 24.7
203 19.5 14.0 21.0



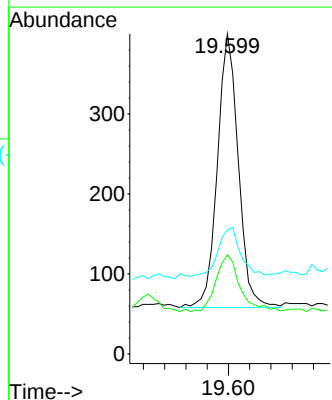



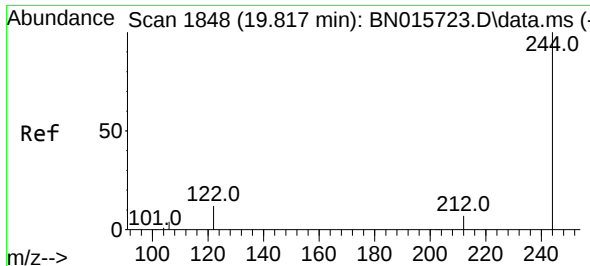

#31
Terphenyl-d14
Concen: 0.445 ng
RT: 19.812 min Scan# 1847
Delta R.T. -0.005 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:244 Resp: 155176
Ion Ratio Lower Upper
244 100
212 7.3 5.9 8.9
122 11.7 9.6 14.4

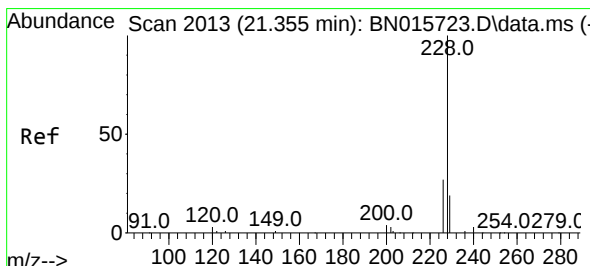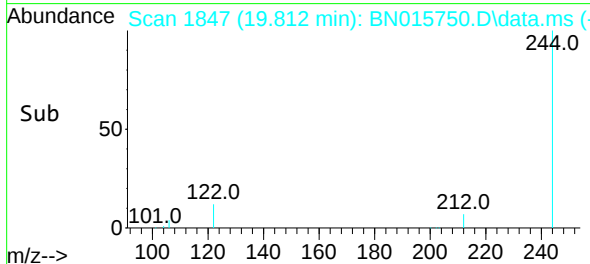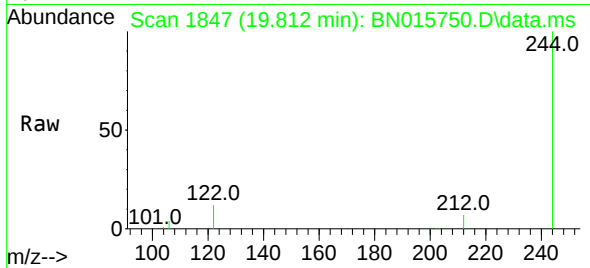

#32
Benzo(a)anthracene
Concen: 0.002 ng
RT: 21.355 min Scan# 2013
Delta R.T. -0.000 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:228 Resp: 943
Ion Ratio Lower Upper
228 100
226 31.1 21.9 32.9
229 29.5 15.4 23.0#


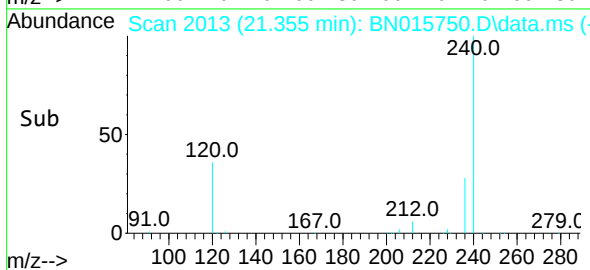
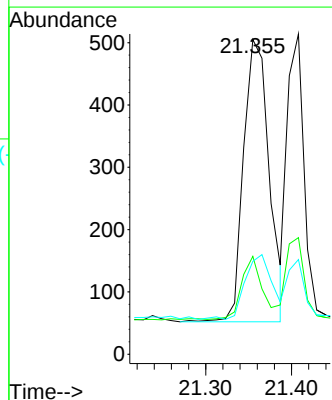
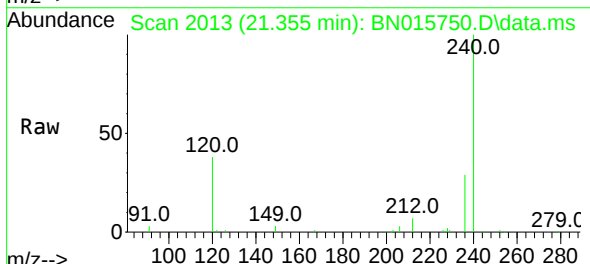


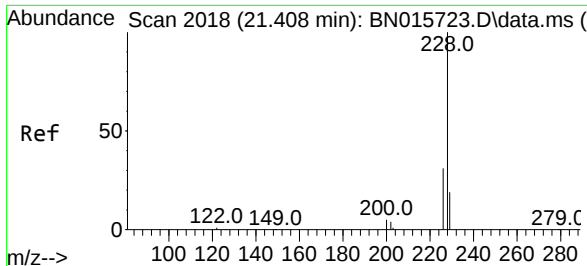

#33
Chrysene
Concen: 0.001 ng
RT: 21.408 min Scan# 2018
Delta R.T. -0.000 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:228 Resp: 641
Ion Ratio Lower Upper
228 100
226 36.4 24.3 36.5
229 29.6 15.3 22.9#

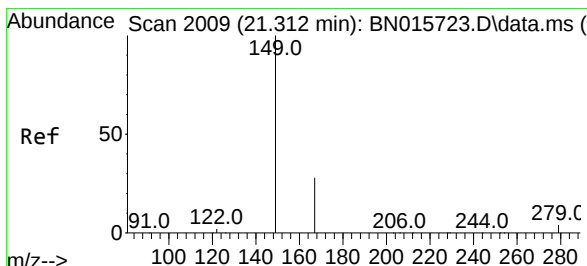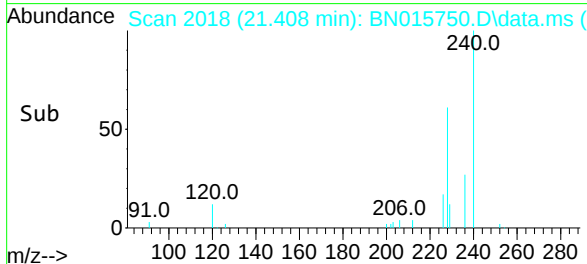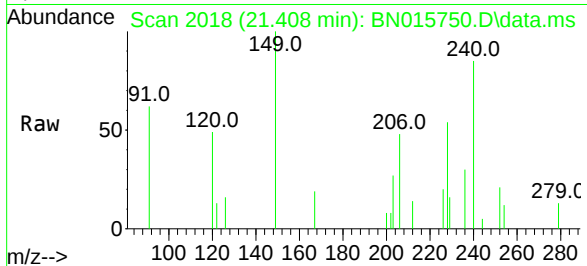

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.006 ng
RT: 21.302 min Scan# 2008
Delta R.T. -0.010 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:149 Resp: 1372
Ion Ratio Lower Upper
149 100
167 24.9 21.5 32.3
279 8.5 3.2 4.8#

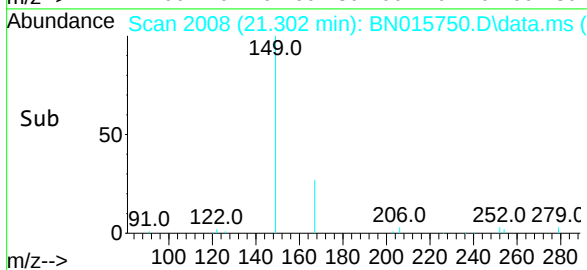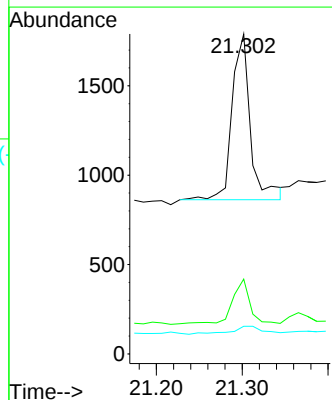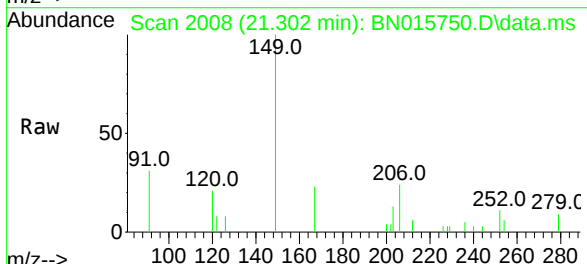



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.710 min Scan# 2493

Delta R.T. -0.010 min

Lab File: BN015750.D

Acq: 01 Aug 2021 01:23





Tgt Ion:264 Resp: 146298

Ion Ratio Lower Upper

264 100

260 24.3 19.4 29.2

265 23.5 19.9 29.9



#36

Indeno(1,2,3-cd)pyrene

Concen: 0.001 ng

RT: 26.113 min Scan# 3195

Delta R.T. -0.014 min

Lab File: BN015750.D

Acq: 01 Aug 2021 01:23




Tgt Ion:276 Resp: 762


Ion Ratio Lower Upper

276 100

138 0.0 20.6 30.8#

277 28.9 20.1 30.1





#37

Benzo(b)fluoranthene

Concen: 0.002 ng

RT: 22.998 min Scan# 2285

Delta R.T. -0.014 min

Lab File: BN015750.D

Acq: 01 Aug 2021 01:23





Tgt Ion:252	Resp:	737
Ion Ratio	Lower	Upper
252	100	
253	90.1	18.1 27.1#
125	68.5	8.3 12.5#

Instrument :

BNA_N

ClientSampleId :

PB137774BL

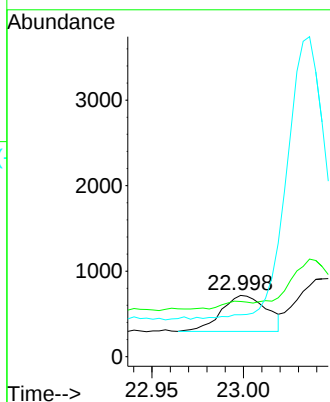

#38

Benzo(k)fluoranthene

Concen: 0.002 ng




RT: 23.046 min Scan# 2299


Delta R.T. -0.010 min

Lab File: BN015750.D

Acq: 01 Aug 2021 01:23

Tgt Ion:252	Resp:	1173
Ion Ratio	Lower	Upper
252	100	
253	105.3	18.1 27.1#
125	224.9	10.4 15.6#




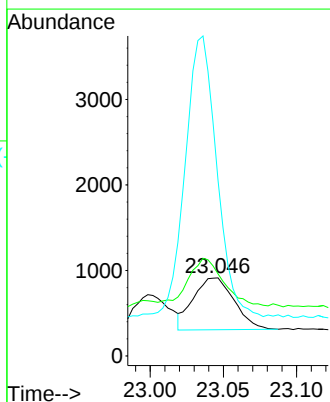




#39
Benzo(a)pyrene
Concen: 0.001 ng
RT: 23.604 min Scan# 2462
Delta R.T. -0.014 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23




Instrument :
BNA_N
ClientSampleId :
PB137774BL


Tgt Ion:252 Resp: 398
Ion Ratio Lower Upper
252 100
253 119.0 18.1 27.1#
125 89.1 9.2 13.8#



#40
Dibenzo(a,h)anthracene
Concen: 0.001 ng
RT: 26.127 min Scan# 3199
Delta R.T. -0.020 min
Lab File: BN015750.D
Acq: 01 Aug 2021 01:23

Tgt Ion:278 Resp: 663
Ion Ratio Lower Upper
278 100
139 554.3 16.0 24.0#
279 101.8 19.2 28.8#

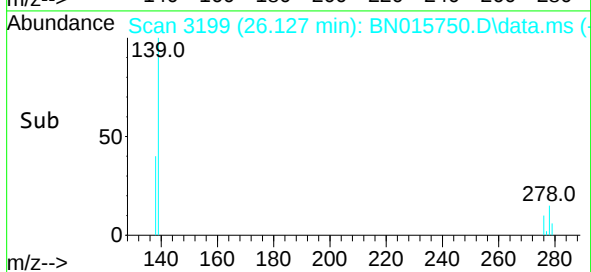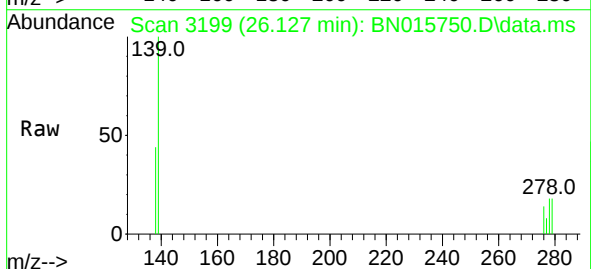

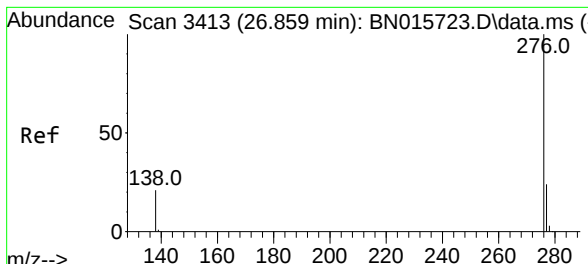

#41
 Benzo(g,h,i)perylene
 Concen: 0.001 ng
 RT: 26.839 min Scan# 3407
 Delta R.T. -0.020 min
 Lab File: BN015750.D
 Acq: 01 Aug 2021 01:23

Instrument :
 BNA_N
 ClientSampleId :
 PB137774BL

Tgt Ion: 276 Resp: 646

Ion	Ratio	Lower	Upper
276	100		
277	56.1	19.2	28.8#
138	61.8	16.8	25.2#

