

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073121\
 Data File : BN015752.D
 Acq On : 01 Aug 2021 02:36
 Operator : CG/JU
 Sample : M2940-07
 Misc : LOD-MDL-WTR-0.2ng
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2021

Manual Integrations
 APPROVED

mohammad
 8/2/2021 3:49:28 PM

Quant Time: Aug 02 04:31:55 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 02 04:24:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.790	152	38331	0.400	ng	0.00
7) Naphthalene-d8	10.572	136	172930	0.400	ng	0.00
13) Acenaphthene-d10	14.421	164	91988	0.400	ng	0.00
19) Phenanthrene-d10	17.164	188	172546	0.400	ng	# 0.00
29) Chrysene-d12	21.366	240	159552	0.400	ng	#-0.01
35) Perylene-d12	23.707	264	158878	0.400	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.383	112	34697	0.337	ng	0.00
5) Phenol-d6	6.951	99	40234	0.323	ng	0.00
8) Nitrobenzene-d5	8.937	82	31975	0.294	ng	0.00
11) 2-Methylnaphthalene-d10	12.163	152	108962	0.418	ng	0.00
14) 2,4,6-Tribromophenol	15.906	330	10074	0.253	ng	-0.01
15) 2-Fluorobiphenyl	13.038	172	112494	0.320	ng	-0.01
27) Fluoranthene-d10	19.207	212	180665	0.397	ng	0.00
31) Terphenyl-d14	19.813	244	121753	0.314	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.355	88	2576m	0.196	ng	
3) n-Nitrosodimethylamine	3.724	42	4314	0.169	ng	# 99
6) bis(2-Chloroethyl)ether	7.218	93	22303	0.219	ng	100
9) Naphthalene	10.622	128	92208	0.205	ng	100
10) Hexachlorobutadiene	10.914	225	15995	0.202	ng	# 100
12) 2-Methylnaphthalene	12.234	142	60407	0.206	ng	99
16) Acenaphthylene	14.129	152	67225	0.166	ng	100
17) Acenaphthene	14.485	154	49598	0.188	ng	99
18) Fluorene	15.461	166	59532	0.186	ng	100
20) 4,6-Dinitro-2-methylph...	15.550	198	1022	0.077	ng	# 79
21) 4-Bromophenyl-phenylether	16.361	248	18588	0.185	ng	# 73
22) Hexachlorobenzene	16.482	284	21982	0.197	ng	100
23) Atrazine	16.628	200	13518	0.176	ng	# 92
24) Pentachlorophenol	16.823	266	9470	0.227	ng	100
25) Phenanthrene	17.212	178	96420	0.195	ng	100
26) Anthracene	17.298	178	78858	0.177	ng	100
28) Fluoranthene	19.237	202	100766	0.191	ng	100
30) Pyrene	19.599	202	98568	0.185	ng	100
32) Benzo(a)anthracene	21.355	228	87963	0.173	ng	98
33) Chrysene	21.408	228	98305	0.190	ng	97
34) Bis(2-ethylhexyl)phtha...	21.302	149	29060	0.108	ng	99
36) Indeno(1,2,3-cd)pyrene	26.107	276	107467	0.188	ng	99
37) Benzo(b)fluoranthene	22.999	252	99115	0.194	ng	100
38) Benzo(k)fluoranthene	23.046	252	109394	0.199	ng	99
39) Benzo(a)pyrene	23.604	252	85426	0.183	ng	99
40) Dibenzo(a,h)anthracene	26.127	278	90913	0.188	ng	98
41) Benzo(g,h,i)perylene	26.842	276	91793	0.184	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073121\
 Data File : BN015752.D
 Acq On : 01 Aug 2021 02:36
 Operator : CG/JU
 Sample : M2940-07
 Misc : LOD-MDL-WTR-0.2ng
 ALS Vial : 21 Sample Multiplier: 1


Instrument :
 BNA_N
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2021

Manual Integrations
 APPROVED

mohammad
 8/2/2021 3:49:28 PM


Quant Time: Aug 02 04:31:55 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 02 04:24:05 2021
 Response via : Initial Calibration

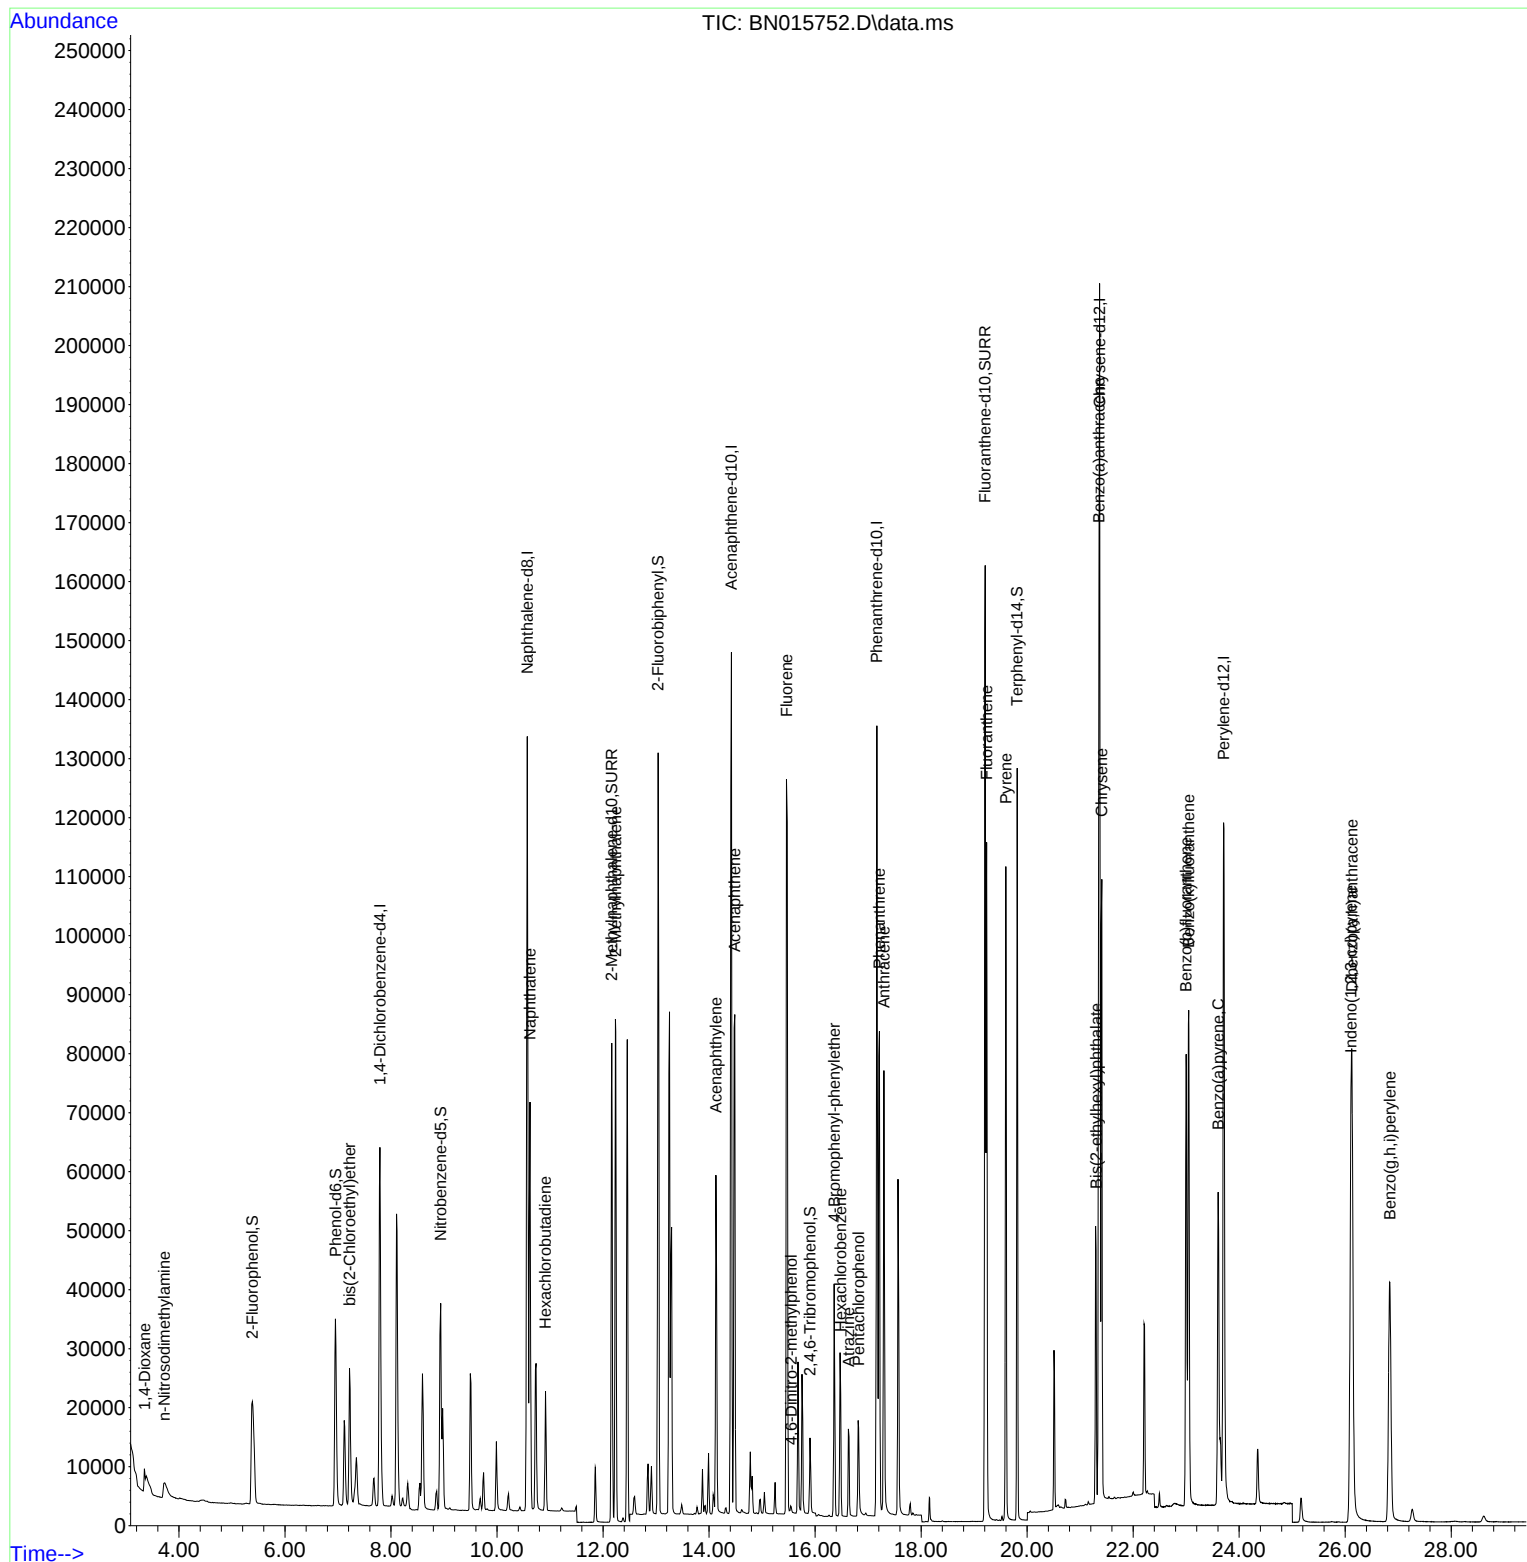



#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.790 min Scan# 511
 Delta R.T. 0.000 min
 Lab File: BN01572.D
 Acq: 01 Aug 2021 02:36




Instrument :
 BNA_N
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2021




Tgt Ion:152 Resp: 38331
 Ion Ratio Lower Upper
 152 100
 150 155.3 123.9 185.9
 115 58.9 47.8 71.6

Manual Integrations
 APPROVED



mohammad
 8/2/2021 3:49:28 PM

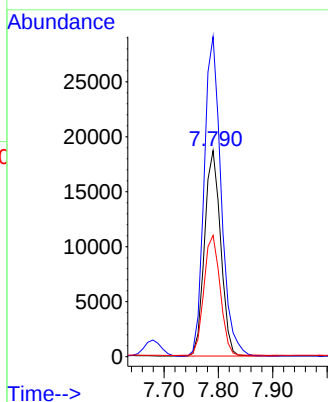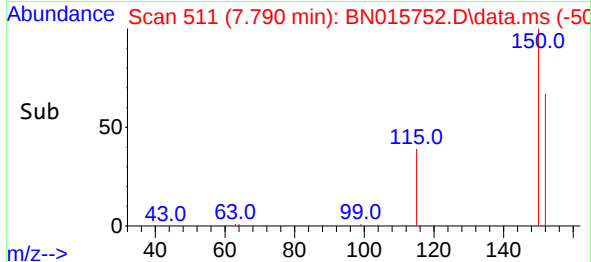


#2
 1,4-Dioxane
 Concen: 0.196 ng m
 RT: 3.355 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: BN015752.D
 Acq: 01 Aug 2021 02:36



Tgt Ion: 88 Resp: 2576
 Ion Ratio Lower Upper
 88 100
 43 28.1 17.2 25.8#
 58 78.1 62.2 93.2

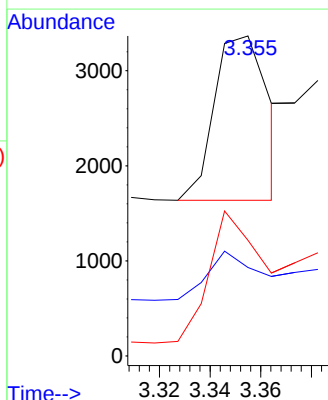







#3
n-Nitrosodimethylamine
Concen: 0.169 ng
RT: 3.724 min Scan# 70
Delta R.T. 0.010 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

Tgt Ion: 42 Resp: 4314
Ion Ratio Lower Upper
42 100
74 146.5 116.6 174.8
44 6.0 6.6 10.0#

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:28 PM



#4
2-Fluorophenol
Concen: 0.337 ng
RT: 5.383 min Scan# 250
Delta R.T. 0.000 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

Tgt Ion: 112 Resp: 34697
Ion Ratio Lower Upper
112 100
64 52.1 42.1 63.1
63 27.4 21.9 32.9

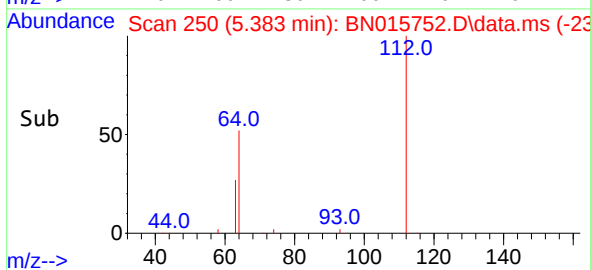







#5
Phenol-d6
Concen: 0.323 ng
RT: 6.951 min Scan# 420
Delta R.T. 0.000 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

Tgt Ion:	99	Resp:	40234
Ion	Ratio	Lower	Upper
99	100		
42	15.8	12.9	19.3
71	29.6	23.8	35.6

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:28 PM



#6
bis(2-Chloroethyl)ether
Concen: 0.219 ng
RT: 7.218 min Scan# 449
Delta R.T. 0.000 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36


Tgt Ion:	93	Resp:	22303
Ion	Ratio	Lower	Upper
93	100		
63	72.9	58.6	87.8
95	33.3	26.9	40.3

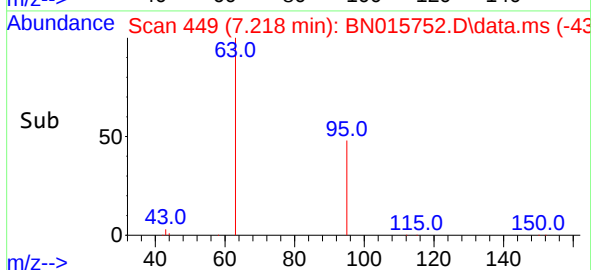



#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.572 min Scan# 746
Delta R.T. 0.000 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021



Tgt Ion:	136	Resp:	172930
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.7	13.1
54	5.6	5.5	8.3
68	4.5	4.5	6.7




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:28 PM




#8
Nitrobenzene-d5
Concen: 0.294 ng
RT: 8.937 min Scan# 617
Delta R.T. 0.000 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

Tgt Ion:	82	Resp:	31975
Ion	Ratio	Lower	Upper
82	100		
128	43.9	33.2	49.8
54	46.1	38.4	57.6

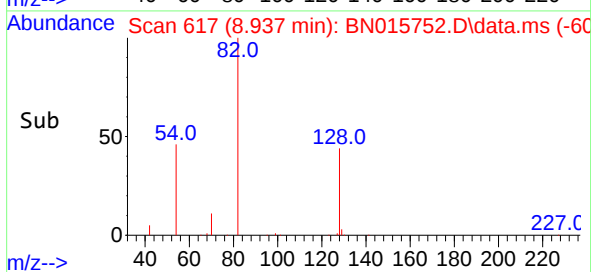






#9
Naphthalene
Concen: 0.205 ng
RT: 10.622 min Scan# 750
Delta R.T. 0.000 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36




Tgt Ion:128 Resp: 92208

Ion	Ratio	Lower	Upper
128	100		
129	11.2	8.9	13.3
127	12.9	10.4	15.6

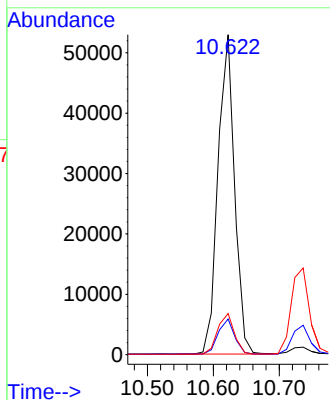



#10
Hexachlorobutadiene
Concen: 0.202 ng
RT: 10.914 min Scan# 773
Delta R.T. 0.000 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36



Tgt Ion:225 Resp: 15995


Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.0	51.0	76.4

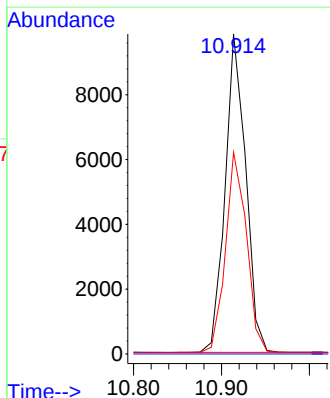

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

Manual Integrations
APPROVED

mohammad
8/2/2021 3:49:28 PM

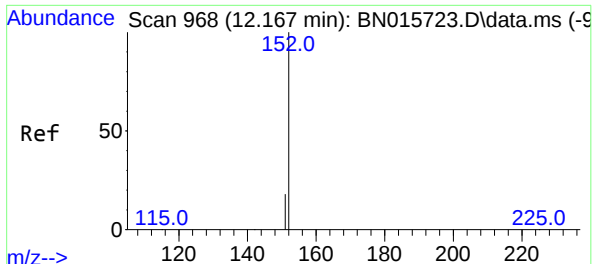





#11
2-Methylnaphthalene-d10
Concen: 0.418 ng
RT: 12.163 min Scan# 967
Delta R.T. -0.004 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

Tgt Ion:152 Resp: 108962
Ion Ratio Lower Upper
152 100
151 18.9 16.2 24.4

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:28 PM

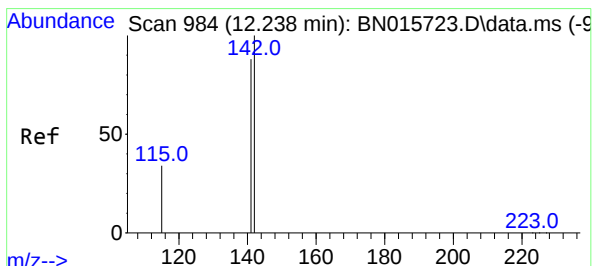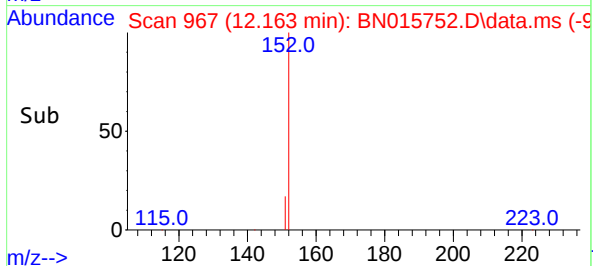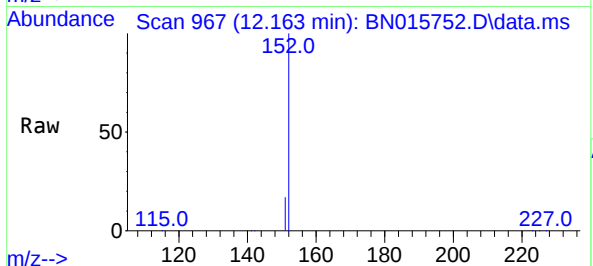

#12
2-Methylnaphthalene
Concen: 0.206 ng
RT: 12.234 min Scan# 983
Delta R.T. -0.004 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36


Tgt Ion:142 Resp: 60407
Ion Ratio Lower Upper
142 100
141 89.0 70.5 105.7
115 34.8 27.3 40.9

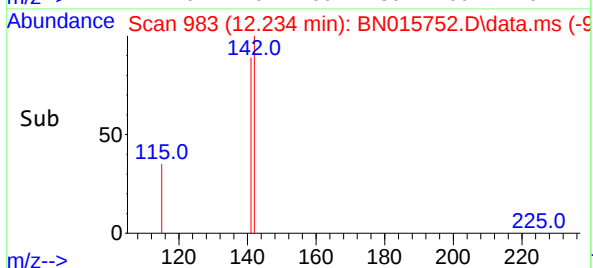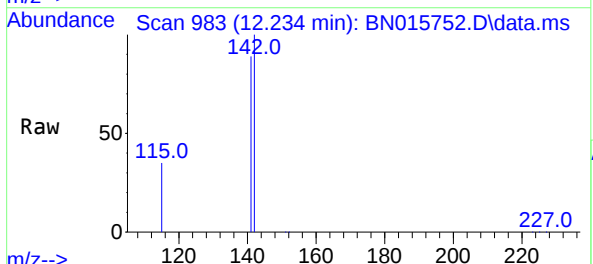



#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.421 min Scan# 1195
Delta R.T. 0.000 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




Tgt Ion:164 Resp: 91988
Ion Ratio Lower Upper
164 100
162 98.4 79.8 119.6
160 43.3 35.8 53.6

Manual Integrations
APPROVED



mohammad
8/2/2021 3:49:28 PM

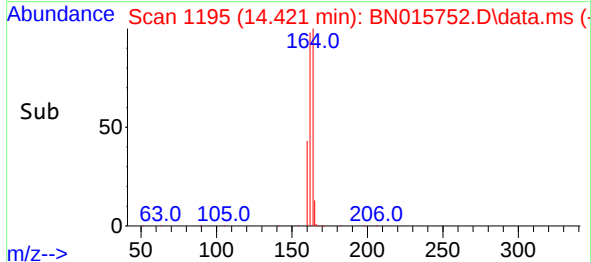


#14
2,4,6-Tribromophenol
Concen: 0.253 ng
RT: 15.906 min Scan# 1312
Delta R.T. -0.012 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36




Tgt Ion:330 Resp: 10074
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.0 28.8 43.2

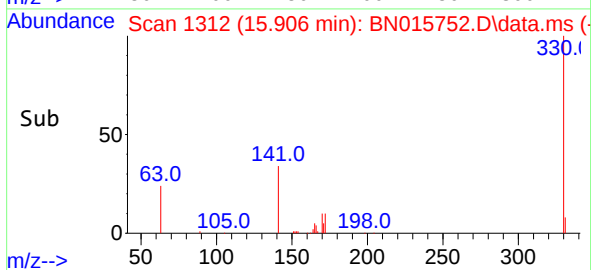

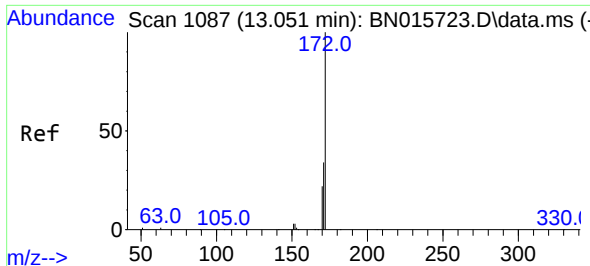

#15
2-Fluorobiphenyl
Concen: 0.320 ng
RT: 13.038 min Scan# 1086
Delta R.T. -0.012 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

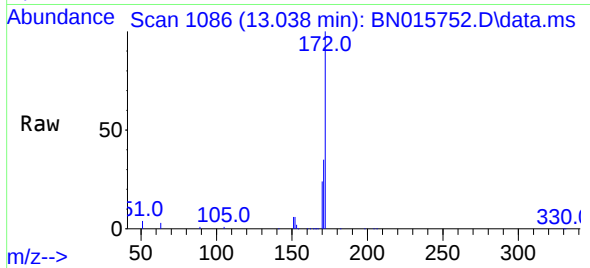


Tgt Ion:172 Resp: 112494
Ion Ratio Lower Upper
172 100
171 35.4 26.9 40.3
170 24.0 17.4 26.0

Manual Integrations
APPROVED



mohammad
8/2/2021 3:49:28 PM

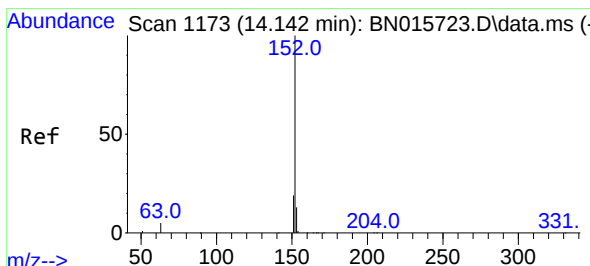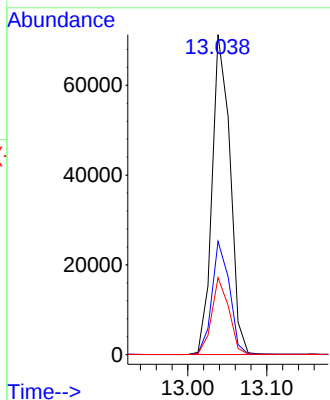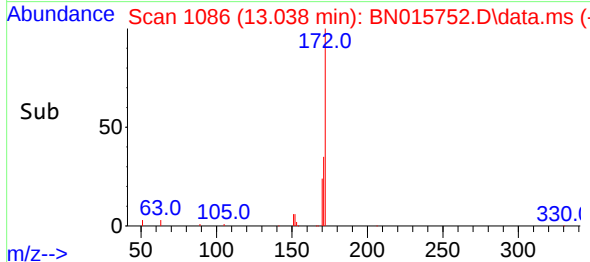


#16
Acenaphthylene
Concen: 0.166 ng
RT: 14.129 min Scan# 1172
Delta R.T. -0.013 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

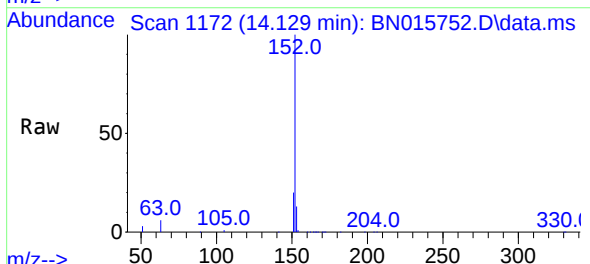


Tgt Ion:152 Resp: 67225
Ion Ratio Lower Upper
152 100
151 19.6 15.7 23.5
153 13.0 10.4 15.6

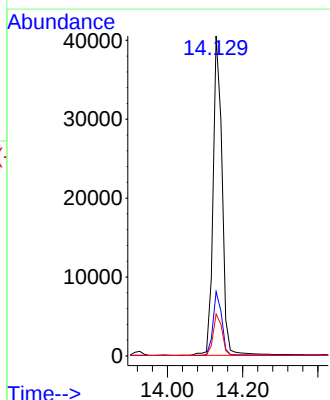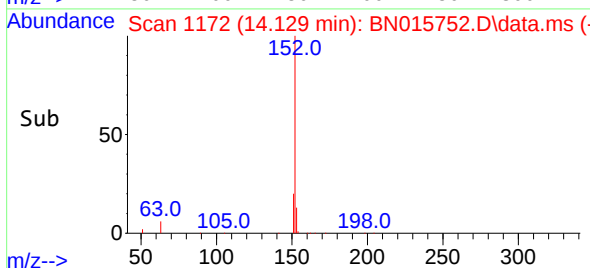

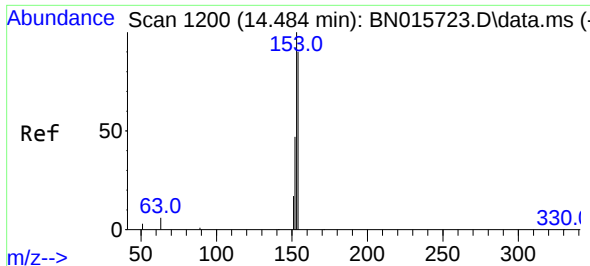

#17
Acenaphthene
Concen: 0.188 ng
RT: 14.485 min Scan# 1200
Delta R.T. 0.001 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

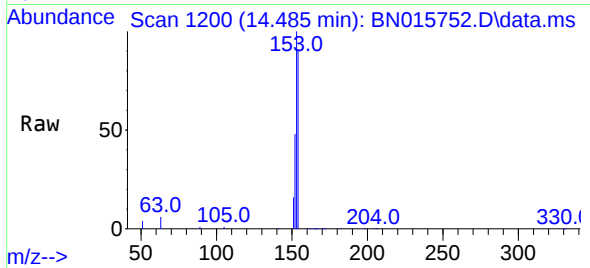


Tgt Ion:154 Resp: 49598
Ion Ratio Lower Upper
154 100
153 112.5 89.7 134.5
152 55.6 43.8 65.6

Manual Integrations
APPROVED



mohammad
8/2/2021 3:49:28 PM

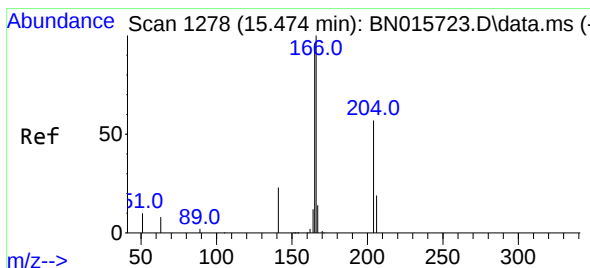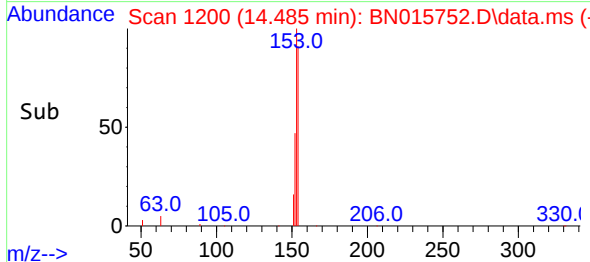


#18
Fluorene
Concen: 0.186 ng
RT: 15.461 min Scan# 1277
Delta R.T. -0.012 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

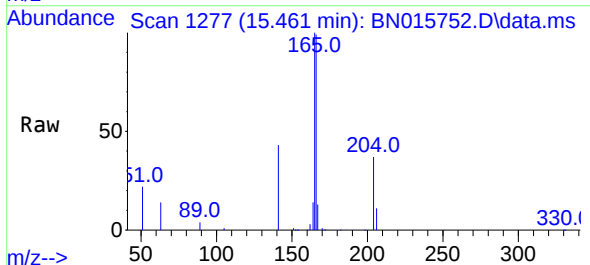

Tgt Ion:166 Resp: 59532
Ion Ratio Lower Upper
166 100
165 97.6 78.1 117.1
167 13.4 10.8 16.2

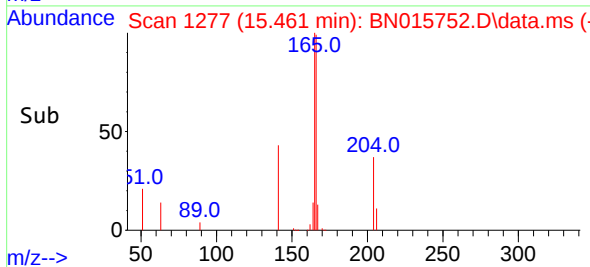

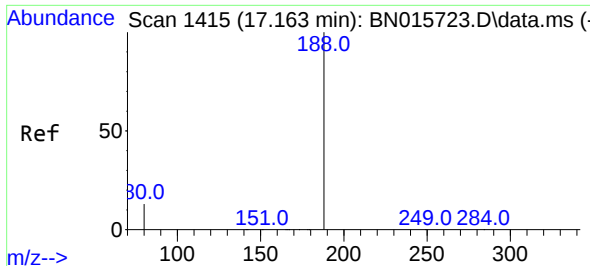





#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.164 min Scan# 1415
Delta R.T. 0.001 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

Tgt Ion:188 Resp: 172546
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.2 10.2 15.4#

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:28 PM

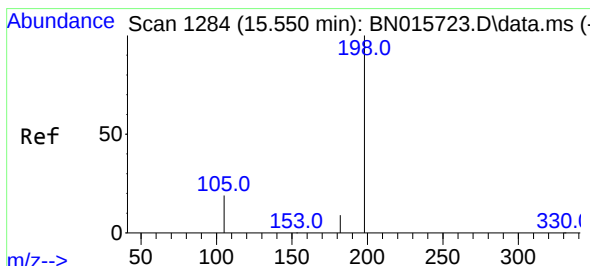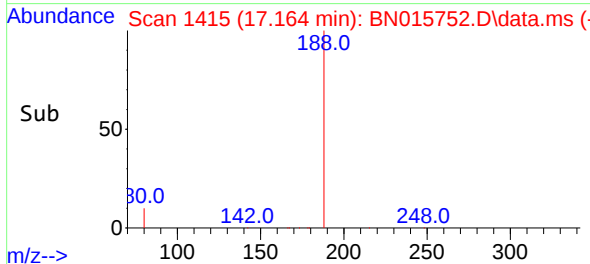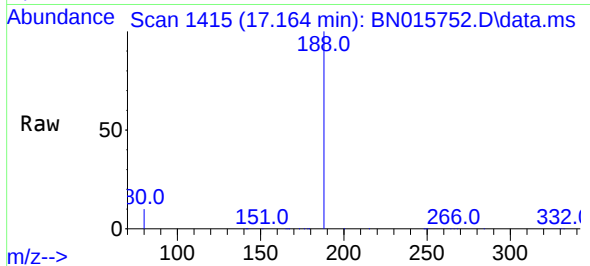

#20
4,6-Dinitro-2-methylphenol
Concen: 0.077 ng
RT: 15.550 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

Tgt Ion:198 Resp: 1022
Ion Ratio Lower Upper
198 100
182 19.8 9.4 14.0#
77 0.0 0.0 0.0

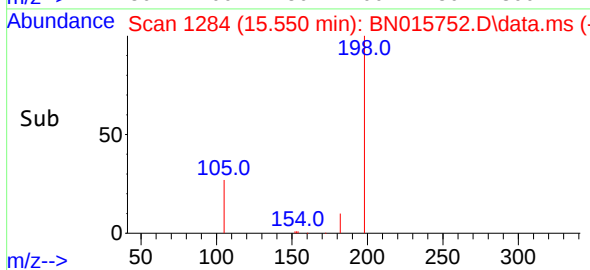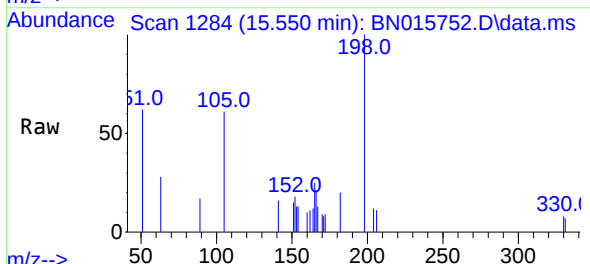







#21
4-Bromophenyl-phenylether
Concen: 0.185 ng
RT: 16.361 min Scan# 1349
Delta R.T. -0.012 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

Tgt Ion:248 Resp: 18588
Ion Ratio Lower Upper
248 100
250 92.1 83.9 125.9
141 75.4 26.9 40.3#

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:28 PM



#22
Hexachlorobenzene
Concen: 0.197 ng
RT: 16.482 min Scan# 1359
Delta R.T. 0.000 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36


Tgt Ion:284 Resp: 21982
Ion Ratio Lower Upper
284 100
142 36.4 29.4 44.0
249 29.6 23.8 35.6

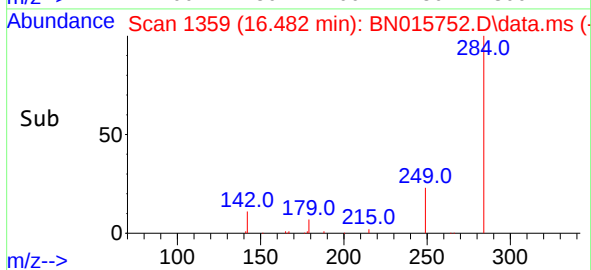



#23
Atrazine
Concen: 0.176 ng
RT: 16.628 min Scan# 1371
Delta R.T. -0.012 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021



Tgt Ion:200 Resp: 13518
Ion Ratio Lower Upper
200 100
173 32.6 18.9 28.3#
215 45.7 38.1 57.1




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:28 PM



#24
Pentachlorophenol
Concen: 0.227 ng
RT: 16.823 min Scan# 1387
Delta R.T. -0.000 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

Tgt Ion:266 Resp: 9470
Ion Ratio Lower Upper
266 100
264 62.3 50.2 75.2
268 63.5 51.1 76.7

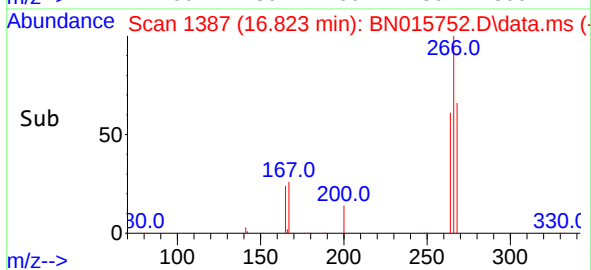







#25
Phenanthrene
Concen: 0.195 ng
RT: 17.212 min Scan# 1419
Delta R.T. 0.000 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

Tgt Ion:178 Resp: 96420
Ion Ratio Lower Upper
178 100
176 18.9 15.3 22.9
179 15.7 12.4 18.6

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:28 PM




#26
Anthracene
Concen: 0.177 ng
RT: 17.298 min Scan# 1426
Delta R.T. 0.000 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

Tgt Ion:178 Resp: 78858
Ion Ratio Lower Upper
178 100
176 18.3 14.6 22.0
179 15.2 12.2 18.4

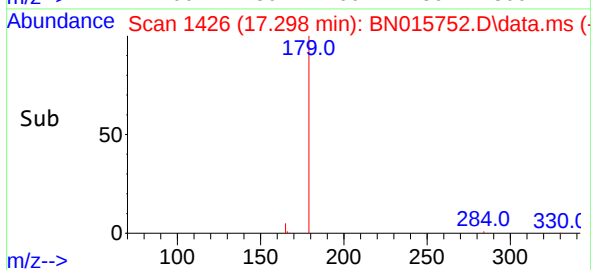







#27
Fluoranthene-d10
Concen: 0.397 ng
RT: 19.207 min Scan# 1725
Delta R.T. -0.005 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36





Tgt Ion:212 Resp: 180665
Ion Ratio Lower Upper
212 100
106 13.4 10.6 16.0
104 7.4 5.9 8.9

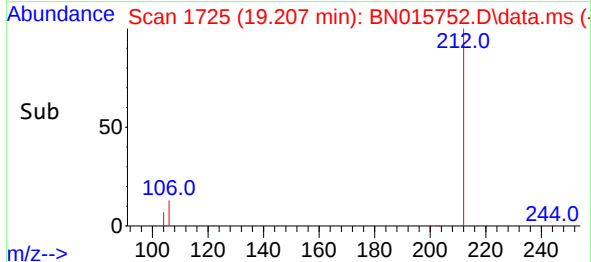

#28
Fluoranthene
Concen: 0.191 ng
RT: 19.237 min Scan# 1731
Delta R.T. -0.005 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

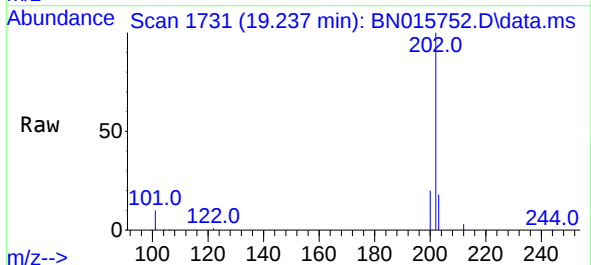


Tgt Ion:202 Resp: 100766
Ion Ratio Lower Upper
202 100
101 11.3 9.0 13.6
203 17.4 13.8 20.8

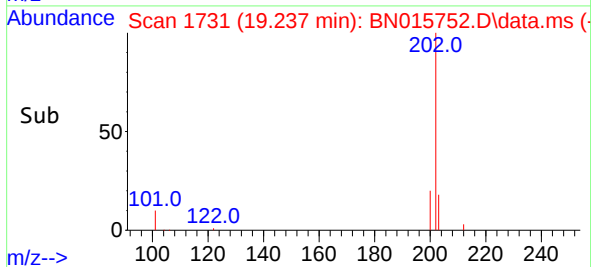

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

Manual Integrations
APPROVED

mohammad
8/2/2021 3:49:28 PM







#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.366 min Scan# 2014
Delta R.T. -0.010 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

Tgt Ion:240 Resp: 159552
Ion Ratio Lower Upper
240 100
120 11.1 7.4 11.0#
236 26.4 20.9 31.3

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:28 PM

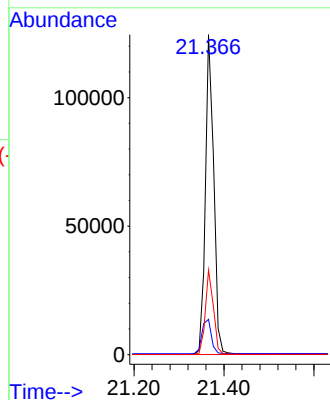

#30
Pyrene
Concen: 0.185 ng
RT: 19.599 min Scan# 1804
Delta R.T. -0.005 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36


Tgt Ion:202 Resp: 98568
Ion Ratio Lower Upper
202 100
200 20.5 16.5 24.7
203 17.7 14.0 21.0

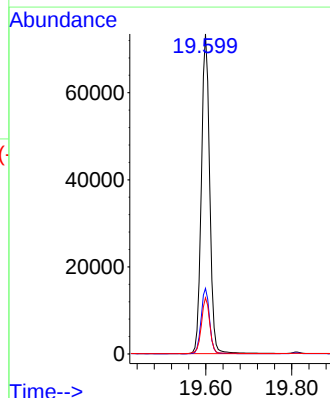

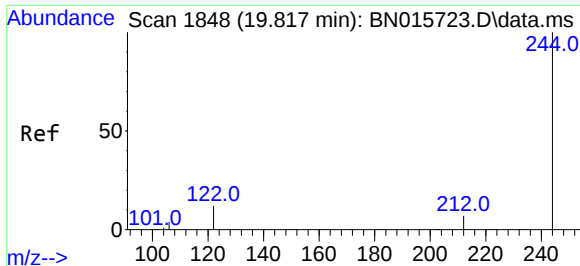

#31
Terphenyl-d14
Concen: 0.314 ng
RT: 19.813 min Scan# 1847
Delta R.T. -0.005 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

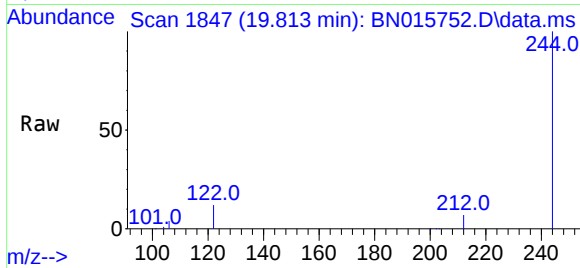

Tgt Ion:244 Resp: 121753
Ion Ratio Lower Upper
244 100
212 7.4 5.9 8.9
122 12.1 9.6 14.4




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:28 PM

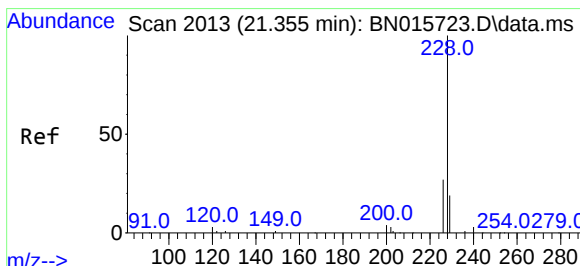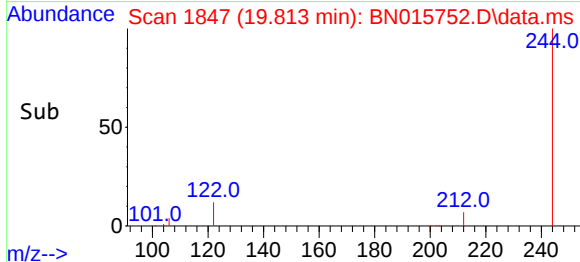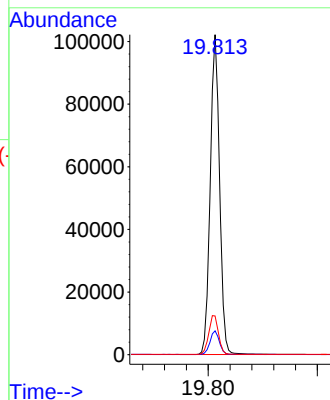

#32
Benzo(a)anthracene
Concen: 0.173 ng
RT: 21.355 min Scan# 2013
Delta R.T. 0.000 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36


Tgt Ion:228 Resp: 87963
Ion Ratio Lower Upper
228 100
226 26.2 21.9 32.9
229 20.0 15.4 23.0

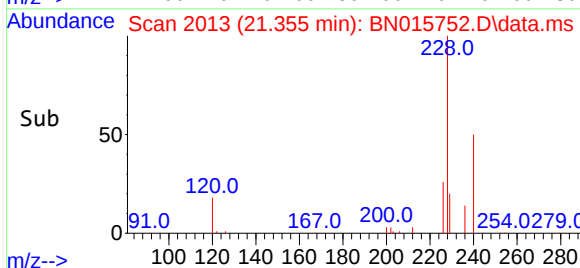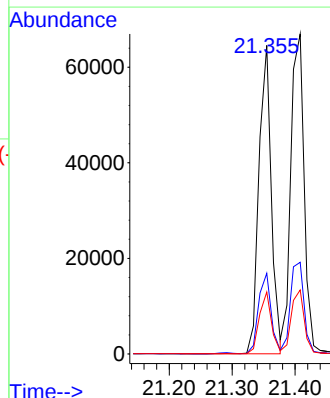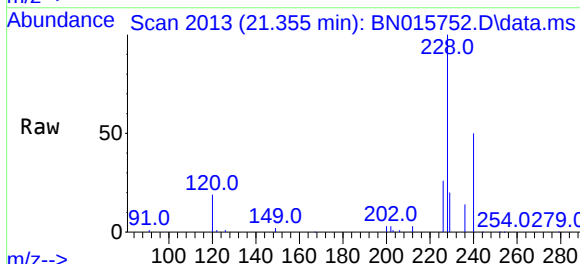

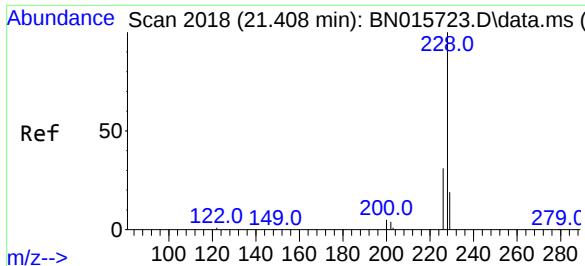

#33
Chrysene
Concen: 0.190 ng
RT: 21.408 min Scan# 2018
Delta R.T. 0.000 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

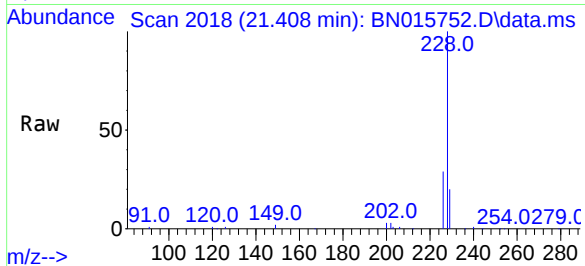


Tgt Ion:228 Resp: 98305
Ion Ratio Lower Upper
228 100
226 28.7 24.3 36.5
229 20.0 15.3 22.9

Manual Integrations
APPROVED



mohammad
8/2/2021 3:49:28 PM

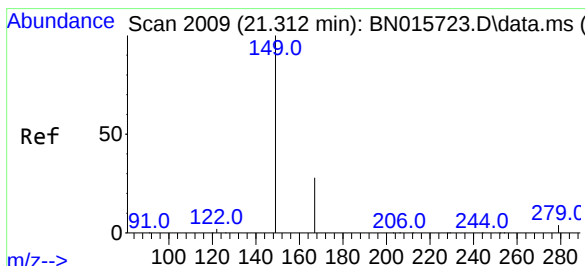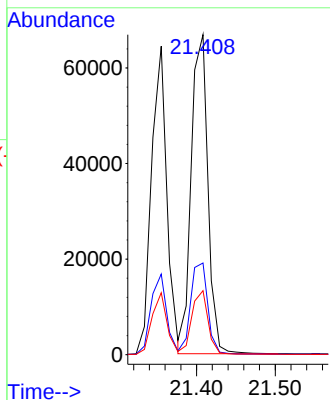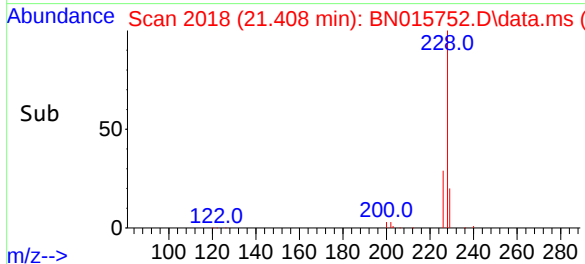


#34
Bis(2-ethylhexyl)phthalate
Concen: 0.108 ng
RT: 21.302 min Scan# 2008
Delta R.T. -0.010 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

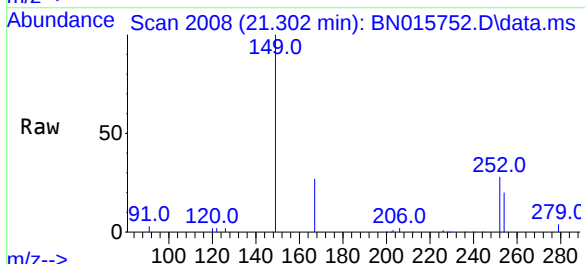


Tgt Ion:149 Resp: 29060
Ion Ratio Lower Upper
149 100
167 26.6 21.5 32.3
279 4.0 3.2 4.8

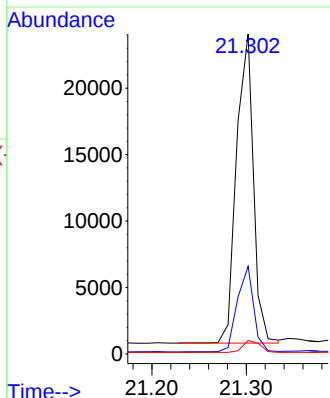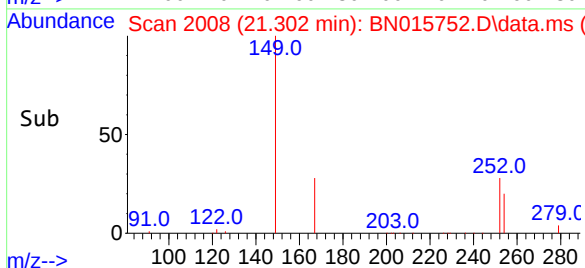



#35
Perylene-d12
Concen: 0.400 ng
RT: 23.707 min Scan# 2492
Delta R.T. -0.013 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36




Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021



Tgt Ion:264 Resp: 158878
Ion Ratio Lower Upper
264 100
260 24.8 19.4 29.2
265 23.7 19.9 29.9




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:28 PM

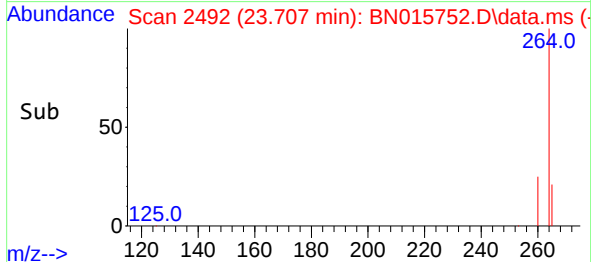


#36
Indeno(1,2,3-cd)pyrene
Concen: 0.188 ng
RT: 26.107 min Scan# 3193
Delta R.T. -0.020 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

Tgt Ion:276 Resp: 107467
Ion Ratio Lower Upper
276 100
138 26.3 20.6 30.8
277 25.0 20.1 30.1

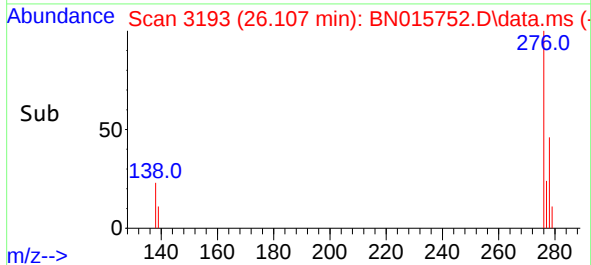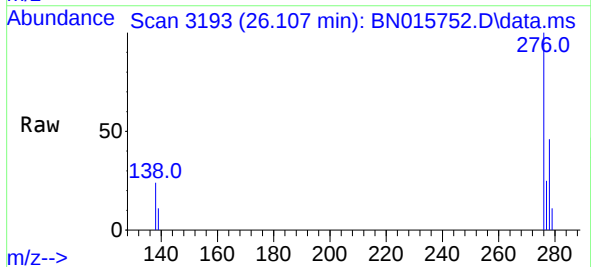






#37
Benzo(b)fluoranthene
Concen: 0.194 ng
RT: 22.999 min Scan# 2285
Delta R.T. -0.013 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36





Tgt Ion:252 Resp: 99115
Ion Ratio Lower Upper
252 100
253 22.4 18.1 27.1
125 10.5 8.3 12.5



#38
Benzo(k)fluoranthene
Concen: 0.199 ng
RT: 23.046 min Scan# 2299
Delta R.T. -0.010 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

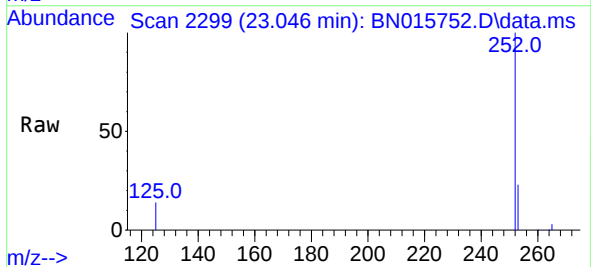


Tgt Ion:252 Resp: 109394
Ion Ratio Lower Upper
252 100
253 22.9 18.1 27.1
125 13.6 10.4 15.6

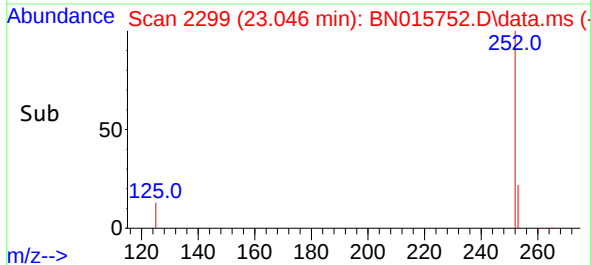


Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

Manual Integrations
APPROVED




mohammad
8/2/2021 3:49:28 PM




#39
Benzo(a)pyrene
Concen: 0.183 ng
RT: 23.604 min Scan# 2462
Delta R.T. -0.013 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36





Tgt Ion:252 Resp: 85426
Ion Ratio Lower Upper
252 100
253 22.9 18.1 27.1
125 11.9 9.2 13.8

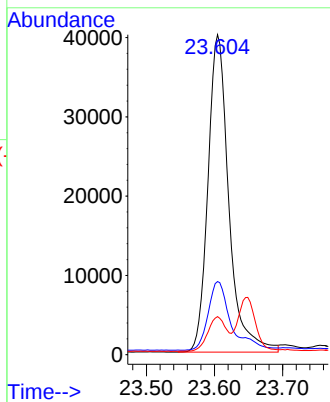

#40
Dibenzo(a,h)anthracene
Concen: 0.188 ng
RT: 26.127 min Scan# 3199
Delta R.T. -0.020 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

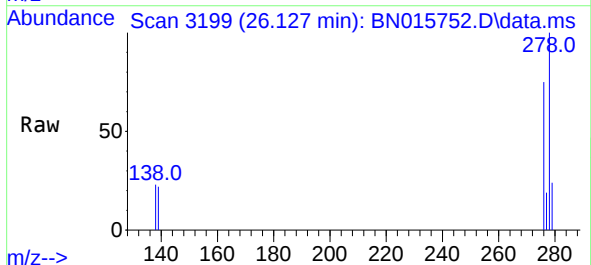


Tgt Ion:278 Resp: 90913
Ion Ratio Lower Upper
278 100
139 22.2 16.0 24.0
279 24.0 19.2 28.8

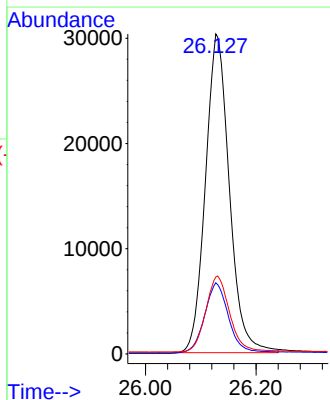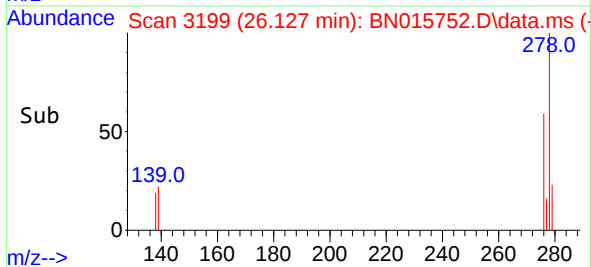

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021


Manual Integrations
APPROVED

mohammad
8/2/2021 3:49:28 PM

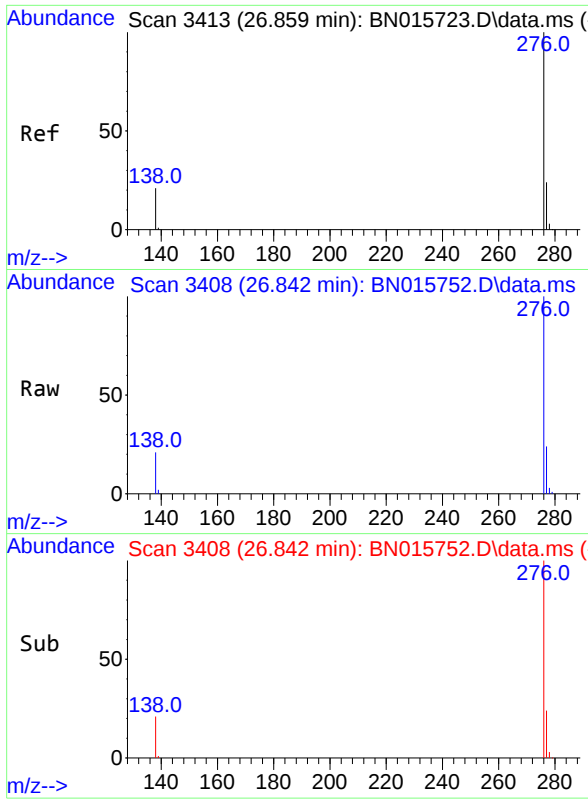

#41
Benzo(g,h,i)perylene
Concen: 0.184 ng
RT: 26.842 min Scan# 3408
Delta R.T. -0.017 min
Lab File: BN015752.D
Acq: 01 Aug 2021 02:36

Tgt Ion:	276	Resp:	91793
Ion Ratio	Lower	Upper	
276	100		
277	23.8	19.2	28.8
138	21.2	16.8	25.2

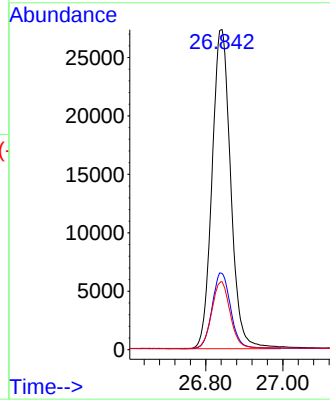

Instrument :
BNA_N
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

Manual Integrations
APPROVED

mohammad
8/2/2021 3:49:28 PM