

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073121\
 Data File : BN015753.D
 Acq On : 01 Aug 2021 03:13
 Operator : CG/JU
 Sample : M2940-08
 Misc : LOQ-WTR-0.1ng
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 LOQ-WATER-02-QT3-2021

Manual Integrations
 APPROVED

mohammad
 8/2/2021 3:49:31 PM

Quant Time: Aug 02 04:32:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 02 04:24:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.790	152	35110	0.400	ng	0.00
7) Naphthalene-d8	10.572	136	156982	0.400	ng	# 0.00
13) Acenaphthene-d10	14.421	164	82780	0.400	ng	0.00
19) Phenanthrene-d10	17.164	188	157961	0.400	ng	# 0.00
29) Chrysene-d12	21.366	240	144056	0.400	ng	#-0.01
35) Perylene-d12	23.707	264	147657	0.400	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.393	112	29142	0.309	ng	0.00
5) Phenol-d6	6.951	99	33470	0.293	ng	0.00
8) Nitrobenzene-d5	8.937	82	30910	0.313	ng	0.00
11) 2-Methylnaphthalene-d10	12.163	152	102545	0.434	ng	0.00
14) 2,4,6-Tribromophenol	15.906	330	8024	0.224	ng	-0.01
15) 2-Fluorobiphenyl	13.038	172	110410	0.348	ng	-0.01
27) Fluoranthene-d10	19.207	212	169551	0.407	ng	0.00
31) Terphenyl-d14	19.813	244	119114	0.340	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.355	88	1268	0.105	ng	88
3) n-Nitrosodimethylamine	3.733	42	1669	0.072	ng	# 99
6) bis(2-Chloroethyl)ether	7.218	93	10437	0.112	ng	100
9) Naphthalene	10.622	128	43655	0.107	ng	100
10) Hexachlorobutadiene	10.914	225	7497	0.104	ng	# 100
12) 2-Methylnaphthalene	12.234	142	28397	0.107	ng	99
16) Acenaphthylene	14.129	152	29692	0.082	ng	100
17) Acenaphthene	14.472	154	22993	0.097	ng	99
18) Fluorene	15.461	166	27271	0.095	ng	100
20) 4,6-Dinitro-2-methylph...	15.550	198	381	0.031	ng	# 41
21) 4-Bromophenyl-phenylether	16.360	248	8594	0.093	ng	# 76
22) Hexachlorobenzene	16.470	284	10437	0.102	ng	98
23) Atrazine	16.628	200	6940	0.099	ng	# 94
24) Pentachlorophenol	16.823	266	7500	0.196	ng	99
25) Phenanthrene	17.200	178	44875	0.099	ng	99
26) Anthracene	17.298	178	35730	0.087	ng	100
28) Fluoranthene	19.237	202	47350	0.098	ng	100
30) Pyrene	19.599	202	44587	0.093	ng	100
32) Benzo(a)anthracene	21.355	228	39183	0.085	ng	98
33) Chrysene	21.408	228	45525	0.098	ng	97
34) Bis(2-ethylhexyl)phtha...	21.302	149	13717	0.056	ng	100
36) Indeno(1,2,3-cd)pyrene	26.110	276	48443	0.091	ng	97
37) Benzo(b)fluoranthene	22.999	252	45424	0.096	ng	98
38) Benzo(k)fluoranthene	23.046	252	50874m	0.099	ng	
39) Benzo(a)pyrene	23.604	252	38324	0.088	ng	96
40) Dibenzo(a,h)anthracene	26.127	278	40846	0.091	ng	# 88
41) Benzo(g,h,i)perylene	26.842	276	41565	0.090	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073121\
Data File : BN015753.D
Acq On : 01 Aug 2021 03:13
Operator : CG/JU
Sample : M2940-08
Misc : LOQ-WTR-0.1ng
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021

Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:31 PM

Quant Time: Aug 02 04:32:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 02 04:24:05 2021
Response via : Initial Calibration









#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.790 min Scan# 511
Delta R.T. 0.000 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13





Tgt Ion: 152 Resp: 35110
Ion Ratio Lower Upper
152 100
150 154.6 123.9 185.9
115 58.5 47.8 71.6



#2
1,4-Dioxane
Concen: 0.105 ng
RT: 3.355 min Scan# 30
Delta R.T. 0.000 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13



Tgt Ion: 88 Resp: 1268
Ion Ratio Lower Upper
88 100
43 24.8 17.2 25.8
58 66.2 62.2 93.2




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021

Manual Integrations
APPROVED

mohammad
8/2/2021 3:49:31 PM

Abundance Scan 69 (3.714 min): BN015723.D\data.ms (-64)



#3

n-Nitrosodimethylamine

Concen: 0.072 ng

RT: 3.733 min Scan# 71

Delta R.T. 0.019 min

Lab File: BN015753.D

Acq: 01 Aug 2021 03:13

Tgt Ion: 42 Resp: 1669

Ion Ratio Lower Upper

42 100

74 145.4 116.6 174.8

44 5.7 6.6 10.0#

Instrument :

BNA_N

ClientSampleId :

LOQ-WATER-02-QT3-2021


Manual Integrations

APPROVED


mohammad

8/2/2021 3:49:31 PM


Abundance Scan 71 (3.733 min): BN015753.D\data.ms




Abundance



Abundance Scan 71 (3.733 min): BN015753.D\data.ms (-58)



Abundance Scan 250 (5.383 min): BN015723.D\data.ms (-24)



#4

2-Fluorophenol

Concen: 0.309 ng

RT: 5.393 min Scan# 251

Delta R.T. 0.009 min

Lab File: BN015753.D

Acq: 01 Aug 2021 03:13

Tgt Ion: 112 Resp: 29142


Ion Ratio Lower Upper

112 100


64 52.1 42.1 63.1

63 27.4 21.9 32.9


Abundance Scan 251 (5.393 min): BN015753.D\data.ms




Abundance



Abundance Scan 251 (5.393 min): BN015753.D\data.ms (-23)









#5
Phenol-d6
Concen: 0.293 ng
RT: 6.951 min Scan# 420
Delta R.T. 0.000 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13

Tgt Ion:	99	Resp:	33470
Ion	Ratio	Lower	Upper
99	100		
42	15.6	12.9	19.3
71	29.4	23.8	35.6

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:31 PM



#6
bis(2-Chloroethyl)ether
Concen: 0.112 ng
RT: 7.218 min Scan# 449
Delta R.T. 0.000 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13


Tgt Ion:	93	Resp:	10437
Ion	Ratio	Lower	Upper
93	100		
63	73.0	58.6	87.8
95	33.9	26.9	40.3





#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.572 min Scan# 746
Delta R.T. 0.000 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021



Tgt Ion:136 Resp: 156982
Ion Ratio Lower Upper
136 100
137 10.9 8.7 13.1
54 5.2 5.5 8.3#
68 4.3 4.5 6.7#




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:31 PM



#8
Nitrobenzene-d5
Concen: 0.313 ng
RT: 8.937 min Scan# 617
Delta R.T. 0.000 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13

Tgt Ion: 82 Resp: 30910
Ion Ratio Lower Upper
82 100
128 44.9 33.2 49.8
54 46.1 38.4 57.6









#9
Naphthalene
Concen: 0.107 ng
RT: 10.622 min Scan# 750
Delta R.T. 0.000 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13

Tgt Ion:	128	Resp:	43655
Ion Ratio	Lower	Upper	
128	100		
129	11.2	8.9	13.3
127	12.8	10.4	15.6

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:31 PM



#10
Hexachlorobutadiene
Concen: 0.104 ng
RT: 10.914 min Scan# 773
Delta R.T. 0.000 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13

Tgt Ion:	225	Resp:	7497
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	63.9	51.0	76.4



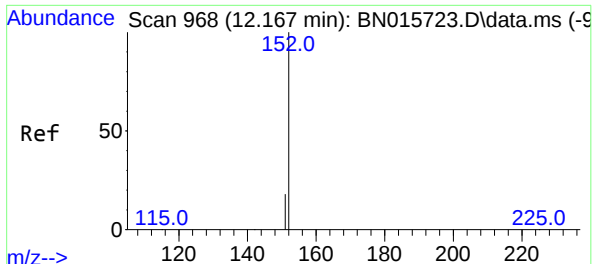





#11
2-Methylnaphthalene-d10
Concen: 0.434 ng
RT: 12.163 min Scan# 967
Delta R.T. -0.004 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13

Tgt Ion:152 Resp: 102545
Ion Ratio Lower Upper
152 100
151 19.0 16.2 24.4

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:31 PM



#12
2-Methylnaphthalene
Concen: 0.107 ng
RT: 12.234 min Scan# 983
Delta R.T. -0.004 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13

Tgt Ion:142 Resp: 28397
Ion Ratio Lower Upper
142 100
141 88.4 70.5 105.7
115 34.6 27.3 40.9









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.421 min Scan# 1195
Delta R.T. 0.000 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13

Tgt Ion:164 Resp: 82780
Ion Ratio Lower Upper
164 100
162 97.6 79.8 119.6
160 42.8 35.8 53.6

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:31 PM




#14
2,4,6-Tribromophenol
Concen: 0.224 ng
RT: 15.906 min Scan# 1312
Delta R.T. -0.012 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13

Tgt Ion:330 Resp: 8024
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 34.8 28.8 43.2




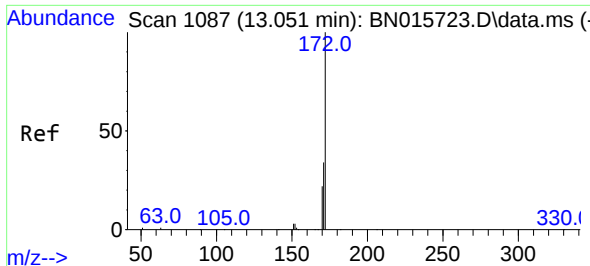

#15
2-Fluorobiphenyl
Concen: 0.348 ng
RT: 13.038 min Scan# 1086
Delta R.T. -0.012 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13





Tgt Ion:172 Resp: 110410
Ion Ratio Lower Upper
172 100
171 34.9 26.9 40.3
170 23.4 17.4 26.0




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021

Manual Integrations
APPROVED



mohammad
8/2/2021 3:49:31 PM

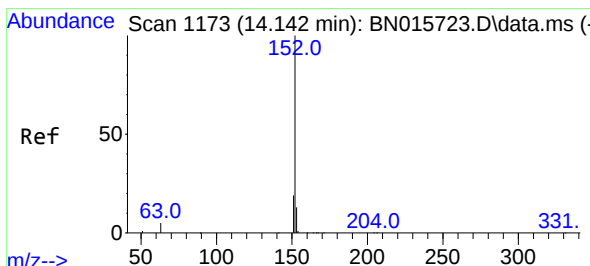


#16
Acenaphthylene
Concen: 0.082 ng
RT: 14.129 min Scan# 1172
Delta R.T. -0.013 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13




Tgt Ion:152 Resp: 29692
Ion Ratio Lower Upper
152 100
151 19.7 15.7 23.5
153 13.2 10.4 15.6



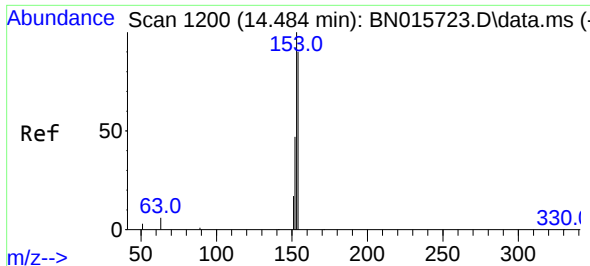

#17
Acenaphthene
Concen: 0.097 ng
RT: 14.472 min Scan# 1199
Delta R.T. -0.012 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021



Tgt Ion:154 Resp: 22993
Ion Ratio Lower Upper
154 100
153 112.4 89.7 134.5
152 55.8 43.8 65.6




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:31 PM




#18
Fluorene
Concen: 0.095 ng
RT: 15.461 min Scan# 1277
Delta R.T. -0.012 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13

Tgt Ion:166 Resp: 27271
Ion Ratio Lower Upper
166 100
165 97.8 78.1 117.1
167 13.4 10.8 16.2







#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.164 min Scan# 1415
Delta R.T. 0.001 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13




Tgt Ion:188 Resp: 157961
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.5 10.2 15.4#




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021

Manual Integrations
APPROVED



mohammad
8/2/2021 3:49:31 PM




#20
4,6-Dinitro-2-methylphenol
Concen: 0.031 ng
RT: 15.550 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13



Tgt Ion:198 Resp: 381
Ion Ratio Lower Upper
198 100
182 34.3 9.4 14.0#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.093 ng
RT: 16.360 min Scan# 1349
Delta R.T. -0.012 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13

Tgt Ion:248 Resp: 8594
Ion Ratio Lower Upper
248 100
250 93.4 83.9 125.9
141 68.9 26.9 40.3#

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:31 PM



#22
Hexachlorobenzene
Concen: 0.102 ng
RT: 16.470 min Scan# 1358
Delta R.T. -0.012 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13


Tgt Ion:284 Resp: 10437
Ion Ratio Lower Upper
284 100
142 35.2 29.4 44.0
249 29.0 23.8 35.6





#23
Atrazine
Concen: 0.099 ng
RT: 16.628 min Scan# 1371
Delta R.T. -0.012 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Tgt Ion:200 Resp: 6940
Ion Ratio Lower Upper
200 100
173 31.3 18.9 28.3#
215 46.6 38.1 57.1

Manual Integrations
APPROVED



mohammad
8/2/2021 3:49:31 PM




#24
Pentachlorophenol
Concen: 0.196 ng
RT: 16.823 min Scan# 1387
Delta R.T. -0.000 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13



Tgt Ion:266 Resp: 7500
Ion Ratio Lower Upper
266 100
264 62.8 50.2 75.2
268 64.9 51.1 76.7









#25
Phenanthrene
Concen: 0.099 ng
RT: 17.200 min Scan# 1418
Delta R.T. -0.012 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13

Tgt Ion:178 Resp: 44875
Ion Ratio Lower Upper
178 100
176 19.1 15.3 22.9
179 16.6 12.4 18.6

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:31 PM




#26
Anthracene
Concen: 0.087 ng
RT: 17.298 min Scan# 1426
Delta R.T. 0.000 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13

Tgt Ion:178 Resp: 35730
Ion Ratio Lower Upper
178 100
176 18.4 14.6 22.0
179 15.4 12.2 18.4









#27
Fluoranthene-d10
Concen: 0.407 ng
RT: 19.207 min Scan# 1725
Delta R.T. -0.005 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13





Tgt Ion:212 Resp: 169551
Ion Ratio Lower Upper
212 100
106 13.4 10.6 16.0
104 7.3 5.9 8.9



#28
Fluoranthene
Concen: 0.098 ng
RT: 19.237 min Scan# 1731
Delta R.T. -0.005 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13




Tgt Ion:202 Resp: 47350
Ion Ratio Lower Upper
202 100
101 11.4 9.0 13.6
203 17.2 13.8 20.8




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021

Manual Integrations
APPROVED




mohammad
8/2/2021 3:49:31 PM




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.366 min Scan# 2014
Delta R.T. -0.010 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13





Tgt Ion:240 Resp: 144056
Ion Ratio Lower Upper
240 100
120 11.2 7.4 11.0#
236 26.4 20.9 31.3



#30
Pyrene
Concen: 0.093 ng
RT: 19.599 min Scan# 1804
Delta R.T. -0.005 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13




Tgt Ion:202 Resp: 44587
Ion Ratio Lower Upper
202 100
200 20.7 16.5 24.7
203 17.6 14.0 21.0



Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021


Manual Integrations
APPROVED

mohammad
8/2/2021 3:49:31 PM



#31
Terphenyl-d14
Concen: 0.340 ng
RT: 19.813 min Scan# 1847
Delta R.T. -0.005 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Tgt Ion:244 Resp: 119114
Ion Ratio Lower Upper
244 100
212 7.3 5.9 8.9
122 11.1 9.6 14.4

Manual Integrations
APPROVED



mohammad
8/2/2021 3:49:31 PM




#32
Benzo(a)anthracene
Concen: 0.085 ng
RT: 21.355 min Scan# 2013
Delta R.T. -0.000 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13




Tgt Ion:228 Resp: 39183
Ion Ratio Lower Upper
228 100
226 26.0 21.9 32.9
229 20.0 15.4 23.0



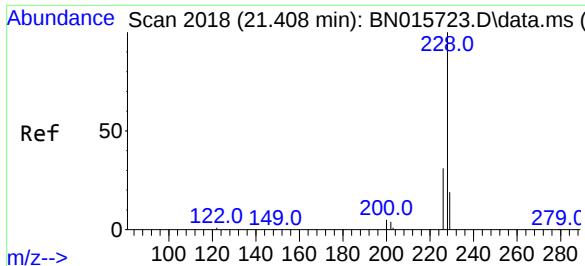

#33
Chrysene
Concen: 0.098 ng
RT: 21.408 min Scan# 2018
Delta R.T. 0.000 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Tgt Ion:228 Resp: 45525
Ion Ratio Lower Upper
228 100
226 28.2 24.3 36.5
229 19.9 15.3 22.9

Manual Integrations
APPROVED



mohammad
8/2/2021 3:49:31 PM

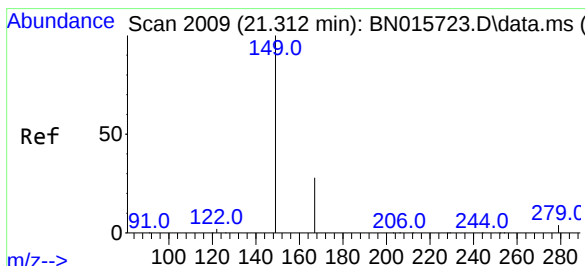


#34
Bis(2-ethylhexyl)phthalate
Concen: 0.056 ng
RT: 21.302 min Scan# 2008
Delta R.T. -0.010 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13




Tgt Ion:149 Resp: 13717
Ion Ratio Lower Upper
149 100
167 26.9 21.5 32.3
279 3.9 3.2 4.8





#35
Perylene-d12
Concen: 0.400 ng
RT: 23.707 min Scan# 2492
Delta R.T. -0.013 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021



Tgt Ion:264 Resp: 147657
Ion Ratio Lower Upper
264 100
260 24.6 19.4 29.2
265 24.1 19.9 29.9




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:31 PM




#36
Indeno(1,2,3-cd)pyrene
Concen: 0.091 ng
RT: 26.110 min Scan# 3194
Delta R.T. -0.017 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13

Tgt Ion:276 Resp: 48443
Ion Ratio Lower Upper
276 100
138 28.8 20.6 30.8
277 25.0 20.1 30.1









#37
Benzo(b)fluoranthene
Concen: 0.096 ng
RT: 22.999 min Scan# 2285
Delta R.T. -0.013 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13





Tgt Ion:252 Resp: 45424
Ion Ratio Lower Upper
252 100
253 23.4 18.1 27.1
125 11.4 8.3 12.5



#38
Benzo(k)fluoranthene
Concen: 0.099 ng m
RT: 23.046 min Scan# 2299
Delta R.T. -0.010 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13




Tgt Ion:252 Resp: 50874
Ion Ratio Lower Upper
252 100
253 24.4 18.1 27.1
125 17.4 10.4 15.6#



Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021

Manual Integrations
APPROVED

mohammad
8/2/2021 3:49:31 PM







#39
Benzo(a)pyrene
Concen: 0.088 ng
RT: 23.604 min Scan# 2462
Delta R.T. -0.013 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13

Tgt Ion:	252	Resp:	38324
Ion Ratio	Lower	Upper	
252	100		
253	24.3	18.1	27.1
125	13.1	9.2	13.8

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021




Manual Integrations
APPROVED


mohammad
8/2/2021 3:49:31 PM



#40
Dibenzo(a,h)anthracene
Concen: 0.091 ng
RT: 26.127 min Scan# 3199
Delta R.T. -0.020 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13


Tgt Ion:	278	Resp:	40846
Ion Ratio	Lower	Upper	
278	100		
139	30.2	16.0	24.0#
279	25.3	19.2	28.8





#41
Benzo(g,h,i)perylene
Concen: 0.090 ng
RT: 26.842 min Scan# 3408
Delta R.T. -0.017 min
Lab File: BN015753.D
Acq: 01 Aug 2021 03:13

Tgt Ion:	276	Resp:	41565
Ion Ratio	Lower	Upper	
276	100		
277	24.3	19.2	28.8
138	21.2	16.8	25.2



Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT3-2021

Manual Integrations
APPROVED

mohammad
8/2/2021 3:49:31 PM