


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073121\
 Data File : BN015730.D
 Acq On : 31 Jul 2021 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 31 04:53:33 2021

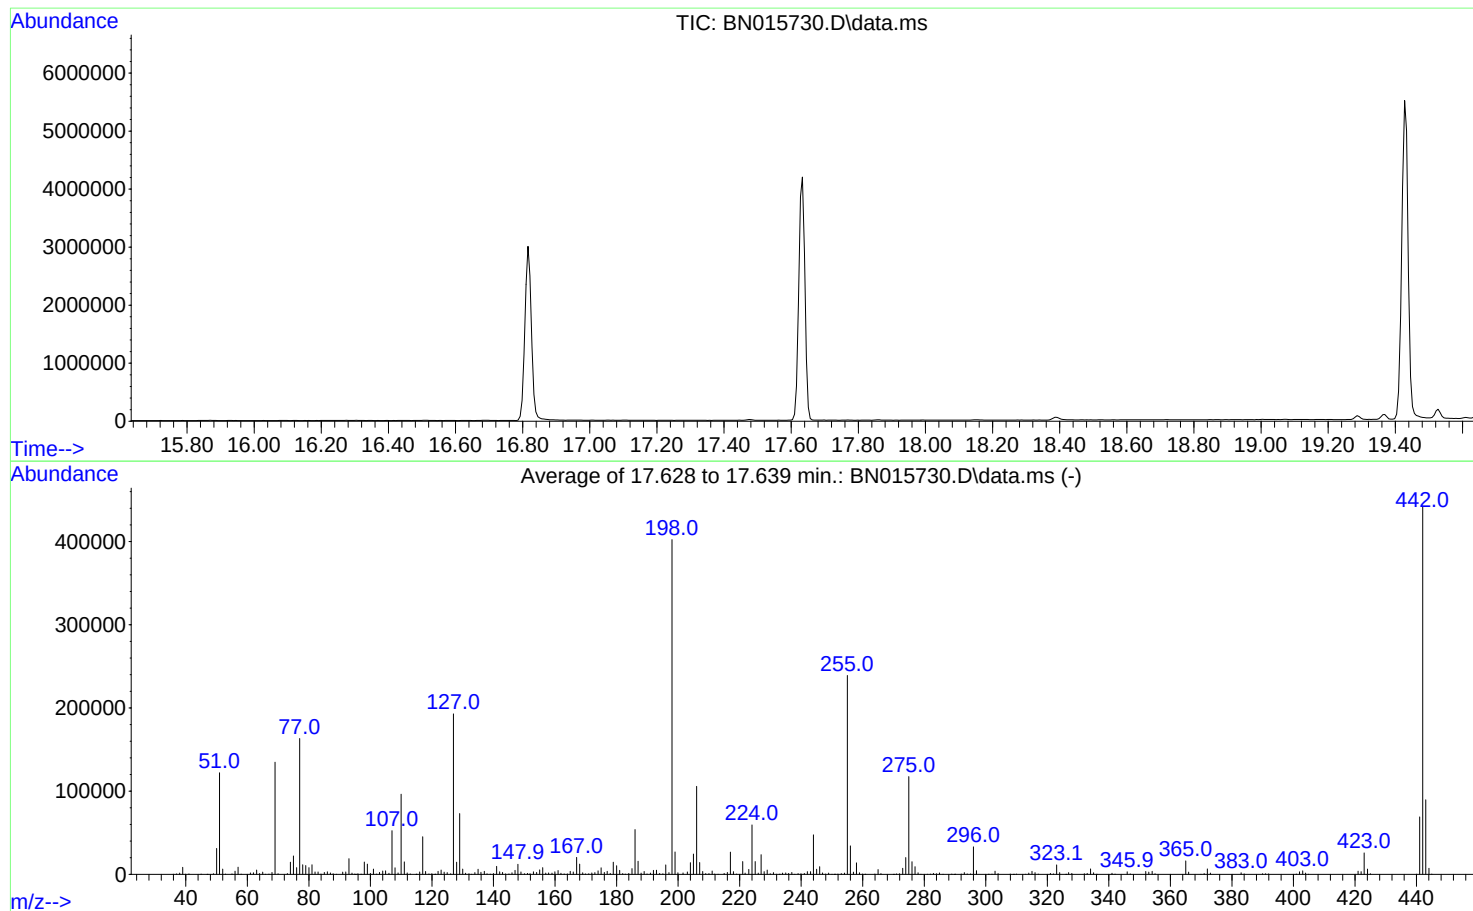




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	122218	PASS
68	69	0.00	2	1.7	2263	PASS
69	198	0.00	100	33.5	134797	PASS
70	69	0.00	2	0.6	848	PASS
127	198	10	80	48.0	192960	PASS
197	198	0.00	2	0.5	2166	PASS
198	198	100	100	100.0	402304	PASS
199	198	5	9	6.7	27005	PASS
275	198	10	60	29.2	117453	PASS
365	198	1	100	4.0	16138	PASS
441	198	0.01	100	17.1	68987	PASS
442	442	50	100	100.0	442133	PASS
443	442	15	24	20.3	89667	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073121\
Data File : BN015730.D
Acq On : 31 Jul 2021 09:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 02 05:34:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 30 07:20:03 2021
Response via : Initial Calibration

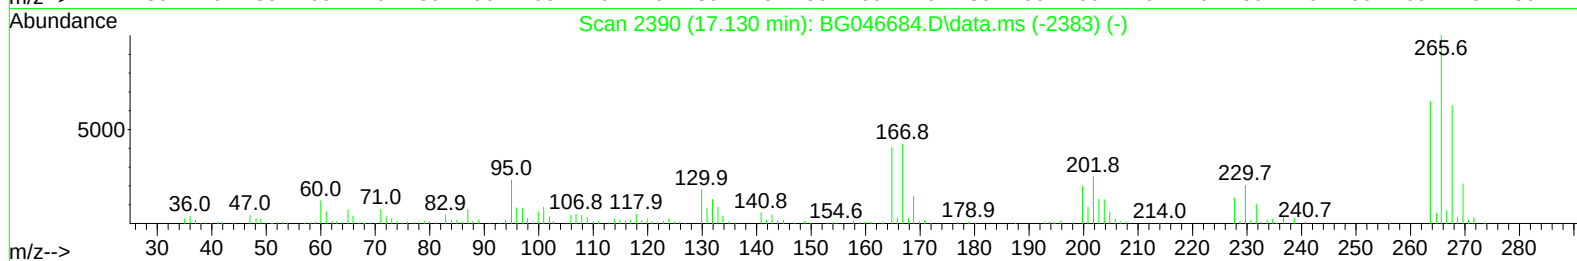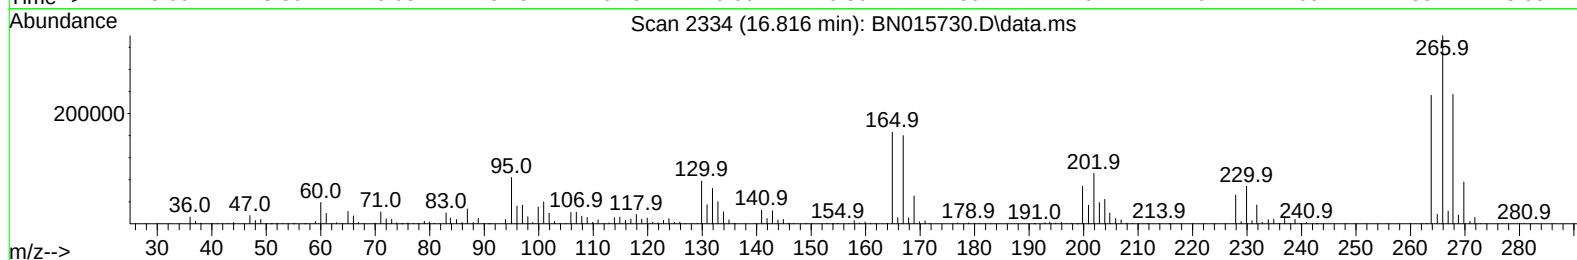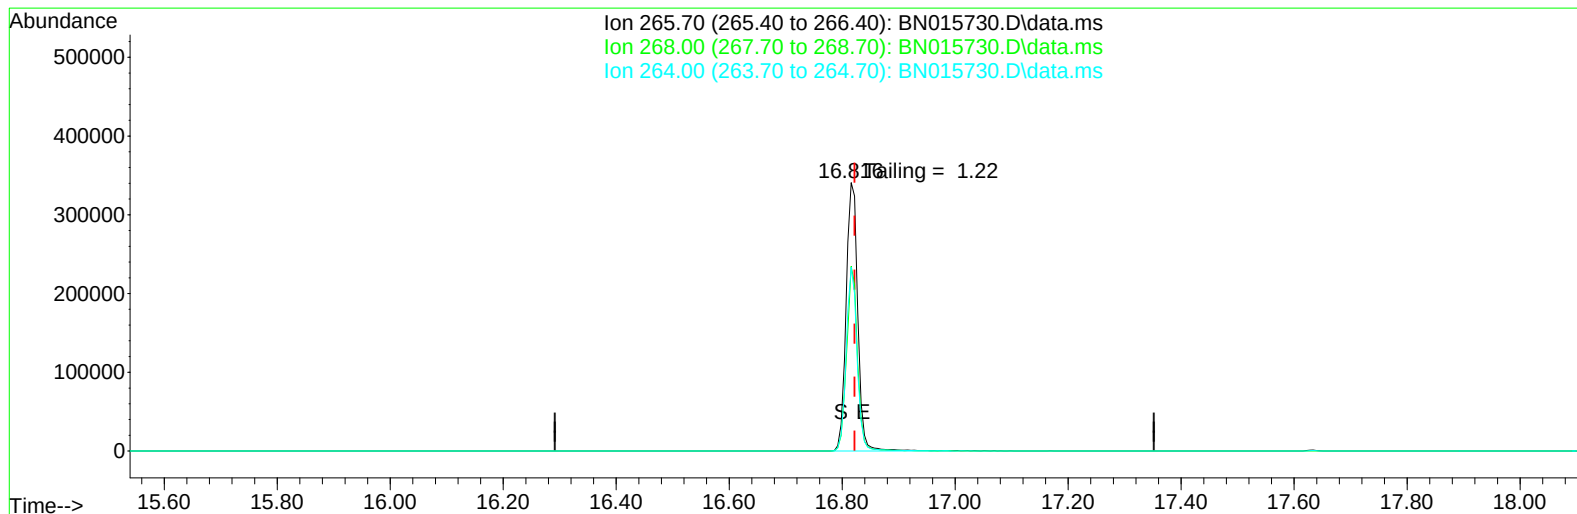

TIC: BN015730.D\data.ms

(70) Pentachlorophenol (C)

16.816min (-0.006) 27608.30 ng




response 487925

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.83
264.00	61.60	68.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073121\
Data File : BN015730.D
Acq On : 31 Jul 2021 09:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 02 05:34:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 30 07:20:03 2021
Response via : Initial Calibration

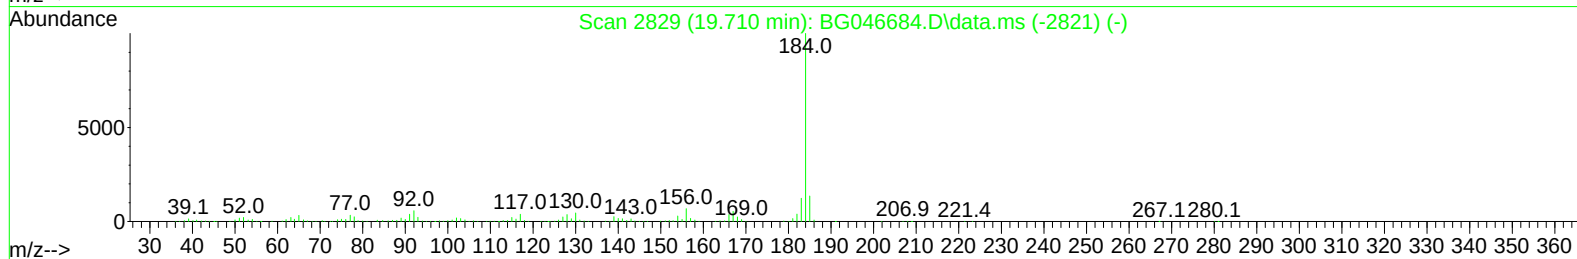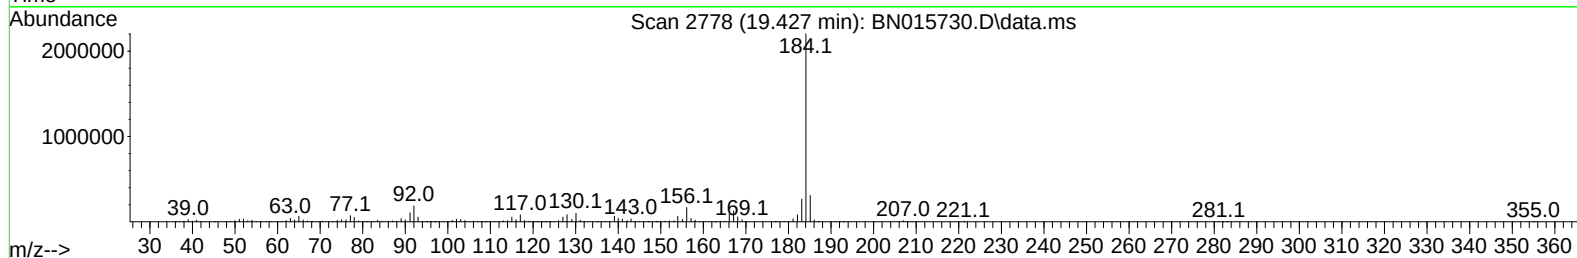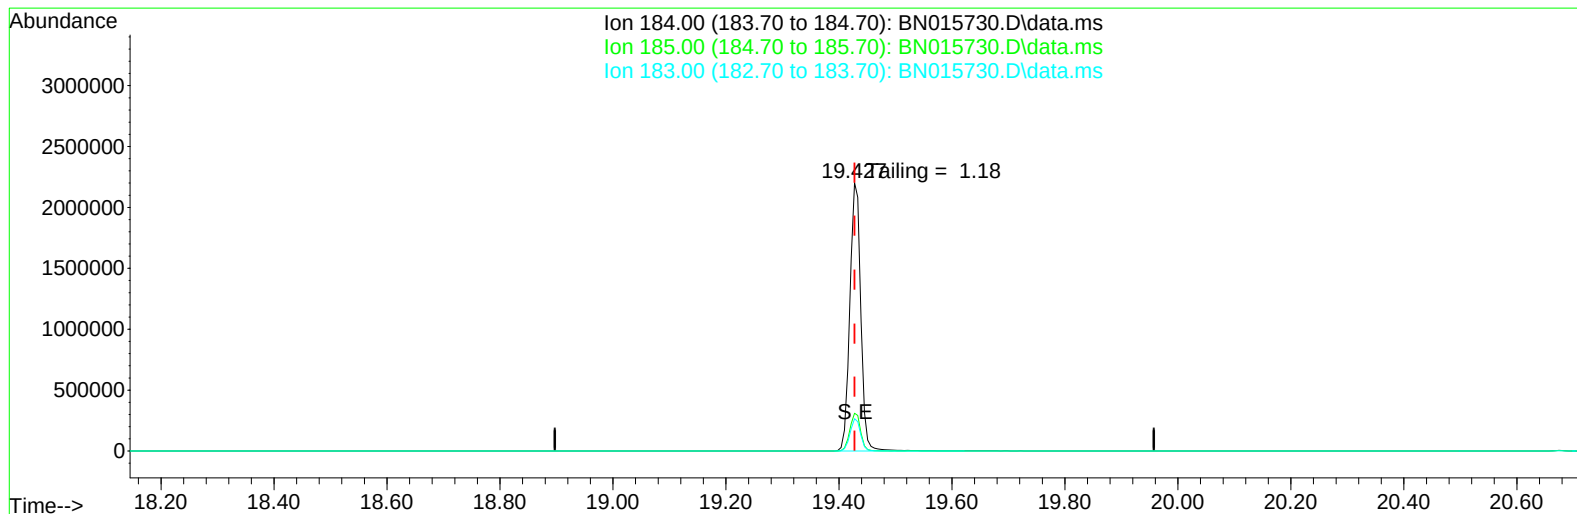

TIC: BN015730.D\data.ms

(77) Benzidine

19.427min (+ 0.000) 0.00 ng

response 2968440

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.07
183.00	13.20	12.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/31/2021	BNA_N	<u>BN015730.D</u>
Compound Name	Response	Retention Time
DDT	1416827	20.674
DDD	9325	20.233
DDE	1491	19.721
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10816	1427643	0.76

Instrument :
BNA_N
ClientSampleId :
DFTPP