


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073121\
 Data File : BN015743.D
 Acq On : 31 Jul 2021 20:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 31 04:53:33 2021

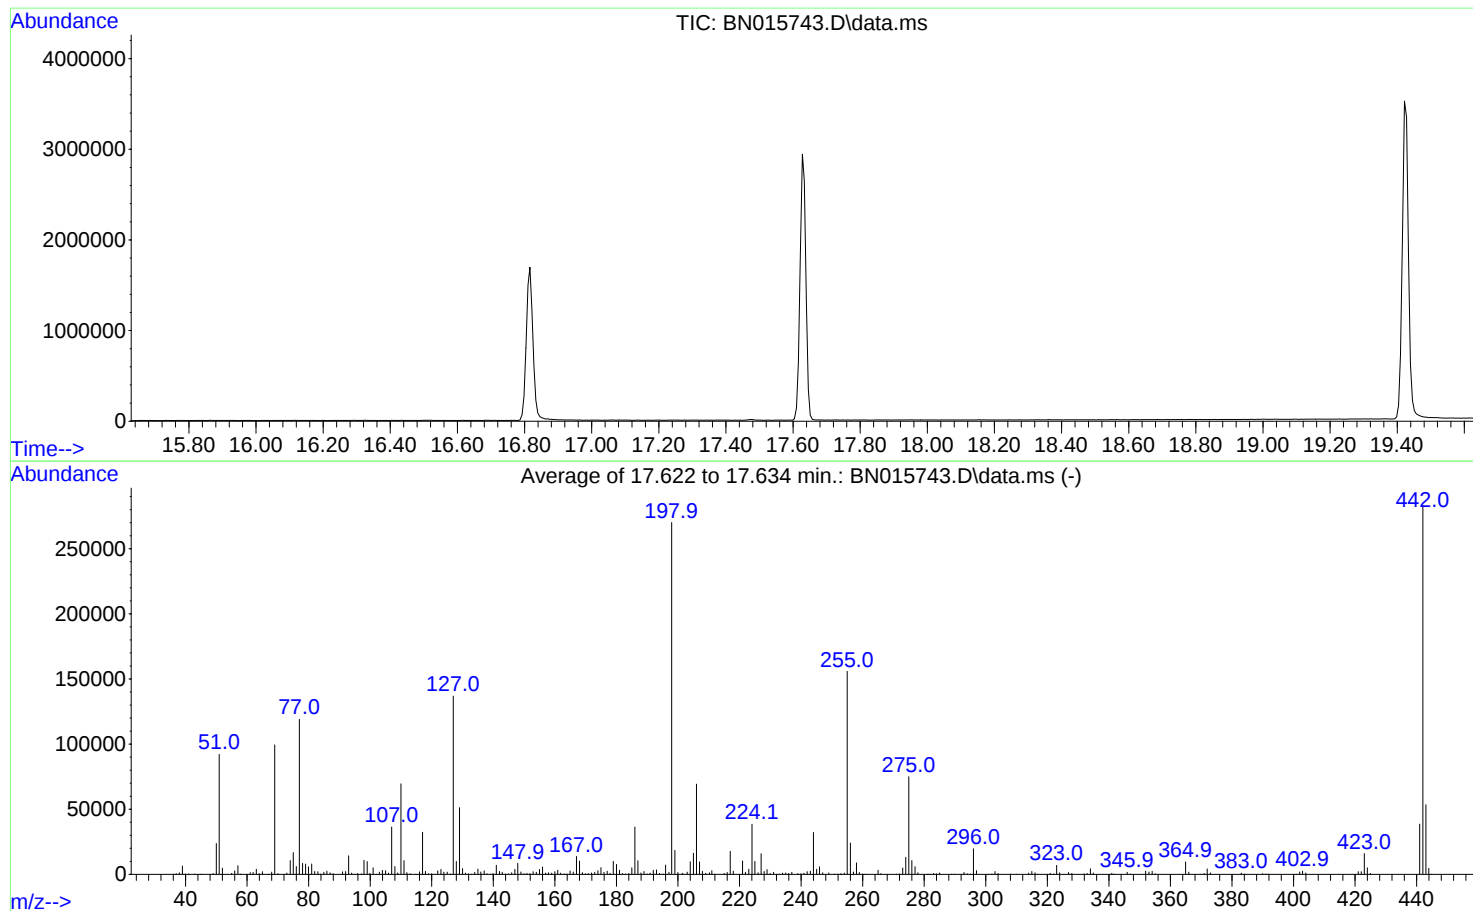




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	92146	PASS
68	69	0.00	2	1.7	1724	PASS
69	198	0.00	100	36.8	99371	PASS
70	69	0.00	2	0.6	637	PASS
127	198	10	80	50.7	136813	PASS
197	198	0.00	2	0.6	1566	PASS
198	198	100	100	100.0	270080	PASS
199	198	5	9	6.8	18434	PASS
275	198	10	60	27.7	74885	PASS
365	198	1	100	3.6	9637	PASS
441	198	0.01	100	14.3	38624	PASS
442	442	50	100	100.0	282432	PASS
443	442	15	24	18.9	53419	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073121\
Data File : BN015743.D
Acq On : 31 Jul 2021 20:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 02 05:38:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 30 07:20:03 2021
Response via : Initial Calibration

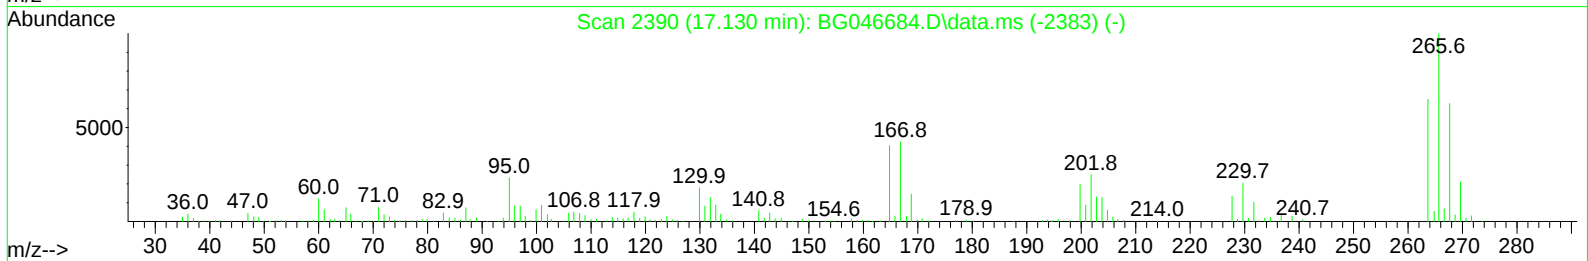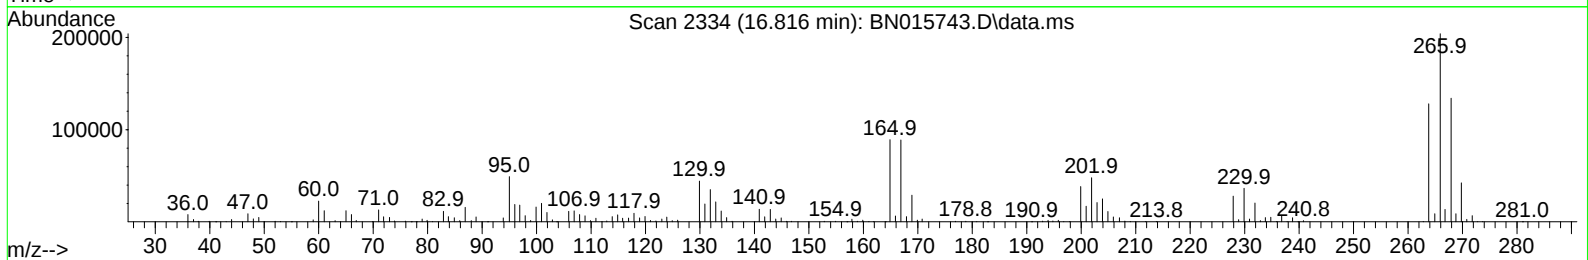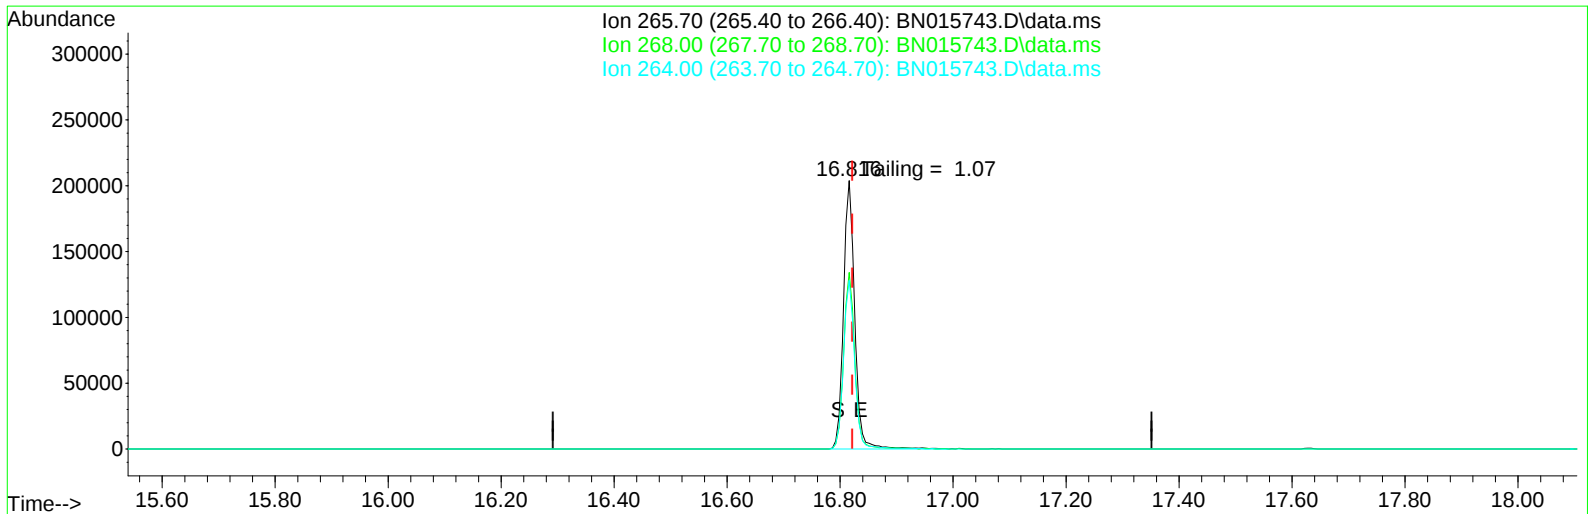

TIC: BN015743.D\data.ms

(70) Pentachlorophenol (C)

16.816min (-0.006) 22820.69 ng




response 279382

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.79
264.00	61.60	62.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073121\
 Data File : BN015743.D
 Acq On : 31 Jul 2021 20:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Aug 02 05:38:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 30 07:20:03 2021
 Response via : Initial Calibration

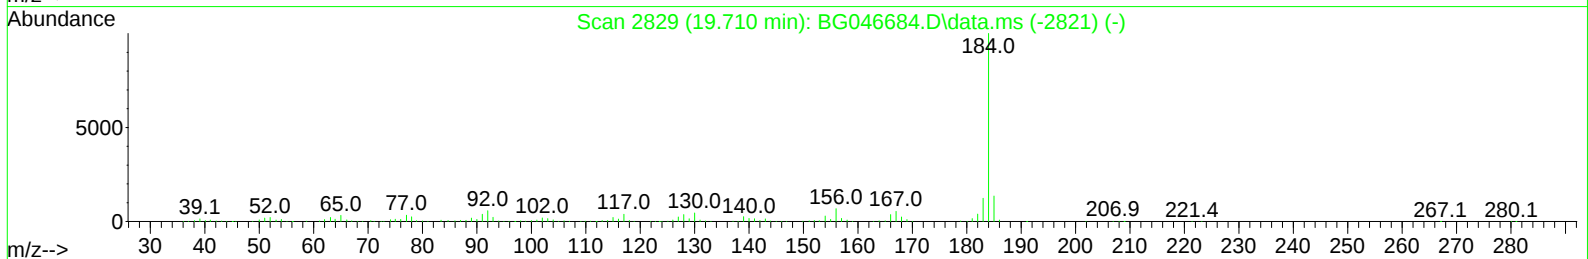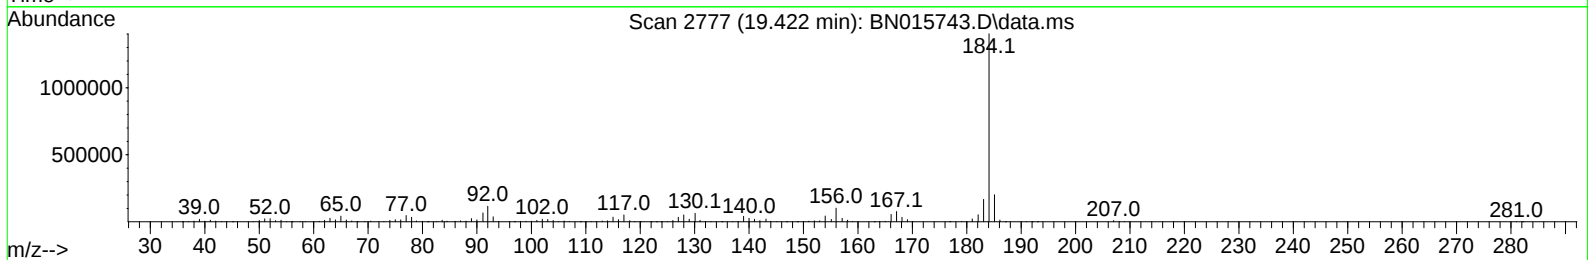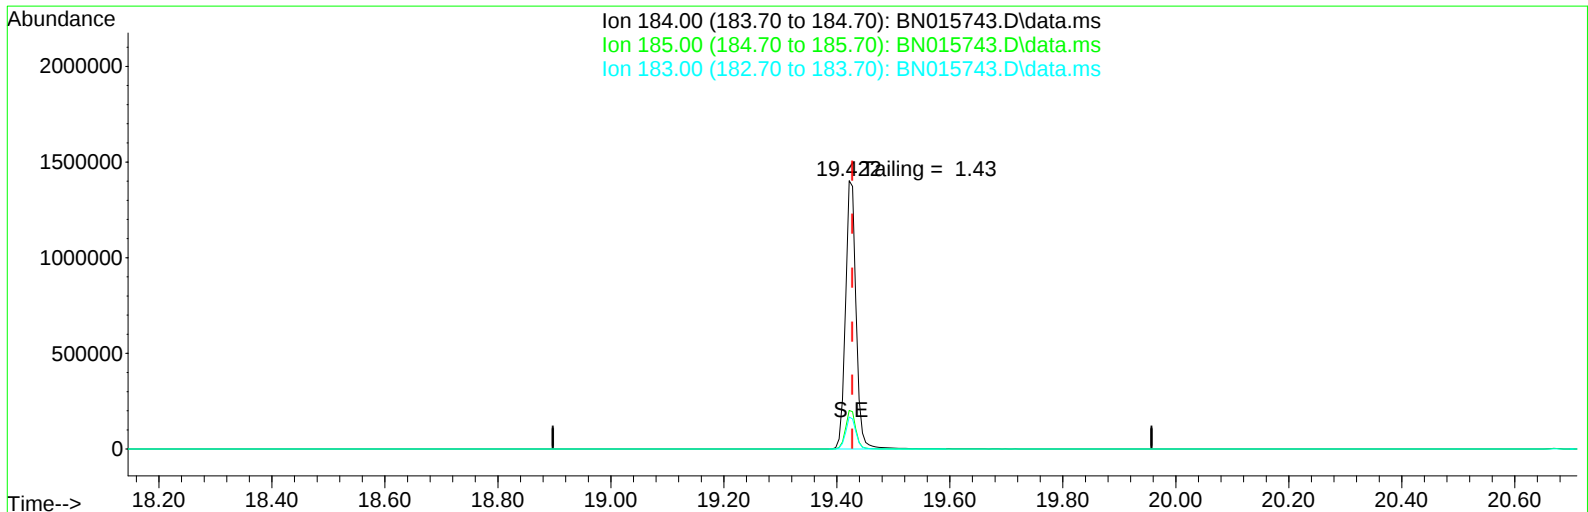

TIC: BN015743.D\data.ms

(77) Benzidine

19.422min (-0.006) 0.00 ng

response 1824584

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.38
183.00	13.20	11.95
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/31/2021	BNA_N	<u>BN015743.D</u>
Compound Name	Response	Retention Time
DDT	878694	20.669
DDD	6483	20.228
DDE	1064	19.722
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7547	886241	0.85

Instrument :
BNA_N
ClientSampleId :
DFTPP