
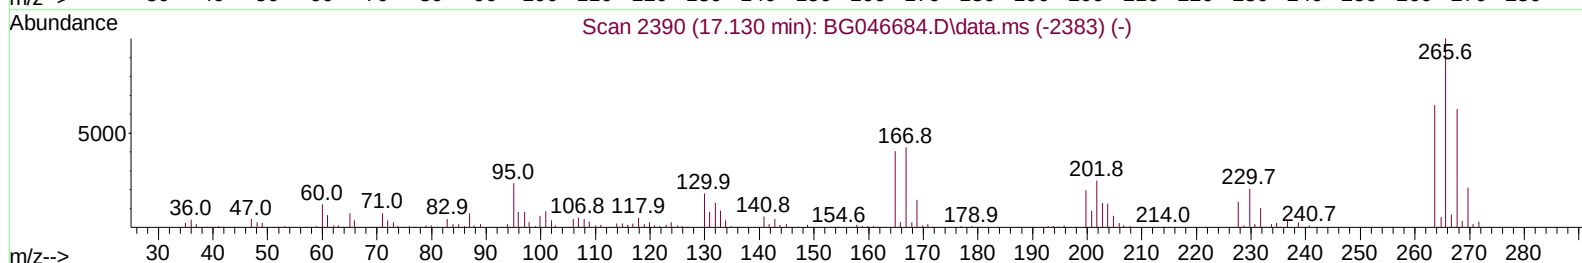
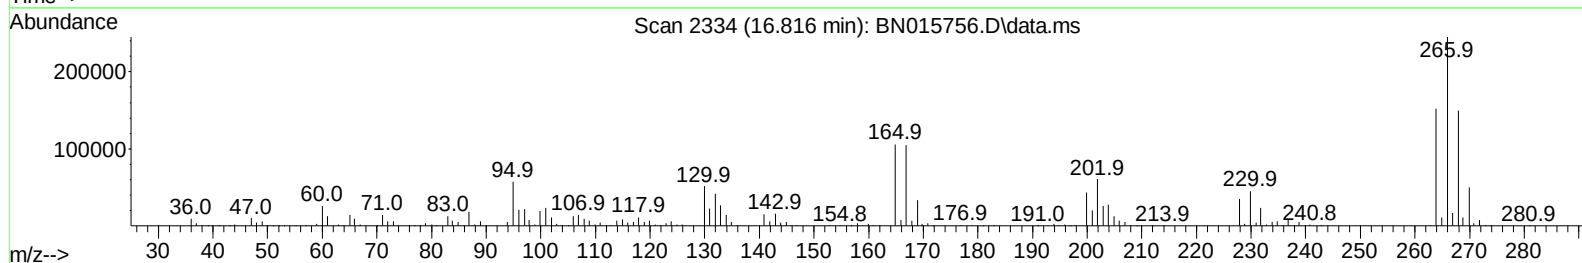


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080221\
Data File : BN015756.D
Acq On : 02 Aug 2021 08:24
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 14:23:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 30 07:20:03 2021
Response via : Initial Calibration

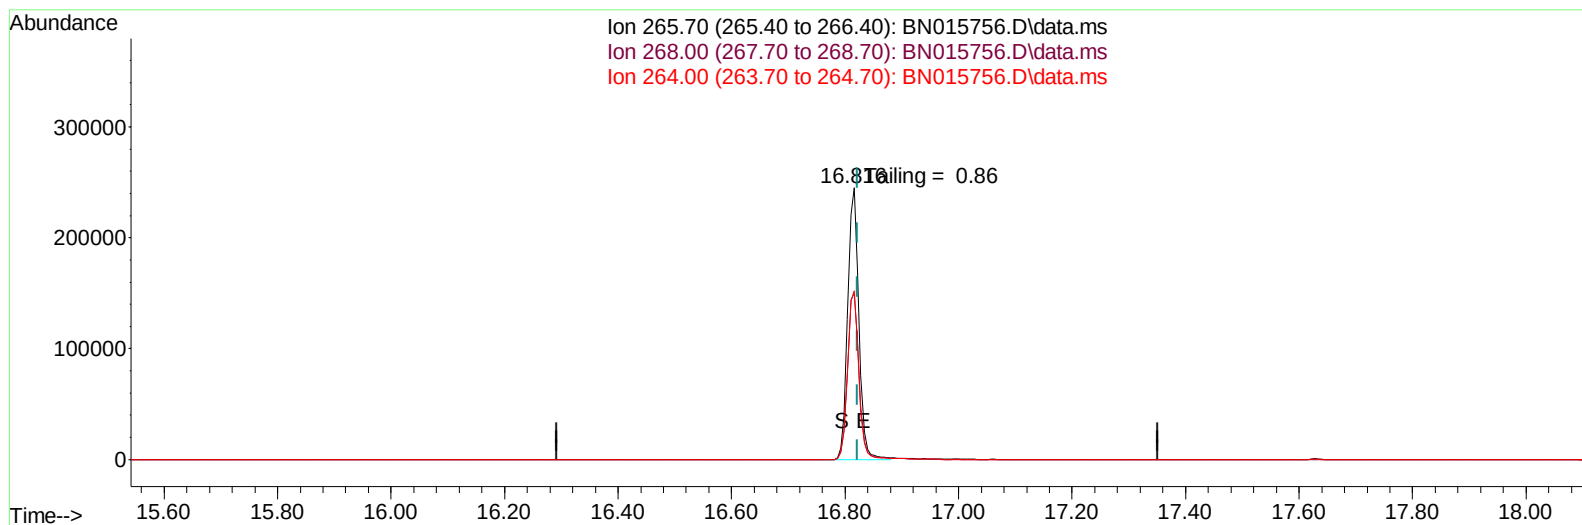




TIC: BN015756.D\data.ms

(70) Pentachlorophenol (C)**16.816min (-0.006) 21494.96 ng****response 334675**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.08
264.00	61.60	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080221\
Data File : BN015756.D
Acq On : 02 Aug 2021 08:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 14:23:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 30 07:20:03 2021
Response via : Initial Calibration

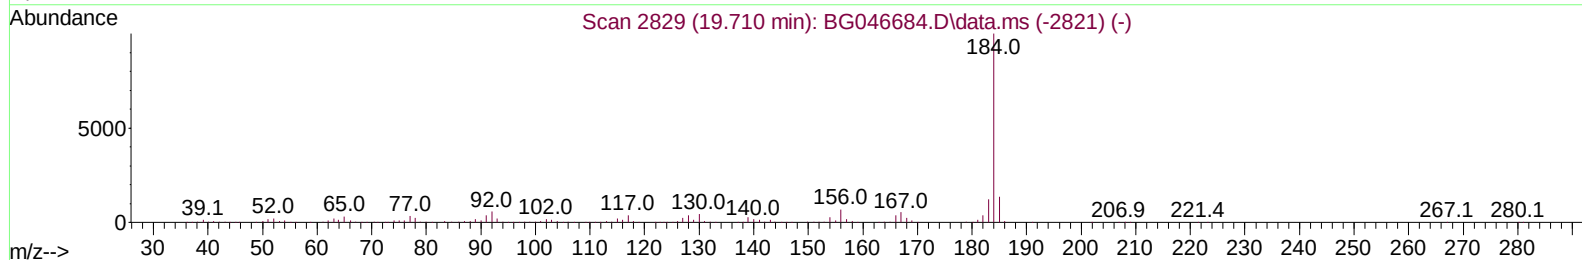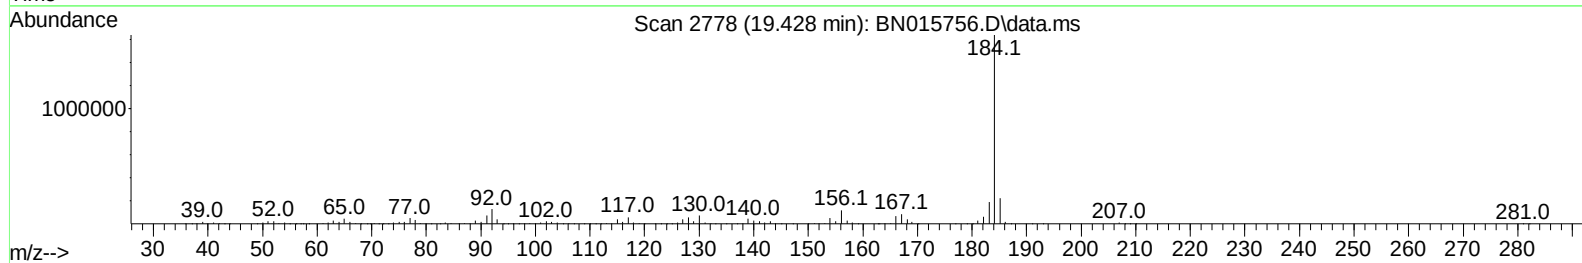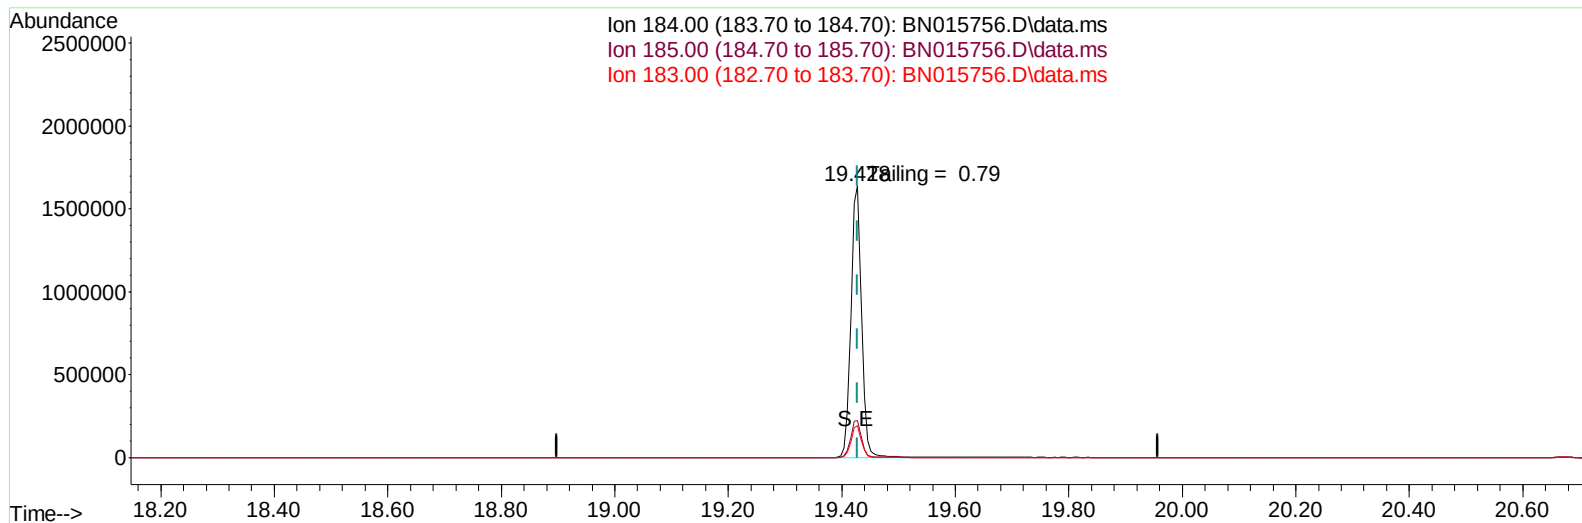

TIC: BN015756.D\data.ms

(77) Benzidine

19.428min (+ 0.000) 0.00 ng

response 2127398

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.70
183.00	13.20	11.62
0.00	0.00	0.00