

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080221\
 Data File : BN015757.D
 Acq On : 02 Aug 2021 09:02
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Aug 02 14:19:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 02 14:09:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	36093	0.400	ng	0.00
7) Naphthalene-d8	10.571	136	158650	0.400	ng	0.00
13) Acenaphthene-d10	14.408	164	81796	0.400	ng	0.00
19) Phenanthrene-d10	17.164	188	149302	0.400	ng	0.00
29) Chrysene-d12	21.376	240	135112	0.400	ng	# 0.01
35) Perylene-d12	23.714	264	117621	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.383	112	34204	0.388	ng	0.00
5) Phenol-d6	6.951	99	40452	0.379	ng	0.00
8) Nitrobenzene-d5	8.924	82	37287	0.366	ng	0.00
11) 2-Methylnaphthalene-d10	12.158	152	95094	0.399	ng	0.00
14) 2,4,6-Tribromophenol	15.905	330	10191	0.344	ng	0.00
15) 2-Fluorobiphenyl	13.038	172	127088	0.390	ng	0.00
27) Fluoranthene-d10	19.207	212	149527	0.385	ng	0.00
31) Terphenyl-d14	19.812	244	129937	0.389	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.345	88	4934	0.422	ng	# 95
3) n-Nitrosodimethylamine	3.714	42	8374	0.348	ng	# 98
6) bis(2-Chloroethyl)ether	7.218	93	39077	0.404	ng	99
9) Naphthalene	10.609	128	164901	0.397	ng	100
10) Hexachlorobutadiene	10.914	225	28866	0.398	ng	# 100
12) 2-Methylnaphthalene	12.234	142	106890	0.399	ng	100
16) Acenaphthylene	14.129	152	123130	0.365	ng	100
17) Acenaphthene	14.472	154	91149	0.387	ng	99
18) Fluorene	15.461	166	109037	0.387	ng	100
20) 4,6-Dinitro-2-methylph...	15.537	198	3342	0.439	ng	98
21) 4-Bromophenyl-phenylether	16.360	248	32880	0.375	ng	94
22) Hexachlorobenzene	16.470	284	39090	0.388	ng	99
23) Atrazine	16.628	200	19449	0.360	ng	99
24) Pentachlorophenol	16.811	266	9849	0.316	ng	99
25) Phenanthrene	17.200	178	173021	0.390	ng	100
26) Anthracene	17.297	178	138208	0.370	ng	100
28) Fluoranthene	19.237	202	181359	0.392	ng	100
30) Pyrene	19.599	202	175950	0.390	ng	100
32) Benzo(a)anthracene	21.355	228	157146	0.381	ng	100
33) Chrysene	21.408	228	174359	0.390	ng	100
34) Bis(2-ethylhexyl)phtha...	21.302	149	48341	0.434	ng	99
36) Indeno(1,2,3-cd)pyrene	26.113	276	152194	0.365	ng	100
37) Benzo(b)fluoranthene	23.005	252	166309	0.407	ng	100
38) Benzo(k)fluoranthene	23.053	252	168571	0.399	ng	100
39) Benzo(a)pyrene	23.611	252	130725	0.385	ng	100
40) Dibenzo(a,h)anthracene	26.134	278	124283	0.356	ng	100
41) Benzo(g,h,i)perylene	26.846	276	141289	0.388	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080221\
Data File : BN015757.D
Acq On : 02 Aug 2021 09:02
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Aug 02 14:19:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 02 14:09:59 2021
Response via : Initial Calibration




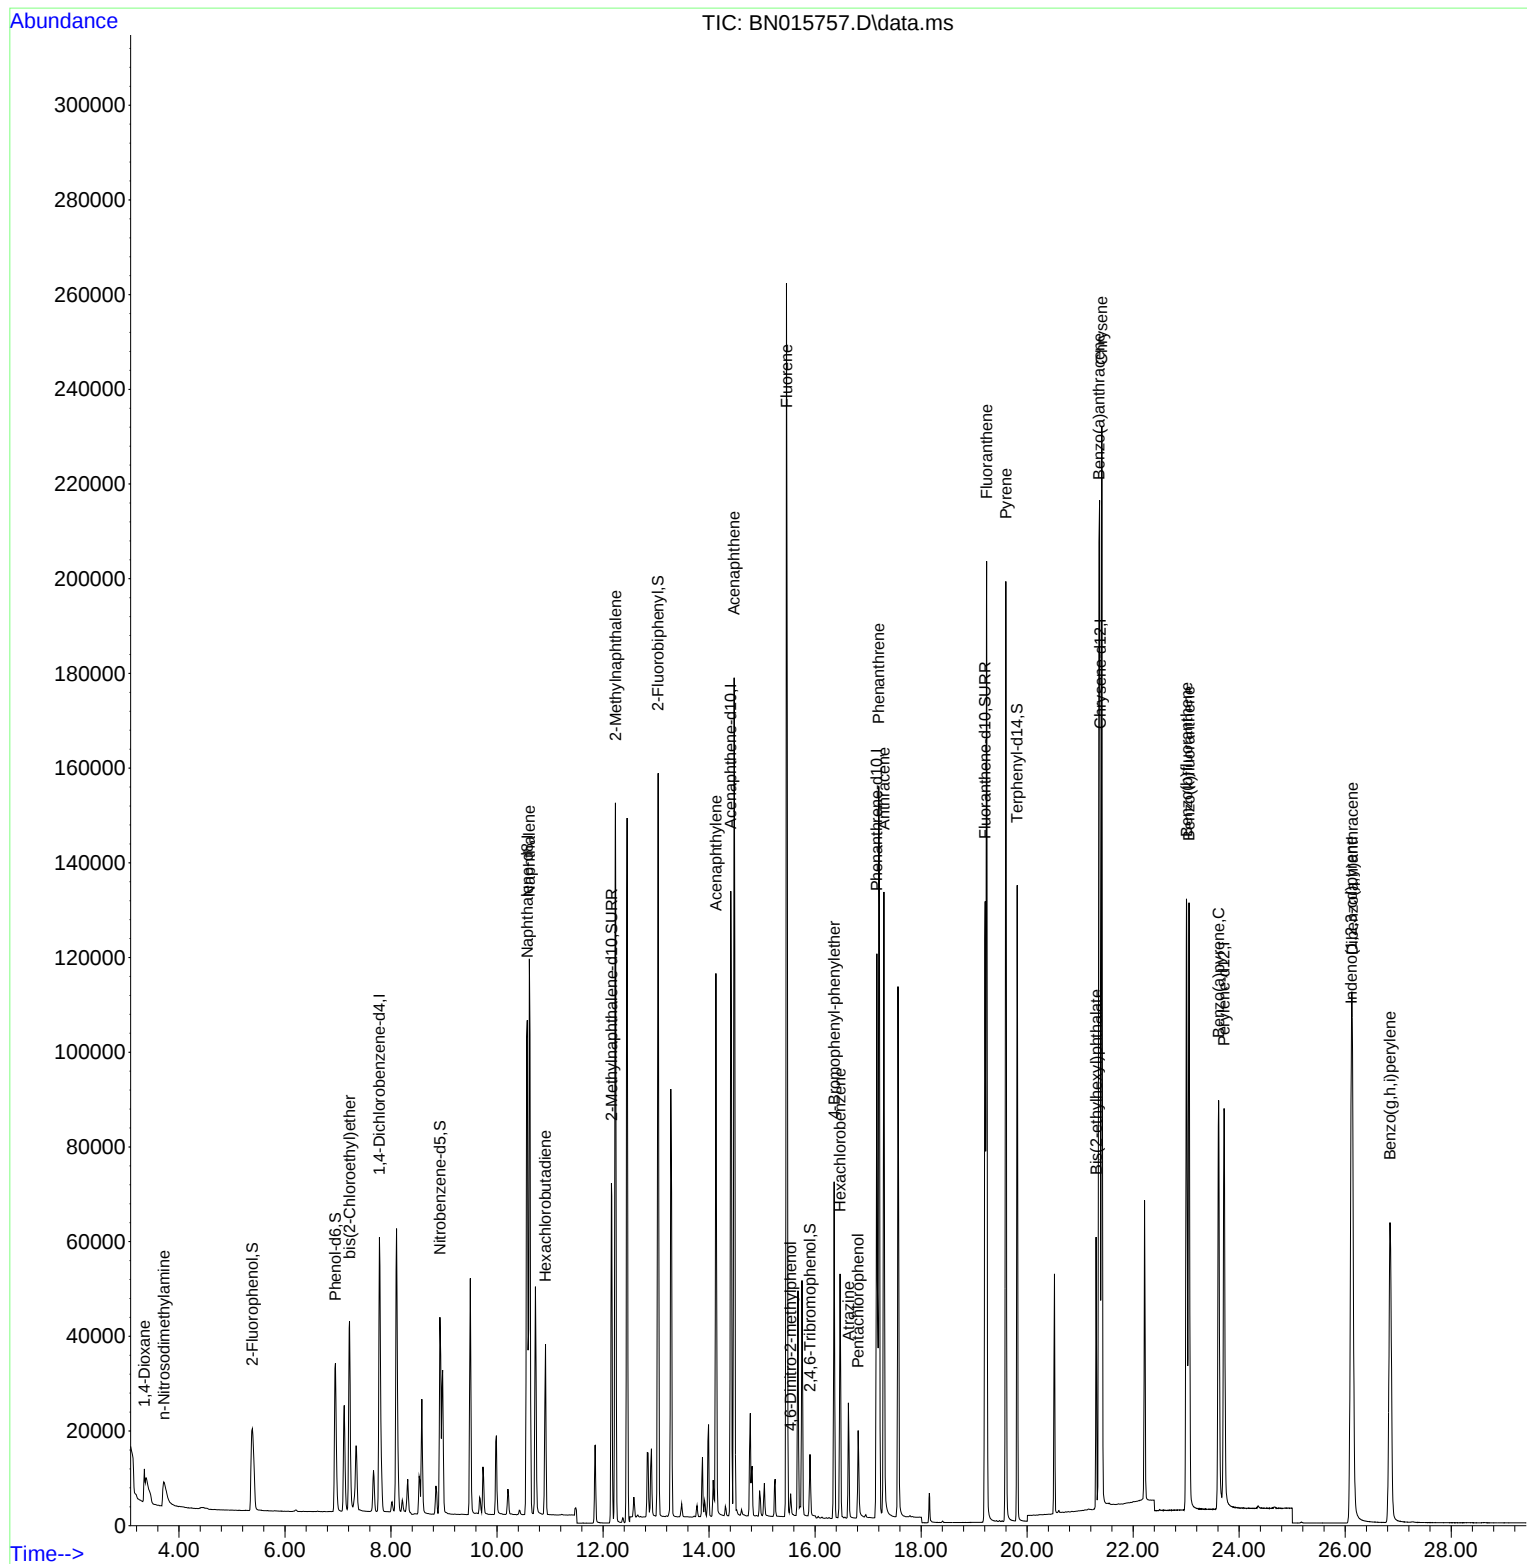




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.781 min Scan# 510
Delta R.T. -0.009 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 36093
Ion Ratio Lower Upper
152 100
150 156.6 123.5 185.3
115 59.7 46.8 70.2

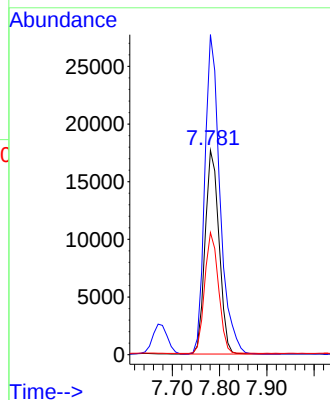

#2
1,4-Dioxane
Concen: 0.422 ng
RT: 3.345 min Scan# 29
Delta R.T. -0.010 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion: 88 Resp: 4934
Ion Ratio Lower Upper
88 100
43 22.9 23.1 34.7#
58 75.5 62.2 93.4


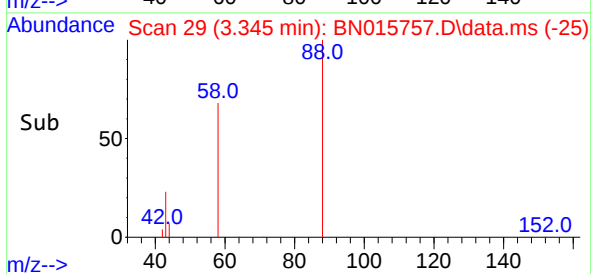
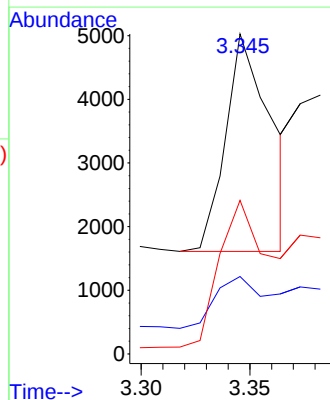



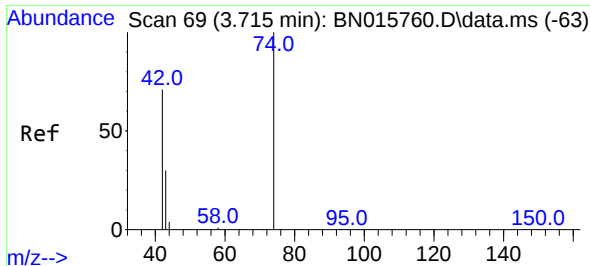

#3
n-Nitrosodimethylamine
Concen: 0.348 ng
RT: 3.714 min Scan# 69
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 42 Resp: 8374
Ion Ratio Lower Upper
42 100
74 145.2 114.4 171.6
44 8.3 3.6 5.4#

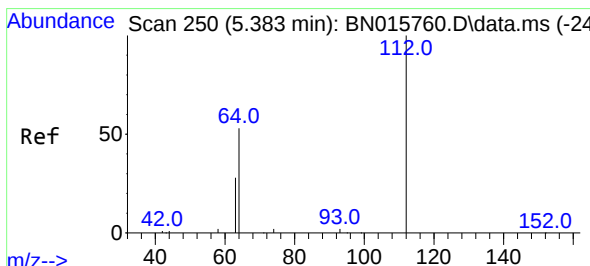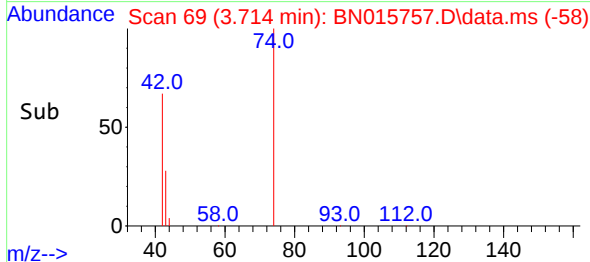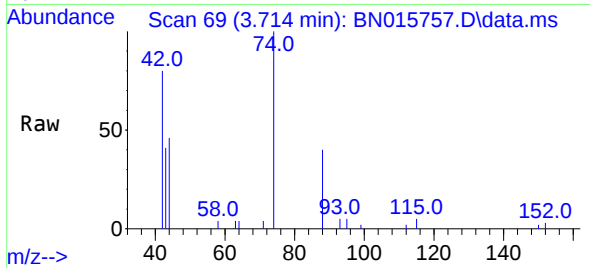

#4
2-Fluorophenol
Concen: 0.388 ng
RT: 5.383 min Scan# 250
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion: 112 Resp: 34204
Ion Ratio Lower Upper
112 100
64 52.7 42.2 63.4
63 27.5 22.2 33.2


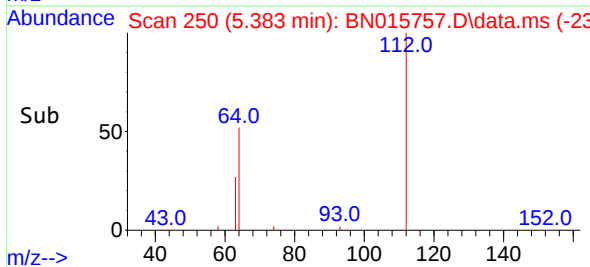

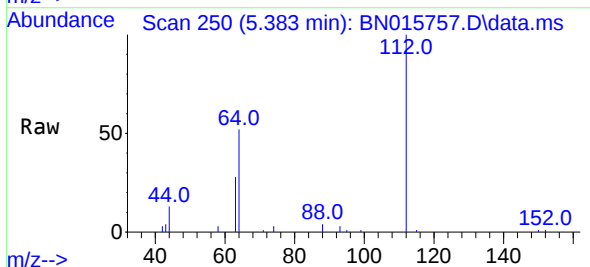


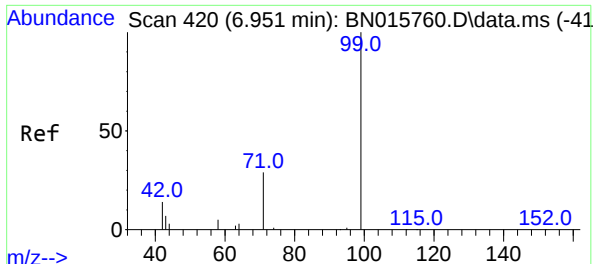

#5
Phenol-d6
Concen: 0.379 ng
RT: 6.951 min Scan# 420
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 99 Resp: 40452
Ion Ratio Lower Upper
99 100
42 16.2 13.2 19.8
71 29.8 23.8 35.8

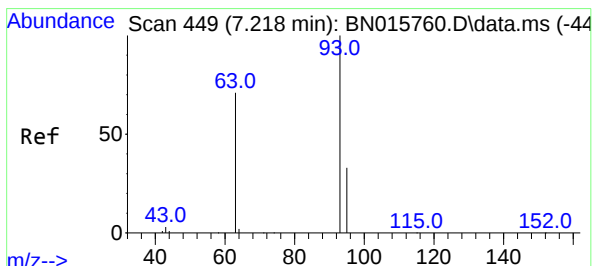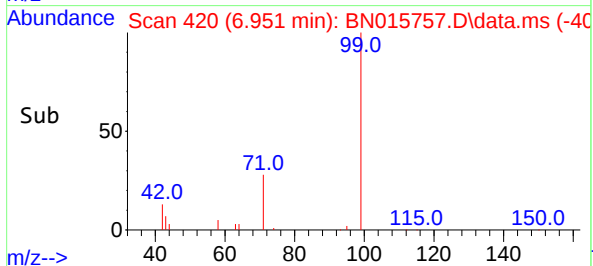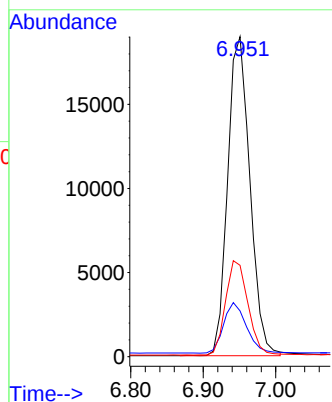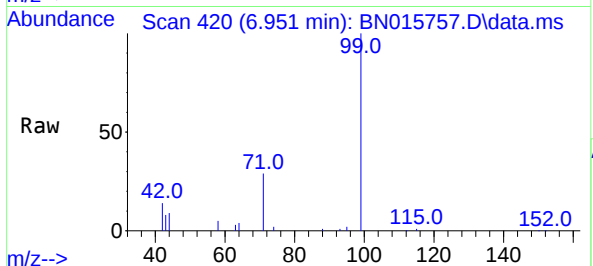

#6
bis(2-Chloroethyl)ether
Concen: 0.404 ng
RT: 7.218 min Scan# 449
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion: 93 Resp: 39077
Ion Ratio Lower Upper
93 100
63 73.9 58.8 88.2
95 33.5 26.6 39.8


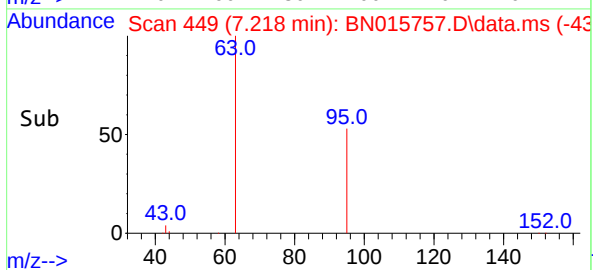
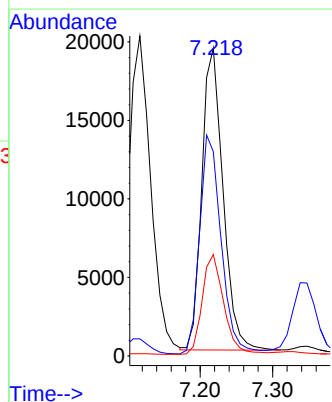
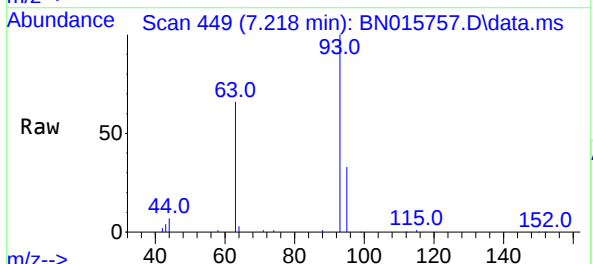




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.571 min Scan# 746
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	158650
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.7	13.1
54	4.4	3.9	5.9
68	3.7	3.3	4.9

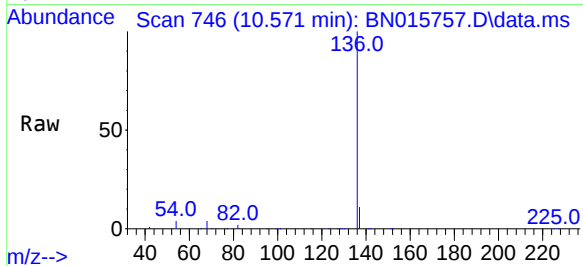

#8
Nitrobenzene-d5
Concen: 0.366 ng
RT: 8.924 min Scan# 616
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion:	82	Resp:	37287
Ion	Ratio	Lower	Upper
82	100		
128	36.3	26.2	39.4
54	52.9	45.1	67.7


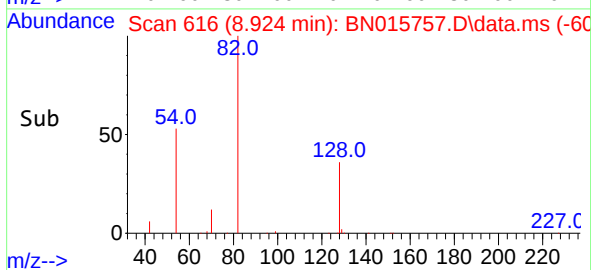

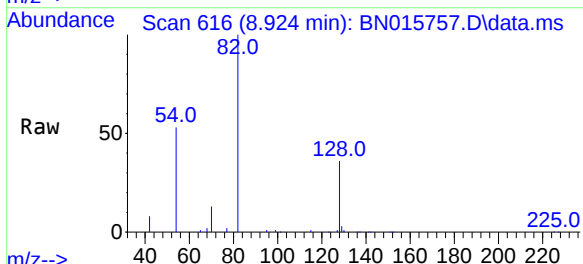




#9
Naphthalene
Concen: 0.397 ng
RT: 10.609 min Scan# 749
Delta R.T. -0.013 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:128 Resp: 164901
Ion Ratio Lower Upper
128 100
129 10.9 8.8 13.2
127 13.0 10.2 15.2

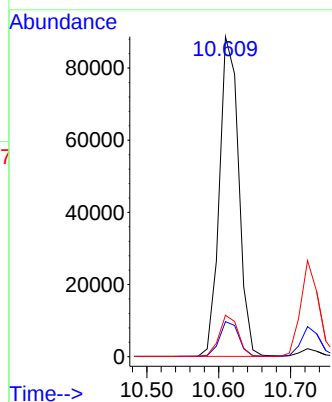

#10
Hexachlorobutadiene
Concen: 0.398 ng
RT: 10.914 min Scan# 773
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion:225 Resp: 28866
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.1 51.5 77.3


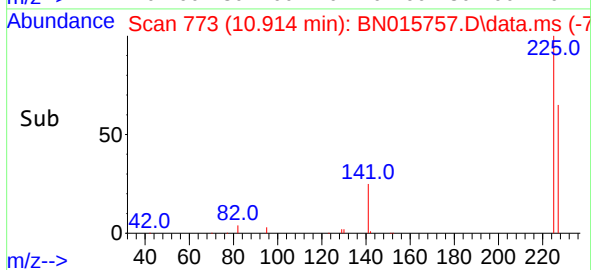
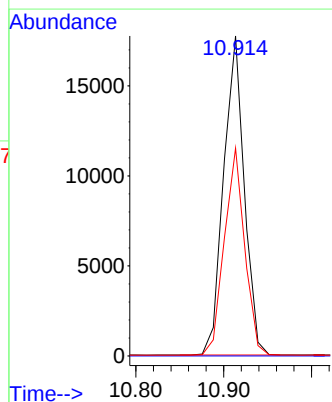





#11
2-Methylnaphthalene-d10
Concen: 0.399 ng
RT: 12.158 min Scan# 966
Delta R.T. -0.005 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:152 Resp: 95094
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.4

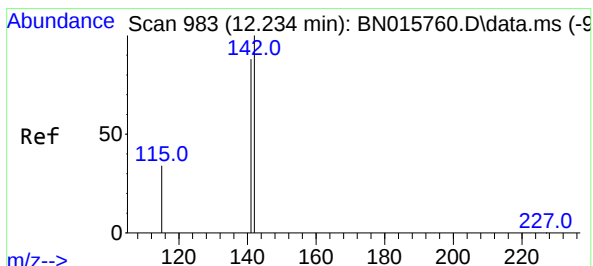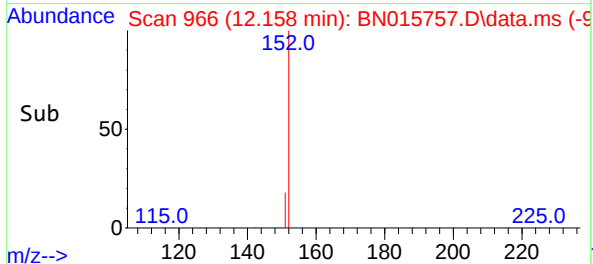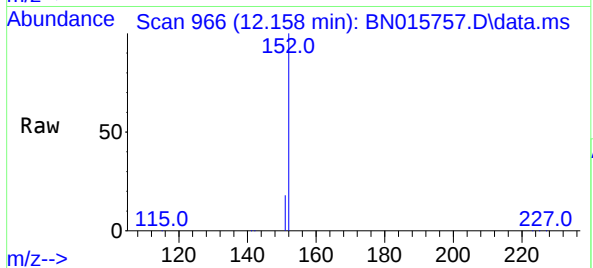

#12
2-Methylnaphthalene
Concen: 0.399 ng
RT: 12.234 min Scan# 983
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion:142 Resp: 106890
Ion Ratio Lower Upper
142 100
141 87.8 70.5 105.7
115 33.8 27.4 41.0


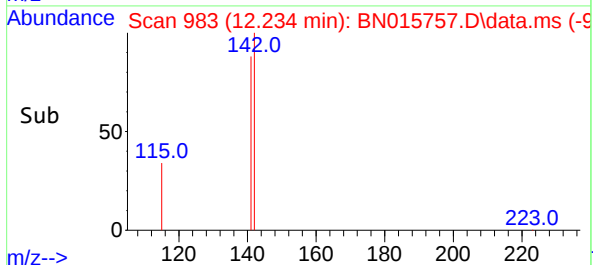

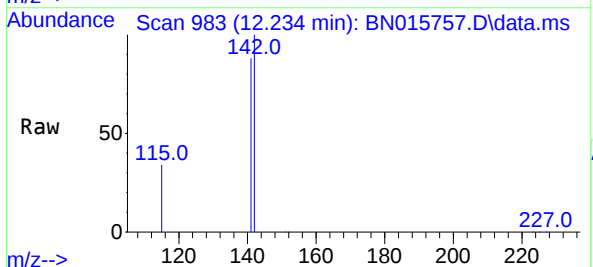




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.408 min Scan# 1194
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 81796
Ion Ratio Lower Upper
164 100
162 103.4 84.2 126.2
160 48.4 39.8 59.6

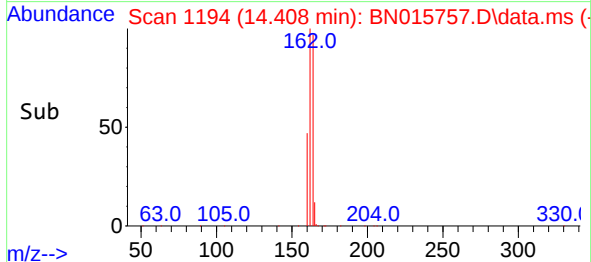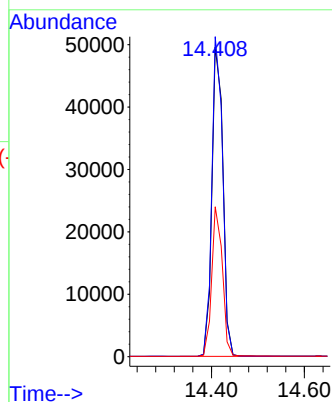

#14
2,4,6-Tribromophenol
Concen: 0.344 ng
RT: 15.905 min Scan# 1312
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion:330 Resp: 10191
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 34.8 28.2 42.2


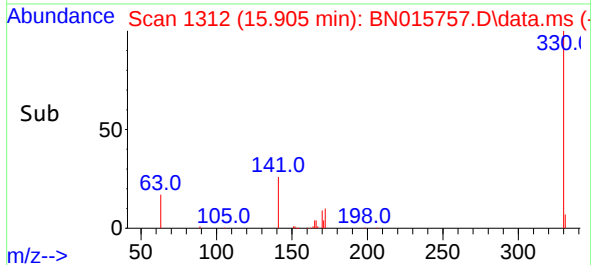
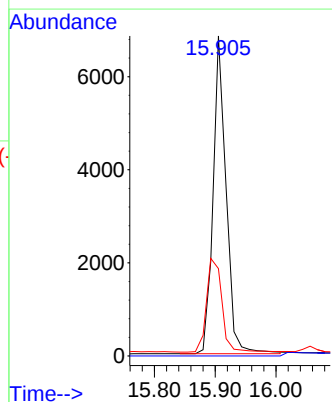
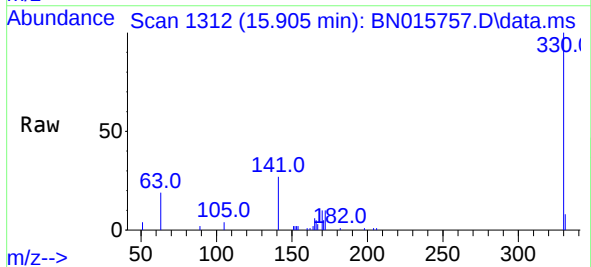




#15
2-Fluorobiphenyl
Concen: 0.390 ng
RT: 13.038 min Scan# 1086
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:172 Resp: 127088
Ion Ratio Lower Upper
172 100
171 34.5 27.8 41.8
170 22.9 18.7 28.1

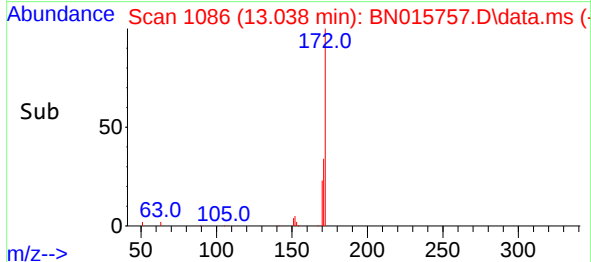

#16
Acenaphthylene
Concen: 0.365 ng
RT: 14.129 min Scan# 1172
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion:152 Resp: 123130
Ion Ratio Lower Upper
152 100
151 19.7 15.7 23.5
153 13.2 10.5 15.7


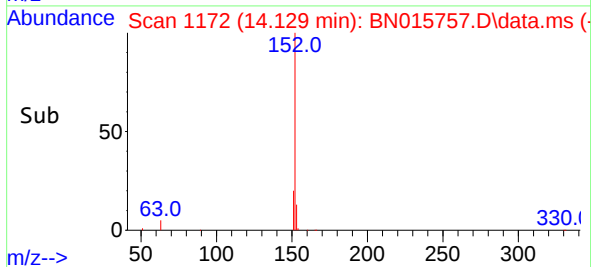

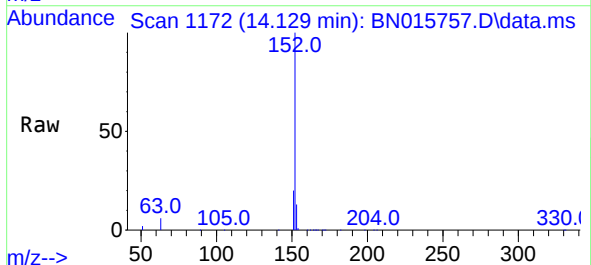




#17
Acenaphthene
Concen: 0.387 ng
RT: 14.472 min Scan# 1199
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:154 Resp: 91149
Ion Ratio Lower Upper
154 100
153 112.5 90.5 135.7
152 55.2 44.4 66.6



#18
Fluorene
Concen: 0.387 ng
RT: 15.461 min Scan# 1277
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion:166 Resp: 109037
Ion Ratio Lower Upper
166 100
165 97.4 78.2 117.2
167 13.4 10.7 16.1


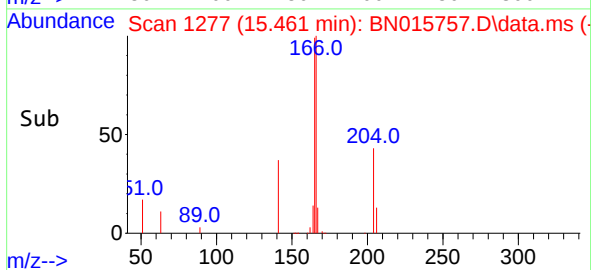






#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.164 min Scan# 1415
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 149302
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.8 7.7 11.5

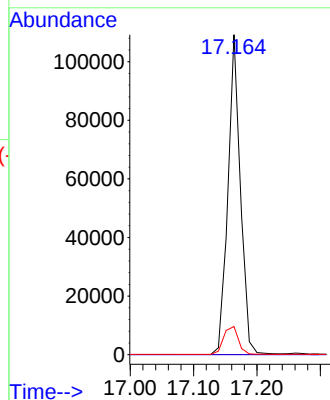

#20
4,6-Dinitro-2-methylphenol
Concen: 0.439 ng
RT: 15.537 min Scan# 1283
Delta R.T. -0.001 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion:198 Resp: 3342
Ion Ratio Lower Upper
198 100
182 13.2 11.1 16.7
77 0.0 0.0 0.0


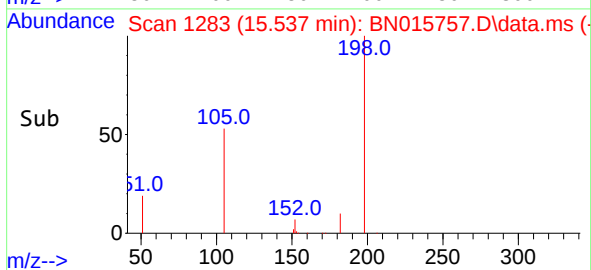
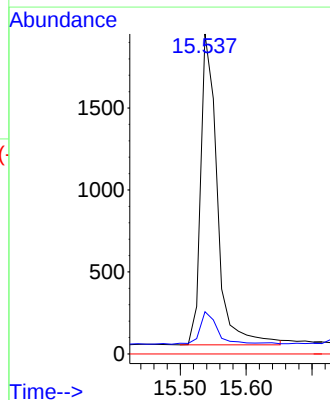





#21
4-Bromophenyl-phenylether
Concen: 0.375 ng
RT: 16.360 min Scan# 1349
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 32880
Ion Ratio Lower Upper
248 100
250 97.8 75.8 113.6
141 58.6 52.8 79.2



#22
Hexachlorobenzene
Concen: 0.388 ng
RT: 16.470 min Scan# 1358
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion:284 Resp: 39090
Ion Ratio Lower Upper
284 100
142 36.4 29.4 44.2
249 29.3 23.8 35.6



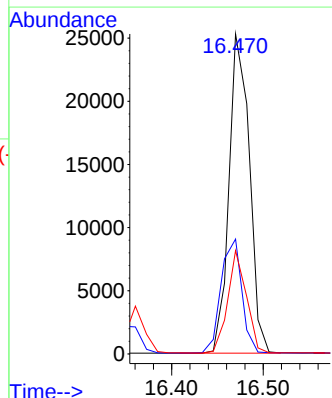



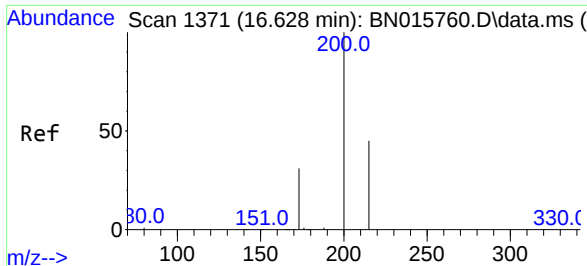

#23
Atrazine
Concen: 0.360 ng
RT: 16.628 min Scan# 1371
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	200	Resp:	19449
Ion Ratio	Lower	Upper	
200	100		
173	29.6	25.0	37.6
215	45.5	36.3	54.5

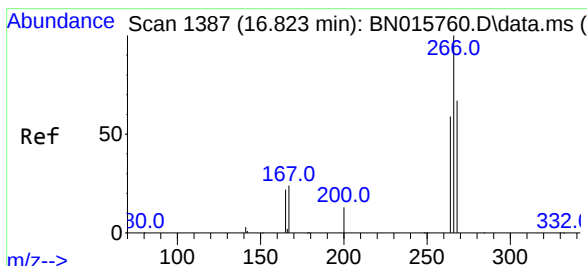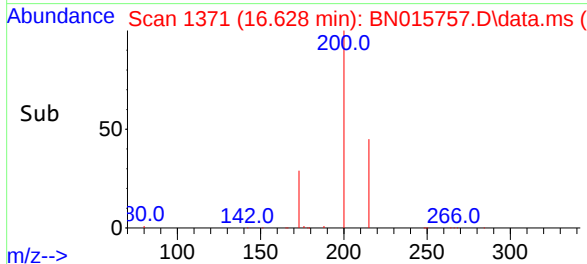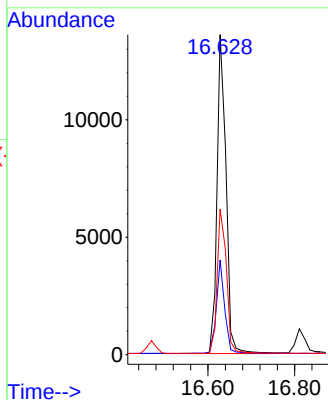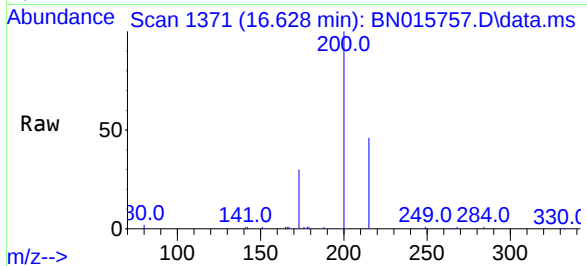

#24
Pentachlorophenol
Concen: 0.316 ng
RT: 16.811 min Scan# 1386
Delta R.T. -0.012 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion:	266	Resp:	9849
Ion Ratio	Lower	Upper	
266	100		
264	61.7	49.7	74.5
268	63.9	51.8	77.6


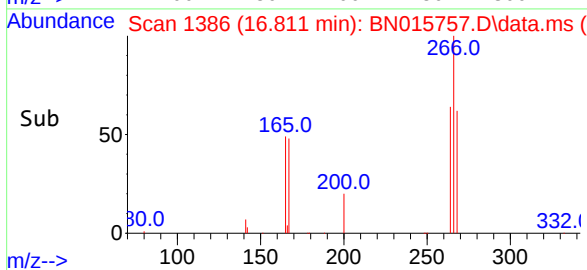
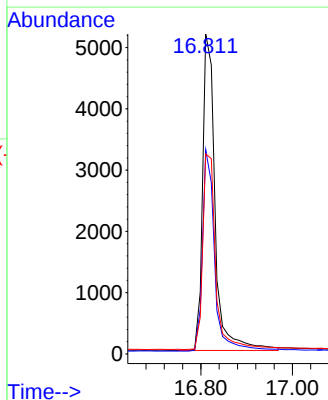
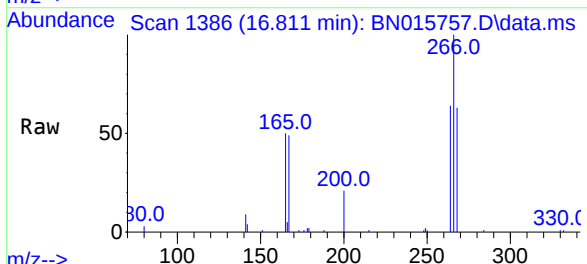




#25
Phenanthrene
Concen: 0.390 ng
RT: 17.200 min Scan# 1418
Delta R.T. -0.012 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:178 Resp: 173021
Ion Ratio Lower Upper
178 100
176 18.9 15.1 22.7
179 15.3 12.2 18.4



#26
Anthracene
Concen: 0.370 ng
RT: 17.297 min Scan# 1426
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion:178 Resp: 138208
Ion Ratio Lower Upper
178 100
176 18.3 14.6 22.0
179 15.2 12.2 18.4


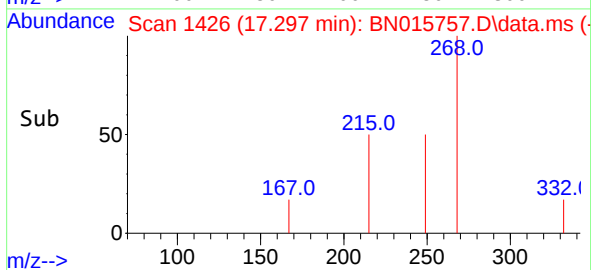






#27
Fluoranthene-d10
Concen: 0.385 ng
RT: 19.207 min Scan# 1725
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 149527
Ion Ratio Lower Upper
212 100
106 13.4 10.8 16.2
104 7.4 6.0 9.0

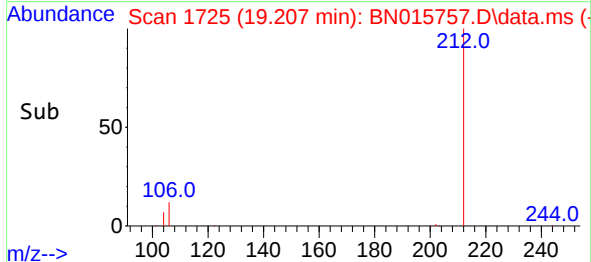

#28
Fluoranthene
Concen: 0.392 ng
RT: 19.237 min Scan# 1731
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion:202 Resp: 181359
Ion Ratio Lower Upper
202 100
101 11.3 9.0 13.6
203 17.3 13.8 20.8


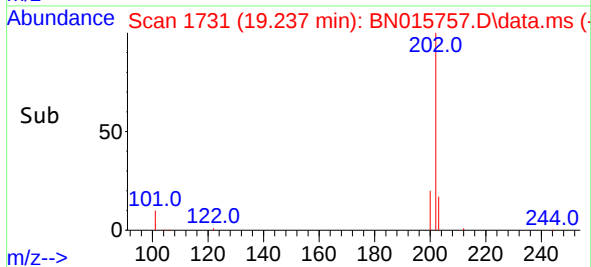

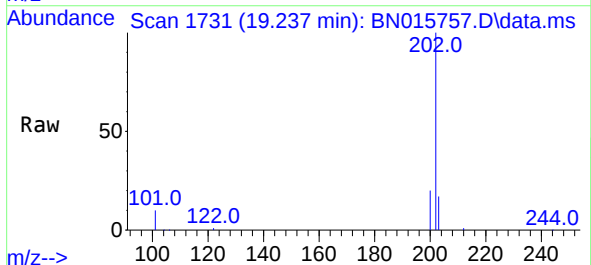


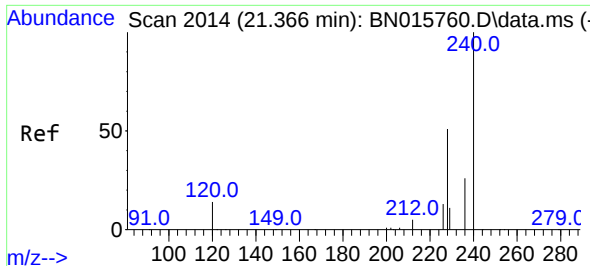

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.376 min Scan# 2015
Delta R.T. 0.010 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:240 Resp: 135112
Ion Ratio Lower Upper
240 100
120 6.3 11.4 17.0#
236 25.1 21.2 31.8

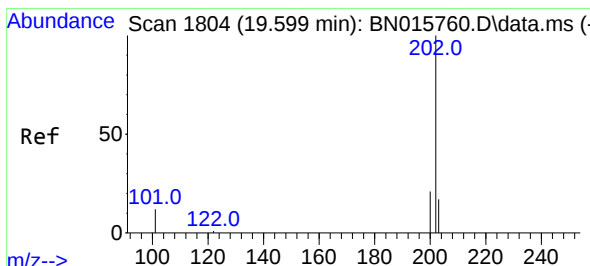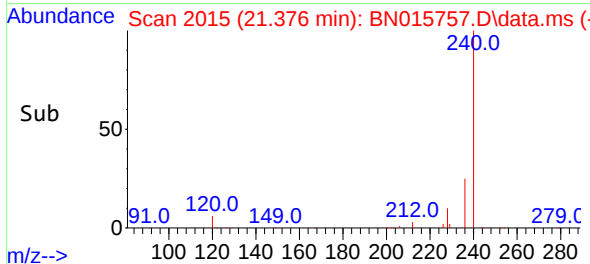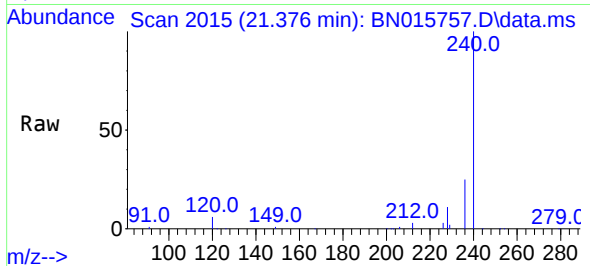

#30
Pyrene
Concen: 0.390 ng
RT: 19.599 min Scan# 1804
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion:202 Resp: 175950
Ion Ratio Lower Upper
202 100
200 20.6 16.5 24.7
203 17.4 13.9 20.9


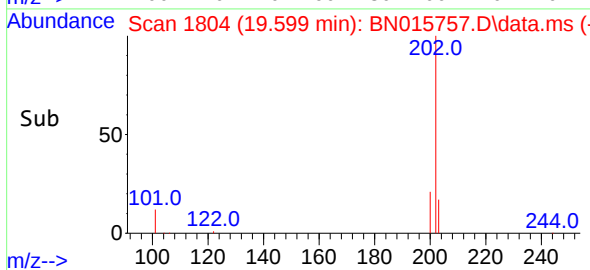

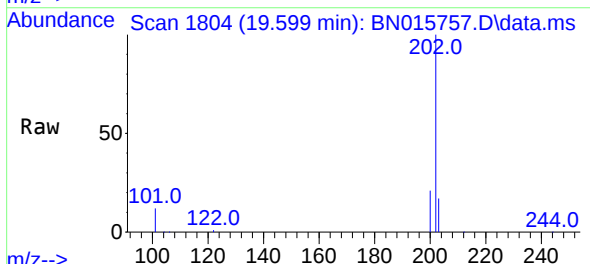




#31
 Terphenyl-d14
 Concen: 0.389 ng
 RT: 19.812 min Scan# 1847
 Delta R.T. -0.000 min
 Lab File: BN015757.D
 Acq: 02 Aug 2021 09:02




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:244 Resp: 129937
 Ion Ratio Lower Upper
 244 100
 212 7.4 5.9 8.9
 122 11.9 9.7 14.5

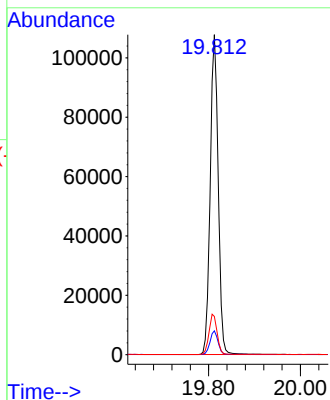

#32
 Benzo(a)anthracene
 Concen: 0.381 ng
 RT: 21.355 min Scan# 2013
 Delta R.T. -0.000 min
 Lab File: BN015757.D
 Acq: 02 Aug 2021 09:02

Tgt Ion:228 Resp: 157146
 Ion Ratio Lower Upper
 228 100
 226 26.8 21.2 31.8
 229 19.5 15.6 23.4

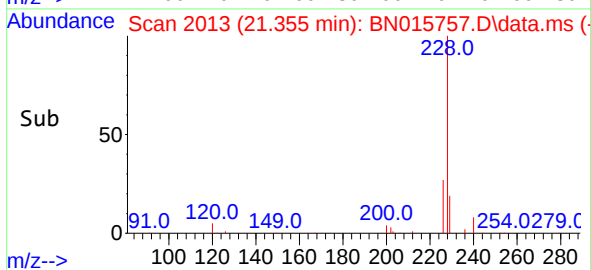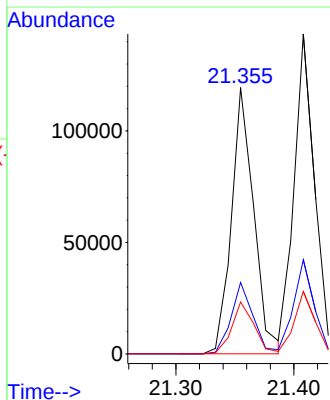







#33
Chrysene
Concen: 0.390 ng
RT: 21.408 min Scan# 2018
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:228 Resp: 174359




Ion	Ratio	Lower	Upper
228	100		
226	29.5	23.3	34.9
229	19.5	15.7	23.5

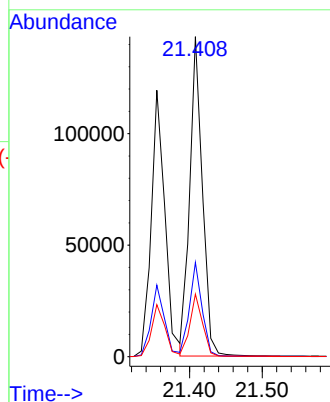

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.434 ng
RT: 21.302 min Scan# 2008
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion:149 Resp: 48341

Ion	Ratio	Lower	Upper
149	100		
167	26.1	21.2	31.8
279	3.9	3.2	4.8

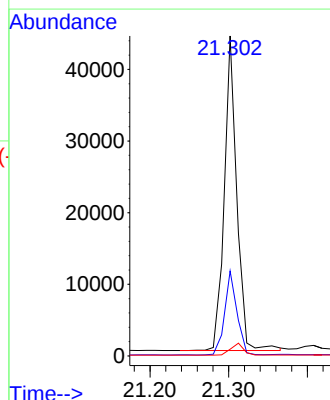







#35
Perylene-d12
Concen: 0.400 ng
RT: 23.714 min Scan# 2494
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:264 Resp: 117621




Ion	Ratio	Lower	Upper
264	100		
260	24.7	19.5	29.3
265	24.9	19.2	28.8

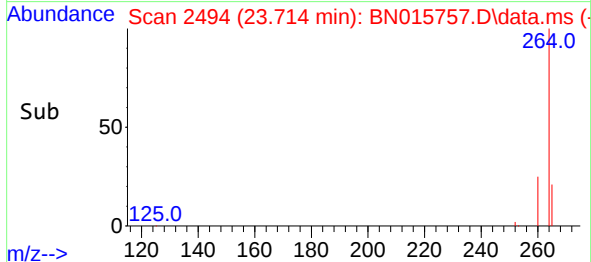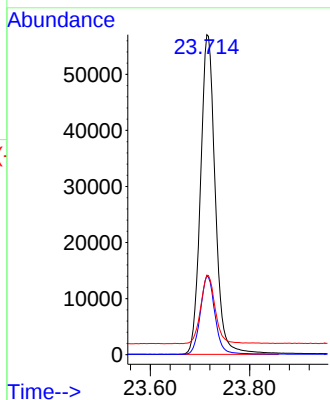

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.365 ng
RT: 26.113 min Scan# 3195
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion:276 Resp: 152194

Ion	Ratio	Lower	Upper
276	100		
138	24.4	19.6	29.4
277	24.9	20.0	30.0


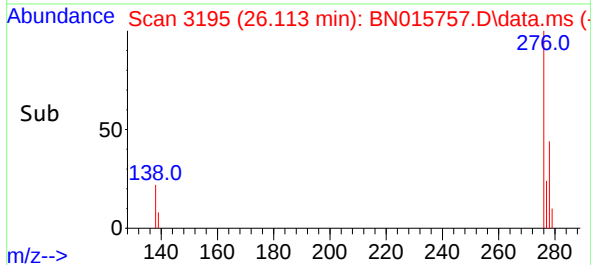
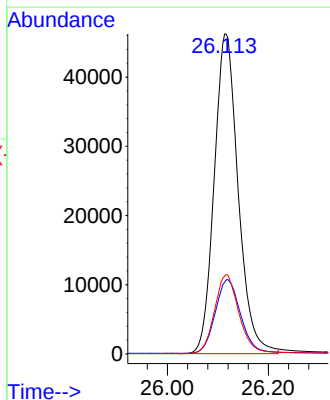
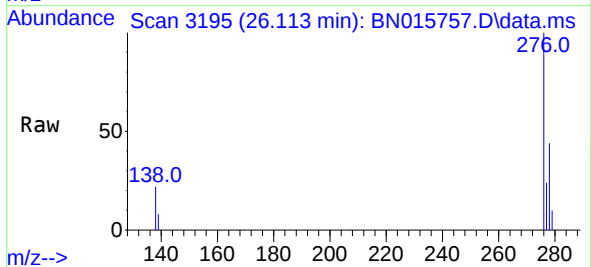




#37
Benzo(b)fluoranthene
Concen: 0.407 ng
RT: 23.005 min Scan# 2287
Delta R.T. 0.003 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:252 Resp: 166309
Ion Ratio Lower Upper
252 100
253 22.2 17.7 26.5
125 10.3 8.2 12.4

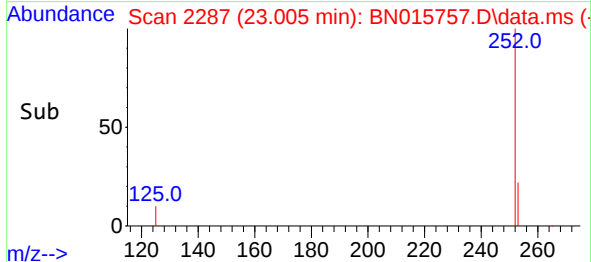

#38
Benzo(k)fluoranthene
Concen: 0.399 ng
RT: 23.053 min Scan# 2301
Delta R.T. 0.003 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02


Tgt Ion:252 Resp: 168571
Ion Ratio Lower Upper
252 100
253 22.4 17.8 26.6
125 10.3 8.3 12.5

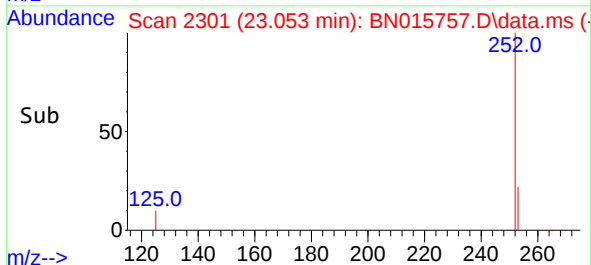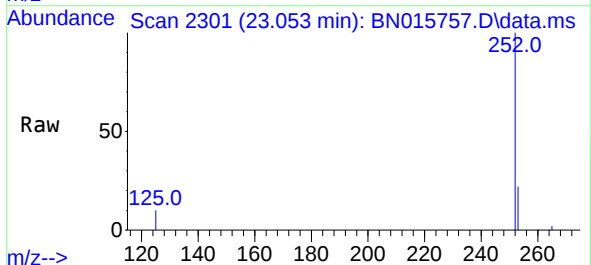






#39
Benzo(a)pyrene
Concen: 0.385 ng
RT: 23.611 min Scan# 2464
Delta R.T. 0.003 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:252 Resp: 130725
Ion Ratio Lower Upper
252 100
253 22.5 17.8 26.8
125 11.5 9.0 13.6

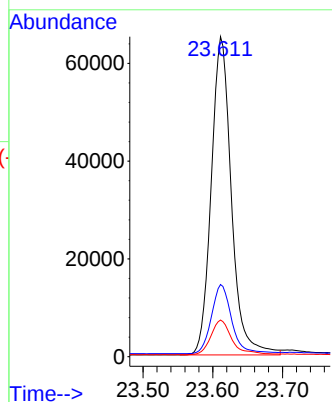

#40
Dibenzo(a,h)anthracene
Concen: 0.356 ng
RT: 26.134 min Scan# 3201
Delta R.T. 0.003 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02


Tgt Ion:278 Resp: 124283
Ion Ratio Lower Upper
278 100
139 16.4 13.1 19.7
279 23.9 19.1 28.7

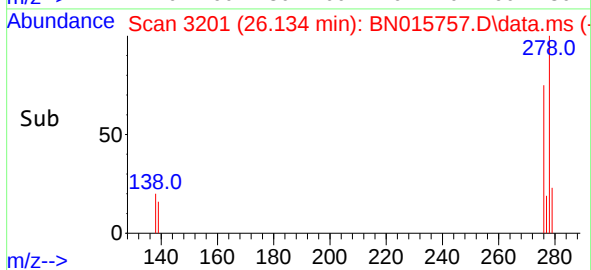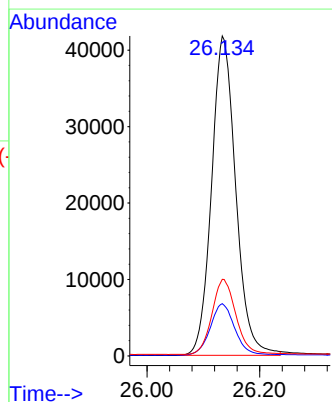

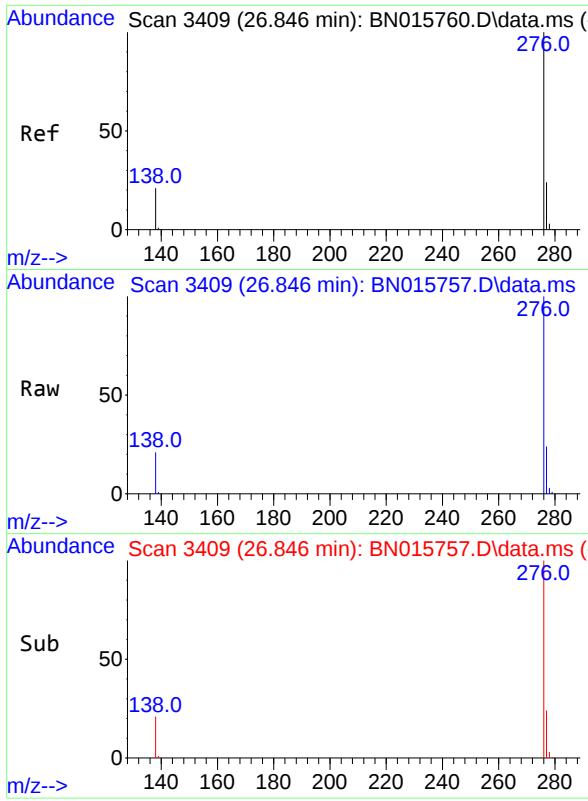

#41
Benzo(g,h,i)perylene
Concen: 0.388 ng
RT: 26.846 min Scan# 3409
Delta R.T. -0.000 min
Lab File: BN015757.D
Acq: 02 Aug 2021 09:02

Tgt Ion:	276	Resp:	141289
Ion	Ratio	Lower	Upper
276	100		
277	23.8	19.0	28.6
138	21.0	16.6	24.8

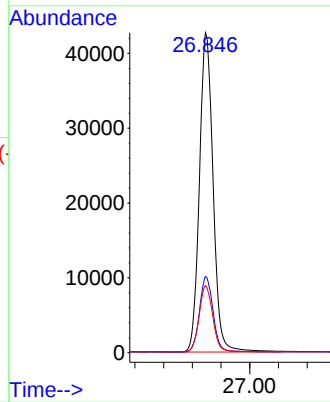

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4