

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080221\
 Data File : BN015762.D
 Acq On : 02 Aug 2021 12:10
 Operator : CG/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Aug 02 12:41:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 02 11:44:42 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.790	152	38621	0.400	ng	0.00
7) Naphthalene-d8	10.571	136	164135	0.400	ng	0.00
13) Acenaphthene-d10	14.421	164	86432	0.400	ng	0.01
19) Phenanthrene-d10	17.163	188	154864	0.400	ng	0.00
29) Chrysene-d12	21.376	240	154151	0.400	ng	# 0.01
35) Perylene-d12	23.713	264	139241	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.383	112	155098	1.495	ng	0.00
5) Phenol-d6	6.950	99	189360	1.508	ng	0.00
8) Nitrobenzene-d5	8.936	82	174035	1.687	ng	0.01
11) 2-Methylnaphthalene-d10	12.162	152	407749	1.650	ng	0.00
14) 2,4,6-Tribromophenol	15.905	330	57526	1.540	ng	0.00
15) 2-Fluorobiphenyl	13.038	172	527955	1.596	ng	0.00
27) Fluoranthene-d10	19.207	212	698660	1.712	ng	0.00
31) Terphenyl-d14	19.812	244	580468	1.547	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.345	88	22463	1.692	ng	# 89
3) n-Nitrosodimethylamine	3.696	42	45935	1.789	ng	# 98
6) bis(2-Chloroethyl)ether	7.218	93	170427	1.659	ng	100
9) Naphthalene	10.622	128	697363	1.631	ng	100
10) Hexachlorobutadiene	10.913	225	121621	1.617	ng	# 100
12) 2-Methylnaphthalene	12.234	142	447176	1.610	ng	100
16) Acenaphthylene	14.129	152	628585	1.655	ng	100
17) Acenaphthene	14.471	154	406058	1.642	ng	98
18) Fluorene	15.461	166	491383	1.631	ng	99
20) 4,6-Dinitro-2-methylph...	15.537	198	19294	1.617	ng	# 87
21) 4-Bromophenyl-phenylether	16.360	248	152781	1.690	ng	100
22) Hexachlorobenzene	16.470	284	171585	1.717	ng	99
23) Atrazine	16.640	200	110506	1.600	ng	# 88
24) Pentachlorophenol	16.822	266	58201	1.552	ng	99
25) Phenanthrene	17.212	178	757115	1.707	ng	100
26) Anthracene	17.297	178	676297	1.687	ng	100
28) Fluoranthene	19.236	202	814934	1.719	ng	100
30) Pyrene	19.599	202	818526	1.590	ng	100
32) Benzo(a)anthracene	21.355	228	815072	1.661	ng	100
33) Chrysene	21.408	228	801058	1.604	ng	100
34) Bis(2-ethylhexyl)phtha...	21.301	149	336190	1.288	ng	100
36) Indeno(1,2,3-cd)pyrene	26.113	276	846751	1.692	ng	100
37) Benzo(b)fluoranthene	23.005	252	816300	1.824	ng	99
38) Benzo(k)fluoranthene	23.053	252	821122	1.702	ng	99
39) Benzo(a)pyrene	23.607	252	702784	1.718	ng	99
40) Dibenzo(a,h)anthracene	26.133	278	706656	1.671	ng	99
41) Benzo(g,h,i)perylene	26.849	276	727609	1.668	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080221\
Data File : BN015762.D
Acq On : 02 Aug 2021 12:10
Operator : CG/JU
Sample : SSTDIC1.6
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDIC1.6

Quant Time: Aug 02 12:41:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 02 11:44:42 2021
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.790 min Scan# 511
 Delta R.T. -0.000 min
 Lab File: BN015762.D
 Acq: 02 Aug 2021 12:10

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Tgt Ion: 152 Resp: 38621




Ion	Ratio	Lower	Upper
152	100		
150	156.3	123.5	185.3
115	58.7	46.8	70.2




#2
 1,4-Dioxane
 Concen: 1.692 ng
 RT: 3.345 min Scan# 29
 Delta R.T. -0.010 min
 Lab File: BN015762.D
 Acq: 02 Aug 2021 12:10

Tgt Ion: 88 Resp: 22463

Ion	Ratio	Lower	Upper
88	100		
43	20.2	23.1	34.7#
58	70.1	62.2	93.4







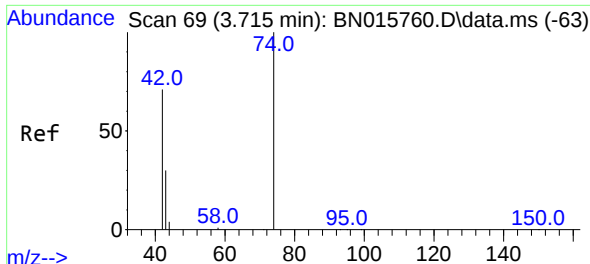

#3
n-Nitrosodimethylamine
Concen: 1.789 ng
RT: 3.696 min Scan# 67
Delta R.T. -0.019 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 42 Resp: 45935
Ion Ratio Lower Upper
42 100
74 145.2 114.4 171.6
44 6.8 3.6 5.4#

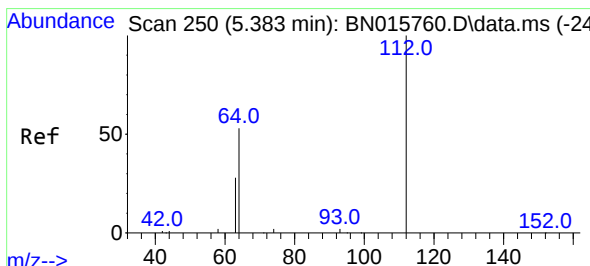

#4
2-Fluorophenol
Concen: 1.495 ng
RT: 5.383 min Scan# 250
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion: 112 Resp: 155098
Ion Ratio Lower Upper
112 100
64 52.7 42.2 63.4
63 27.6 22.2 33.2









#5
Phenol-d6
Concen: 1.508 ng
RT: 6.950 min Scan# 420
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 99 Resp: 189360
Ion Ratio Lower Upper
99 100
42 16.3 13.2 19.8
71 29.6 23.8 35.8



#6
bis(2-Chloroethyl)ether
Concen: 1.659 ng
RT: 7.218 min Scan# 449
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion: 93 Resp: 170427
Ion Ratio Lower Upper
93 100
63 73.1 58.8 88.2
95 33.1 26.6 39.8









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.571 min Scan# 746
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	136	Resp:	164135
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.7	13.1
54	5.1	3.9	5.9
68	4.1	3.3	4.9



#8
Nitrobenzene-d5
Concen: 1.687 ng
RT: 8.936 min Scan# 617
Delta R.T. 0.012 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion:	82	Resp:	174035
Ion	Ratio	Lower	Upper
82	100		
128	47.9	26.2	39.4#
54	44.1	45.1	67.7#









#9
Naphthalene
Concen: 1.631 ng
RT: 10.622 min Scan# 750
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:128 Resp: 697363
Ion Ratio Lower Upper
128 100
129 11.0 8.8 13.2
127 12.6 10.2 15.2



#10
Hexachlorobutadiene
Concen: 1.617 ng
RT: 10.913 min Scan# 773
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion:225 Resp: 121621
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.1 51.5 77.3









#11
2-Methylnaphthalene-d10
Concen: 1.650 ng
RT: 12.162 min Scan# 967
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:152 Resp: 407749
Ion Ratio Lower Upper
152 100
151 20.1 16.2 24.4

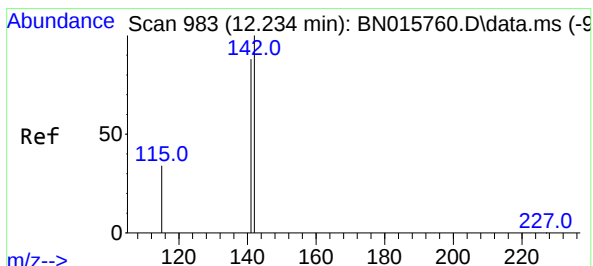

#12
2-Methylnaphthalene
Concen: 1.610 ng
RT: 12.234 min Scan# 983
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion:142 Resp: 447176
Ion Ratio Lower Upper
142 100
141 88.0 70.5 105.7
115 33.8 27.4 41.0









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.421 min Scan# 1195
Delta R.T. 0.012 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:164 Resp: 86432
Ion Ratio Lower Upper
164 100
162 98.0 84.2 126.2
160 43.2 39.8 59.6



#14
2,4,6-Tribromophenol
Concen: 1.540 ng
RT: 15.905 min Scan# 1312
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion:330 Resp: 57526
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.1 28.2 42.2









#15
2-Fluorobiphenyl
Concen: 1.596 ng
RT: 13.038 min Scan# 1086
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:172 Resp: 527955
Ion Ratio Lower Upper
172 100
171 34.6 27.8 41.8
170 23.1 18.7 28.1



#16
Acenaphthylene
Concen: 1.655 ng
RT: 14.129 min Scan# 1172
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion:152 Resp: 628585
Ion Ratio Lower Upper
152 100
151 19.3 15.7 23.5
153 13.1 10.5 15.7









#17
Acenaphthene
Concen: 1.642 ng
RT: 14.471 min Scan# 1199
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:154 Resp: 406058
Ion Ratio Lower Upper
154 100
153 111.3 90.5 135.7
152 54.3 44.4 66.6



#18
Fluorene
Concen: 1.631 ng
RT: 15.461 min Scan# 1277
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion:166 Resp: 491383
Ion Ratio Lower Upper
166 100
165 97.0 78.2 117.2
167 13.5 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.163 min Scan# 1415
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:188 Resp: 154864
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.3 7.7 11.5



#20
4,6-Dinitro-2-methylphenol
Concen: 1.617 ng
RT: 15.537 min Scan# 1283
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion:198 Resp: 19294
Ion Ratio Lower Upper
198 100
182 8.8 11.1 16.7#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 1.690 ng
RT: 16.360 min Scan# 1349
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:248 Resp: 152781
Ion Ratio Lower Upper
248 100
250 94.1 75.8 113.6
141 66.1 52.8 79.2



#22
Hexachlorobenzene
Concen: 1.717 ng
RT: 16.470 min Scan# 1358
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion:284 Resp: 171585
Ion Ratio Lower Upper
284 100
142 36.1 29.4 44.2
249 29.5 23.8 35.6









#23
Atrazine
Concen: 1.600 ng
RT: 16.640 min Scan# 1372
Delta R.T. 0.012 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:200 Resp: 110506
Ion Ratio Lower Upper
200 100
173 19.6 25.0 37.6#
215 49.3 36.3 54.5



#24
Pentachlorophenol
Concen: 1.552 ng
RT: 16.822 min Scan# 1387
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion:266 Resp: 58201
Ion Ratio Lower Upper
266 100
264 62.8 49.7 74.5
268 64.2 51.8 77.6









#25
Phenanthrene
Concen: 1.707 ng
RT: 17.212 min Scan# 1419
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:178 Resp: 757115
Ion Ratio Lower Upper
178 100
176 18.9 15.1 22.7
179 15.4 12.2 18.4



#26
Anthracene
Concen: 1.687 ng
RT: 17.297 min Scan# 1426
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion:178 Resp: 676297
Ion Ratio Lower Upper
178 100
176 18.3 14.6 22.0
179 15.4 12.2 18.4









#27
Fluoranthene-d10
Concen: 1.712 ng
RT: 19.207 min Scan# 1725
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:212 Resp: 698660
Ion Ratio Lower Upper
212 100
106 13.6 10.8 16.2
104 7.5 6.0 9.0



#28
Fluoranthene
Concen: 1.719 ng
RT: 19.236 min Scan# 1731
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion:202 Resp: 814934
Ion Ratio Lower Upper
202 100
101 11.3 9.0 13.6
203 17.4 13.8 20.8







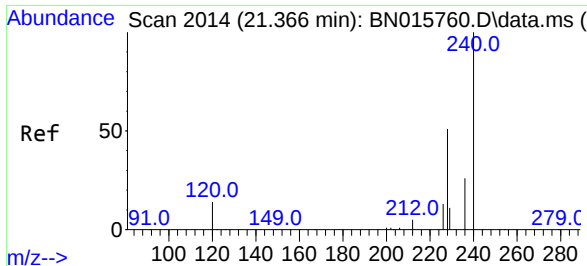

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.376 min Scan# 2015
Delta R.T. 0.010 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:240 Resp: 154151
Ion Ratio Lower Upper
240 100
120 5.8 11.4 17.0#
236 25.2 21.2 31.8



#30
Pyrene
Concen: 1.590 ng
RT: 19.599 min Scan# 1804
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion:202 Resp: 818526
Ion Ratio Lower Upper
202 100
200 20.7 16.5 24.7
203 17.6 13.9 20.9









#31
Terphenyl-d14
Concen: 1.547 ng
RT: 19.812 min Scan# 1847
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:244 Resp: 580468
Ion Ratio Lower Upper
244 100
212 7.4 5.9 8.9
122 12.4 9.7 14.5



#32
Benzo(a)anthracene
Concen: 1.661 ng
RT: 21.355 min Scan# 2013
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion:228 Resp: 815072
Ion Ratio Lower Upper
228 100
226 26.8 21.2 31.8
229 19.5 15.6 23.4









#33
Chrysene
Concen: 1.604 ng
RT: 21.408 min Scan# 2018
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:228 Resp: 801058
Ion Ratio Lower Upper
228 100
226 29.2 23.3 34.9
229 19.6 15.7 23.5



#34
Bis(2-ethylhexyl)phthalate
Concen: 1.288 ng
RT: 21.301 min Scan# 2008
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10


Tgt Ion:149 Resp: 336190
Ion Ratio Lower Upper
149 100
167 26.6 21.2 31.8
279 3.8 3.2 4.8







#35
Perylene-d12
Concen: 0.400 ng
RT: 23.713 min Scan# 2494
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6



Tgt Ion:264 Resp: 139241




Ion	Ratio	Lower	Upper
264	100		
260	24.6	19.5	29.3
265	23.5	19.2	28.8



#36
Indeno(1,2,3-cd)pyrene
Concen: 1.692 ng
RT: 26.113 min Scan# 3195
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Tgt Ion:276 Resp: 846751

Ion	Ratio	Lower	Upper
276	100		
138	24.4	19.6	29.4
277	24.9	20.0	30.0









#37
Benzo(b)fluoranthene
Concen: 1.824 ng
RT: 23.005 min Scan# 2287
Delta R.T. 0.003 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:252 Resp: 816300
Ion Ratio Lower Upper
252 100
253 21.9 17.7 26.5
125 10.0 8.2 12.4



#38
Benzo(k)fluoranthene
Concen: 1.702 ng
RT: 23.053 min Scan# 2301
Delta R.T. 0.003 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10


Tgt Ion:252 Resp: 821122
Ion Ratio Lower Upper
252 100
253 21.9 17.8 26.6
125 10.1 8.3 12.5








#39
Benzo(a)pyrene
Concen: 1.718 ng
RT: 23.607 min Scan# 2463
Delta R.T. -0.000 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10


Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6





Tgt Ion:252 Resp: 702784
Ion Ratio Lower Upper
252 100
253 21.8 17.8 26.8
125 11.0 9.0 13.6




#40
Dibenzo(a,h)anthracene
Concen: 1.671 ng
RT: 26.133 min Scan# 3201
Delta R.T. 0.003 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10



Tgt Ion:278 Resp: 706656
Ion Ratio Lower Upper
278 100
139 16.1 13.1 19.7
279 23.5 19.1 28.7





#41
Benzo(g,h,i)perylene
Concen: 1.668 ng
RT: 26.849 min Scan# 3410
Delta R.T. 0.003 min
Lab File: BN015762.D
Acq: 02 Aug 2021 12:10

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:276 Resp: 727609
Ion Ratio Lower Upper
276 100
277 23.9 19.0 28.6
138 20.8 16.6 24.8

