

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080221\
 Data File : BN015764.D
 Acq On : 02 Aug 2021 13:23
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Aug 02 13:52:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 02 11:44:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.790	152	46471	0.400	ng	0.00
7) Naphthalene-d8	10.571	136	184348	0.400	ng	0.00
13) Acenaphthene-d10	14.421	164	97489	0.400	ng	0.01
19) Phenanthrene-d10	17.164	188	176683	0.400	ng	0.00
29) Chrysene-d12	21.376	240	170345	0.400	ng	# 0.01
35) Perylene-d12	23.714	264	169906	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.383	112	540515	4.331	ng	0.00
5) Phenol-d6	6.951	99	658713	4.361	ng	0.00
8) Nitrobenzene-d5	8.937	82	660298	5.700	ng	0.01
11) 2-Methylnaphthalene-d10	12.163	152	1310614	4.721	ng	0.00
14) 2,4,6-Tribromophenol	0.000	330	0d	0.000	ng	
15) 2-Fluorobiphenyl	13.038	172	1716167	4.599	ng	0.00
27) Fluoranthene-d10	19.207	212	2340420	5.027	ng	0.00
31) Terphenyl-d14	19.813	244	1914338	4.617	ng	0.00
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.346	88	79506	4.977	ng	92
3) n-Nitrosodimethylamine	3.696	42	170847	5.530	ng	# 94
6) bis(2-Chloroethyl)ether	7.218	93	550455	4.454	ng	99
9) Naphthalene	10.622	128	2238691	4.662	ng	100
10) Hexachlorobutadiene	10.914	225	398991	4.723	ng	# 100
12) 2-Methylnaphthalene	12.234	142	1435090	4.601	ng	99
16) Acenaphthylene	14.129	152	2150390	5.021	ng	100
17) Acenaphthene	14.484	154	1364984	4.893	ng	96
18) Fluorene	15.461	166	1640610	4.828	ng	98
21) 4-Bromophenyl-phenylether	16.360	248	532111	5.159	ng	97
22) Hexachlorobenzene	16.482	284	571687	5.015	ng	99
24) Pentachlorophenol	16.823	266	263124	6.150	ng	99
25) Phenanthrene	17.212	178	2475431	4.892	ng	100
26) Anthracene	17.298	178	2324985	5.085	ng	99
28) Fluoranthene	19.237	202	2625056	4.853	ng	99
30) Pyrene	19.599	202	2755365	4.843	ng	99
32) Benzo(a)anthracene	21.355	228	2753295	5.076	ng	99
33) Chrysene	21.408	228	2602241	4.715	ng	99
34) Bis(2-ethylhexyl)phtha...	21.302	149	1675992	5.812	ng	98
36) Indeno(1,2,3-cd)pyrene	26.120	276	3115093	5.101	ng	99
37) Benzo(b)fluoranthene	23.009	252	2788933	5.106	ng	99
38) Benzo(k)fluoranthene	23.053	252	2858907	4.855	ng	100
39) Benzo(a)pyrene	23.611	252	2573339	5.157	ng	99
40) Dibenzo(a,h)anthracene	26.141	278	2627219	5.091	ng	100
41) Benzo(g,h,i)perylene	26.853	276	2646321	4.970	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080221\
Data File : BN015764.D
Acq On : 02 Aug 2021 13:23
Operator : CG/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Aug 02 13:52:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 02 11:44:42 2021
Response via : Initial Calibration









#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.790 min Scan# 511
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 46471
Ion Ratio Lower Upper
152 100
150 158.2 123.5 185.3
115 58.7 46.8 70.2



#2
1,4-Dioxane
Concen: 4.977 ng
RT: 3.346 min Scan# 29
Delta R.T. -0.009 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion: 88 Resp: 79506
Ion Ratio Lower Upper
88 100
43 25.0 23.1 34.7
58 70.3 62.2 93.4







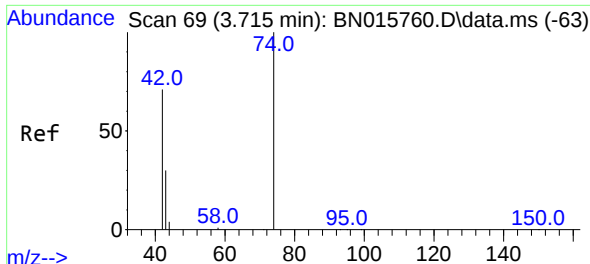

#3
n-Nitrosodimethylamine
Concen: 5.530 ng
RT: 3.696 min Scan# 67
Delta R.T. -0.018 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 42 Resp: 170847
Ion Ratio Lower Upper
42 100
74 150.5 114.4 171.6
44 6.5 3.6 5.4#

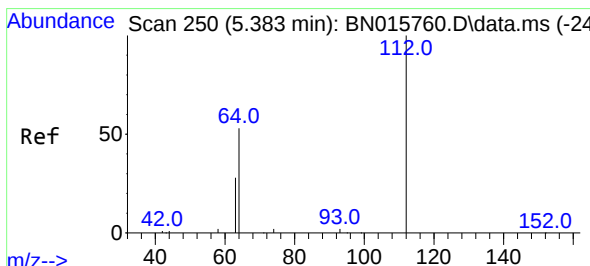

#4
2-Fluorophenol
Concen: 4.331 ng
RT: 5.383 min Scan# 250
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion: 112 Resp: 540515
Ion Ratio Lower Upper
112 100
64 52.4 42.2 63.4
63 27.3 22.2 33.2









#5
Phenol-d6
Concen: 4.361 ng
RT: 6.951 min Scan# 420
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 658713
Ion Ratio Lower Upper
99 100
42 15.9 13.2 19.8
71 29.5 23.8 35.8

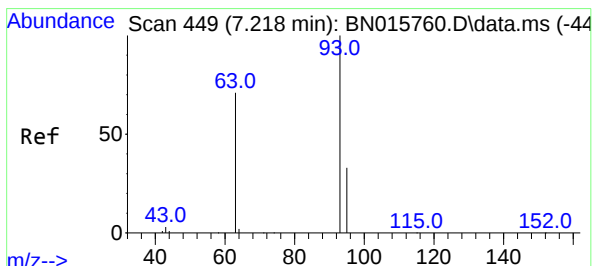

#6
bis(2-Chloroethyl)ether
Concen: 4.454 ng
RT: 7.218 min Scan# 449
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion: 93 Resp: 550455
Ion Ratio Lower Upper
93 100
63 72.2 58.8 88.2
95 33.1 26.6 39.8









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.571 min Scan# 746
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	184348
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.7	13.1
54	5.1	3.9	5.9
68	4.2	3.3	4.9



#8
Nitrobenzene-d5
Concen: 5.700 ng
RT: 8.937 min Scan# 617
Delta R.T. 0.013 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion:	82	Resp:	660298
Ion	Ratio	Lower	Upper
82	100		
128	52.0	26.2	39.4#
54	42.3	45.1	67.7#









#9
Naphthalene
Concen: 4.662 ng
RT: 10.622 min Scan# 750
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:128 Resp: 2238691
Ion Ratio Lower Upper
128 100
129 11.1 8.8 13.2
127 12.6 10.2 15.2



#10
Hexachlorobutadiene
Concen: 4.723 ng
RT: 10.914 min Scan# 773
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion:225 Resp: 398991
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.0 51.5 77.3









#11
2-Methylnaphthalene-d10
Concen: 4.721 ng
RT: 12.163 min Scan# 967
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:152 Resp: 1310614
Ion Ratio Lower Upper
152 100
151 20.0 16.2 24.4

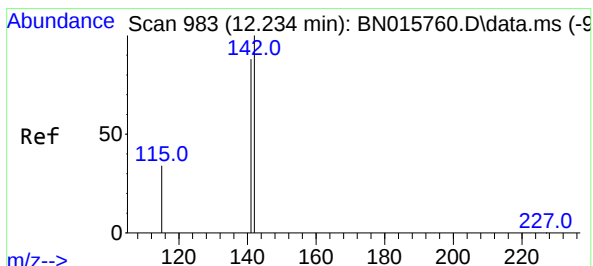

#12
2-Methylnaphthalene
Concen: 4.601 ng
RT: 12.234 min Scan# 983
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion:142 Resp: 1435090
Ion Ratio Lower Upper
142 100
141 87.7 70.5 105.7
115 33.6 27.4 41.0









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.421 min Scan# 1195
Delta R.T. 0.013 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:164 Resp: 97489
Ion Ratio Lower Upper
164 100
162 97.8 84.2 126.2
160 43.0 39.8 59.6



#14
2,4,6-Tribromophenol
Concen: 0.000 ng
Expected RT: 15.91 min


Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion: 330
Sig Exp Ratio
330 100
332 0.0
141 35.2



Ion 331.80 (331.50 to 332.50): BN015764.D\data.ms

Ion 141.00 (140.70 to 141.70): BN015764.D\data.ms







#15
2-Fluorobiphenyl
Concen: 4.599 ng
RT: 13.038 min Scan# 1086
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:172 Resp: 1716167




Ion	Ratio	Lower	Upper
172	100		
171	34.5	27.8	41.8
170	23.2	18.7	28.1




#16
Acenaphthylene
Concen: 5.021 ng
RT: 14.129 min Scan# 1172
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion:152 Resp: 2150390

Ion	Ratio	Lower	Upper
152	100		
151	19.3	15.7	23.5
153	13.2	10.5	15.7









#17
Acenaphthene
Concen: 4.893 ng
RT: 14.484 min Scan# 1200
Delta R.T. 0.013 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:154 Resp: 1364984
Ion Ratio Lower Upper
154 100
153 108.7 90.5 135.7
152 51.8 44.4 66.6



#18
Fluorene
Concen: 4.828 ng
RT: 15.461 min Scan# 1277
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion:166 Resp: 1640610
Ion Ratio Lower Upper
166 100
165 95.7 78.2 117.2
167 13.6 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.164 min Scan# 1415
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:188 Resp: 176683
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.6 7.7 11.5



#21
4-Bromophenyl-phenylether
Concen: 5.159 ng
RT: 16.360 min Scan# 1349
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion:248 Resp: 532111
Ion Ratio Lower Upper
248 100
250 95.1 75.8 113.6
141 60.4 52.8 79.2









#22
Hexachlorobenzene
Concen: 5.015 ng
RT: 16.482 min Scan# 1359
Delta R.T. 0.012 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:284 Resp: 571687
Ion Ratio Lower Upper
284 100
142 35.6 29.4 44.2
249 29.5 23.8 35.6



#24
Pentachlorophenol
Concen: 6.150 ng
RT: 16.823 min Scan# 1387
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion:266 Resp: 263124
Ion Ratio Lower Upper
266 100
264 62.6 49.7 74.5
268 63.8 51.8 77.6









#25
Phenanthrene
Concen: 4.892 ng
RT: 17.212 min Scan# 1419
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 2475431
Ion Ratio Lower Upper
178 100
176 18.8 15.1 22.7
179 15.6 12.2 18.4



#26
Anthracene
Concen: 5.085 ng
RT: 17.298 min Scan# 1426
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion:178 Resp: 2324985
Ion Ratio Lower Upper
178 100
176 18.3 14.6 22.0
179 15.7 12.2 18.4









#27
Fluoranthene-d10
Concen: 5.027 ng
RT: 19.207 min Scan# 1725
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 2340420
Ion Ratio Lower Upper
212 100
106 13.9 10.8 16.2
104 7.6 6.0 9.0



#28
Fluoranthene
Concen: 4.853 ng
RT: 19.237 min Scan# 1731
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion:202 Resp: 2625056
Ion Ratio Lower Upper
202 100
101 11.8 9.0 13.6
203 17.8 13.8 20.8









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.376 min Scan# 2015
Delta R.T. 0.011 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:240 Resp: 170345
Ion Ratio Lower Upper
240 100
120 5.9 11.4 17.0#
236 25.2 21.2 31.8



#30
Pyrene
Concen: 4.843 ng
RT: 19.599 min Scan# 1804
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion:202 Resp: 2755365
Ion Ratio Lower Upper
202 100
200 20.7 16.5 24.7
203 17.9 13.9 20.9









#31
Terphenyl-d14
Concen: 4.617 ng
RT: 19.813 min Scan# 1847
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:244 Resp: 1914338
Ion Ratio Lower Upper
244 100
212 7.5 5.9 8.9
122 12.5 9.7 14.5



#32
Benzo(a)anthracene
Concen: 5.076 ng
RT: 21.355 min Scan# 2013
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion:228 Resp: 2753295
Ion Ratio Lower Upper
228 100
226 26.5 21.2 31.8
229 20.4 15.6 23.4









#33
Chrysene
Concen: 4.715 ng
RT: 21.408 min Scan# 2018
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:228 Resp: 2602241
Ion Ratio Lower Upper
228 100
226 29.5 23.3 34.9
229 20.1 15.7 23.5



#34
Bis(2-ethylhexyl)phthalate
Concen: 5.812 ng
RT: 21.302 min Scan# 2008
Delta R.T. -0.000 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion:149 Resp: 1675992
Ion Ratio Lower Upper
149 100
167 27.5 21.2 31.8
279 3.9 3.2 4.8









#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.714 min Scan# 2494
 Delta R.T. -0.000 min
 Lab File: BN015764.D
 Acq: 02 Aug 2021 13:23

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:264 Resp: 169906




Ion	Ratio	Lower	Upper
264	100		
260	24.3	19.5	29.3
265	23.0	19.2	28.8




#36
 Indeno(1,2,3-cd)pyrene
 Concen: 5.101 ng
 RT: 26.120 min Scan# 3197
 Delta R.T. 0.007 min
 Lab File: BN015764.D
 Acq: 02 Aug 2021 13:23

Tgt Ion:276 Resp: 3115093

Ion	Ratio	Lower	Upper
276	100		
138	24.9	19.6	29.4
277	25.2	20.0	30.0









#37
Benzo(b)fluoranthene
Concen: 5.106 ng
RT: 23.009 min Scan# 2288
Delta R.T. 0.007 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 2788933
Ion Ratio Lower Upper
252 100
253 22.4 17.7 26.5
125 10.1 8.2 12.4



#38
Benzo(k)fluoranthene
Concen: 4.855 ng
RT: 23.053 min Scan# 2301
Delta R.T. 0.003 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion:252 Resp: 2858907
Ion Ratio Lower Upper
252 100
253 22.2 17.8 26.6
125 10.3 8.3 12.5









#39
Benzo(a)pyrene
Concen: 5.157 ng
RT: 23.611 min Scan# 2464
Delta R.T. 0.003 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 2573339
Ion Ratio Lower Upper
252 100
253 22.1 17.8 26.8
125 11.1 9.0 13.6



#40
Dibenzo(a,h)anthracene
Concen: 5.091 ng
RT: 26.141 min Scan# 3203
Delta R.T. 0.010 min
Lab File: BN015764.D
Acq: 02 Aug 2021 13:23

Tgt Ion:278 Resp: 2627219
Ion Ratio Lower Upper
278 100
139 16.2 13.1 19.7
279 23.8 19.1 28.7





#41
 Benzo(g,h,i)perylene
 Concen: 4.970 ng
 RT: 26.853 min Scan# 3411
 Delta R.T. 0.007 min
 Lab File: BN015764.D
 Acq: 02 Aug 2021 13:23

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion: 276 Resp: 2646321

Ion	Ratio	Lower	Upper
276	100		
277	24.0	19.0	28.6
138	21.4	16.6	24.8

