


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080221\
 Data File : BN015756.D
 Acq On : 02 Aug 2021 08:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN080221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 02 14:09:59 2021

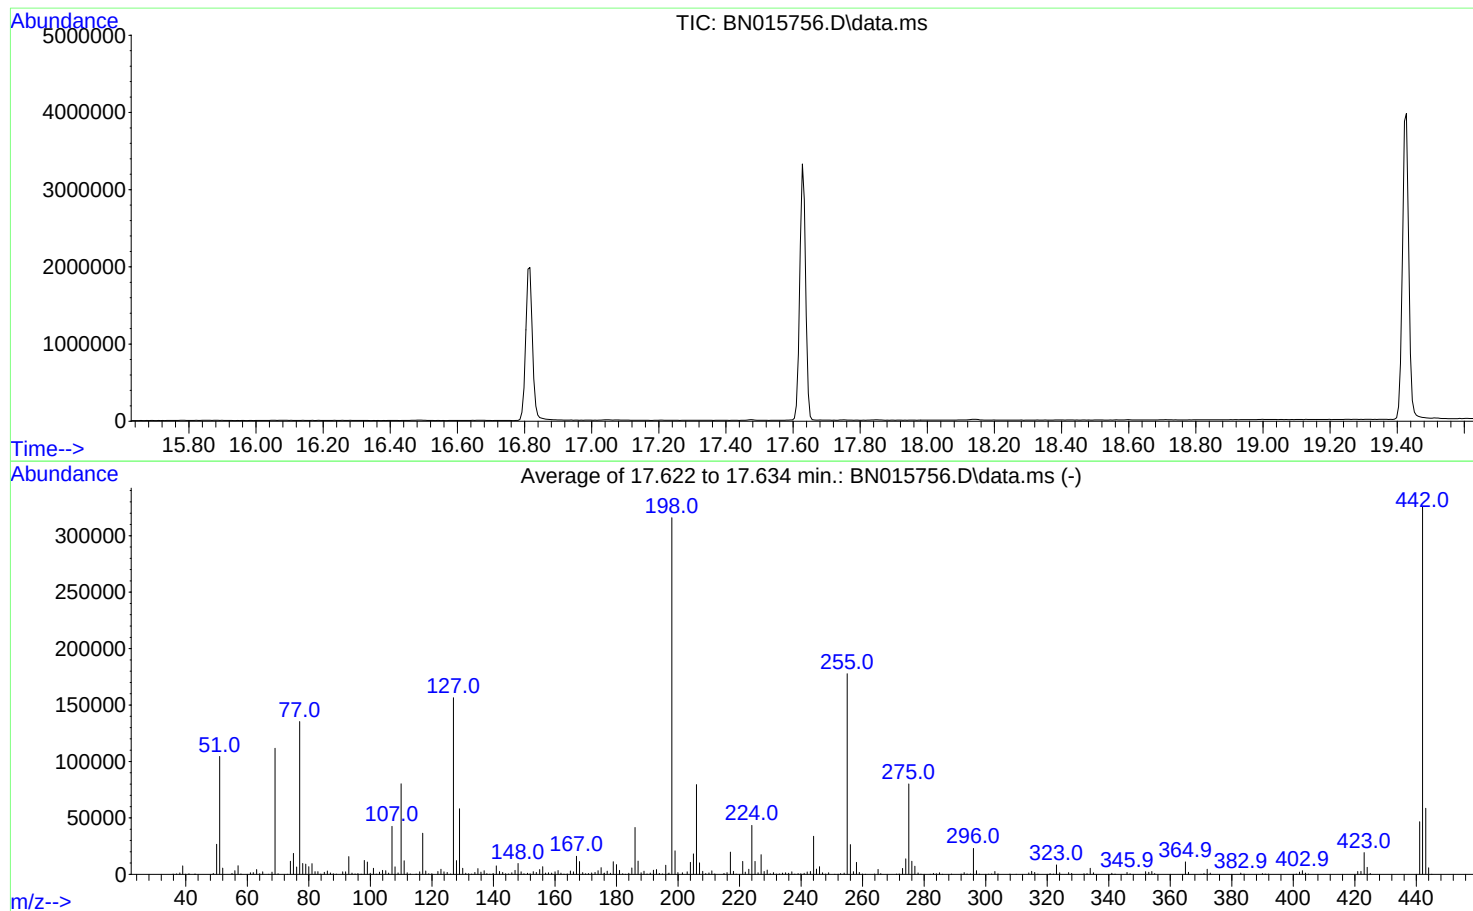




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	104437	PASS
68	69	0.00	2	1.7	1938	PASS
69	198	0.00	100	35.3	111677	PASS
70	69	0.00	2	0.6	653	PASS
127	198	10	80	49.5	156523	PASS
197	198	0.00	2	0.4	1129	PASS
198	198	100	100	100.0	315989	PASS
199	198	5	9	6.6	20832	PASS
275	198	10	60	25.4	80160	PASS
365	198	1	100	3.5	11131	PASS
441	198	0.01	100	14.8	46683	PASS
442	442	50	100	100.0	325909	PASS
443	442	15	24	18.0	58600	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080221\
Data File : BN015756.D
Acq On : 02 Aug 2021 08:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 02 14:23:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 30 07:20:03 2021
Response via : Initial Calibration

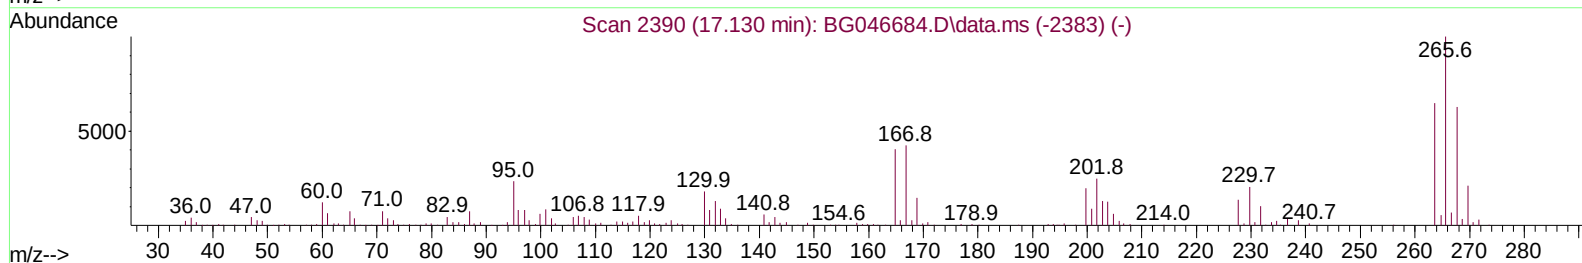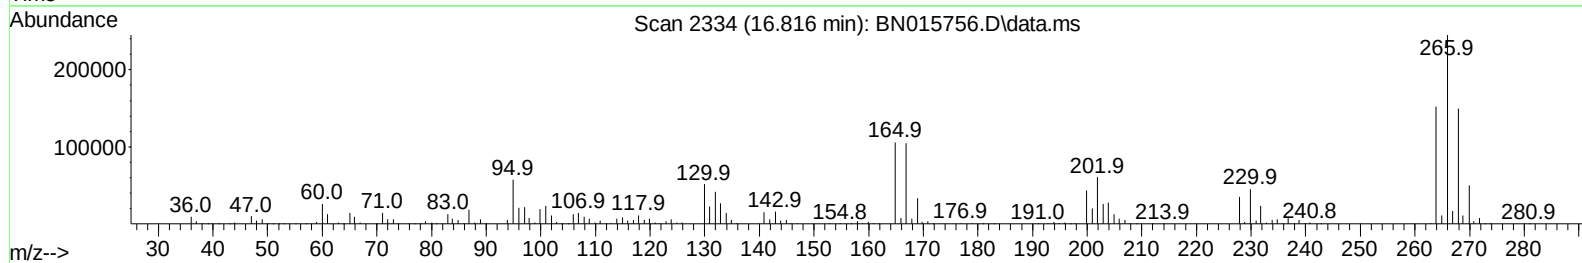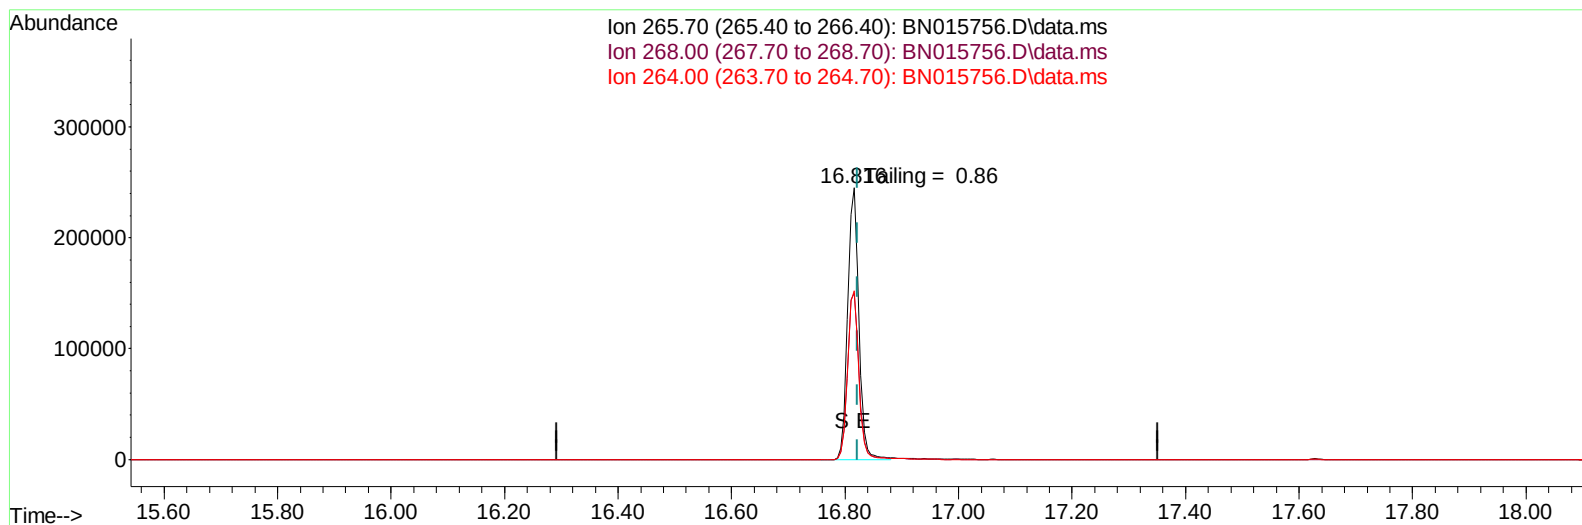

TIC: BN015756.D\data.ms

(70) Pentachlorophenol (C)

16.816min (-0.006) 21494.96 ng




response 334675

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.08
264.00	61.60	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080221\
Data File : BN015756.D
Acq On : 02 Aug 2021 08:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 02 14:23:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 30 07:20:03 2021
Response via : Initial Calibration

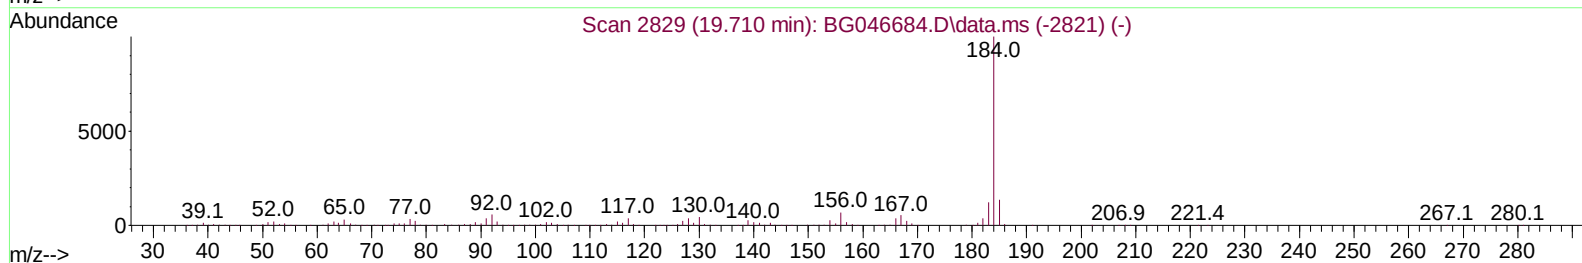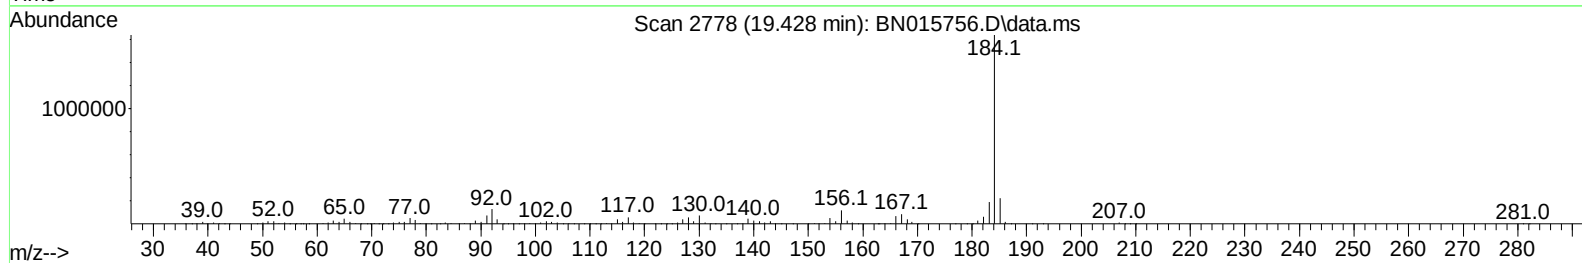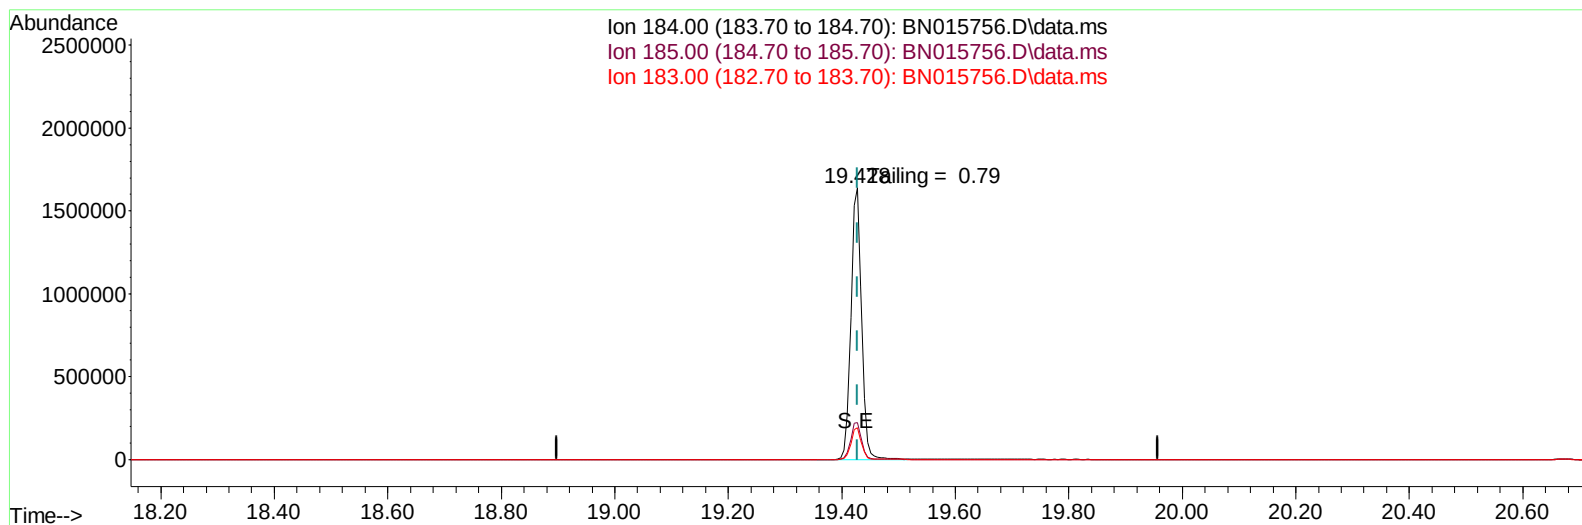

TIC: BN015756.D\data.ms

(77) Benzidine

19.428min (+ 0.000) 0.00 ng

response 2127398

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.70
183.00	13.20	11.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/2/2021	BNA_N	<u>BN015756.D</u>
Compound Name	Response	Retention Time
DDT	987361	20.675
DDD	6204	20.227
DDE	1184	19.722
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7388	994749	0.74

Instrument :
BNA_N
ClientSampleId :
DFTPP