

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080222\
 Data File : BN020942.D
 Acq On : 02 Aug 2022 14:30
 Operator : CG/JU
 Sample : PB146575BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 02 22:33:43 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 04:19:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	3742	0.400	ng/ul	0.00
4) Naphthalene-d8	10.602	136	10690	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.461	164	7043	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.210	188	14124	0.400	ng/ul	0.00
17) Chrysene-d12	21.430	240	7572	0.400	ng/ul	0.00
23) Perylene-d12	23.768	264	10925	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.206	96	25343	5.553	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.218	152	4366	0.277	ng/ul	0.01
18) Fluoranthene-d10	19.254	212	11637	0.502	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.451	166	1800	0.065	ng/ul#	15
20) Pyrene	19.612	202	1628	0.046	ng/ul#	1
26) Benzo(a)pyrene	23.610	252	3373	0.069	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080222\
Data File : BN020942.D
Acq On : 02 Aug 2022 14:30
Operator : CG/JU
Sample : PB146575BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 02 22:33:43 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 04:19:04 2022
Response via : Initial Calibration




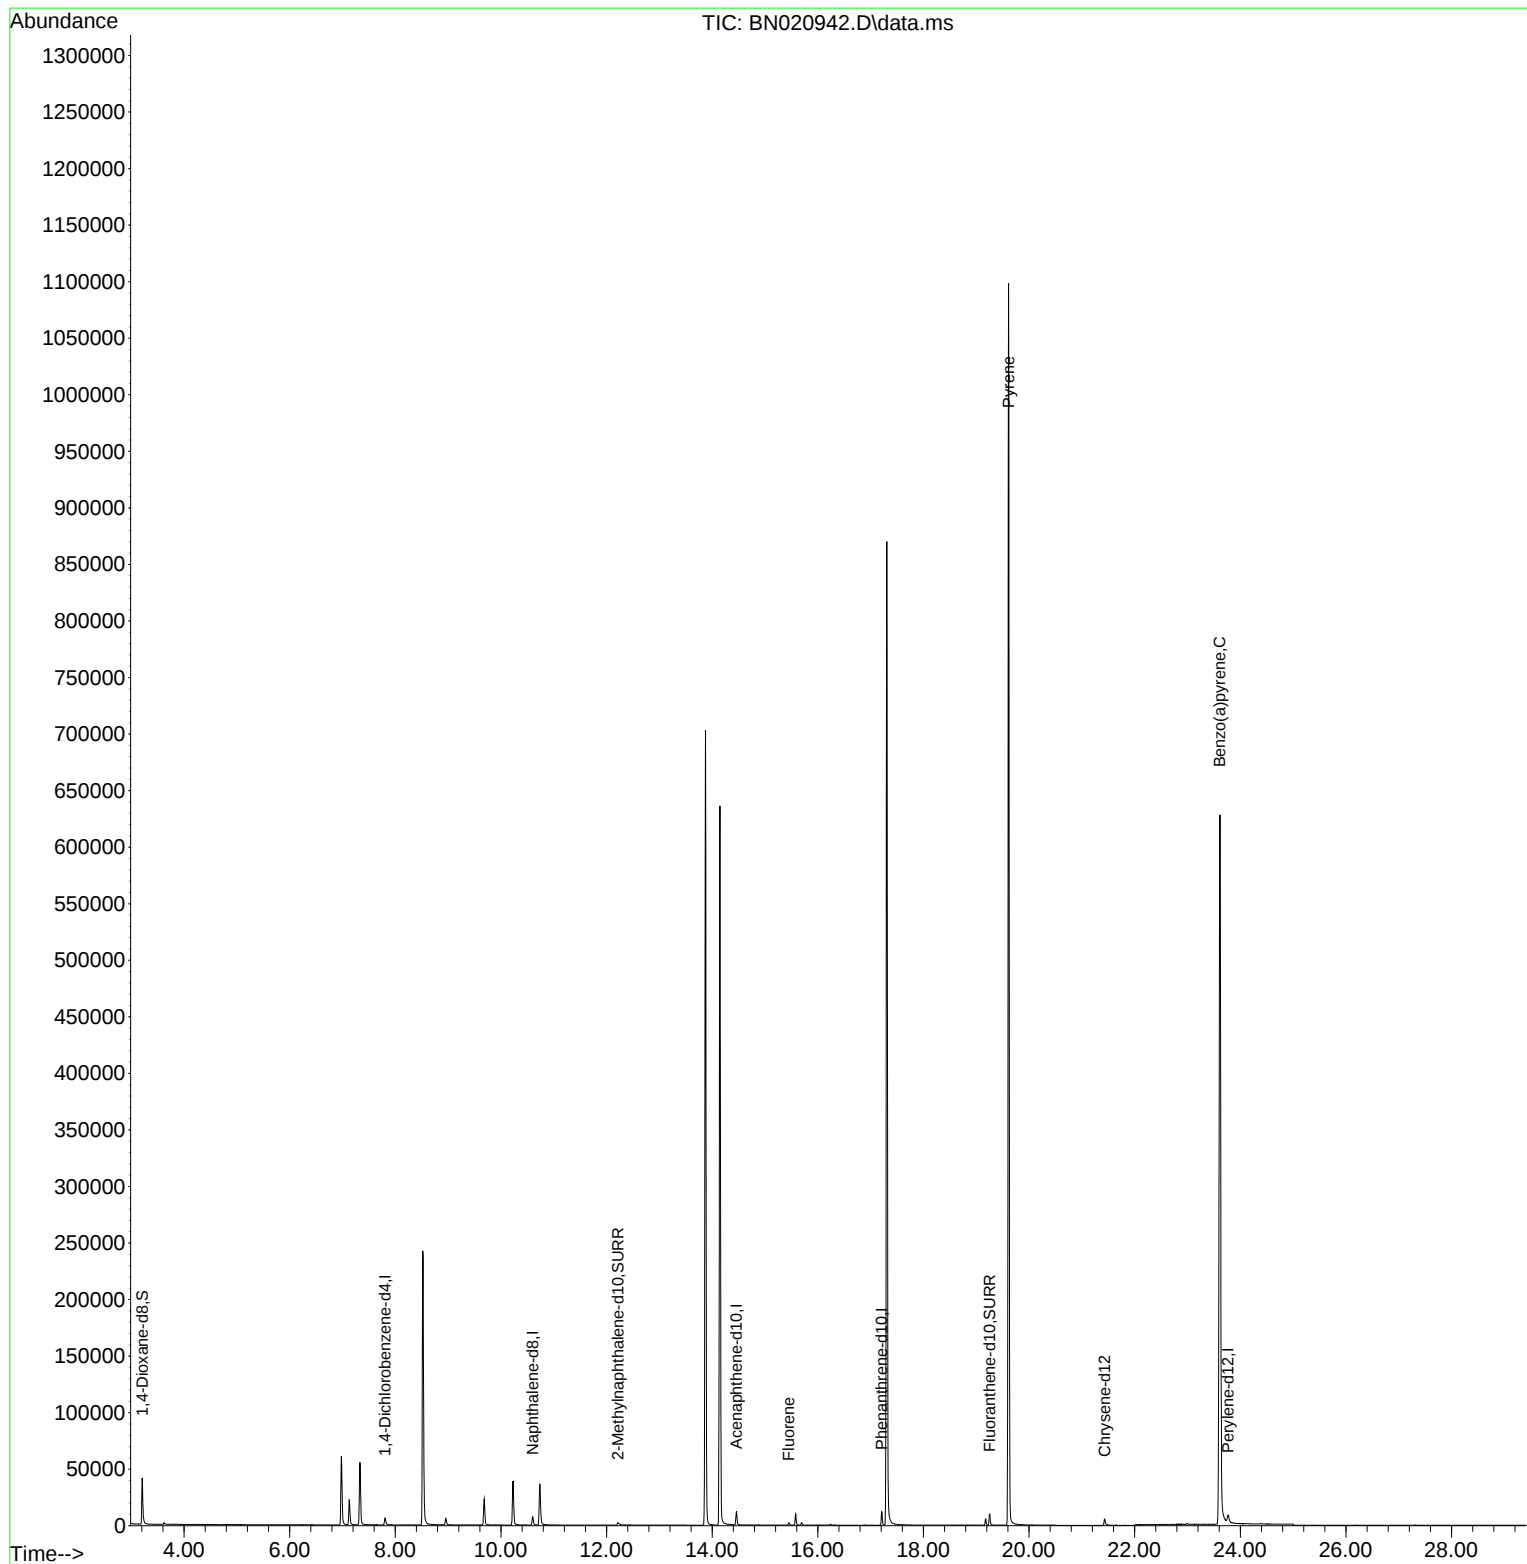


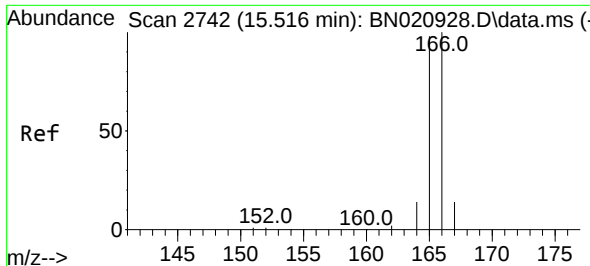

#12
Fluorene
Concen: 0.065 ng/ul
RT: 15.451 min Scan# 21
Delta R.T. -0.065 min
Lab File: BN020942.D
Acq: 02 Aug 2022 14:30




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:166 Resp: 1800
Ion Ratio Lower Upper
166 100
165 7.3 78.6 117.8#
167 32.0 11.8 17.6#

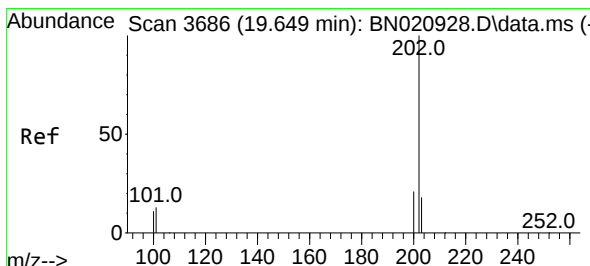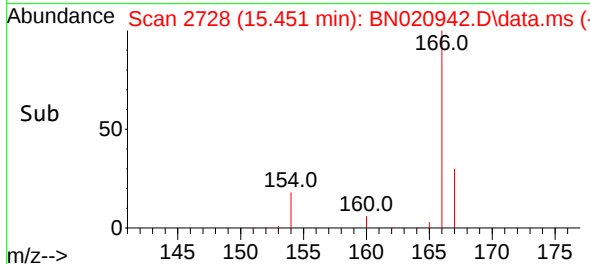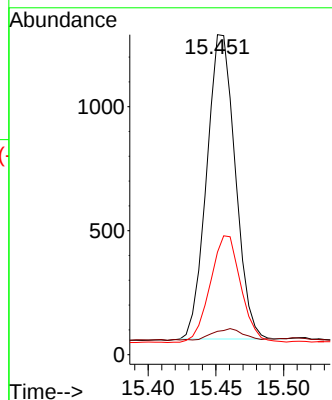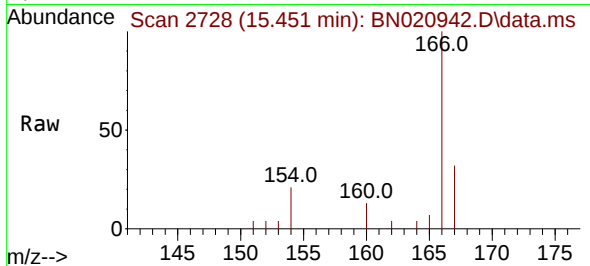

#20
Pyrene
Concen: 0.046 ng/ul
RT: 19.612 min Scan# 3678
Delta R.T. -0.037 min
Lab File: BN020942.D
Acq: 02 Aug 2022 14:30


Tgt Ion:202 Resp: 1628
Ion Ratio Lower Upper
202 100
101 180.8 11.3 16.9#
100 1346.0 9.0 13.4#

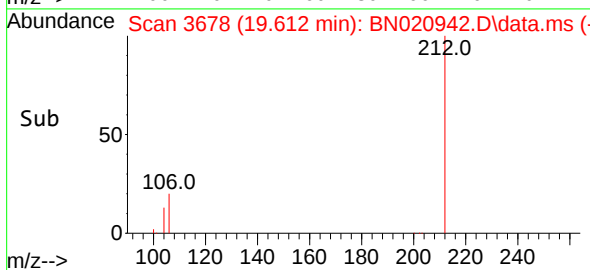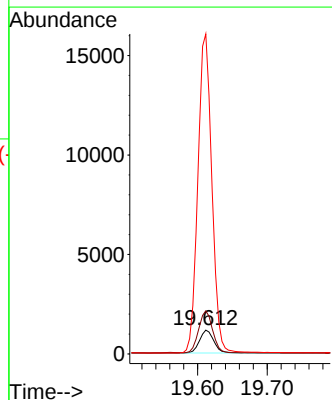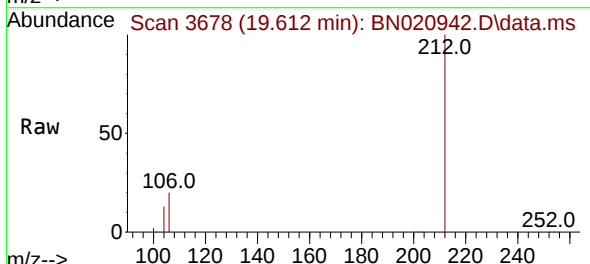

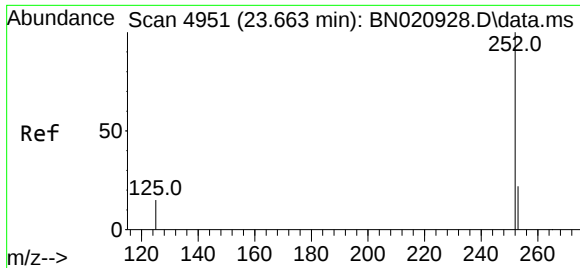

#26
Benzo(a)pyrene
Concen: 0.069 ng/ul
RT: 23.610 min Scan# 49
Delta R.T. -0.053 min
Lab File: BN020942.D
Acq: 02 Aug 2022 14:30

Instrument :
BNA_N
ClientSampleId :

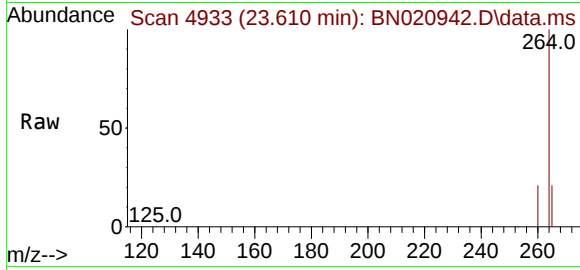

Tgt Ion:252 Resp: 3373
Ion Ratio Lower Upper
252 100
253 41.1 22.1 33.1#
125 34.4 14.7 22.1#

