

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080222\
 Data File : BN020944.D
 Acq On : 02 Aug 2022 15:44
 Operator : CG/JU
 Sample : N3943-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 02 22:33:53 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 04:19:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	4212	0.400	ng/ul	0.00
4) Naphthalene-d8	10.602	136	10906	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.457	164	8149	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.210	188	16562	0.400	ng/ul	0.00
17) Chrysene-d12	21.427	240	13117	0.400	ng/ul	0.00
23) Perylene-d12	23.768	264	9880	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.211	96	24609	4.791	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.208	152	5971	0.371	ng/ul	0.00
18) Fluoranthene-d10	19.249	212	16099	0.401	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.612	202	2180	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.616	252	3299	0.074	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080222\
Data File : BN020944.D
Acq On : 02 Aug 2022 15:44
Operator : CG/JU
Sample : N3943-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Aug 02 22:33:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 04:19:04 2022
Response via : Initial Calibration

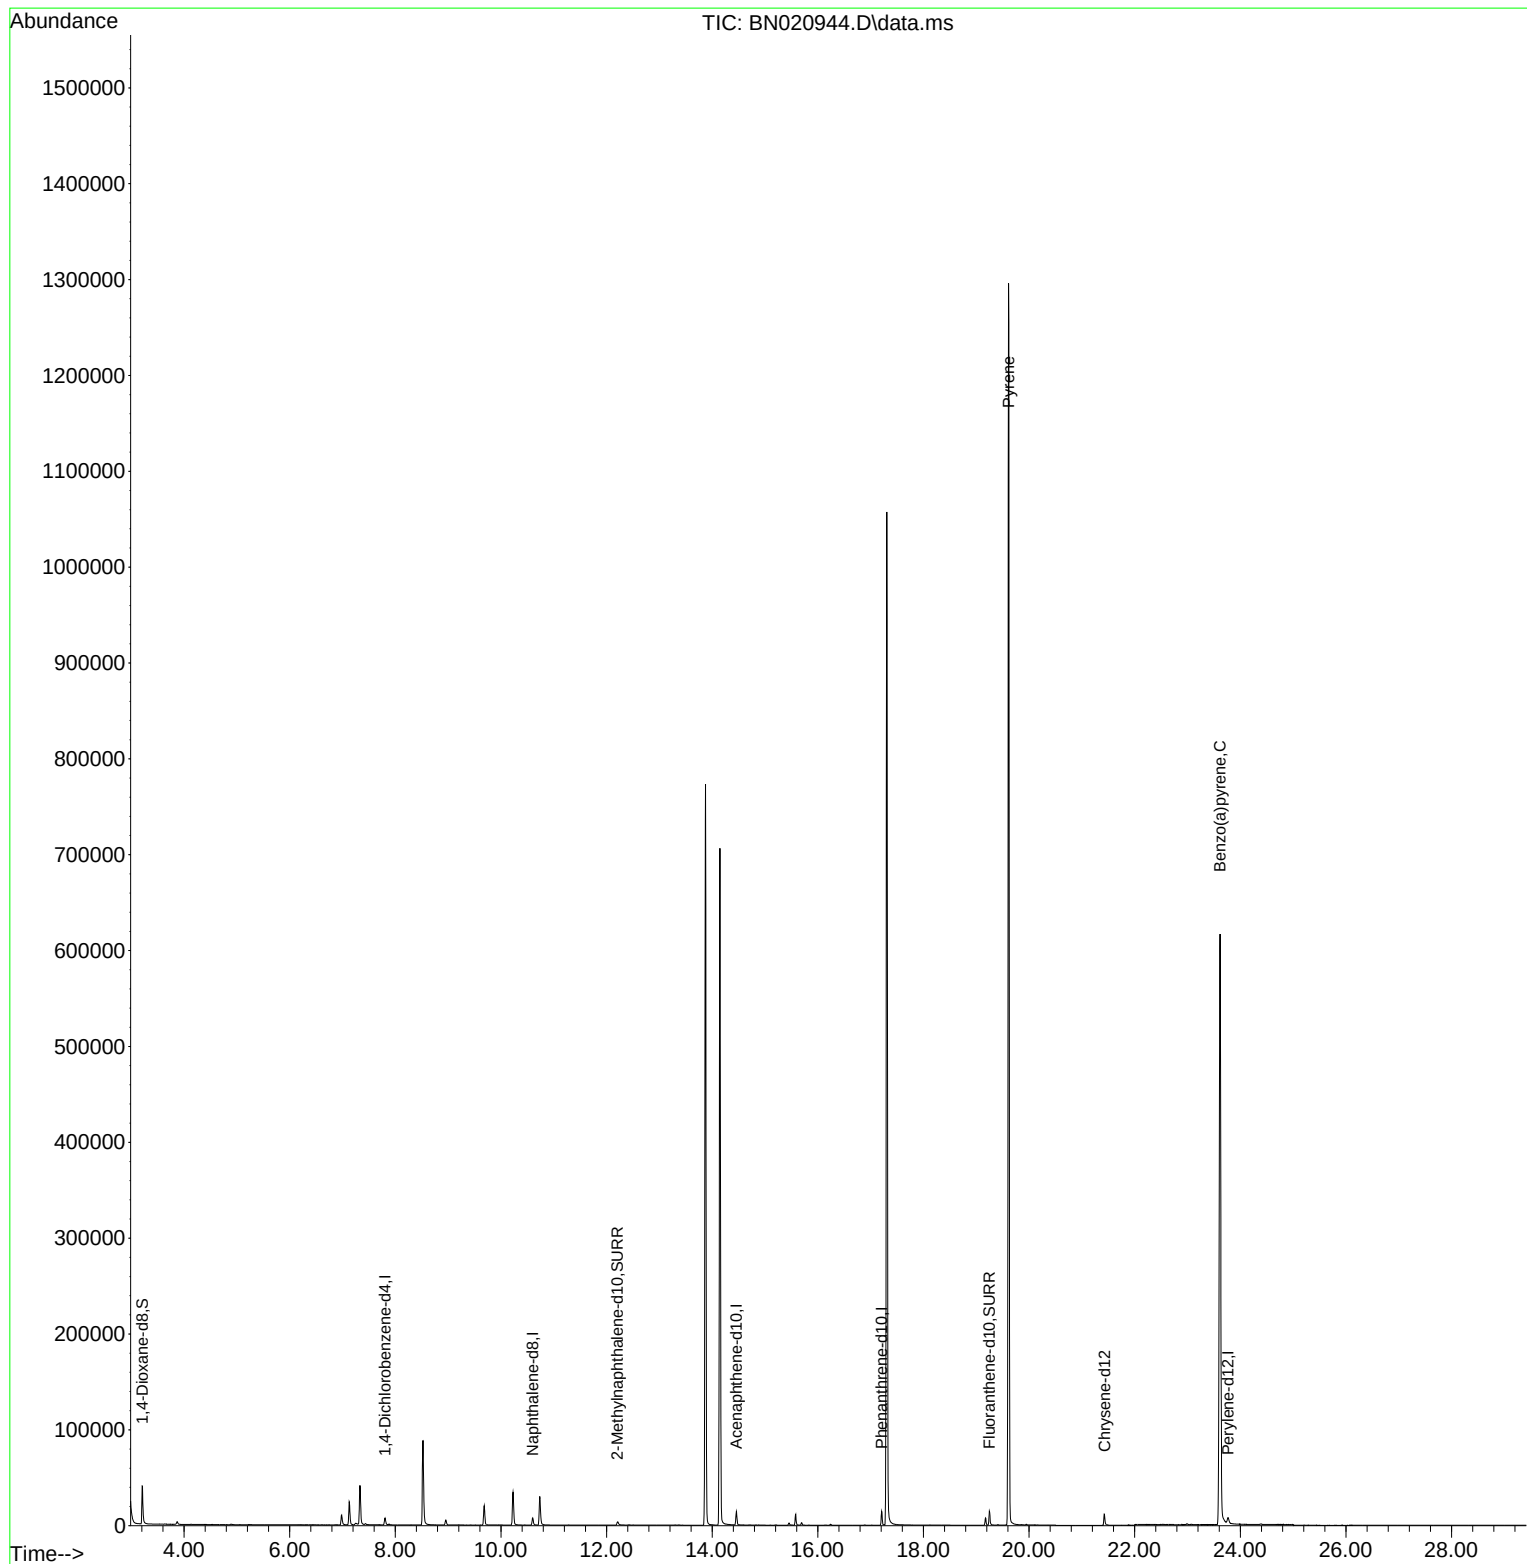



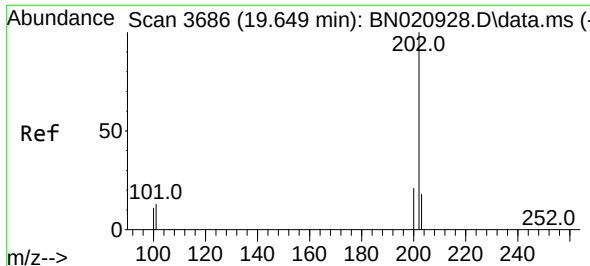


#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.612 min Scan# 3678
Delta R.T. -0.037 min
Lab File: BN020944.D
Acq: 02 Aug 2022 15:44

Instrument :
BNA_N
ClientSampleId :

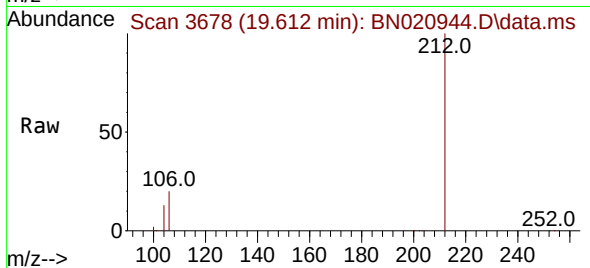

Tgt Ion:202 Resp: 2180
Ion Ratio Lower Upper
202 100
101 186.0 11.3 16.9#
100 1403.4 9.0 13.4#

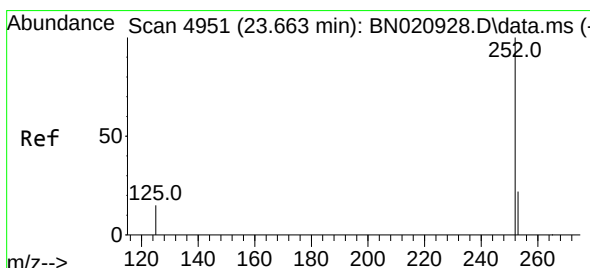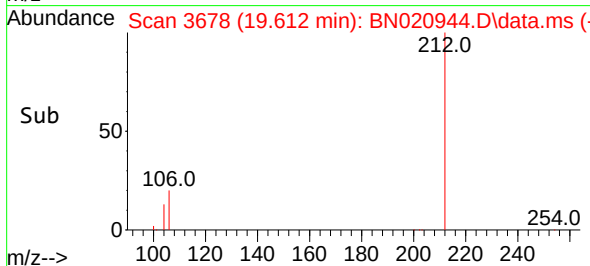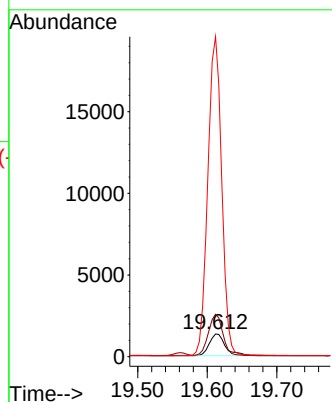

#26
Benzo(a)pyrene
Concen: 0.074 ng/ul
RT: 23.616 min Scan# 4935
Delta R.T. -0.047 min
Lab File: BN020944.D
Acq: 02 Aug 2022 15:44

Tgt Ion:252 Resp: 3299
Ion Ratio Lower Upper
252 100
253 43.0 22.1 33.1#
125 35.1 14.7 22.1#

