

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080222\
 Data File : BN020949.D
 Acq On : 02 Aug 2022 18:53
 Operator : CG/JU
 Sample : PB146650BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 02 22:34:16 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 04:19:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	2912	0.400	ng/ul	0.00
4) Naphthalene-d8	10.602	136	9222	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.461	164	5465	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.210	188	10815	0.400	ng/ul	0.00
17) Chrysene-d12	21.427	240	7886	0.400	ng/ul	0.00
23) Perylene-d12	23.765	264	8510	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	18573	5.230	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.213	152	3817	0.281	ng/ul	0.00
18) Fluoranthene-d10	19.254	212	8429	0.349	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.456	166	1334	0.062	ng/ul#	15
20) Pyrene	19.612	202	1192	0.032	ng/ul#	1
26) Benzo(a)pyrene	23.613	252	2543	0.066	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080222\
Data File : BN020949.D
Acq On : 02 Aug 2022 18:53
Operator : CG/JU
Sample : PB146650BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Aug 02 22:34:16 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 04:19:04 2022
Response via : Initial Calibration

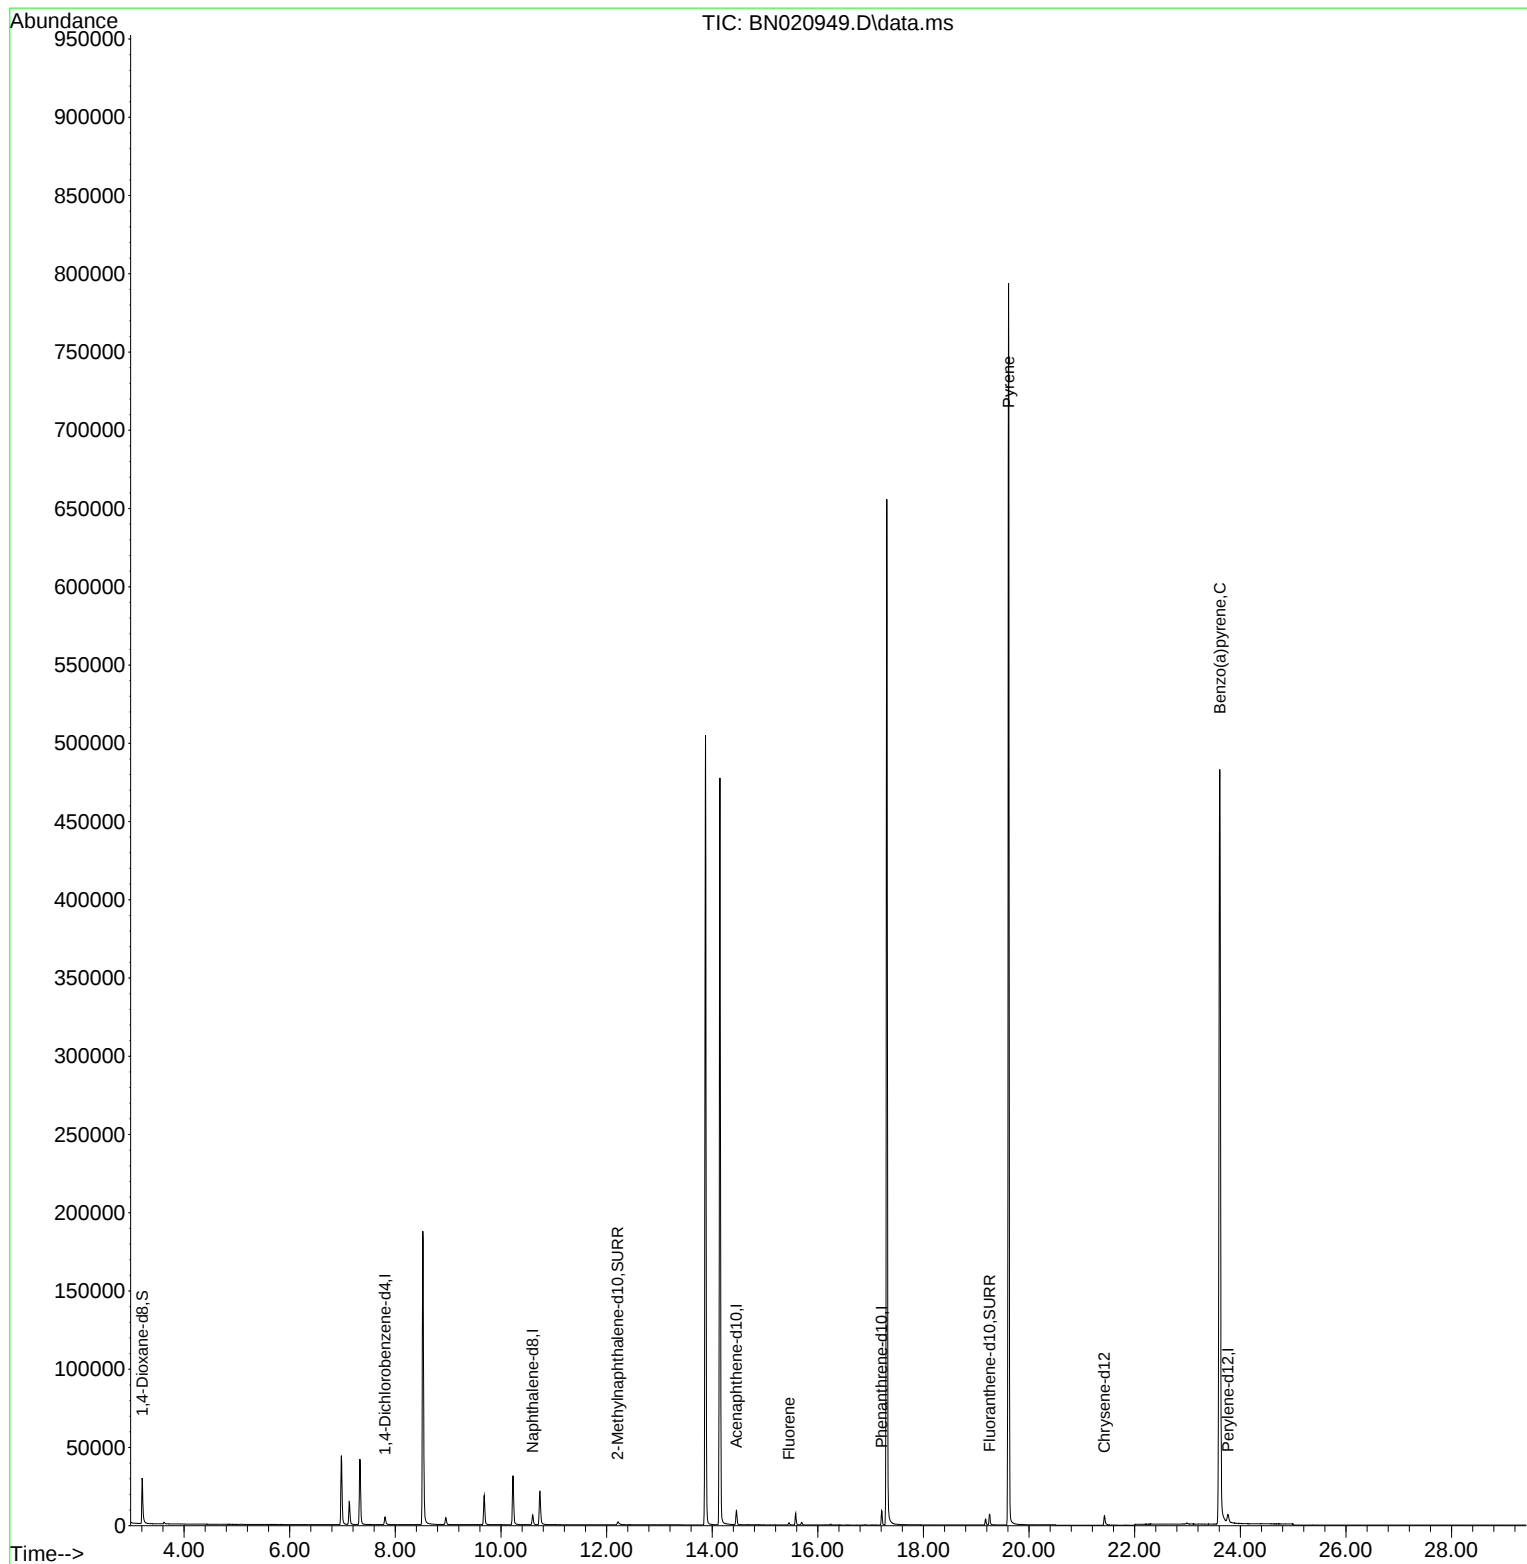



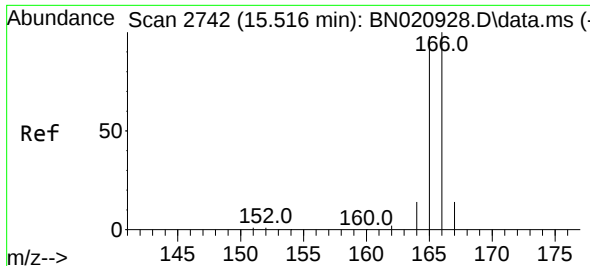


#12
Fluorene
Concen: 0.062 ng/ul
RT: 15.456 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN020949.D
Acq: 02 Aug 2022 18:53

Instrument :
BNA_N
ClientSampleId :



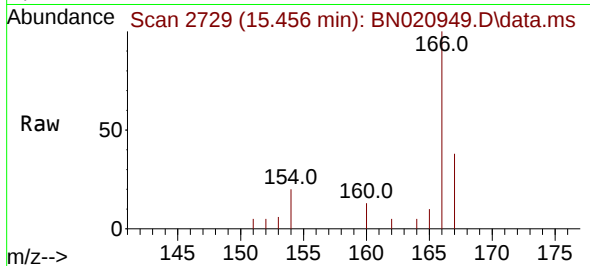



Tgt Ion:166 Resp: 1334
Ion Ratio Lower Upper
166 100
165 9.7 78.6 117.8#
167 37.8 11.8 17.6#

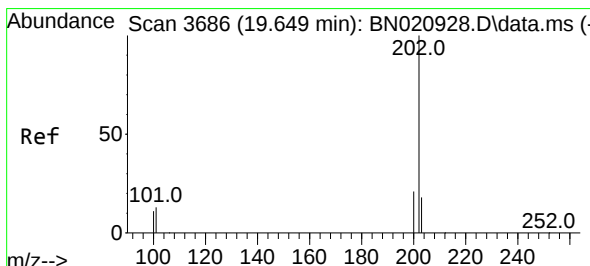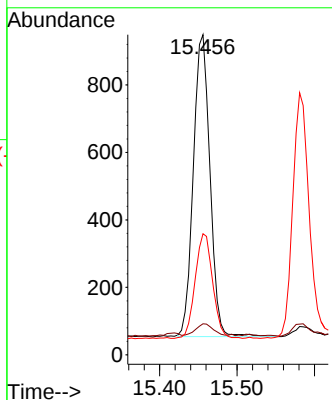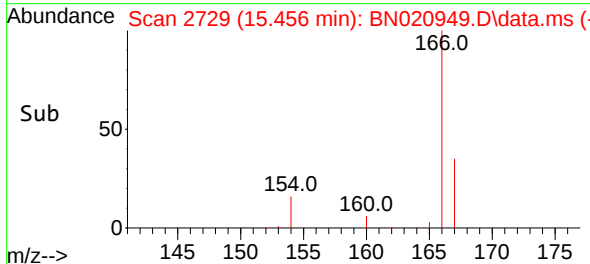

#20
Pyrene
Concen: 0.032 ng/ul
RT: 19.612 min Scan# 3678
Delta R.T. -0.037 min
Lab File: BN020949.D
Acq: 02 Aug 2022 18:53

Tgt Ion:202 Resp: 1192
Ion Ratio Lower Upper
202 100
101 184.3 11.3 16.9#
100 1335.0 9.0 13.4#

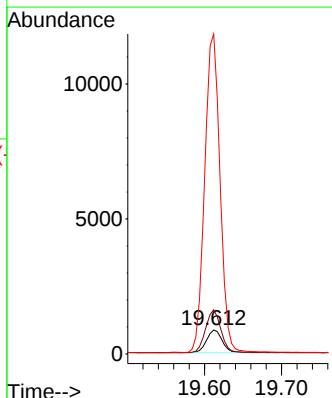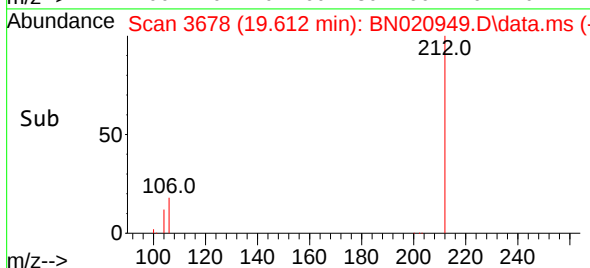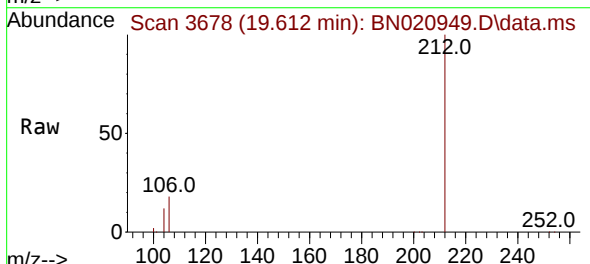

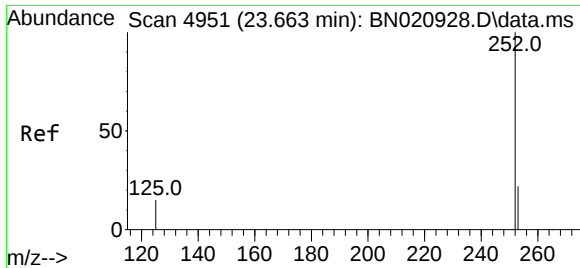

#26

Benzo(a)pyrene

Concen: 0.066 ng/ul

RT: 23.613 min Scan# 49

Delta R.T. -0.050 min


Lab File: BN020949.D

Acq: 02 Aug 2022 18:53

Instrument :

BNA_N

ClientSampleId :

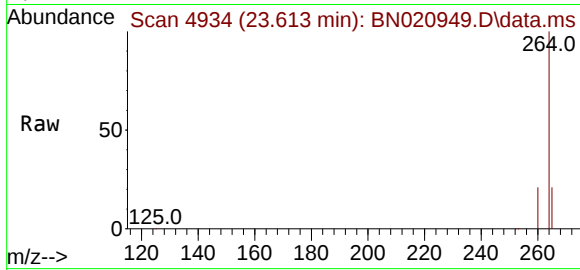

Tgt Ion:252 Resp: 2543

Ion Ratio Lower Upper

252 100

253 44.1 22.1 33.1#

125 35.6 14.7 22.1#

