

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080222\
 Data File : BN020954.D
 Acq On : 02 Aug 2022 22:01
 Operator : CG/JU
 Sample : N3943-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 02 22:34:36 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 04:19:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	2737	0.400	ng/ul	0.00
4) Naphthalene-d8	10.602	136	7759	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.457	164	4607	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.210	188	9722	0.400	ng/ul	0.00
17) Chrysene-d12	21.418	240	10072	0.400	ng/ul	0.00
23) Perylene-d12	23.757	264	10561	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.206	96	19016	5.697	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.213	152	3665	0.320	ng/ul	0.00
18) Fluoranthene-d10	19.249	212	12052	0.391	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.456	166	1270	0.070	ng/ul#	15
20) Pyrene	19.612	202	1576	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.605	252	3510	0.074	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080222\
Data File : BN020954.D
Acq On : 02 Aug 2022 22:01
Operator : CG/JU
Sample : N3943-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Aug 02 22:34:36 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 04:19:04 2022
Response via : Initial Calibration

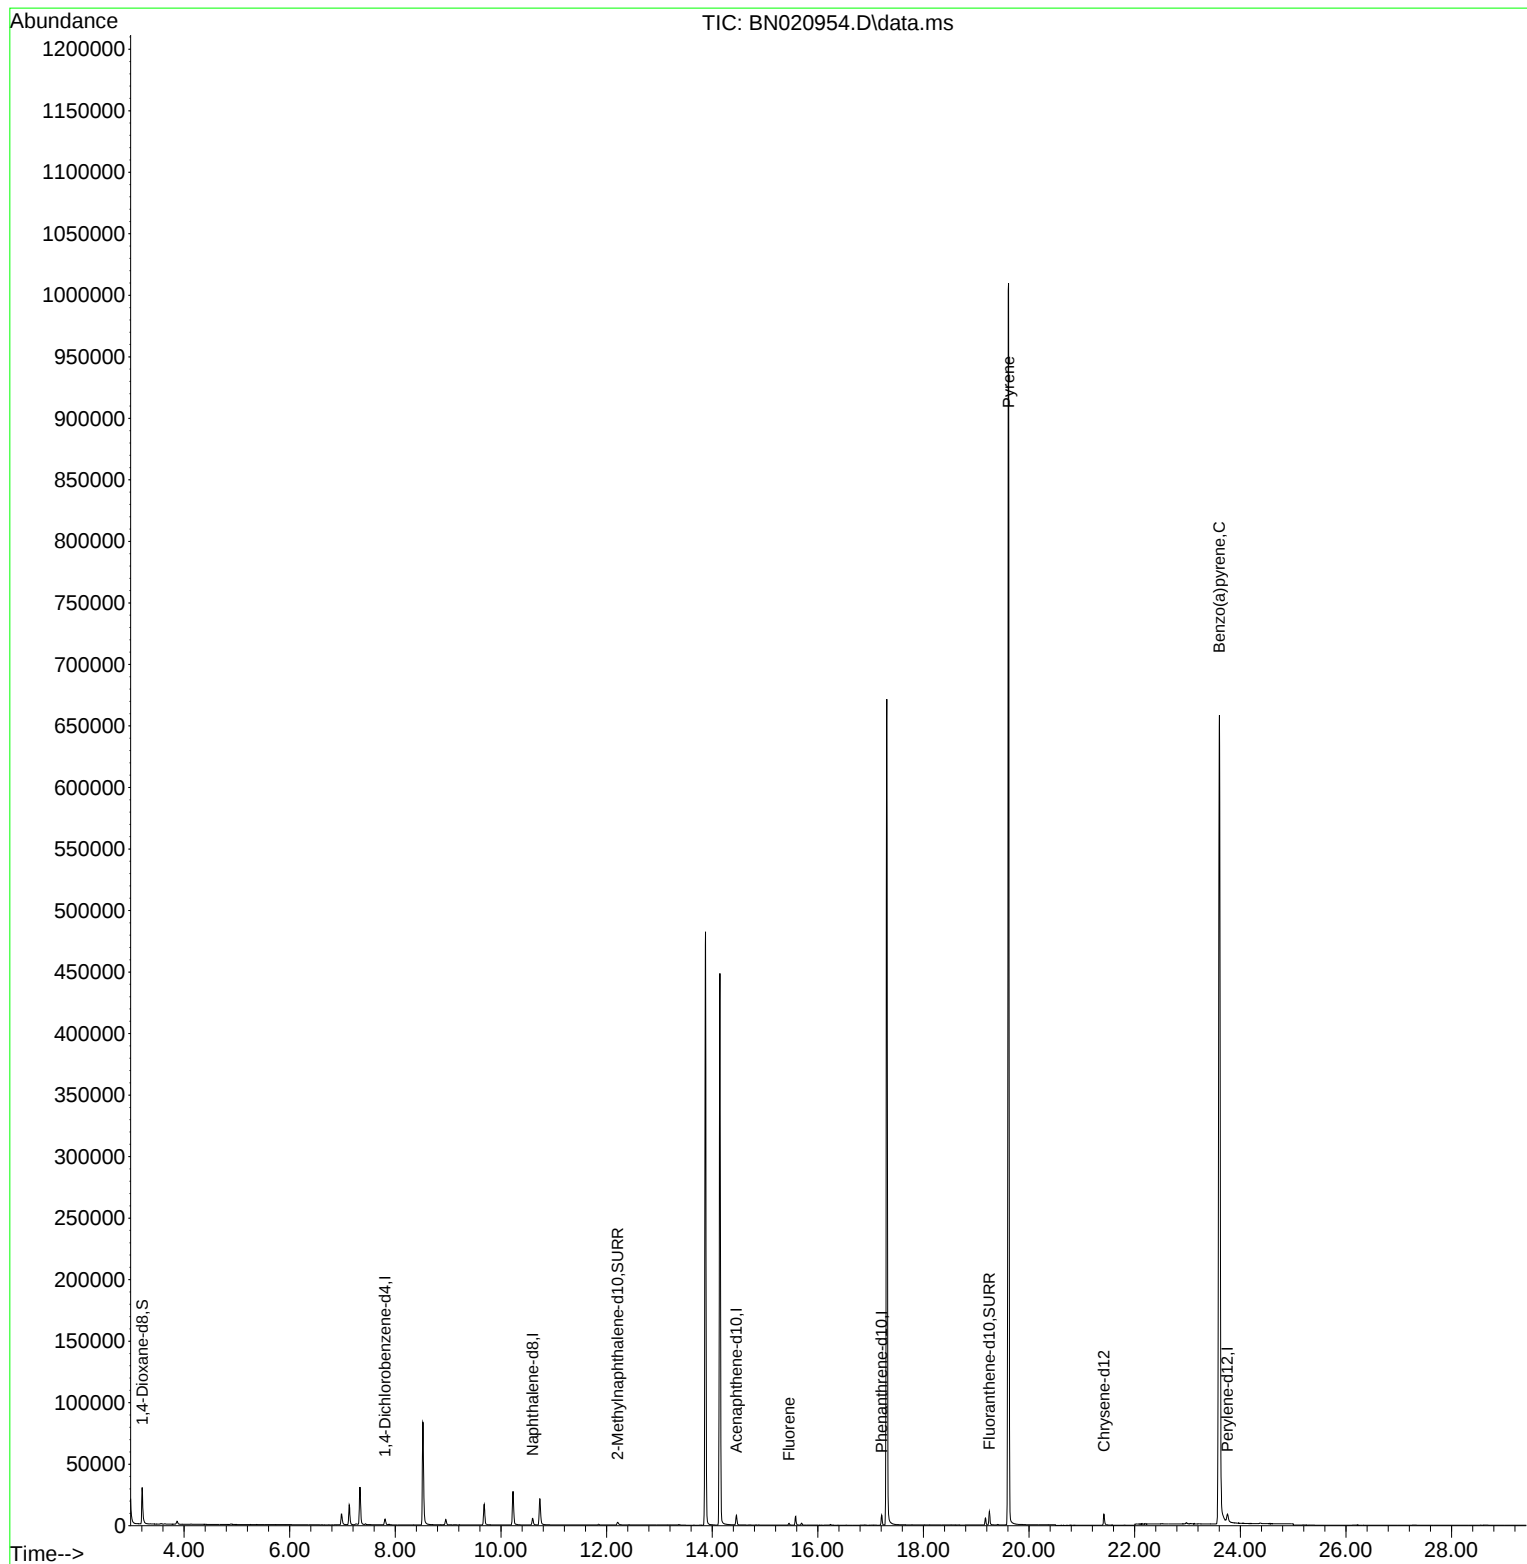



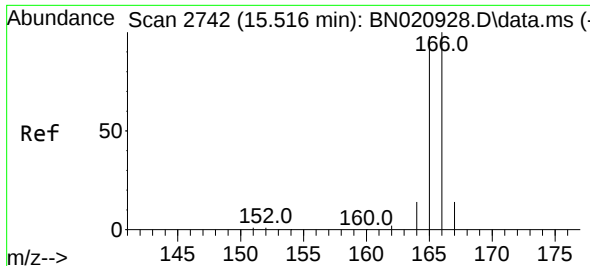


#12
Fluorene
Concen: 0.070 ng/ul
RT: 15.456 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN020954.D
Acq: 02 Aug 2022 22:01

Instrument :
BNA_N
ClientSampleId :



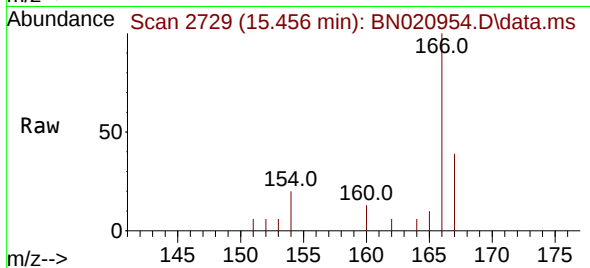



Tgt Ion:166 Resp: 1270
Ion Ratio Lower Upper
166 100
165 10.1 78.6 117.8#
167 38.8 11.8 17.6#

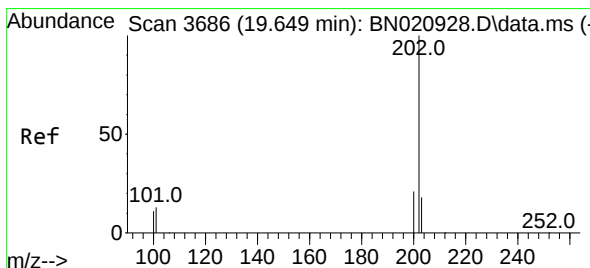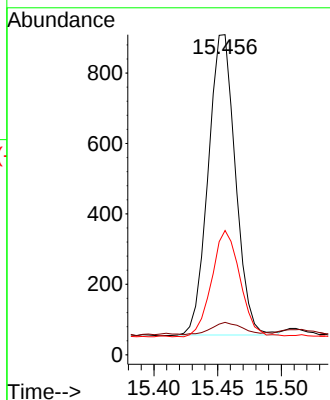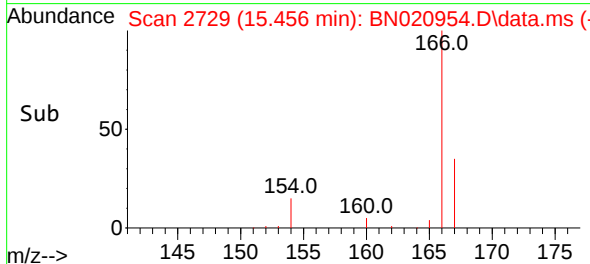

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.612 min Scan# 3678
Delta R.T. -0.037 min
Lab File: BN020954.D
Acq: 02 Aug 2022 22:01

Tgt Ion:202 Resp: 1576
Ion Ratio Lower Upper
202 100
101 181.9 11.3 16.9#
100 1290.9 9.0 13.4#

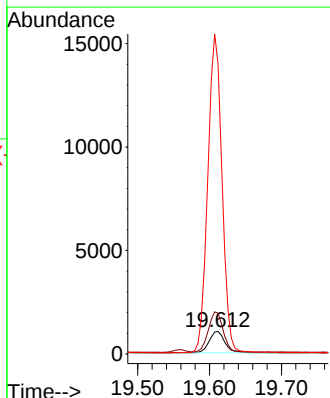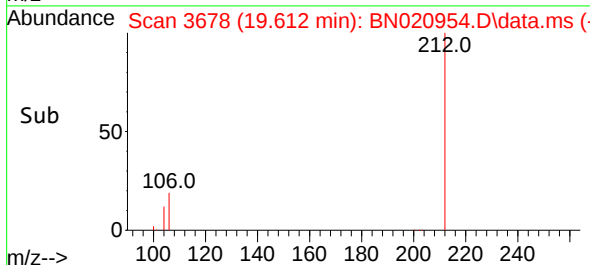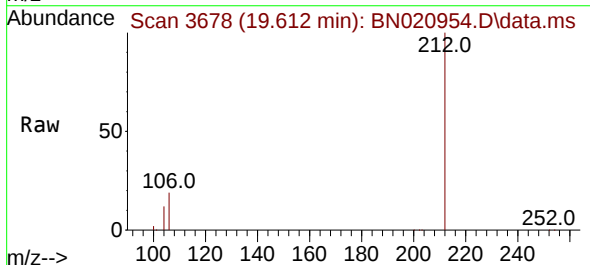

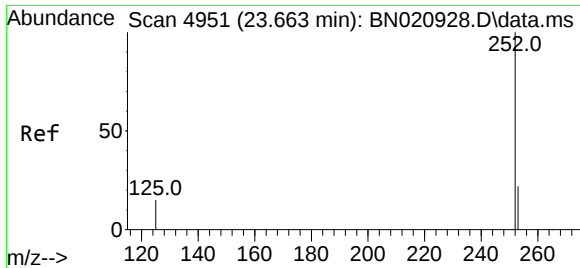

#26

Benzo(a)pyrene

Concen: 0.074 ng/ul

RT: 23.605 min Scan# 49

Delta R.T. -0.059 min


Lab File: BN020954.D

Acq: 02 Aug 2022 22:01

Instrument :

BNA_N

ClientSampleId :

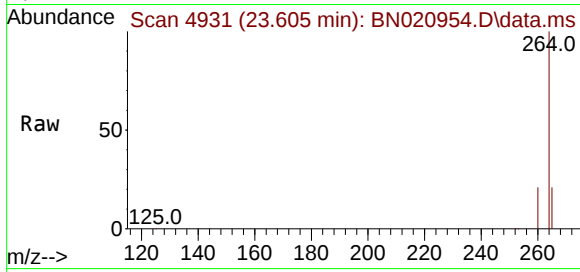

Tgt Ion:252 Resp: 3510

Ion Ratio Lower Upper

252 100

253 44.9 22.1 33.1#

125 35.2 14.7 22.1#

