

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080222\
 Data File : BN020937.D
 Acq On : 02 Aug 2022 11:11
 Operator : CG/JU
 Sample : N3943-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C59

Quant Time: Aug 02 11:40:26 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 04:19:04 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.818	152	2135	0.400	ng/ul	0.00
4) Naphthalene-d8	10.618	136	7144	0.400	ng/ul #	0.01
9) Acenaphthene-d10	14.461	164	4251	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.222	188	7463	0.400	ng/ul	0.00
17) Chrysene-d12	21.427	240	7121	0.400	ng/ul	0.00
23) Perylene-d12	23.771	264	6586	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.211	96	1850	0.711	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.224	152	3317	0.315	ng/ul	0.02
18) Fluoranthene-d10	19.254	212	8269	0.379	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.240	88	11460	4.088	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080222\
 Data File : BN020937.D
 Acq On : 02 Aug 2022 11:11
 Operator : CG/JU
 Sample : N3943-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C59


Quant Time: Aug 02 11:40:26 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 04:19:04 2022
 Response via : Initial Calibration

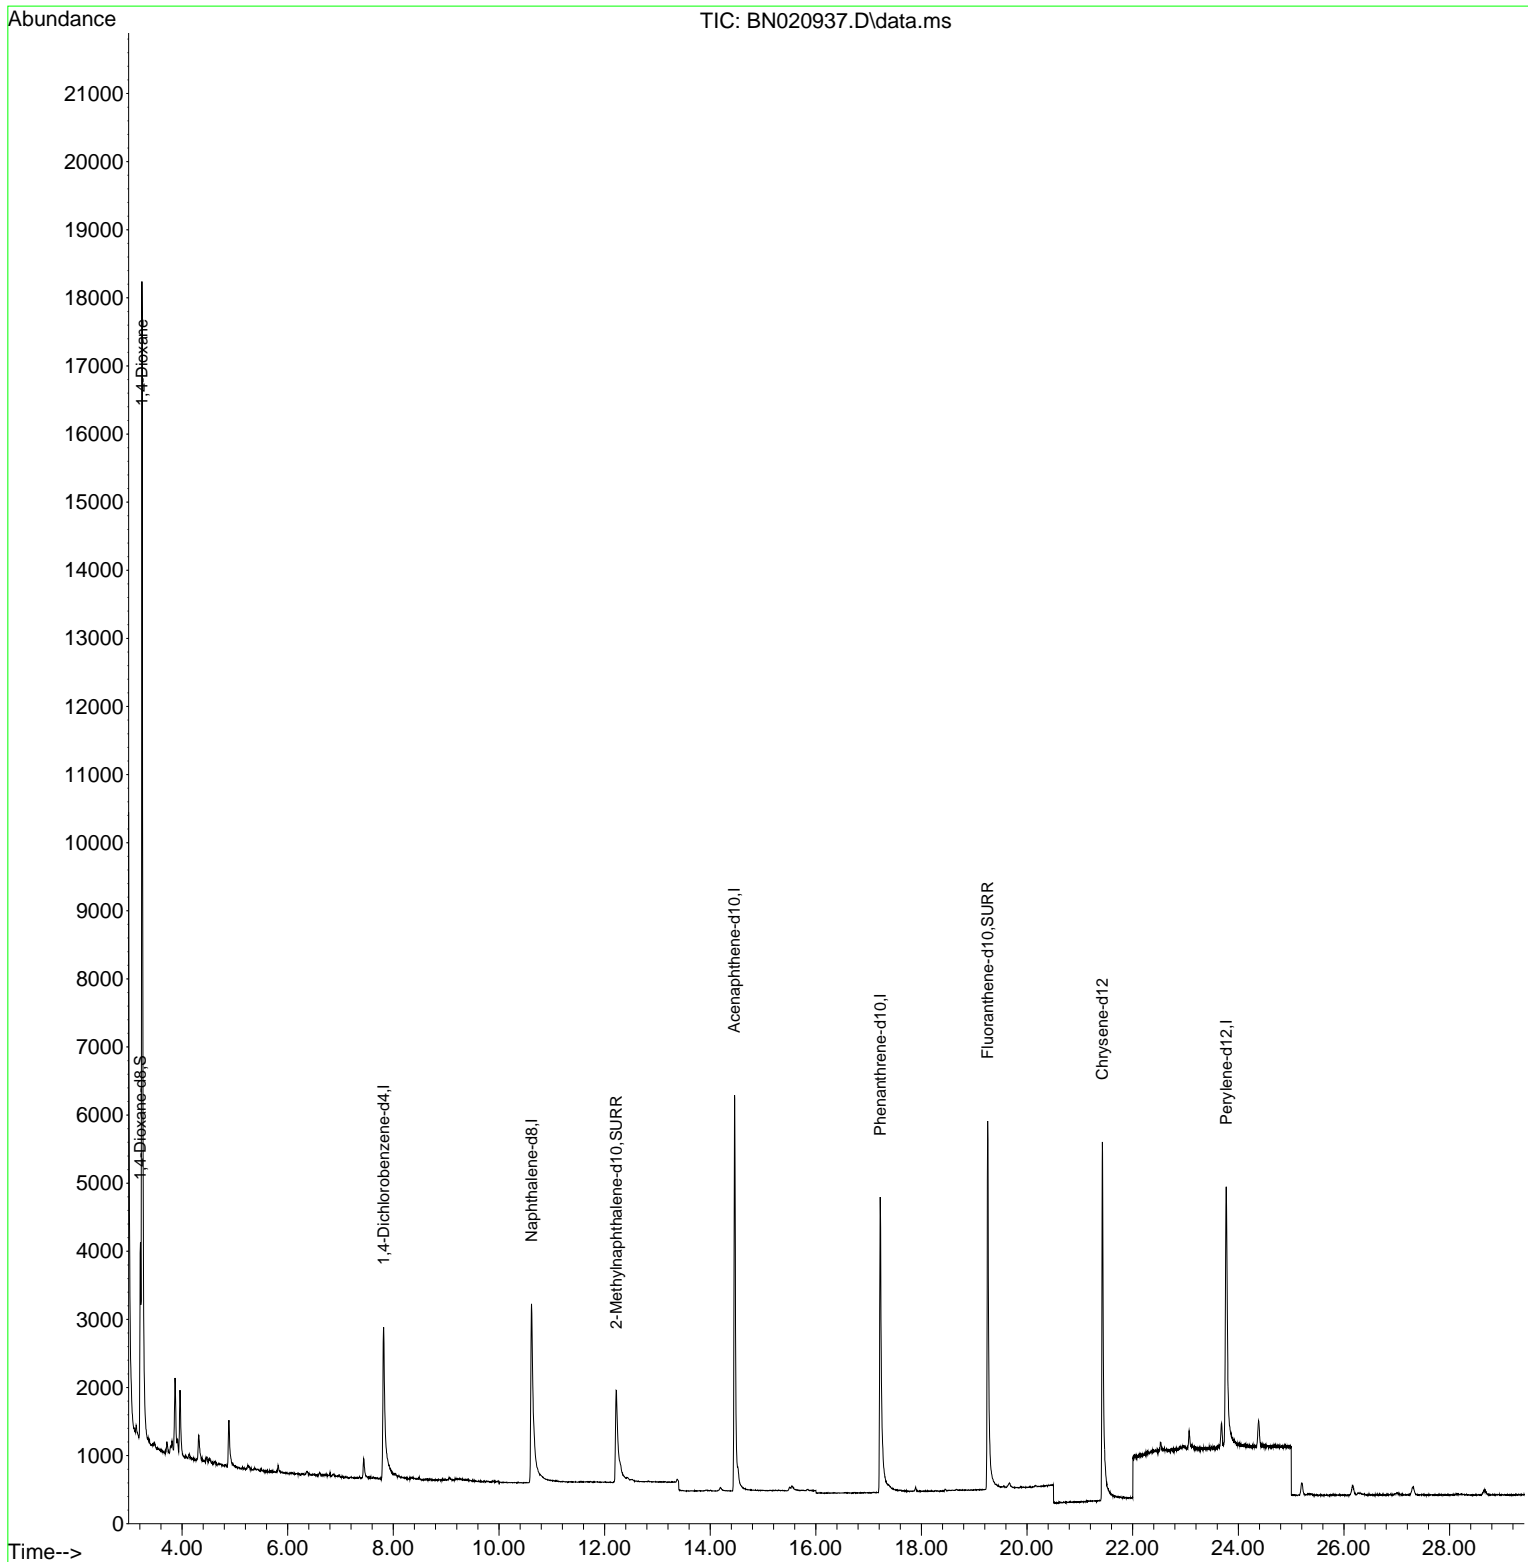

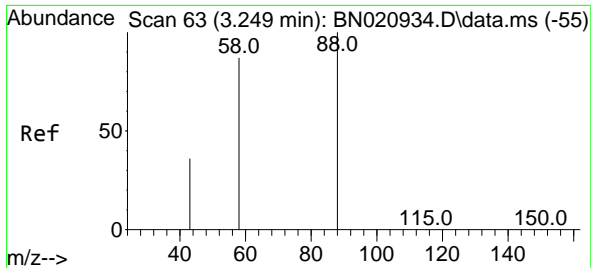

#2
 1,4-Dioxane
 Concen: 4.088 ng/ul
 RT: 3.240 min Scan# 61
 Delta R.T. -0.004 min
 Lab File: BN020937.D
 Acq: 02 Aug 2022 11:11

Instrument :
 BNA_N
 ClientSampleId :
 C0C59

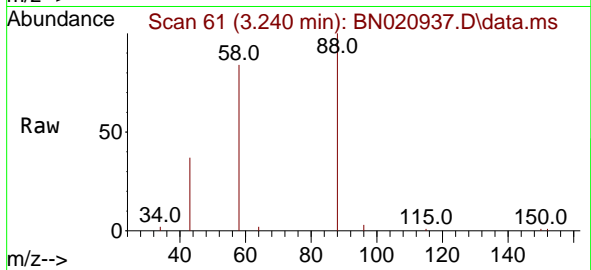

Tgt Ion: 88 Resp: 11460
 Ion Ratio Lower Upper
 88 100
 43 36.7 31.4 47.0
 58 83.7 49.0 73.6#

