

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080222\
 Data File : BN020938.D
 Acq On : 02 Aug 2022 12:02
 Operator : CG/JU
 Sample : N3943-07DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C59DL

Quant Time: Aug 02 12:29:12 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 04:19:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.806	152	3010	0.400	ng/u1	0.00
4) Naphthalene-d8	10.607	136	9767	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.461	164	5793	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.218	188	10601	0.400	ng/u1	0.00
17) Chrysene-d12	21.427	240	9744	0.400	ng/u1	0.00
23) Perylene-d12	23.771	264	9139	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.215	96	474	0.129	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.230	152	716	0.050	ng/u1	0.02
18) Fluoranthene-d10	19.263	212	1934	0.065	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.245	88	2591	0.656	ng/u1	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080222\
Data File : BN020938.D
Acq On : 02 Aug 2022 12:02
Operator : CG/JU
Sample : N3943-07DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C59DL


Quant Time: Aug 02 12:29:12 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 04:19:04 2022
Response via : Initial Calibration

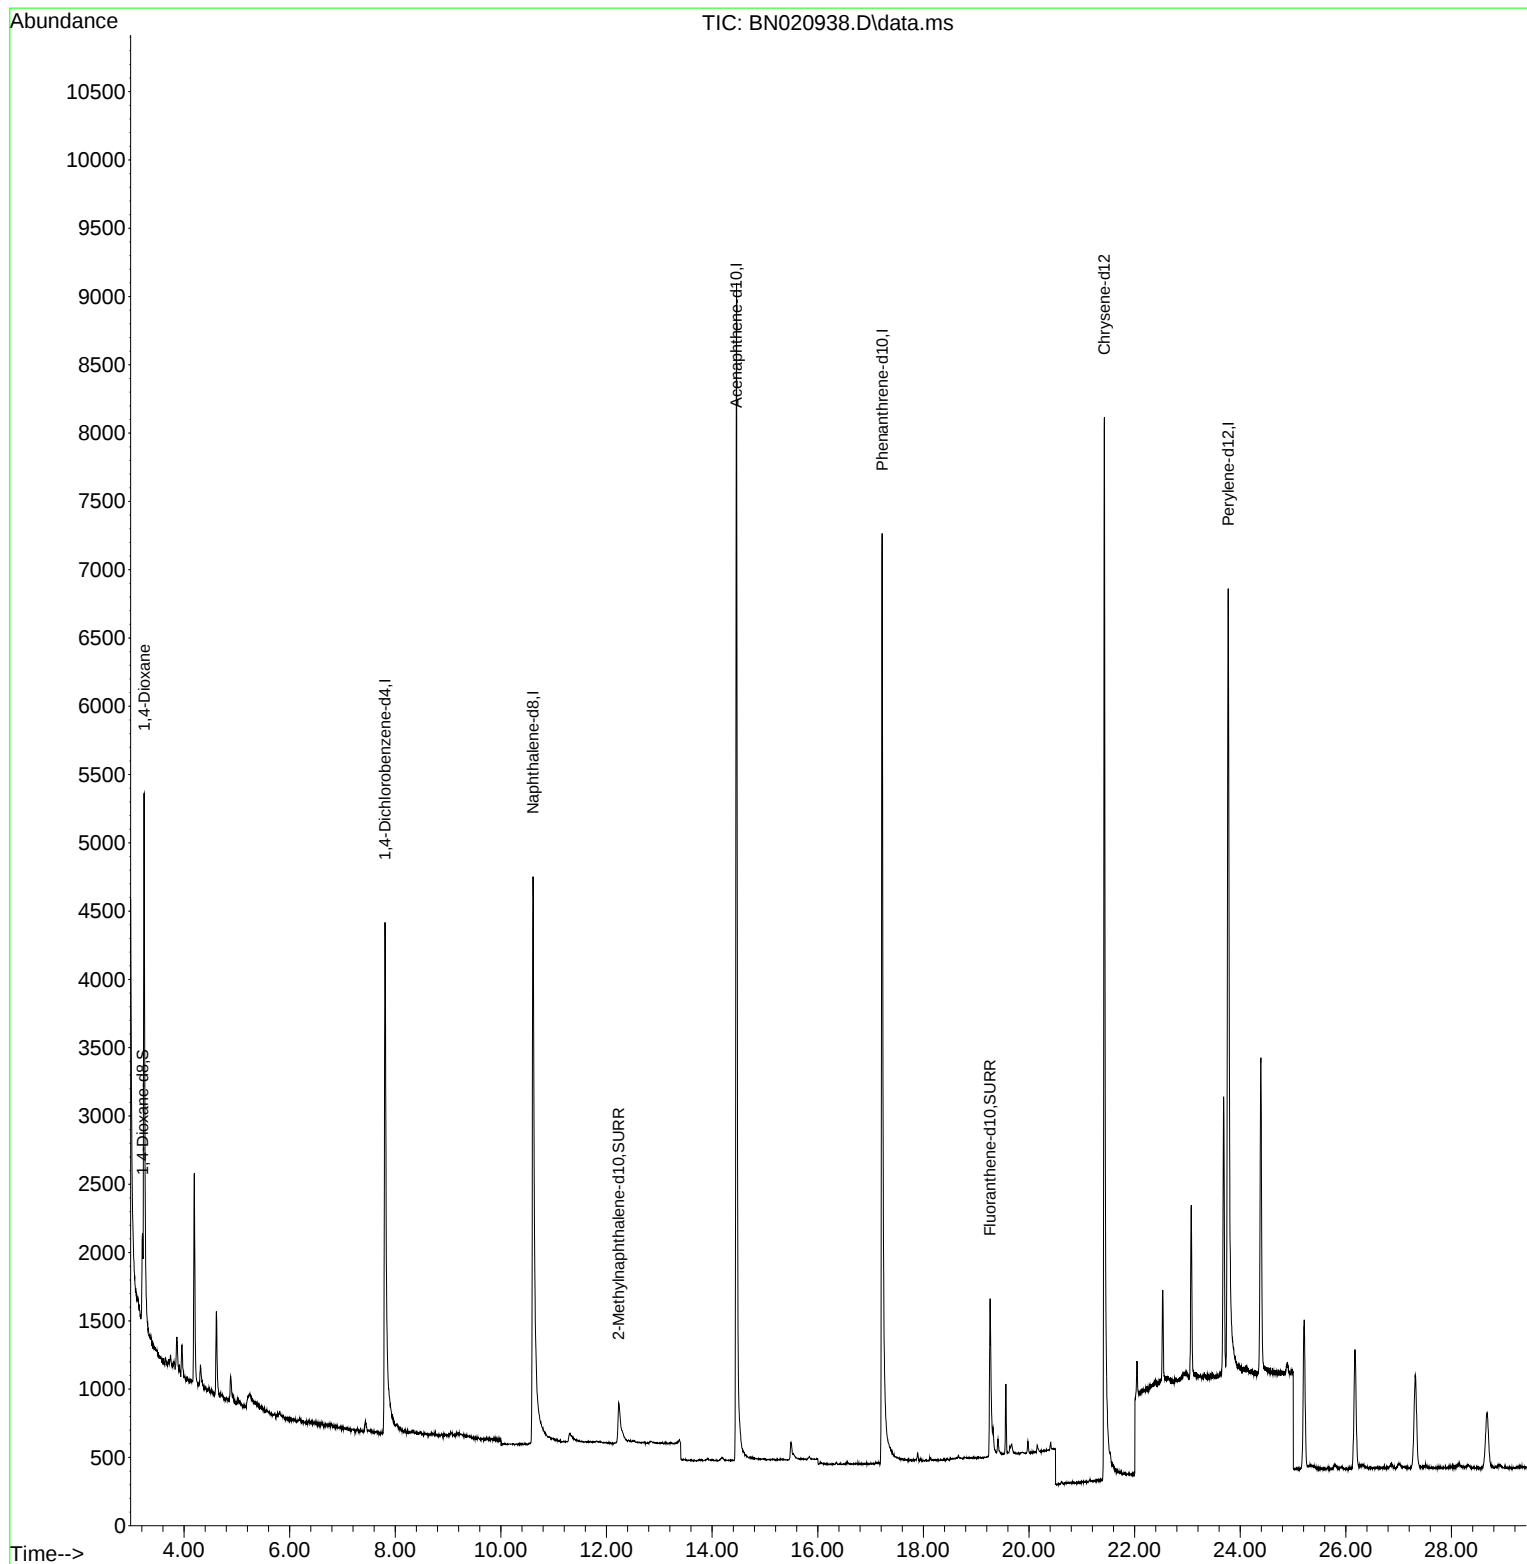

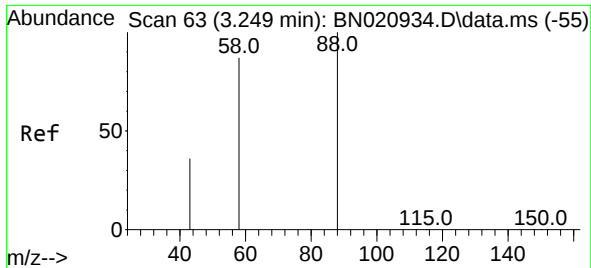

#2
 1,4-Dioxane
 Concen: 0.656 ng/ul
 RT: 3.245 min Scan# 61
 Delta R.T. 0.001 min
 Lab File: BN020938.D
 Acq: 02 Aug 2022 12:02

Instrument :
 BNA_N
 ClientSampleId :
 C0C59DL

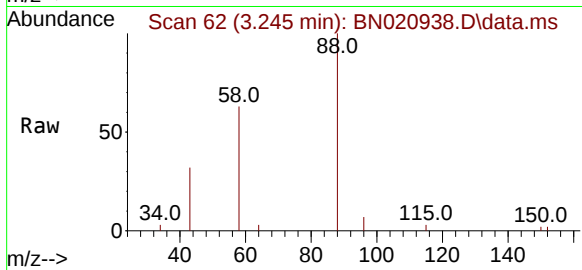

Tgt Ion:	88	Resp:	2591
Ion	Ratio	Lower	Upper
88	100		
43	32.4	31.4	47.0
58	62.7	49.0	73.6

