




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

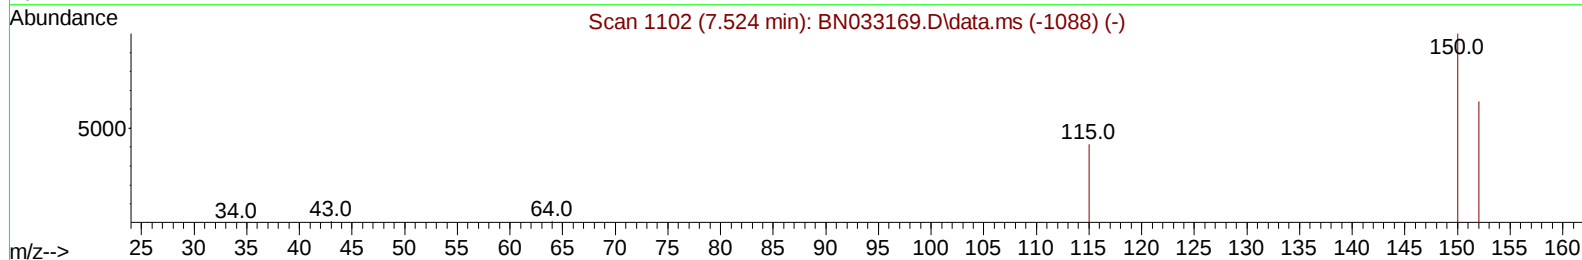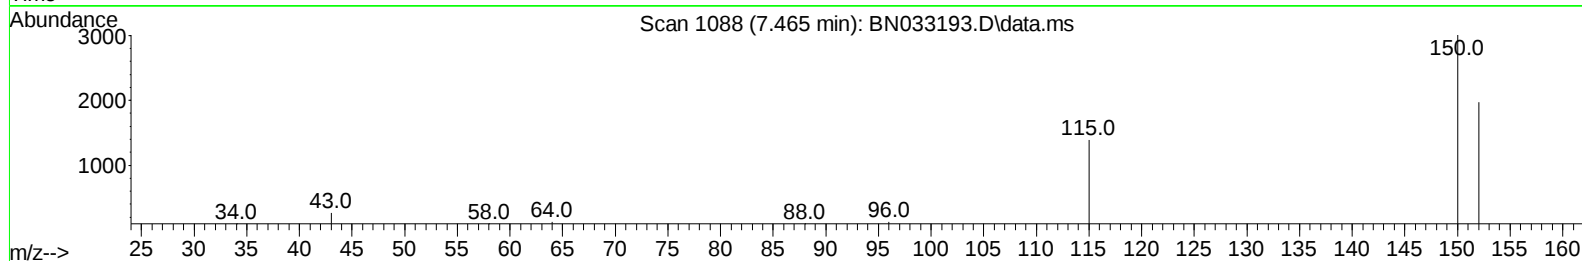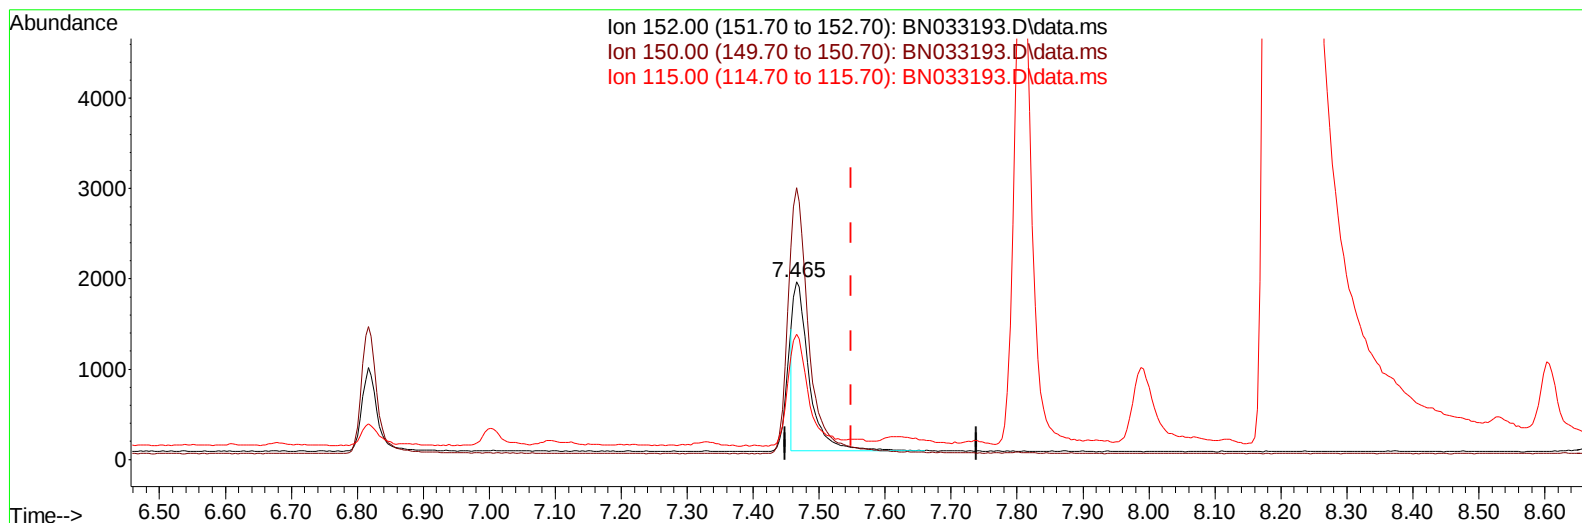

TIC: BN033193.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.465min (-0.084) 0.40 ng/u1

response 3190

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	143.10	152.61
115.00	84.50	70.37
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

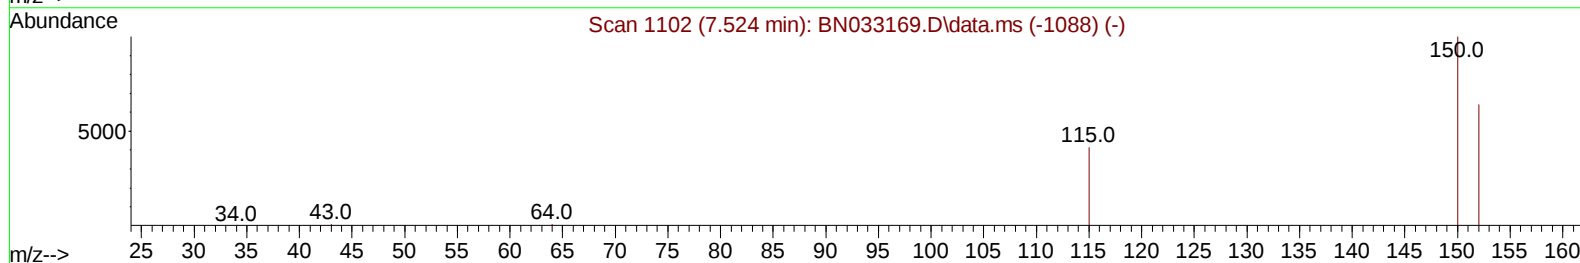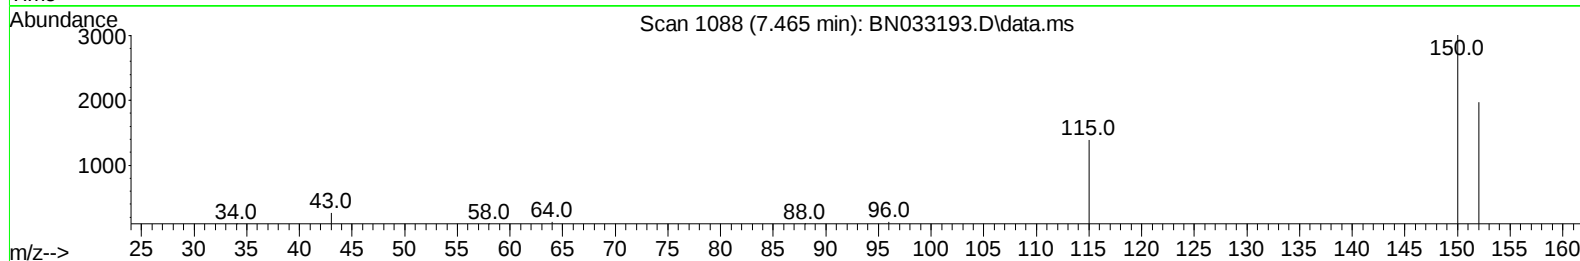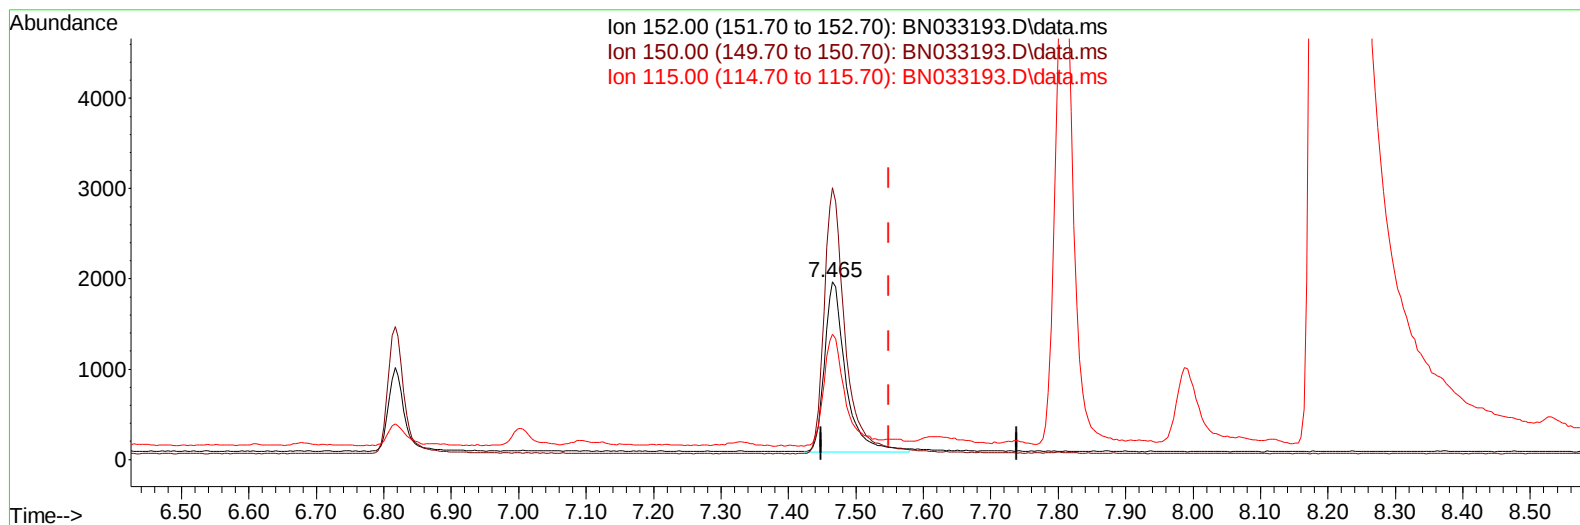

TIC: BN033193.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.465min (-0.084) 0.40 ng/ul m

response 4111

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	143.10	152.61
115.00	84.50	70.37
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

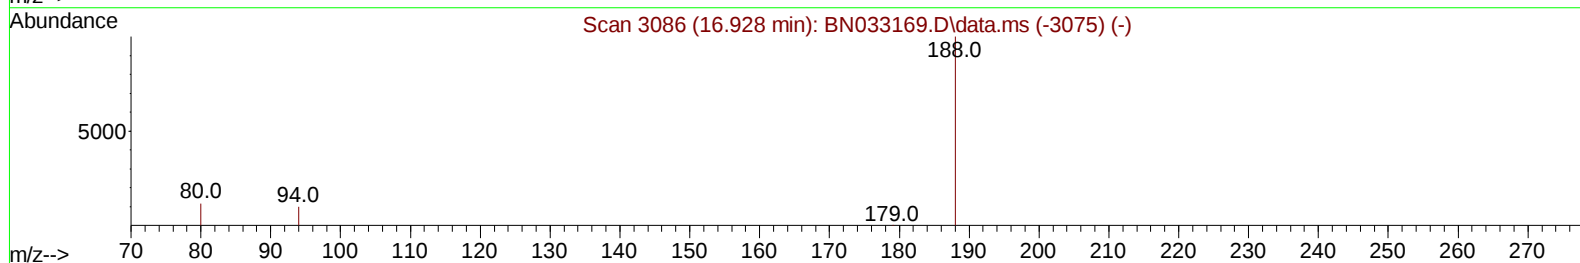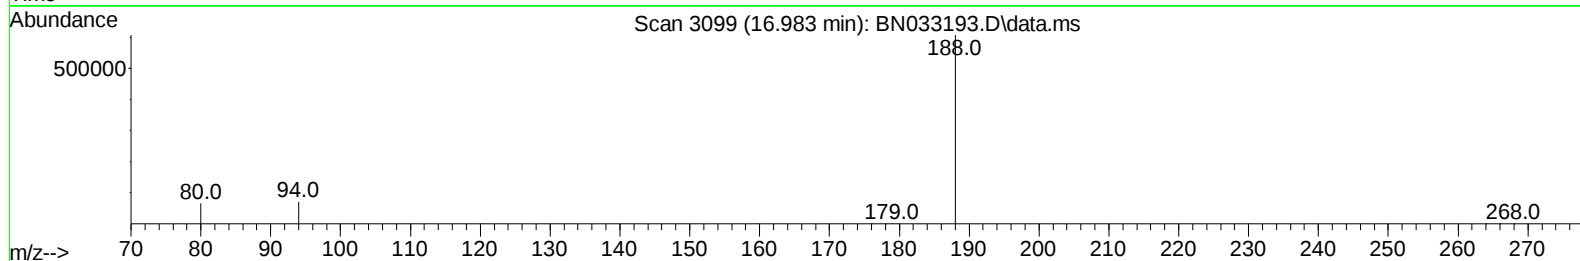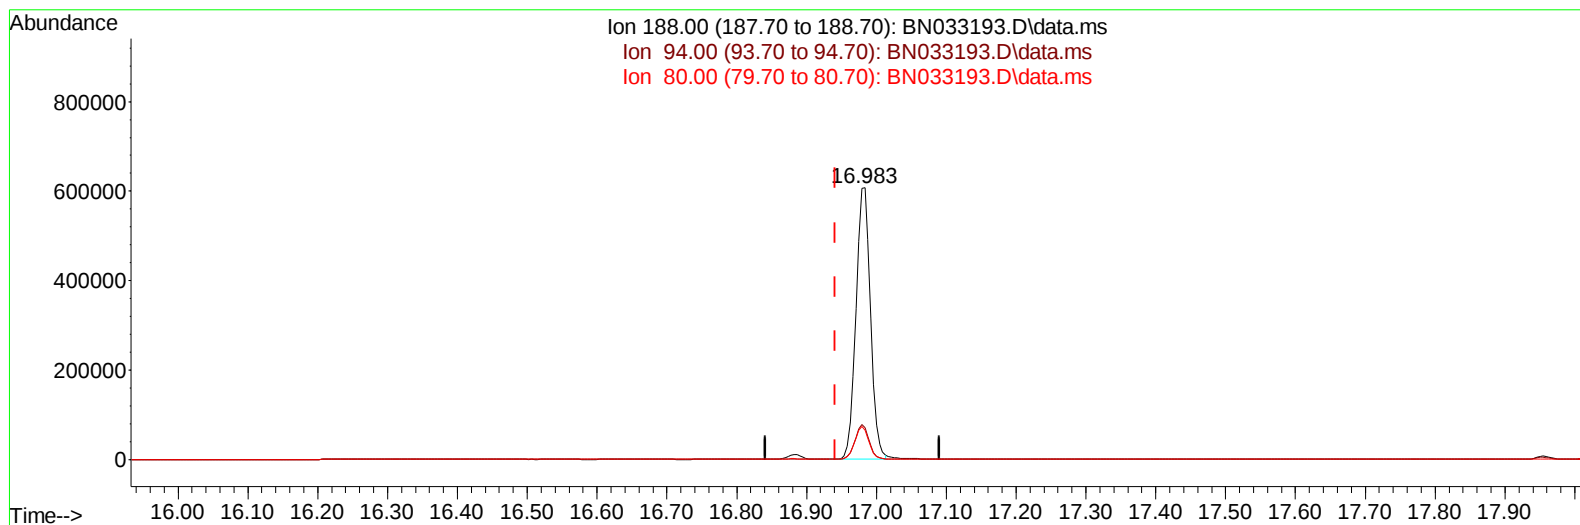

TIC: BN033193.D\data.ms

(13) Phenanthrene-d10 (I)

16.983min (+ 0.042) 0.40 ng/u1

response 874611

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	11.64
80.00	13.10	10.81
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

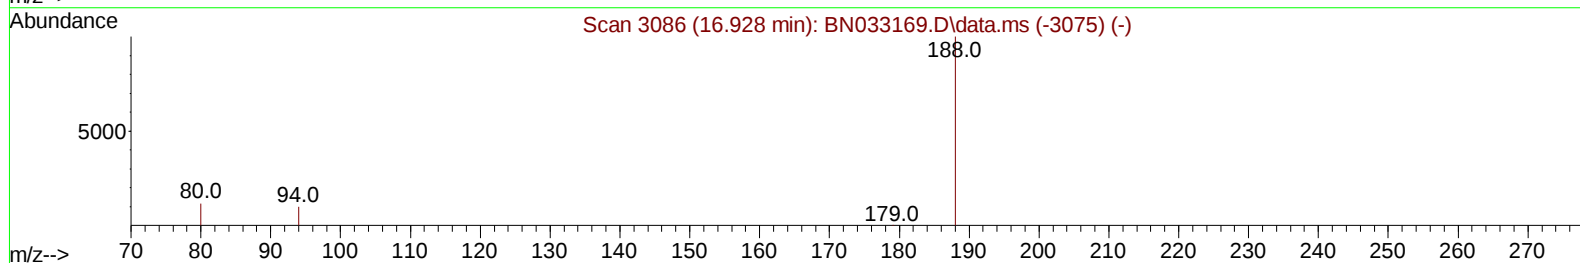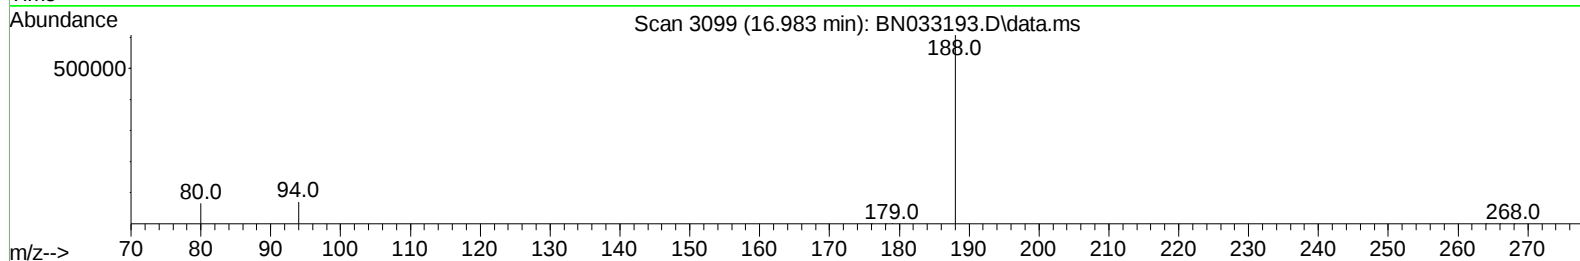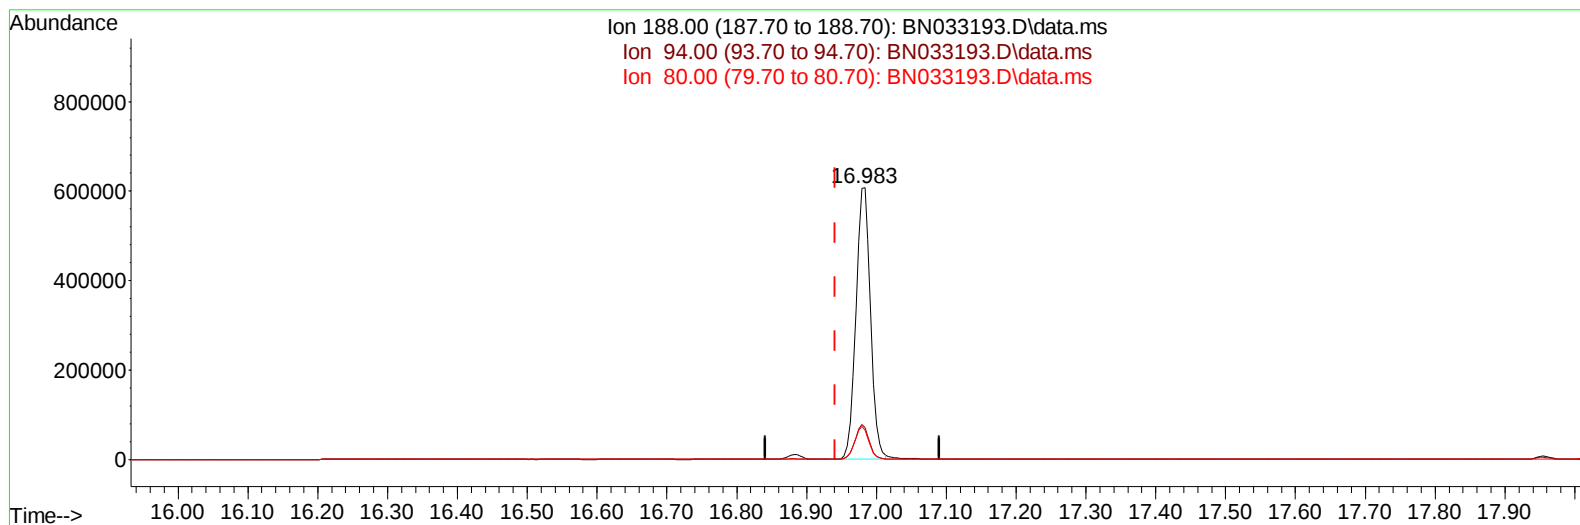

TIC: BN033193.D\data.ms

(13) Phenanthrene-d10 (I)

16.983min (+ 0.042) 0.40 ng/u1

response 874611

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	11.64
80.00	13.10	10.81
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

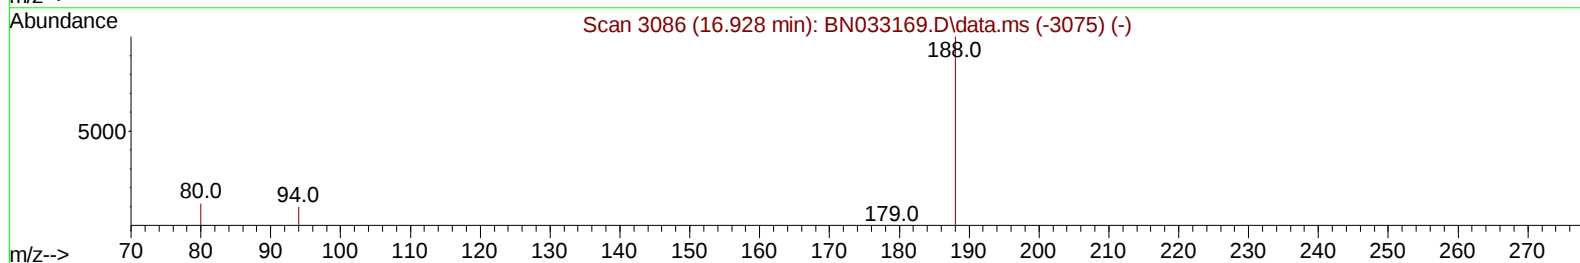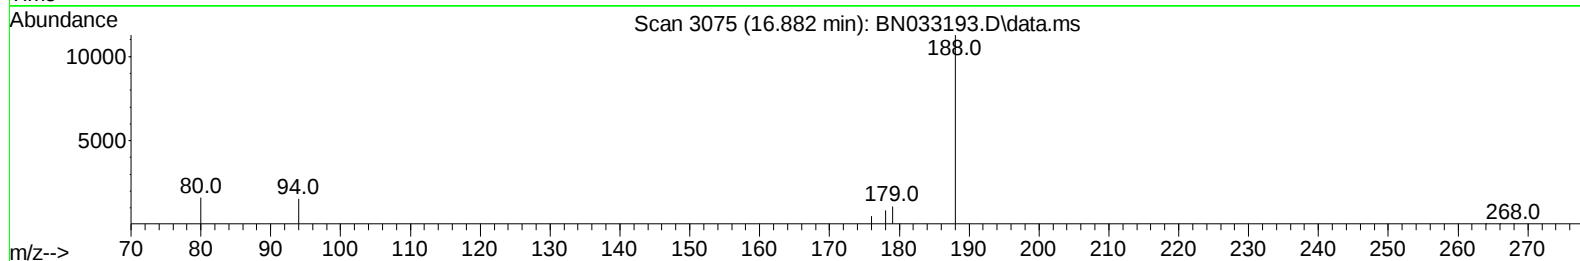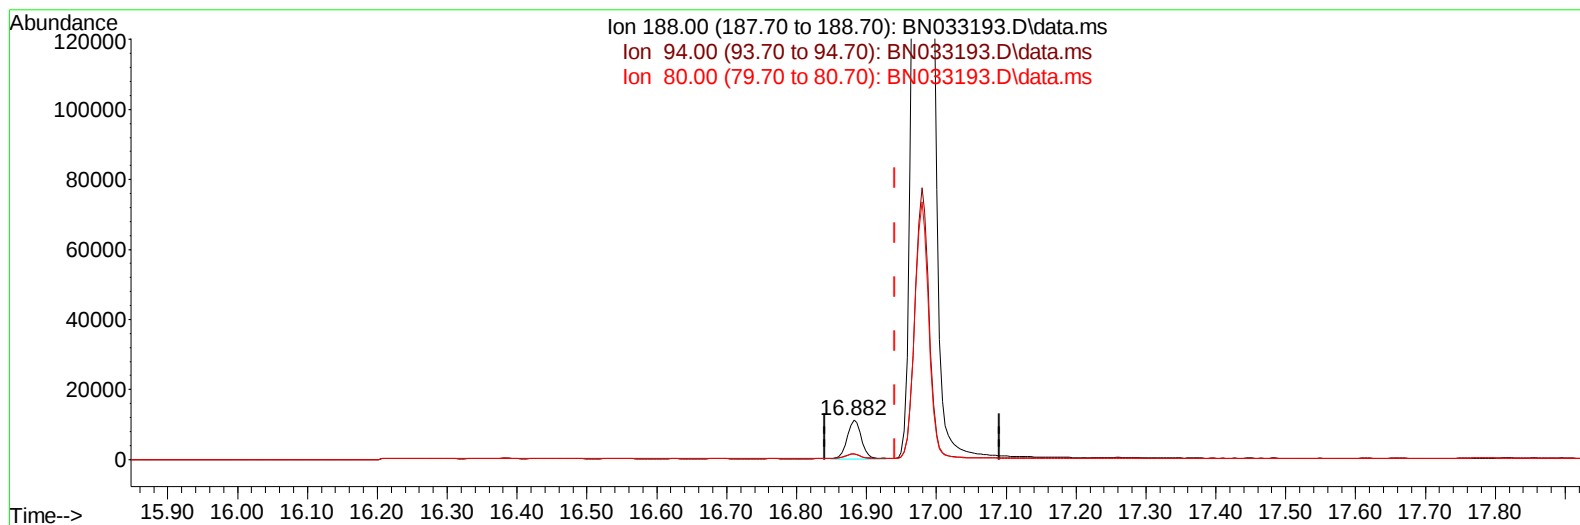

TIC: BN033193.D\data.ms

(13) Phenanthrene-d10 (I)

16.882min (-0.059) 0.40 ng/ul m

response 15883

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.40	13.57
80.00	13.10	14.34
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

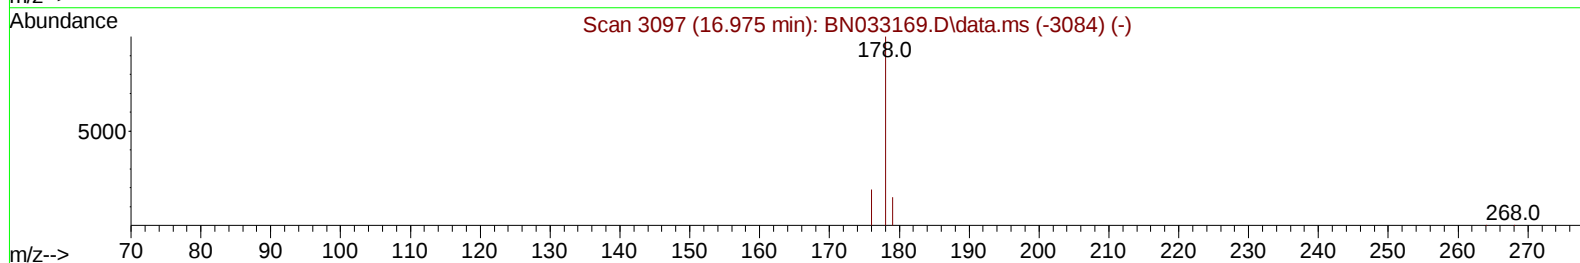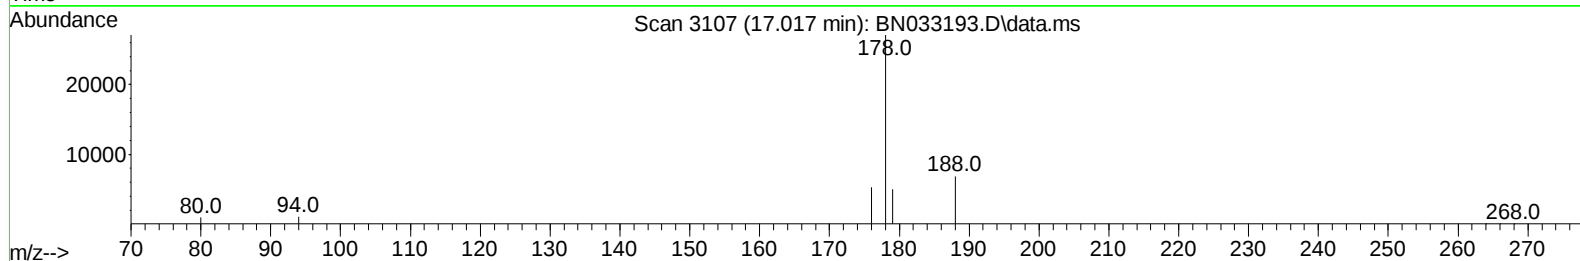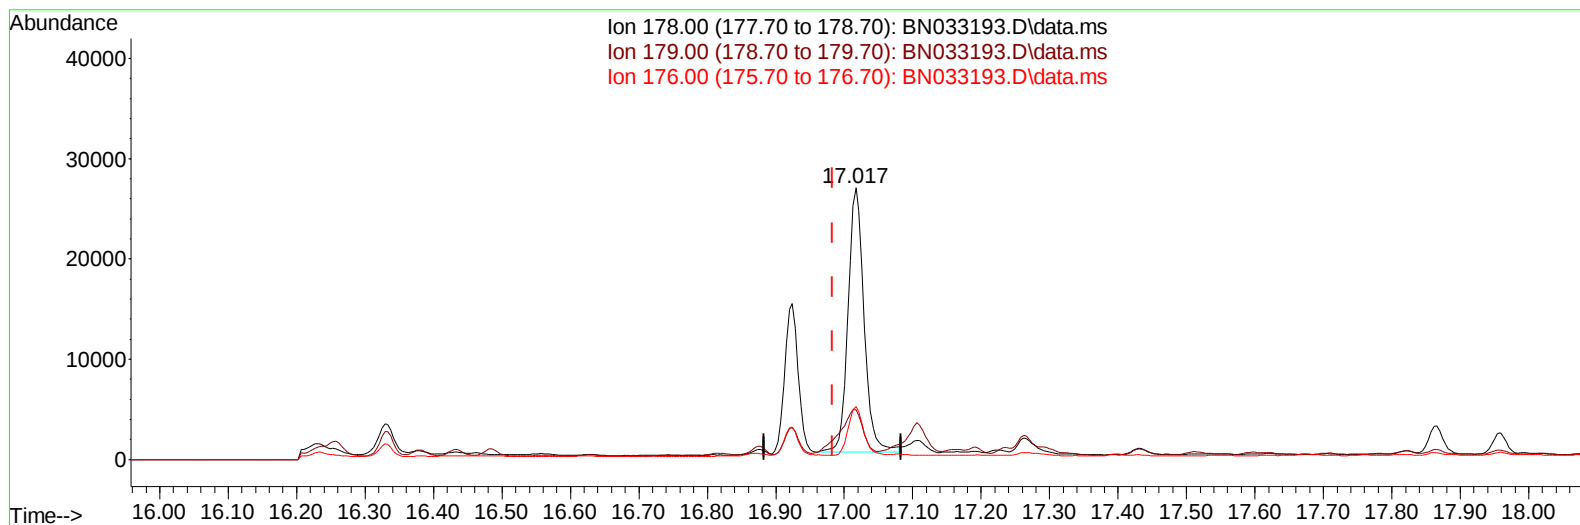

TIC: BN033193.D\data.ms

(15) Phenanthrene

17.017min (+ 0.034) 1.01 ng/u1

response 42918

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.10	18.36
176.00	19.90	19.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

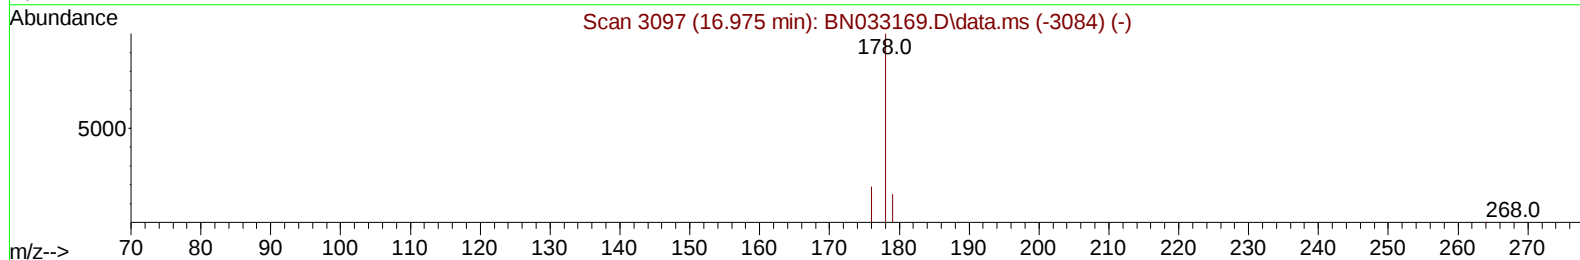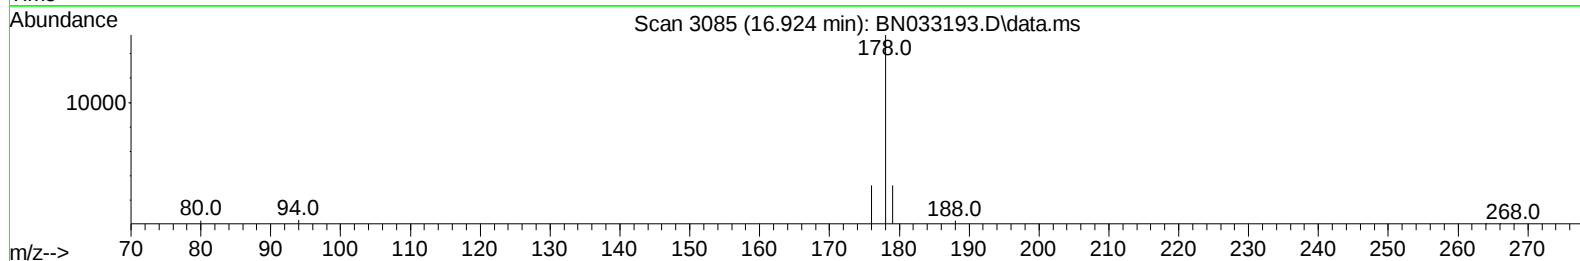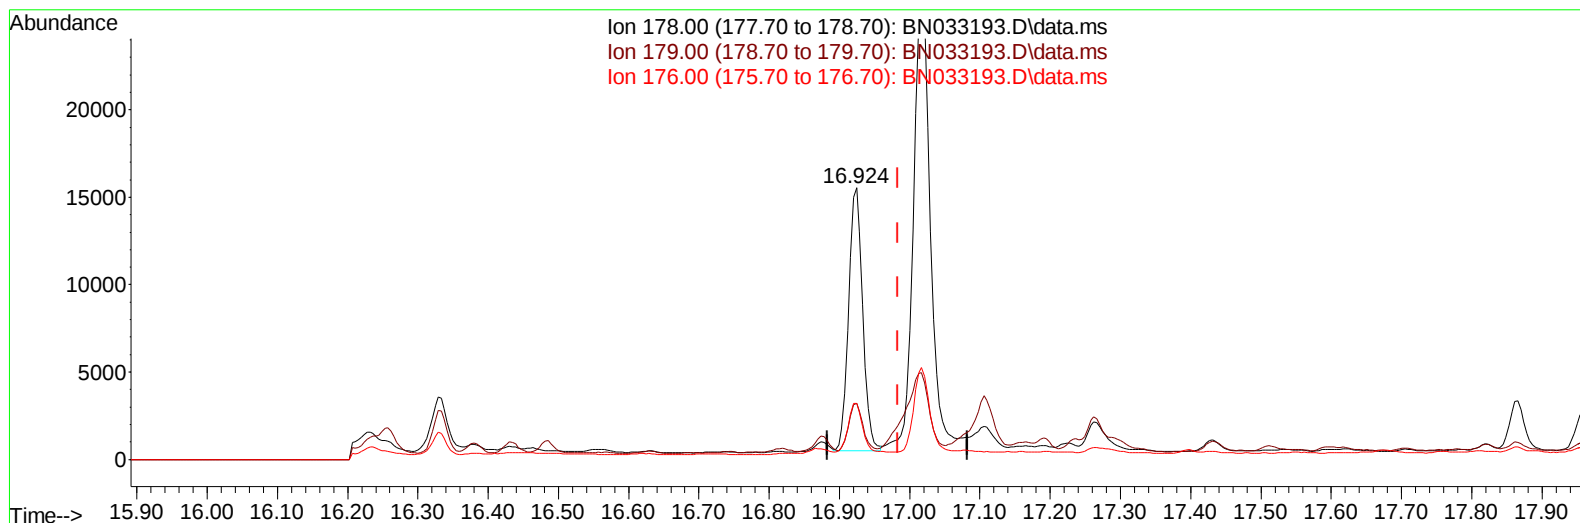

TIC: BN033193.D\data.ms

(15) Phenanthrene

16.924min (-0.059) 0.49 ng/u1 m

response 20922

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.10	20.58#
176.00	19.90	20.72
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
 Data File : BN033193.D
 Acq On : 02 Aug 2024 07:33
 Operator : MA/JU
 Sample : P3378-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
 Supervised By :mohammad ahmed 08/03/2024

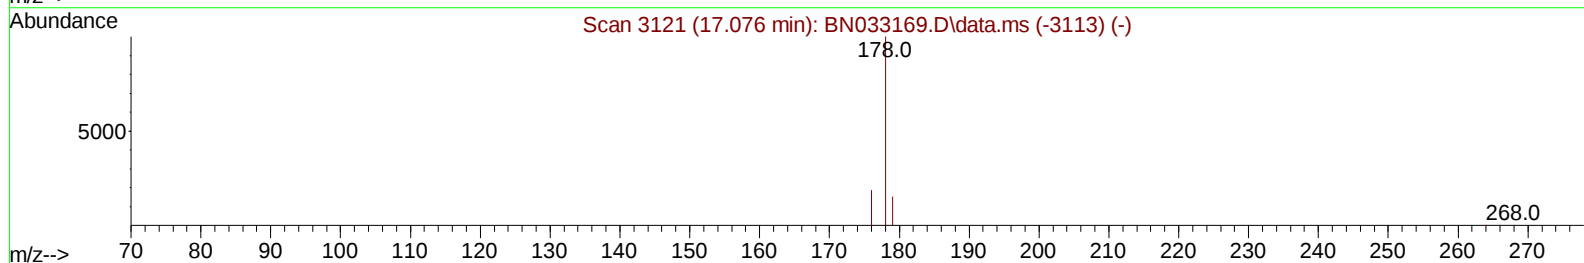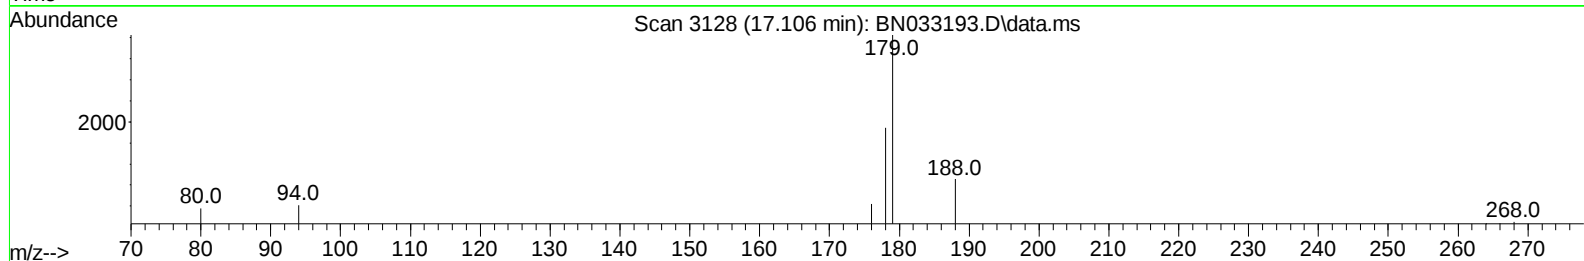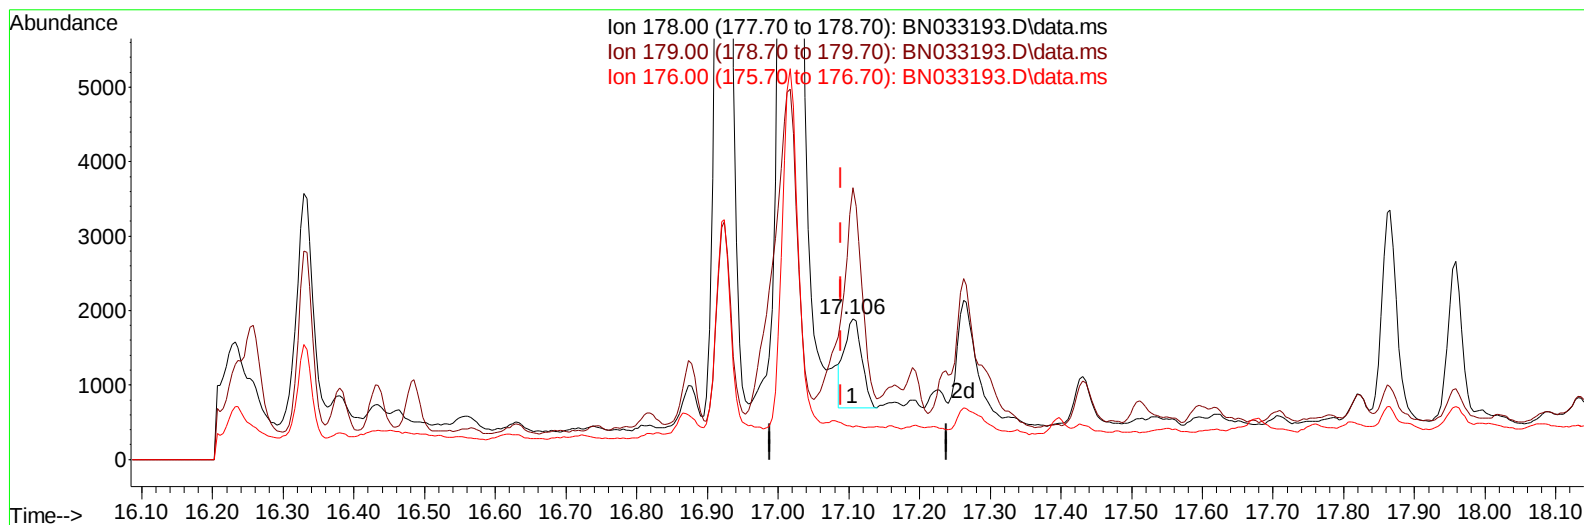

TIC: BN033193.D\data.ms

(16) Anthracene

17.106min (+ 0.017) 0.05 ng/u1

response 2080

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.90	193.07#
176.00	19.80	23.13
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

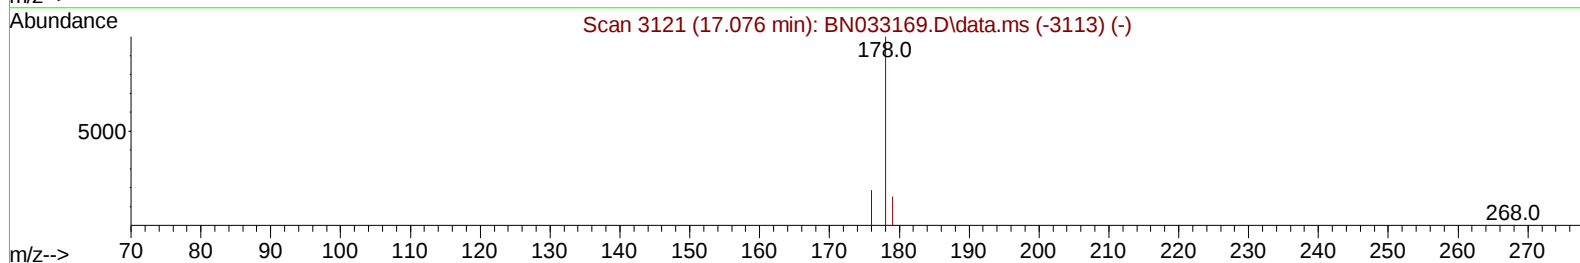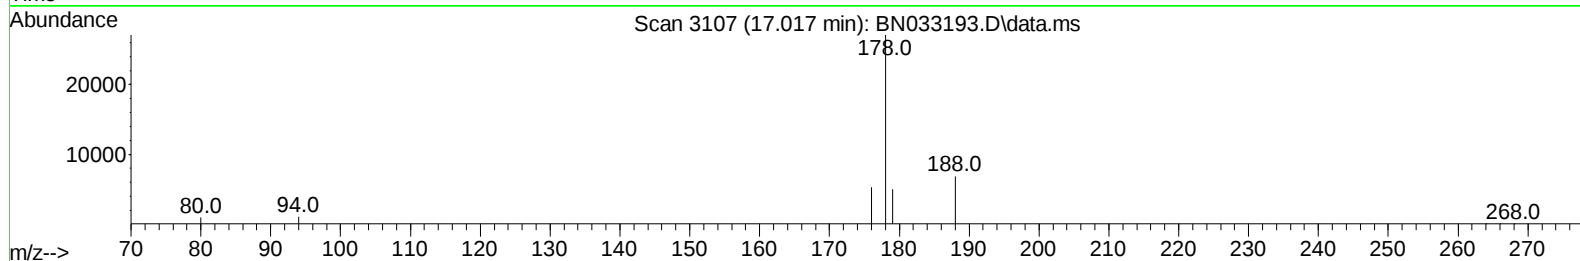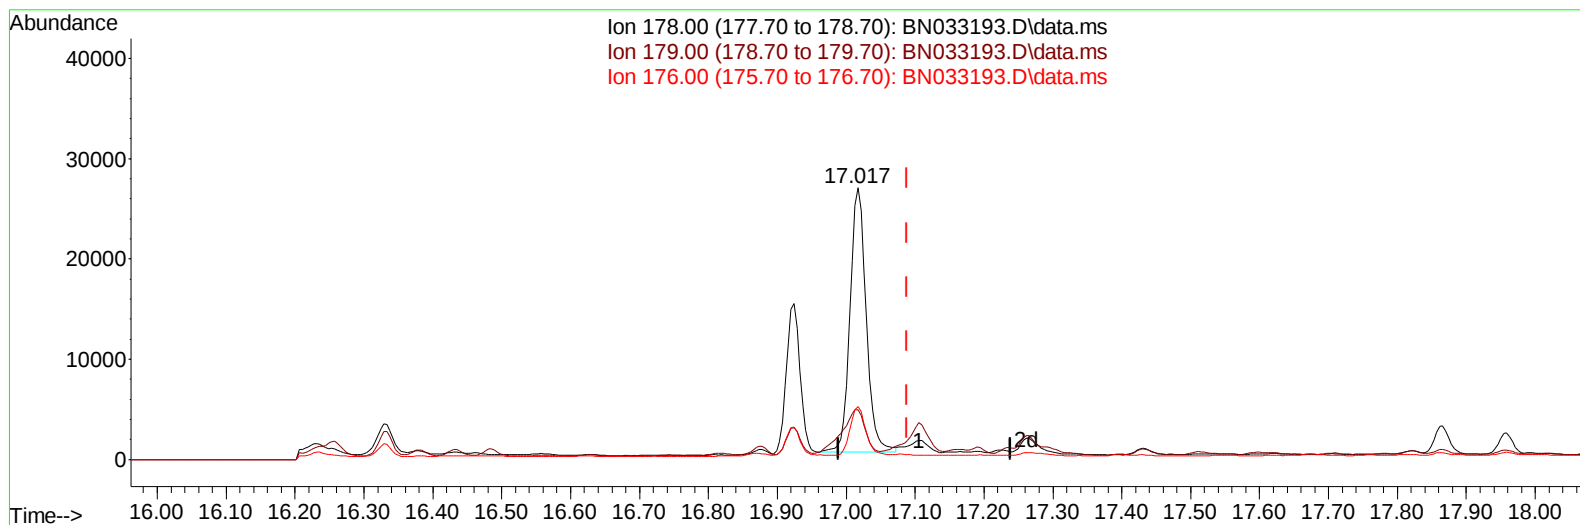

TIC: BN033193.D\data.ms

(16) Anthracene

17.017min (-0.072) 1.12 ng/ul m

response 42743

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.90	18.36
176.00	19.80	19.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

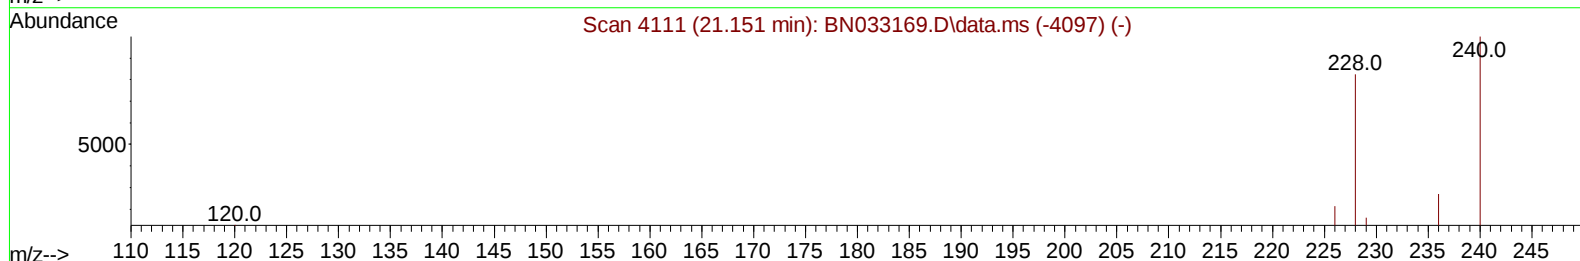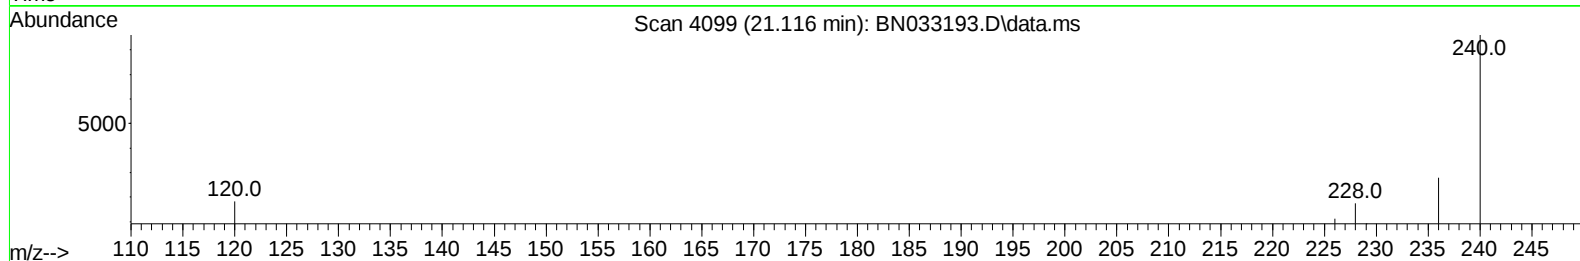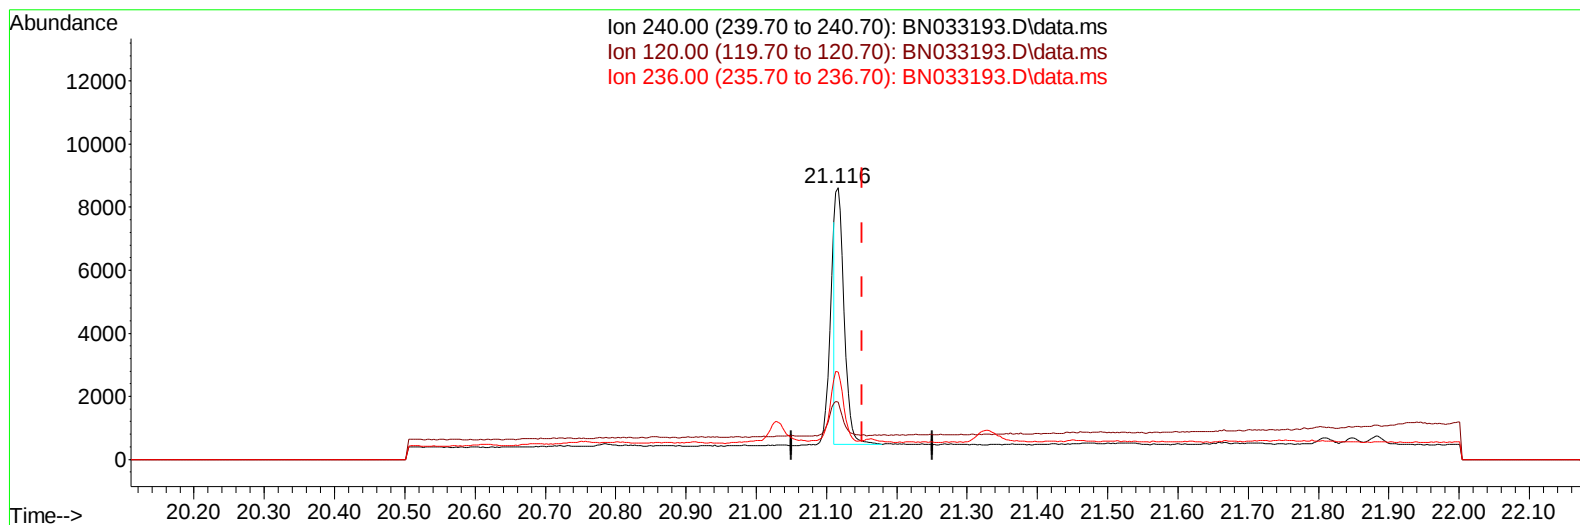

TIC: BN033193.D\data.ms

(17) Chrysene-d12

21.116min (-0.035) 0.40 ng/u1

response 7159

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	21.40	21.16
236.00	29.50	32.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

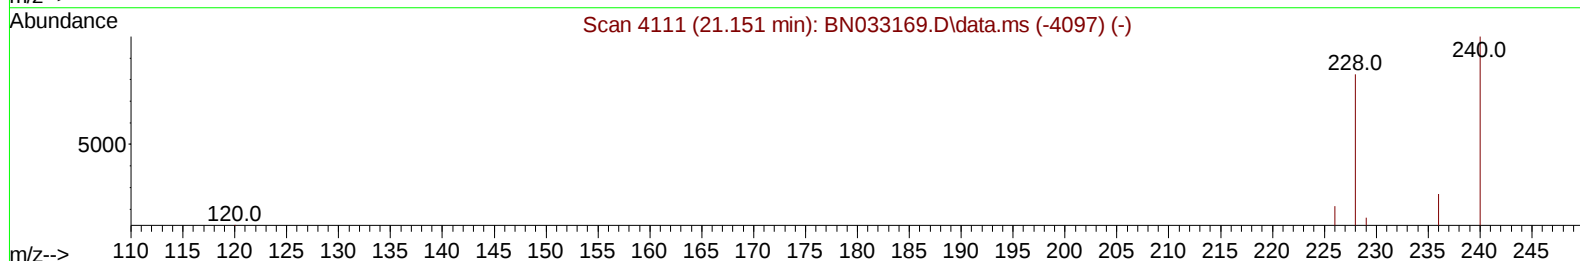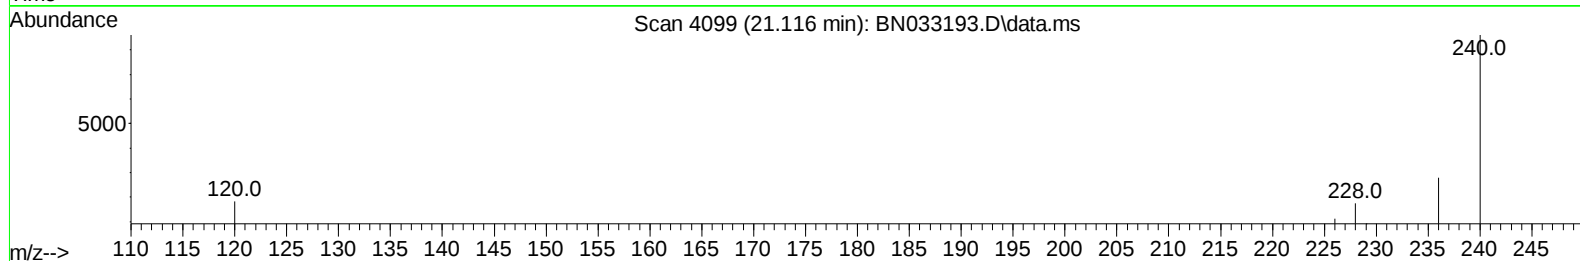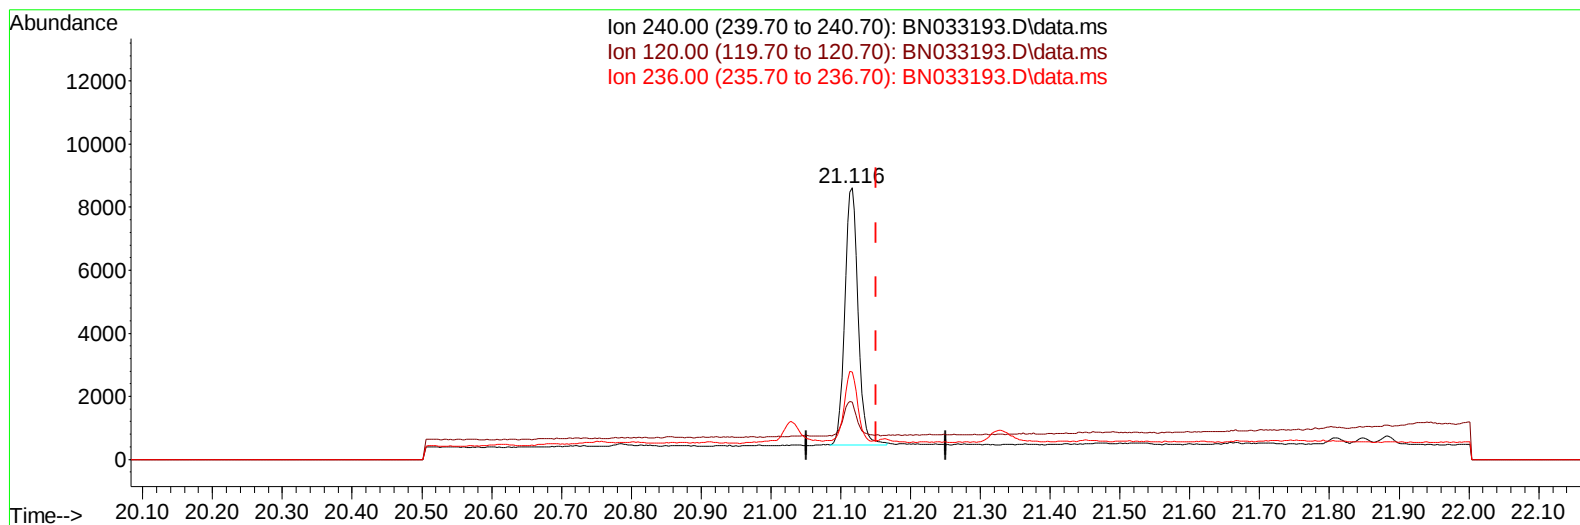

TIC: BN033193.D\data.ms

(17) Chrysene-d12

21.116min (-0.035) 0.40 ng/ul m

response 10775

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	21.40	21.16
236.00	29.50	32.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

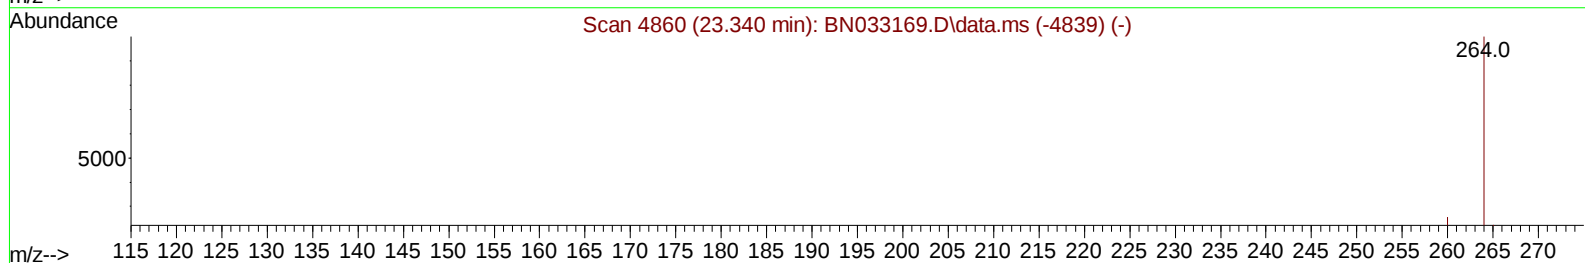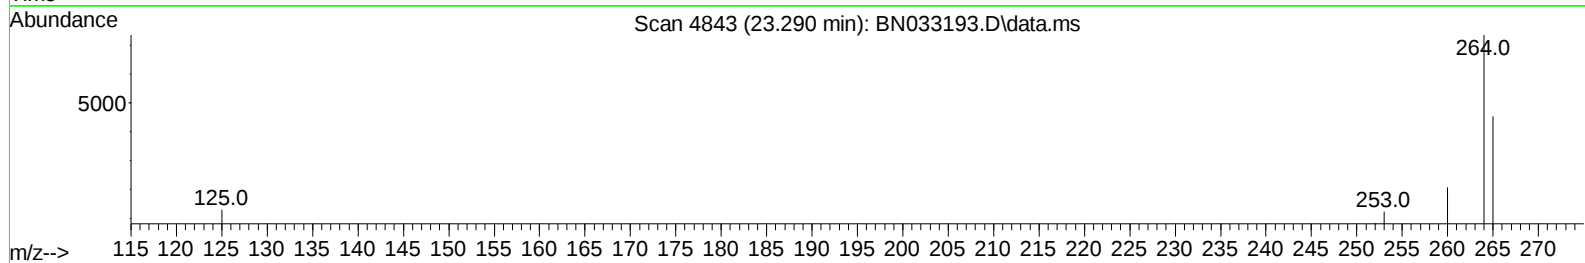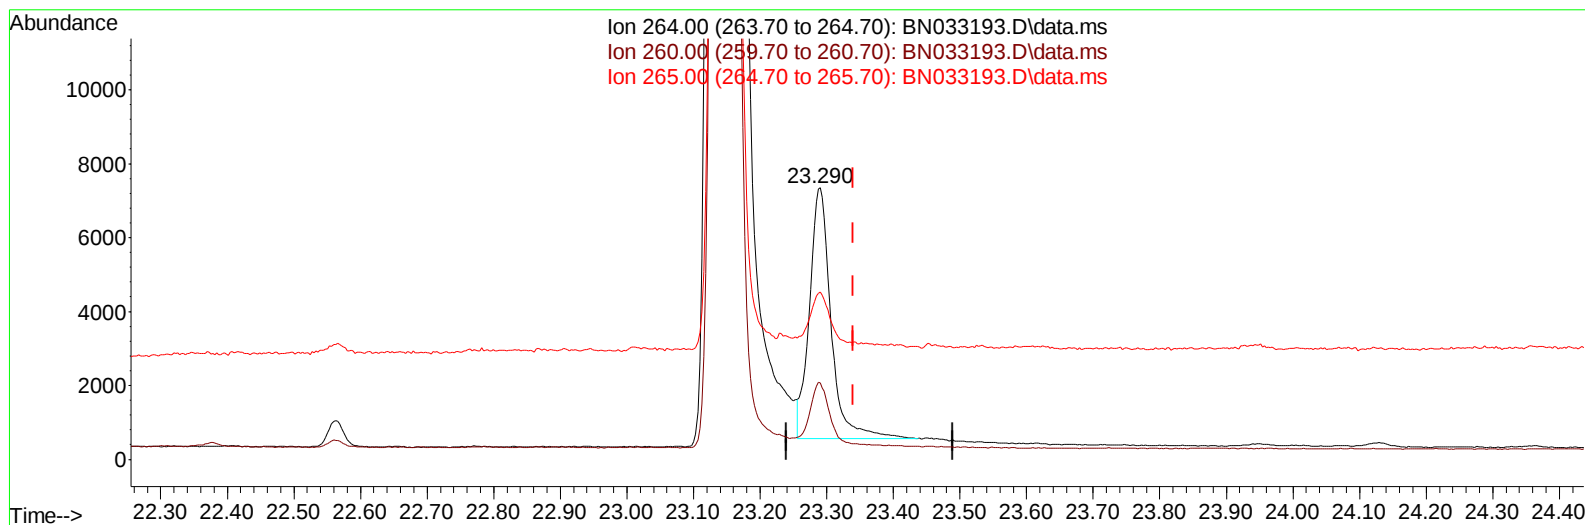

TIC: BN033193.D\data.ms

(23) Perylene-d12 (I)

23.290min (-0.049) 0.40 ng/u1

response 15286

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.50	28.12
265.00	80.60	61.60#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

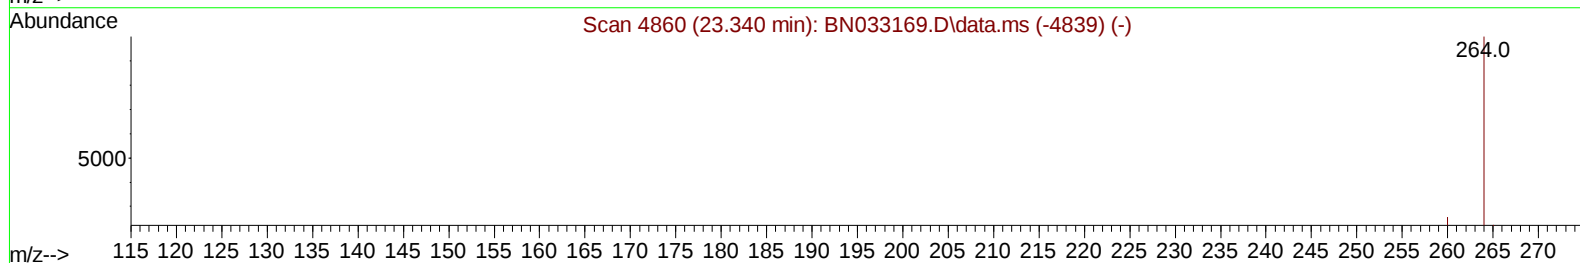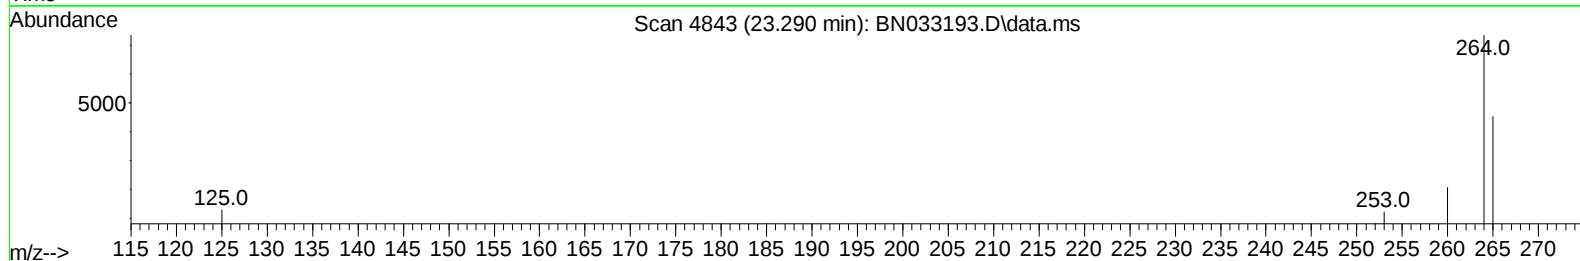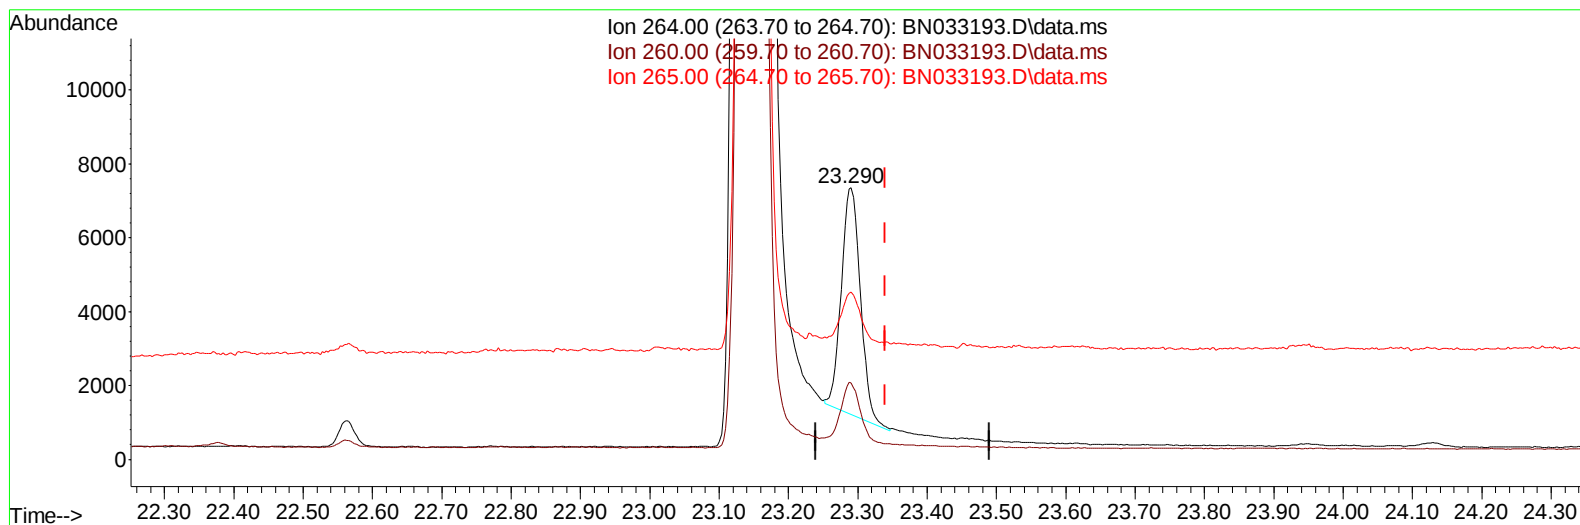

TIC: BN033193.D\data.ms

(23) Perylene-d12 (I)

23.290min (-0.049) 0.40 ng/ul m

response 11705

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.50	28.12
265.00	80.60	61.60#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

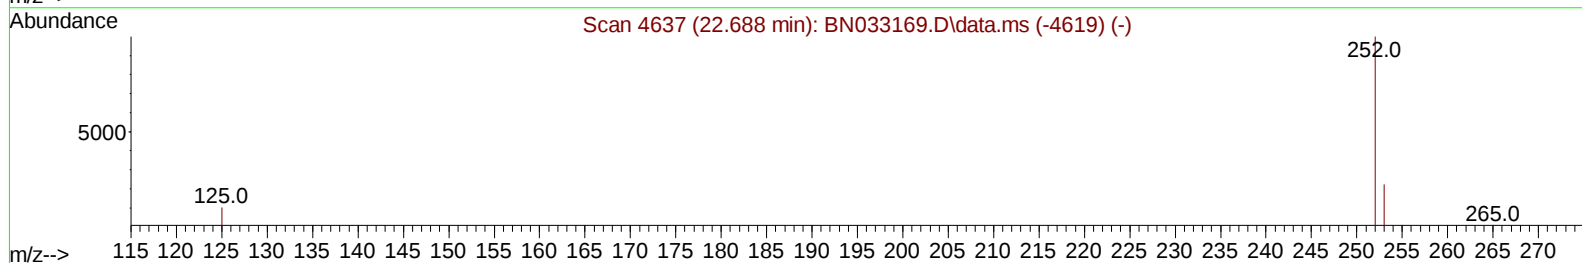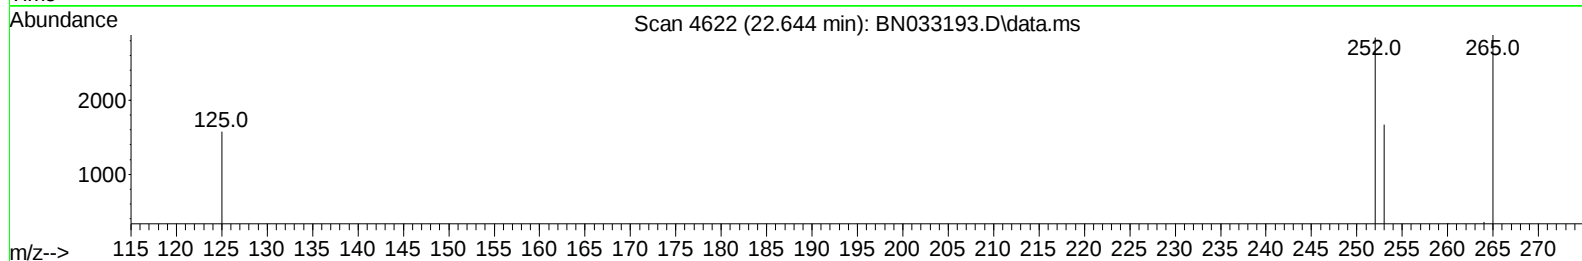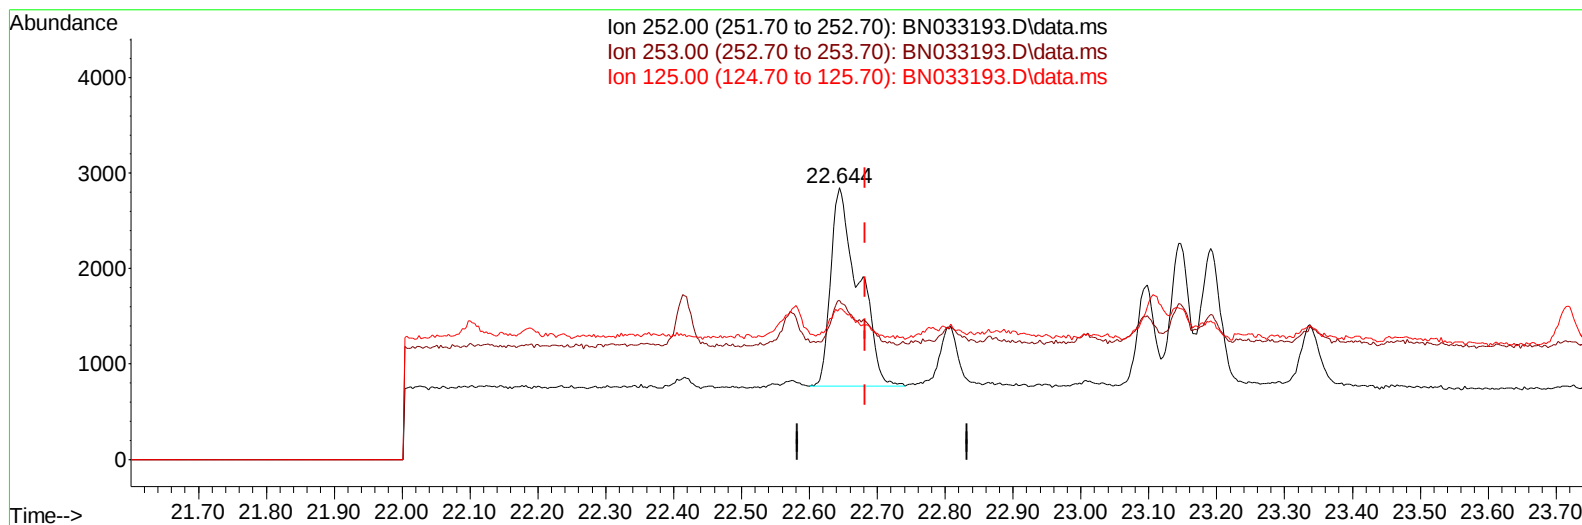

TIC: BN033193.D\data.ms

(24) Benzo(b)fluoranthene

22.644min (-0.038) 0.17 ng/u1

response 5910

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	30.30	58.59
125.00	25.50	55.43#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

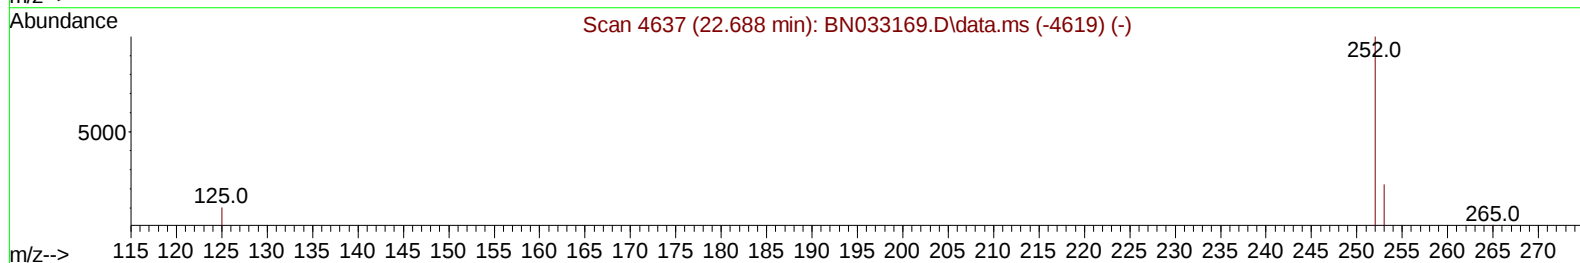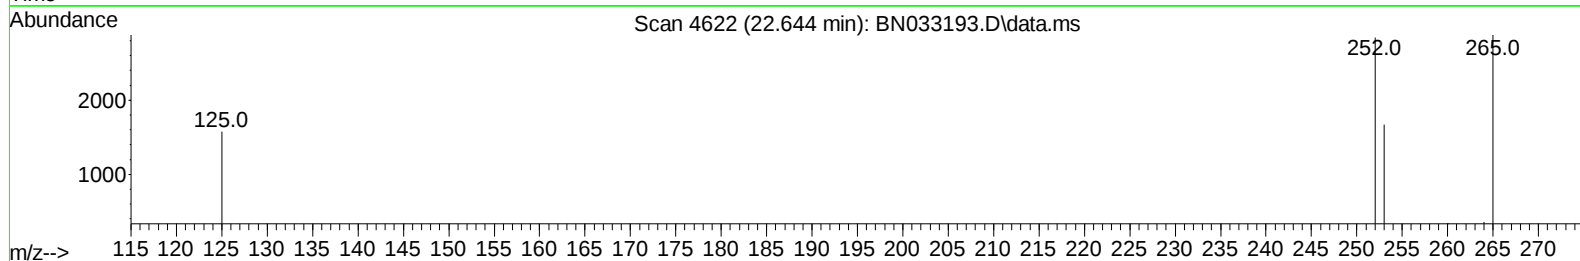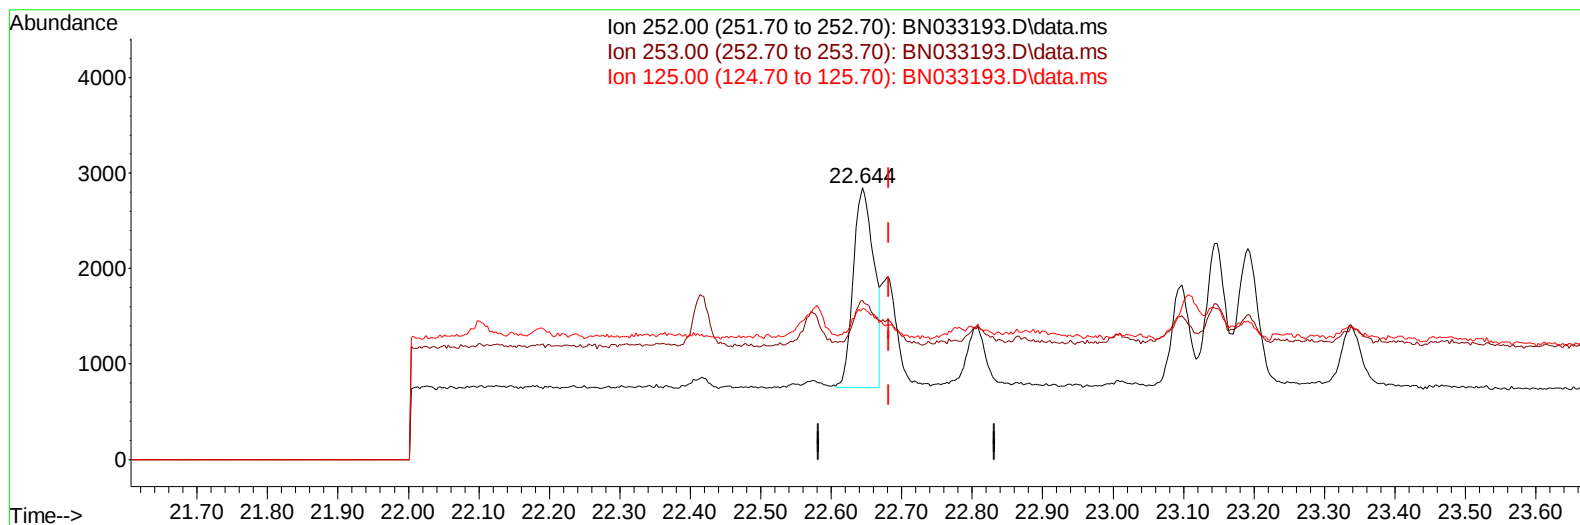

TIC: BN033193.D\data.ms

(24) Benzo(b)fluoranthene

22.644min (-0.038) 0.12 ng/ul m

response 4200

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	30.30	58.59
125.00	25.50	55.43#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
 Data File : BN033193.D
 Acq On : 02 Aug 2024 07:33
 Operator : MA/JU
 Sample : P3378-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
 Supervised By :mohammad ahmed 08/03/2024

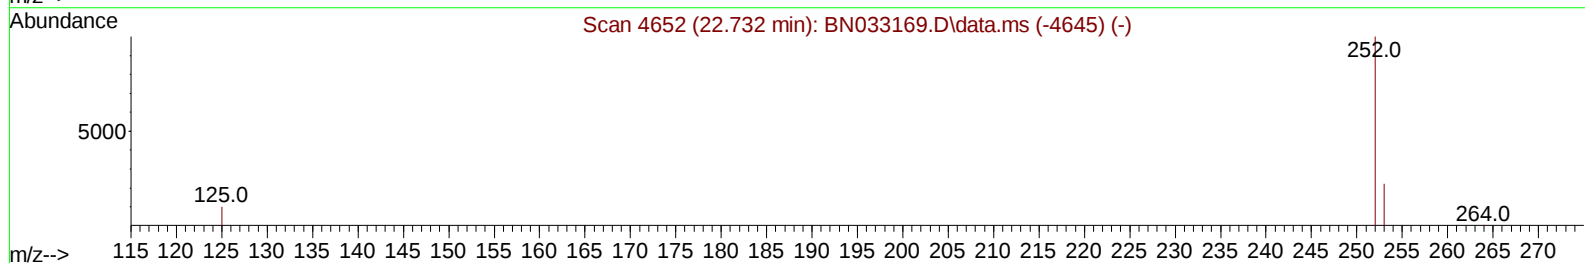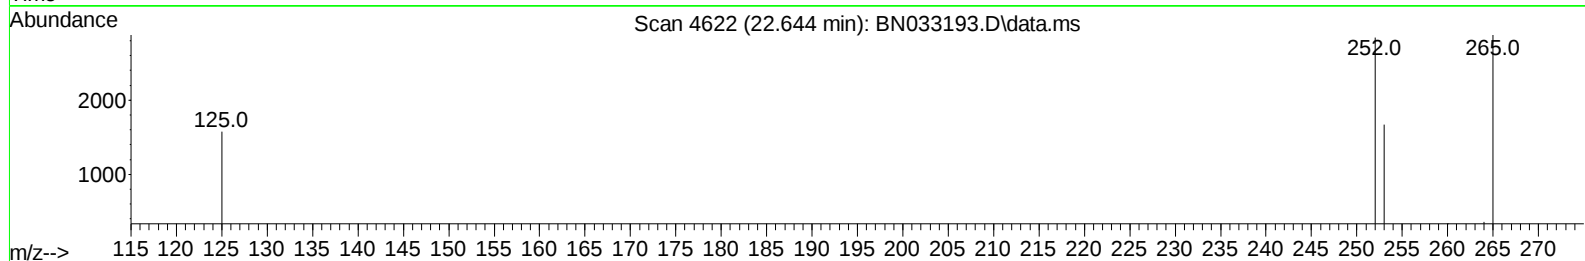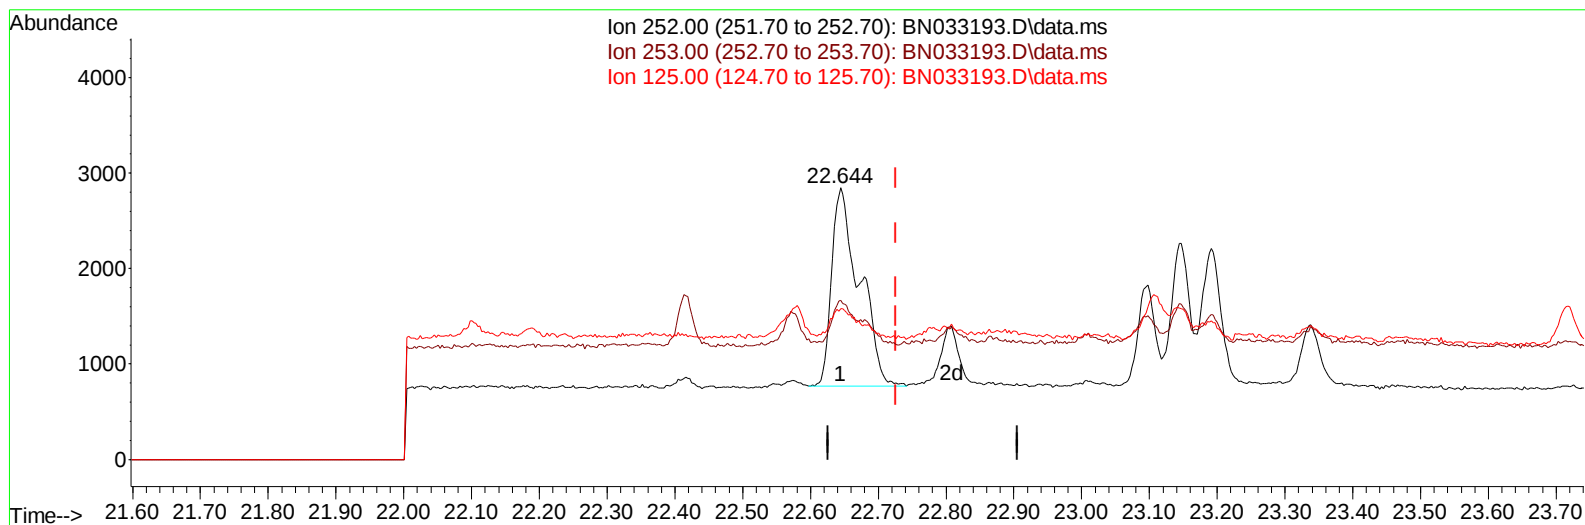

TIC: BN033193.D\data.ms

(25) Benzo(k)fluoranthene

22.644min (-0.082) 0.14 ng/u1

response 5914

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	31.10	58.59#
125.00	26.10	55.43#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

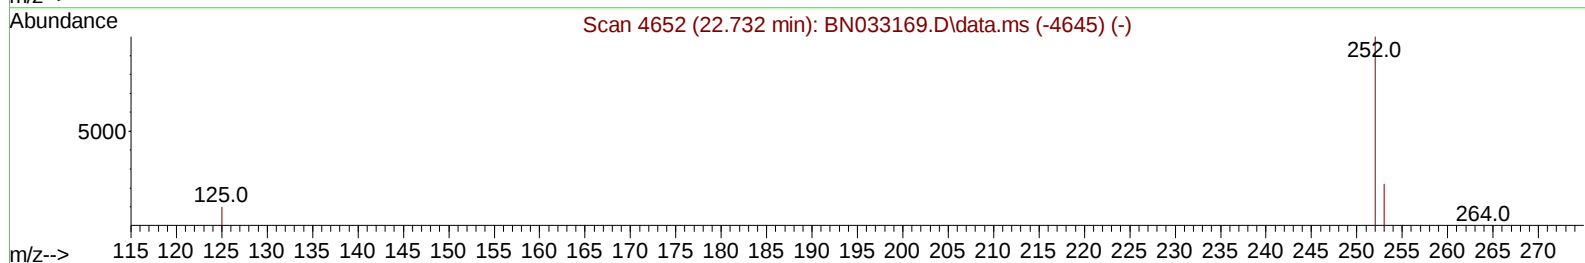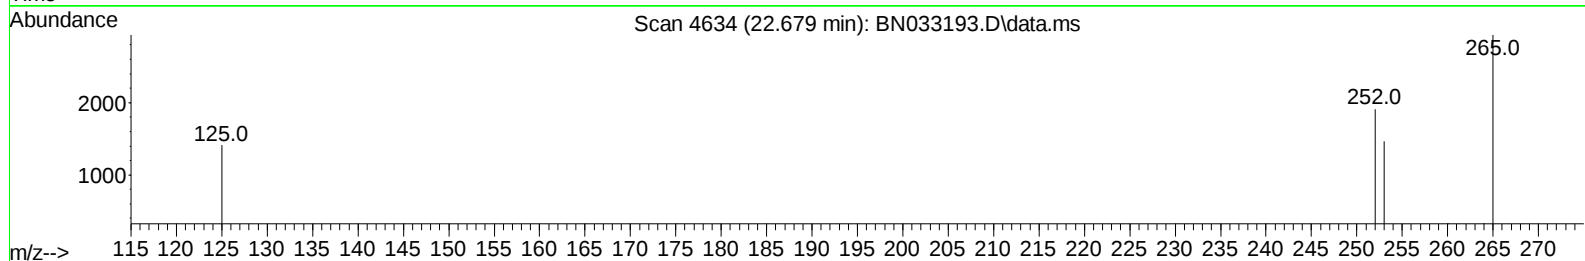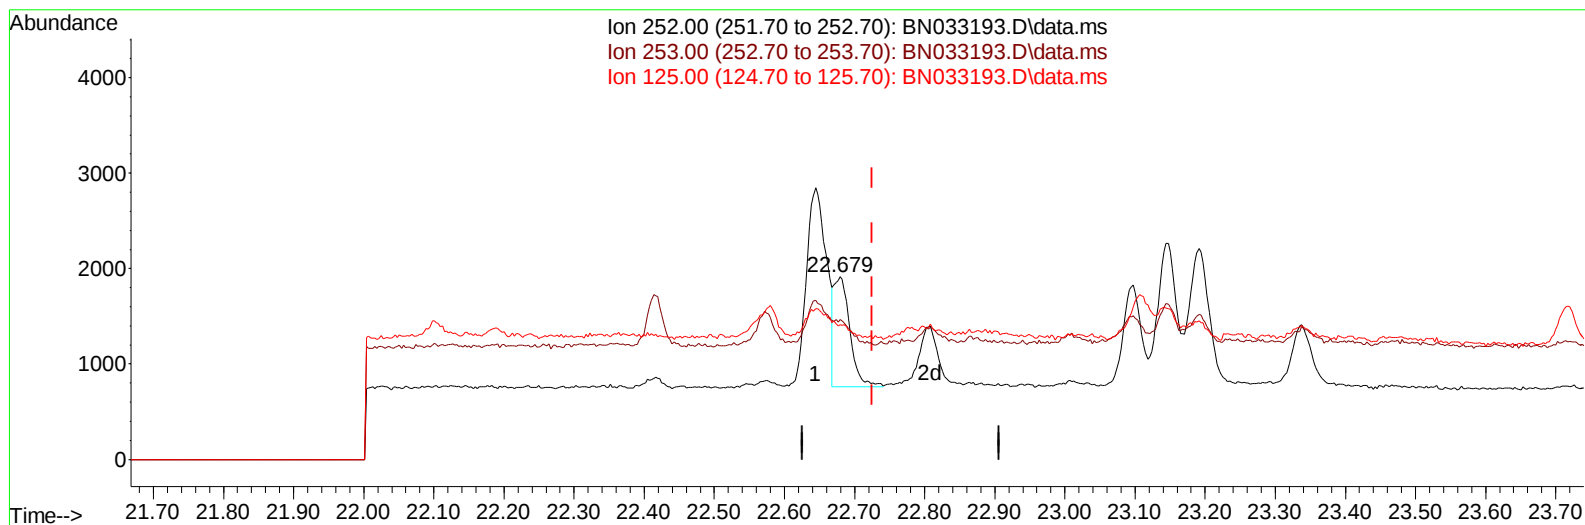

TIC: BN033193.D\data.ms

(25) Benzo(k)fluoranthene

22.679min (-0.047) 0.04 ng/u1 m

response 1808

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	31.10	76.78#
125.00	26.10	73.69#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
 Data File : BN033193.D
 Acq On : 02 Aug 2024 07:33
 Operator : MA/JU
 Sample : P3378-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AX2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
 Supervised By :mohammad ahmed 08/03/2024

Quant Time: Aug 02 08:01:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.465	152	4111m	0.400	ng/ul	-0.08
4) Naphthalene-d8	10.223	136	13534	0.400	ng/ul	#-0.09
9) Acenaphthene-d10	14.111	164	8246	0.400	ng/ul	-0.05
13) Phenanthrene-d10	16.882	188	15883m	0.400	ng/ul	-0.06
17) Chrysene-d12	21.116	240	10775m	0.400	ng/ul	-0.03
23) Perylene-d12	23.290	264	11705m	0.400	ng/ul	-0.05
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.048	96	18149	3.490	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.835	152	4759	0.215	ng/ul	-0.09
18) Fluoranthene-d10	18.930	212	11247	0.369	ng/ul	-0.04
Target Compounds						
					Qvalue	
5) Naphthalene	10.273	128	28228	0.812	ng/ul#	94
7) 2-Methylnaphthalene	11.912	142	1292	0.055	ng/ul	100
8) 1-Methylnaphthalene	12.126	142	49002	1.925	ng/ul	100
10) Acenaphthylene	13.833	152	19971	0.592	ng/ul#	96
11) Acenaphthene	14.176	153	803933	31.670	ng/ul	98
12) Fluorene	15.175	166	342412	11.573	ng/ul	99
15) Phenanthrene	16.924	178	20922m	0.491	ng/ul	
16) Anthracene	17.017	178	42743m	1.116	ng/ul	
19) Fluoranthene	18.958	202	201334	5.675	ng/ul	98
20) Pyrene	19.325	202	154315	4.056	ng/ul	98
21) Benzo(a)anthracene	21.099	228	8271	0.225	ng/ul#	86
22) Chrysene	21.151	228	5874	0.137	ng/ul#	81
24) Benzo(b)fluoranthene	22.644	252	4200m	0.123	ng/ul	
25) Benzo(k)fluoranthene	22.679	252	1808m	0.044	ng/ul	
26) Benzo(a)pyrene	23.191	252	2614	0.081	ng/ul#	42
27) Indeno(1,2,3-cd)pyrene	25.477	276	1836	0.038	ng/ul#	98
29) Benzo(g,h,i)perylene	26.151	276	1735	0.045	ng/ul#	37

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033193.D
Acq On : 02 Aug 2024 07:33
Operator : MA/JU
Sample : P3378-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AX2

Manual IntegrationsAPPROVED

Quant Time: Aug 02 08:01:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

