

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
 Data File : BN033177.D
 Acq On : 01 Aug 2024 21:18
 Operator : MA/JU
 Sample : P3401-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1GG3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
 Supervised By :mohammad ahmed 08/03/2024

Quant Time: Aug 01 23:16:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.486	152	3016m	0.400	ng/ul	-0.06
4) Naphthalene-d8	10.234	136	10523	0.400	ng/ul	#-0.08
9) Acenaphthene-d10	14.125	164	5717	0.400	ng/ul	-0.04
13) Phenanthrene-d10	16.895	188	12103m	0.400	ng/ul	-0.05
17) Chrysene-d12	21.139	240	9005m	0.400	ng/ul	-0.01
23) Perylene-d12	23.314	264	6326m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.048	96	16298	4.272	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.857	152	3990	0.232	ng/ul	-0.07
18) Fluoranthene-d10	18.944	212	10052	0.394	ng/ul	-0.03
Target Compounds						Qvalue
5) Naphthalene	10.284	128	585	0.022	ng/ul#	68

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033177.D
Acq On : 01 Aug 2024 21:18
Operator : MA/JU
Sample : P3401-03
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E1GG3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024


Quant Time: Aug 01 23:16:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

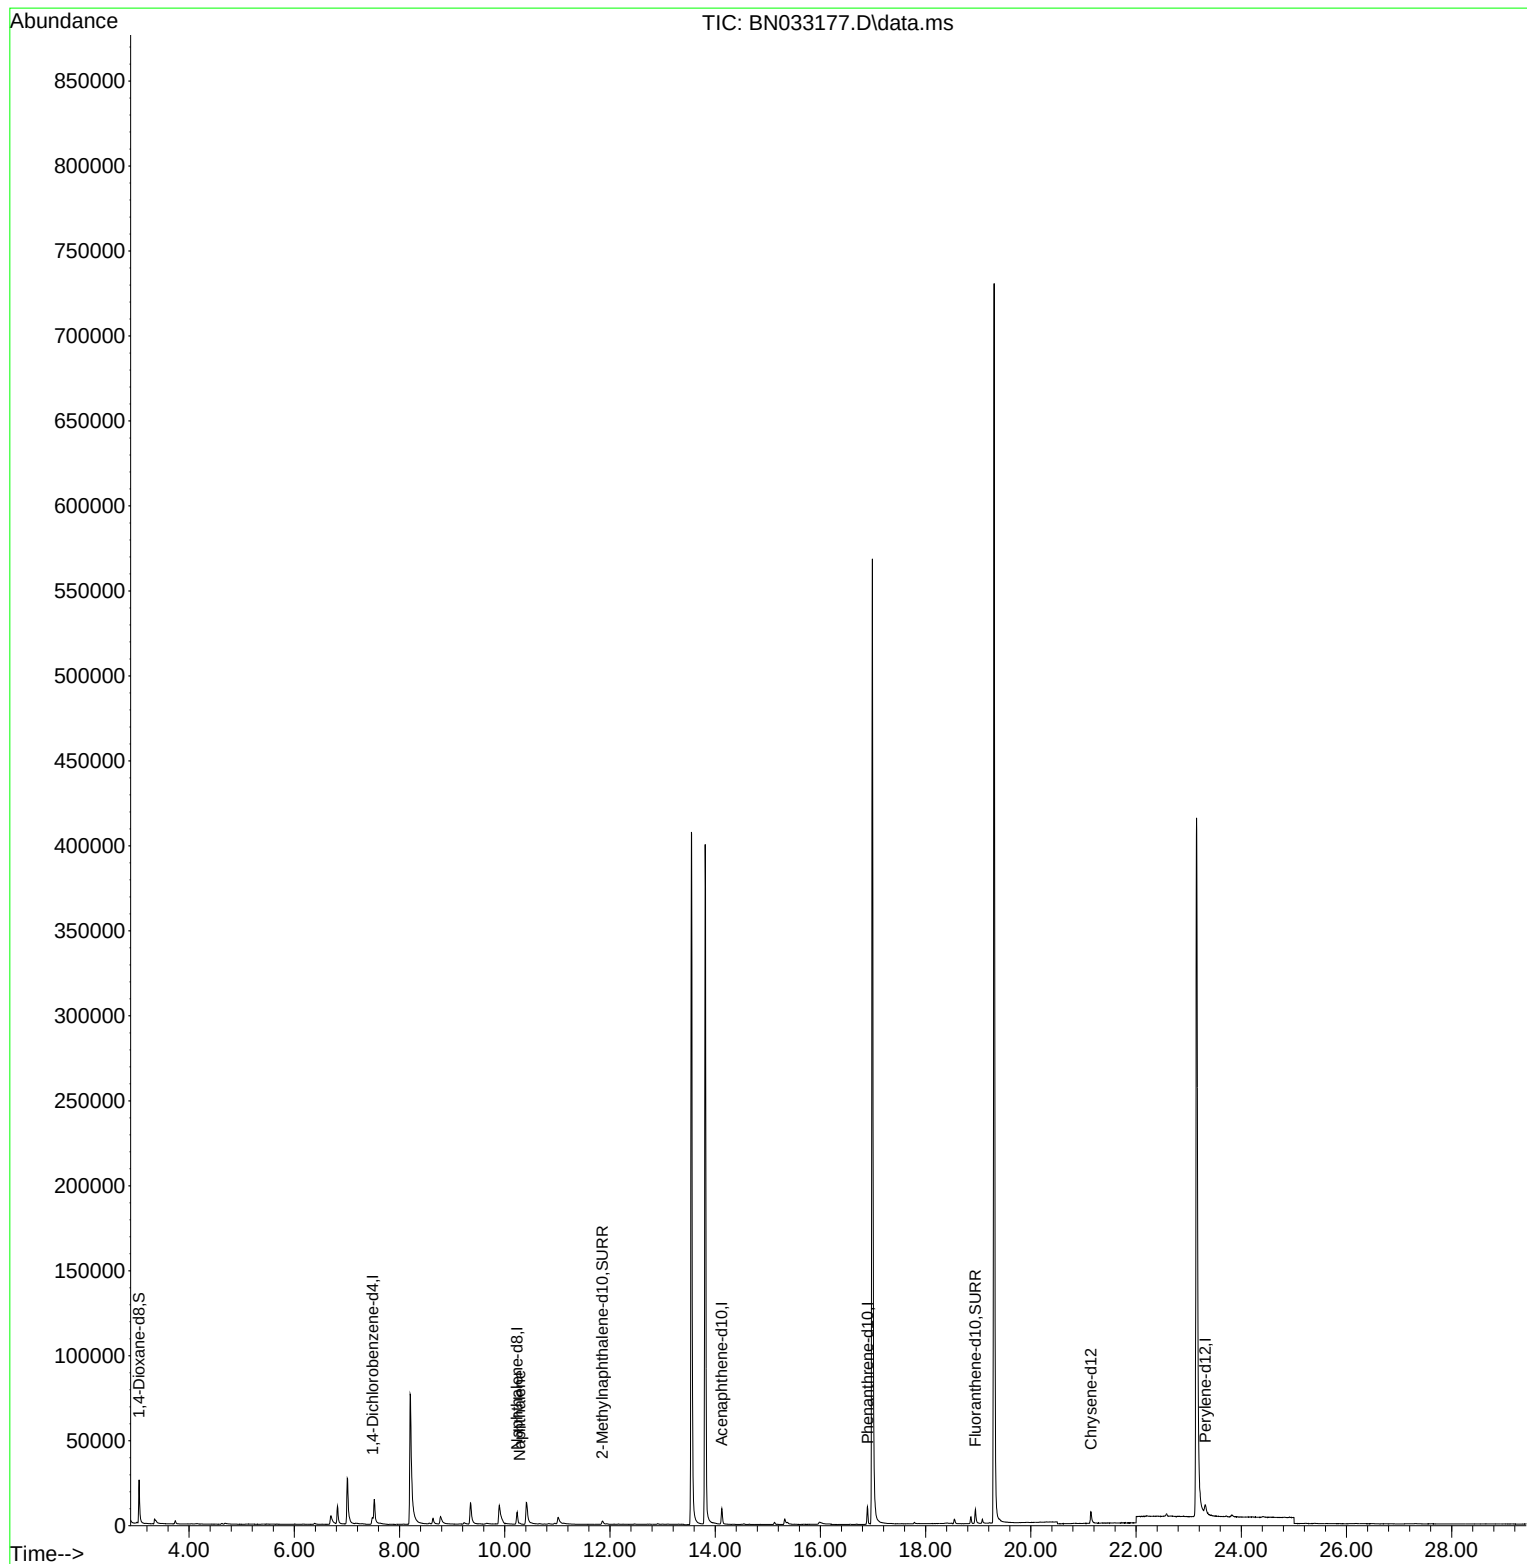

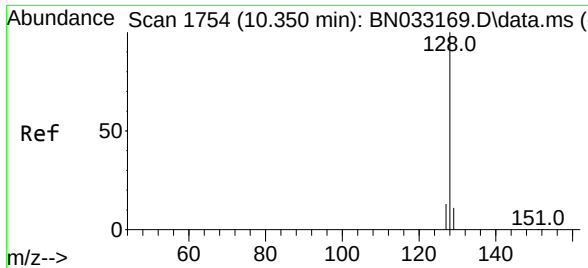

#5
Naphthalene
Concen: 0.022 ng/ul
RT: 10.284 min Scan# 1754
Delta R.T. -0.093 min
Lab File: BN033177.D
Acq: 01 Aug 2024 21:18

Instrument :
BNA_N
ClientSampleId :
E1GG3

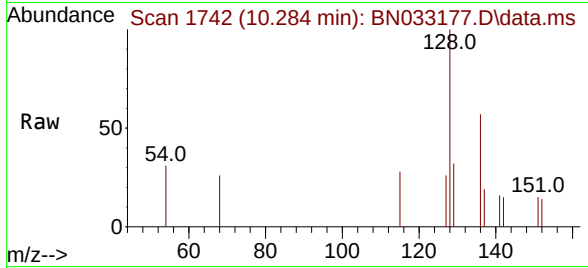

Tgt Ion:	128	Resp:	58
Ion	Ratio	Lower	Upper
128	100		
129	32.1	12.0	18.0
127	26.0	12.7	19.1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

