

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
 Data File : BN033181.D
 Acq On : 01 Aug 2024 23:42
 Operator : MA/JU
 Sample : P3359-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1GF1

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
 Supervised By :mohammad ahmed 08/03/2024

Quant Time: Aug 02 00:52:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 14:49:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.486	152	2942m	0.400	ng/ul	-0.06
4) Naphthalene-d8	10.234	136	9235	0.400	ng/ul	#-0.08
9) Acenaphthene-d10	14.124	164	5647	0.400	ng/ul	#-0.04
13) Phenanthrene-d10	16.894	188	11856m	0.400	ng/ul	-0.05
17) Chrysene-d12	21.154	240	8490	0.400	ng/ul	0.00
23) Perylene-d12	23.317	264	4884m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.047	96	16948	4.554	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.873	152	4424	0.294	ng/ul	-0.05
18) Fluoranthene-d10	18.949	212	10120	0.421	ng/ul	-0.02
Target Compounds						
					Qvalue	
5) Naphthalene	10.284	128	967	0.041	ng/ul#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN080224\
Data File : BN033181.D
Acq On : 01 Aug 2024 23:42
Operator : MA/JU
Sample : P3359-13
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E1GF1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024


Quant Time: Aug 02 00:52:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN072524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 14:49:49 2024
Response via : Initial Calibration

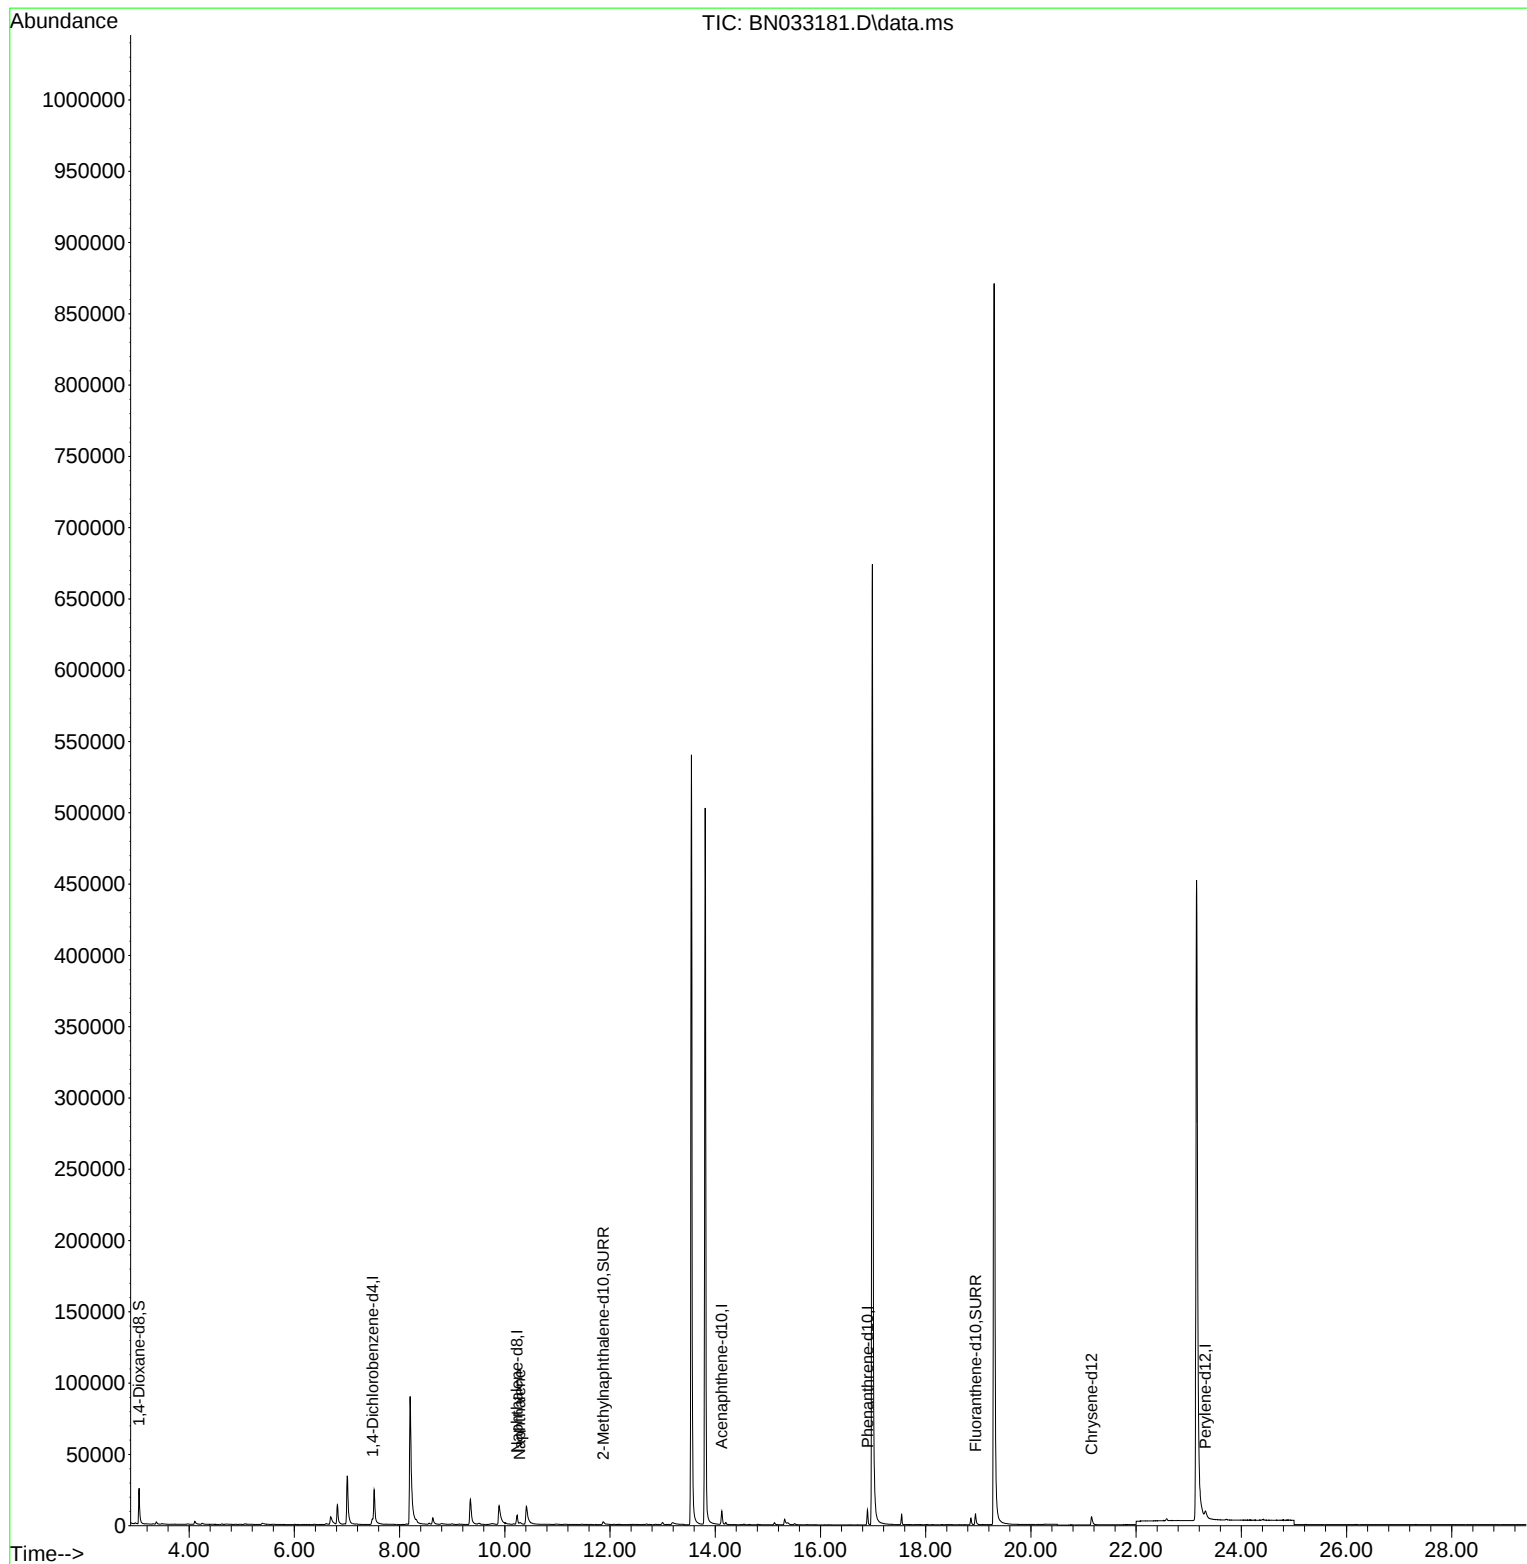

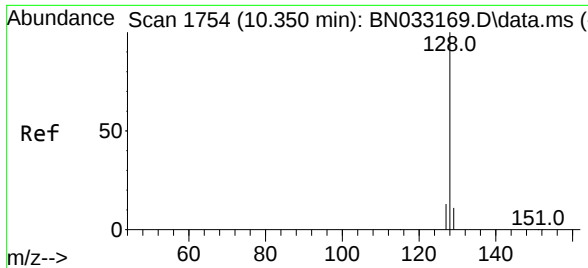

#5
Naphthalene
Concen: 0.041 ng/ul
RT: 10.284 min Scan# 11
Delta R.T. -0.093 min
Lab File: BN033181.D
Acq: 01 Aug 2024 23:42

Instrument :
BNA_N
ClientSampleId :
E1GF1

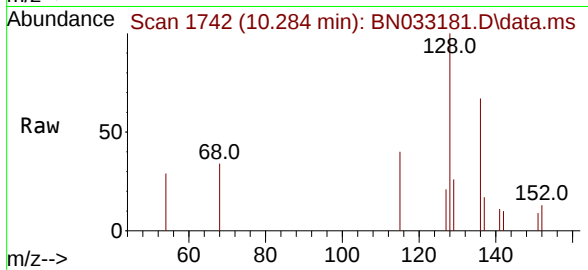

Tgt Ion:128 Resp: 96
Ion Ratio Lower Upper
128 100
129 25.6 12.0 18.0
127 21.0 12.7 19.1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/02/2024
Supervised By :mohammad ahmed 08/03/2024

